

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121619\
 Data File : P0064713.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Dec 2019 17:12
 Operator : SM/AJ
 Sample : K6294-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 00:38:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 13 08:19:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.179	3.455	664529	833266	27.296	32.871
2) SA Decachlor...	9.695	8.375	584678	694469	19.051	19.997

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121619\
Data File : P0064713.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Dec 2019 17:12
Operator : SM/AJ
Sample : K6294-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 00:38:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 13 08:19:24 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

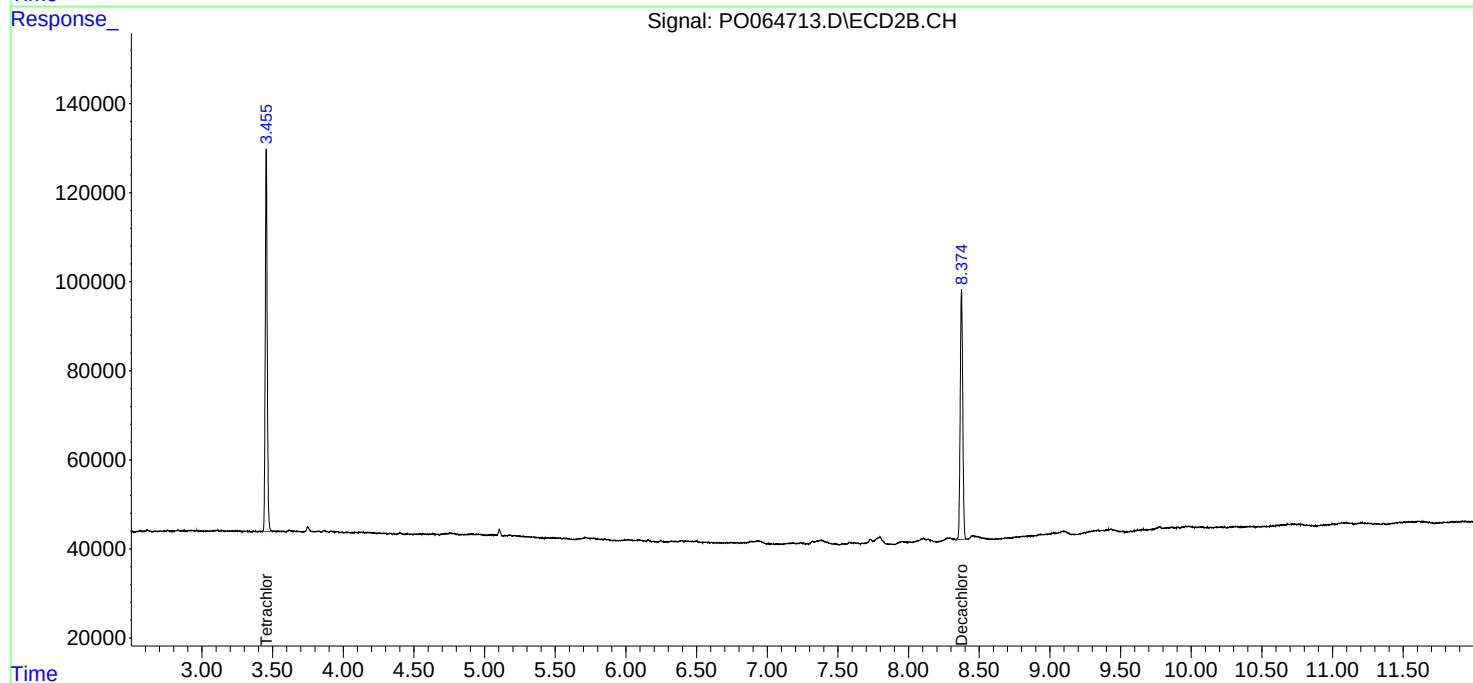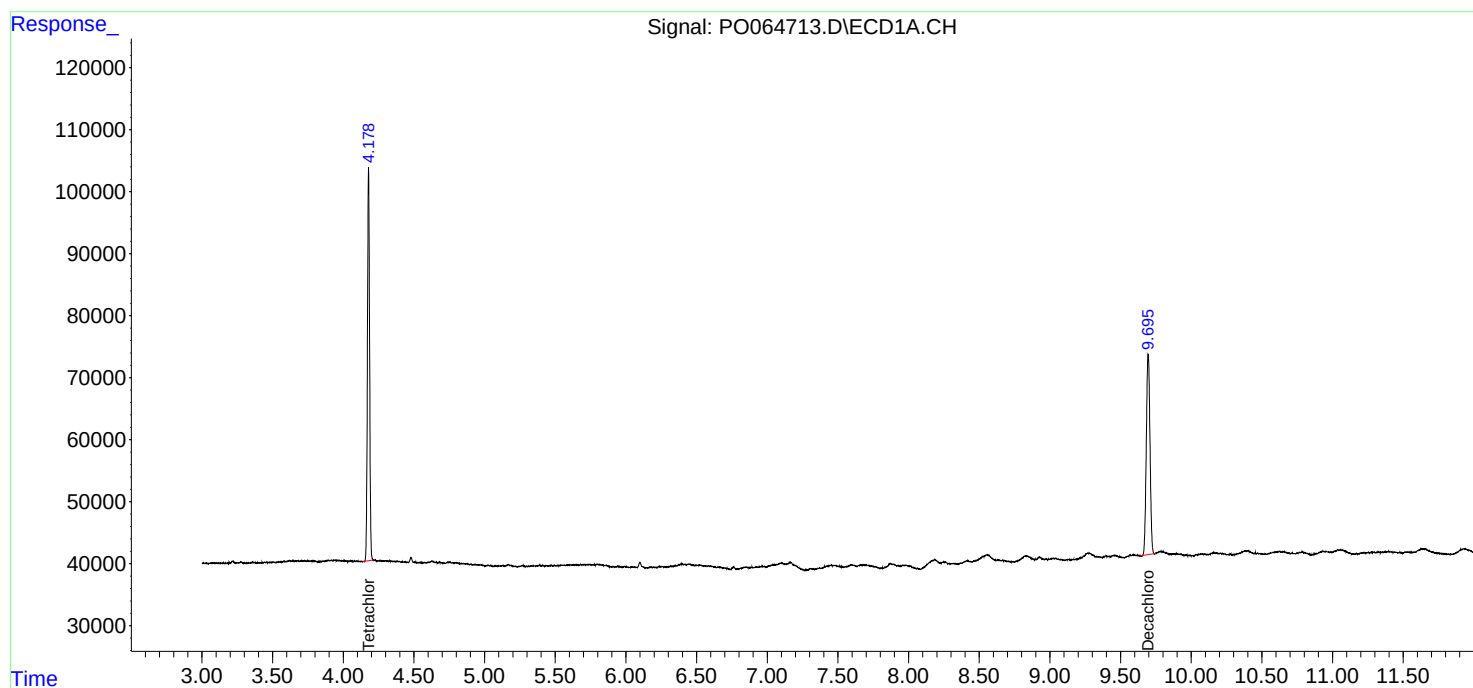


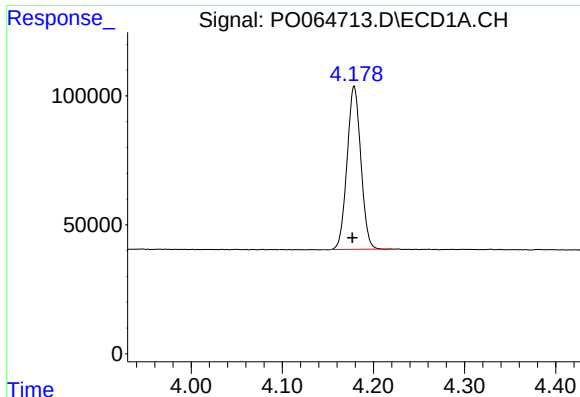

#1 Tetrachloro-m-xylene


R.T.: 4.179 min
Delta R.T.: 0.002 min
Response: 664529
Conc: 27.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1

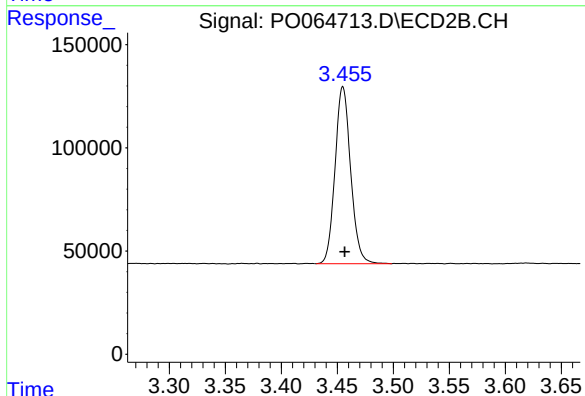


#1 Tetrachloro-m-xylene

R.T.: 3.455 min
Delta R.T.: -0.002 min
Response: 833266
Conc: 32.87 ng/ml

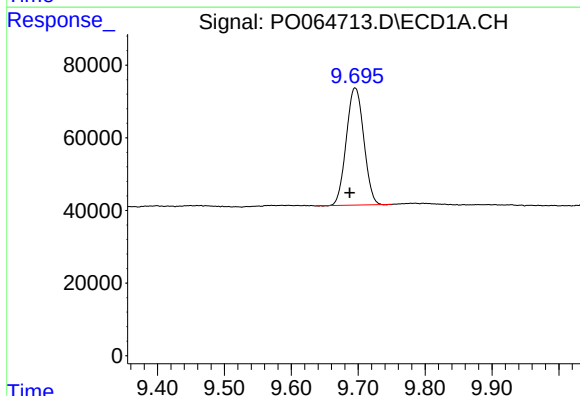

#2 Decachlorobiphenyl

R.T.: 9.695 min
Delta R.T.: 0.008 min
Response: 584678
Conc: 19.05 ng/ml

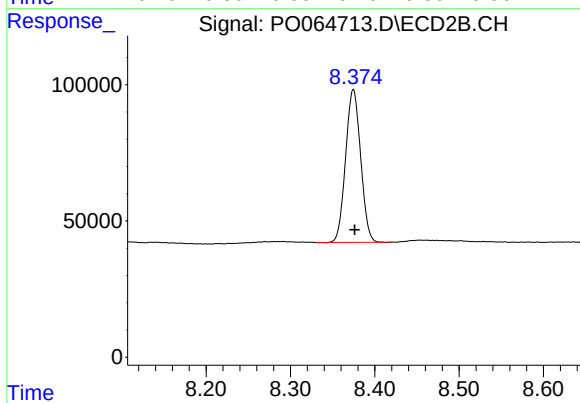

#2 Decachlorobiphenyl

R.T.: 8.375 min
Delta R.T.: -0.002 min
Response: 694469
Conc: 20.00 ng/ml