

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121619\
 Data File : P0064728.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Dec 2019 21:24
 Operator : SM/AJ
 Sample : K6309-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 30789

Manual Integrations
 APPROVED

Ankita
 12/17/2019 10:46:07 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 00:43:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 13 08:19:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.179	3.455	501149	692198	20.585	27.306m#
2) SA Decachlor...	9.697	8.374	742181	911439	24.183	26.245

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121619\
Data File : P0064728.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Dec 2019 21:24
Operator : SM/AJ
Sample : K6309-06
Misc :
ALS Vial : 24 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
30789


Manual Integrations
APPROVED

Ankita
12/17/2019 10:46:07 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 00:43:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 13 08:19:24 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

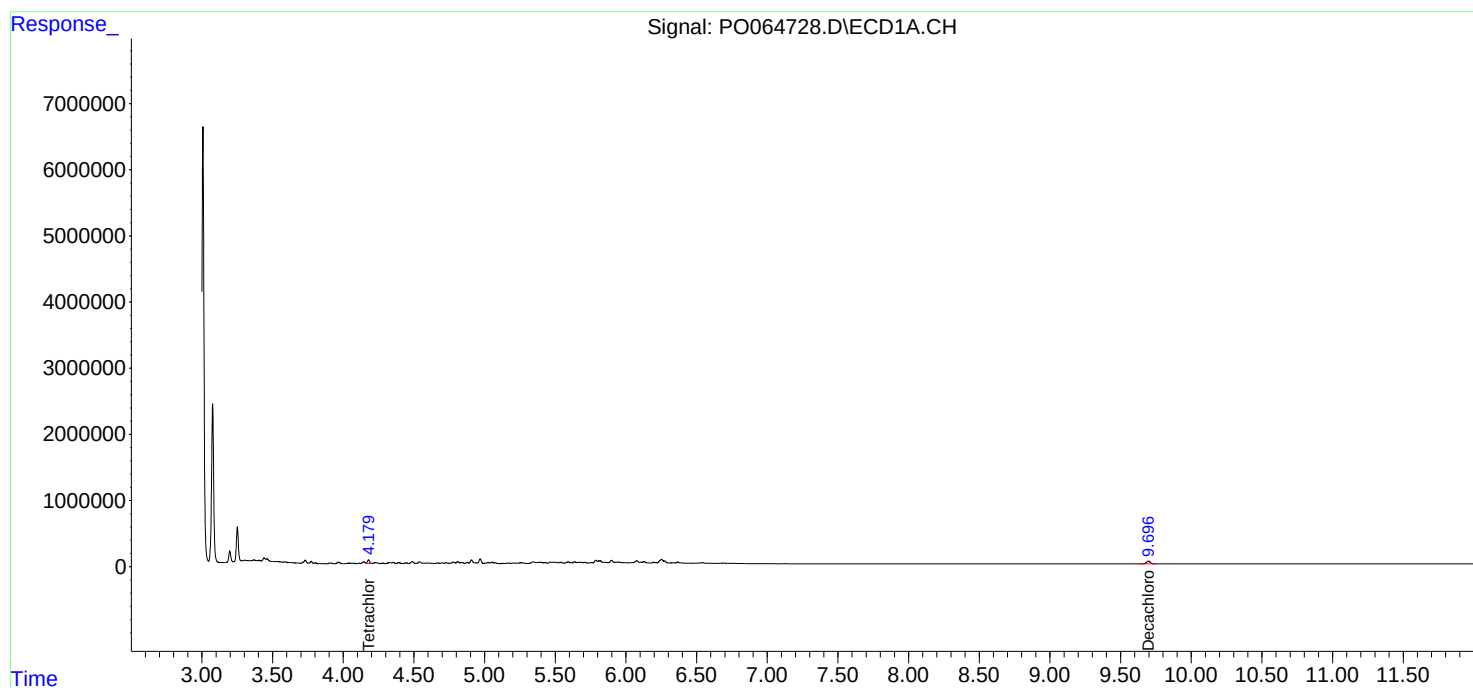

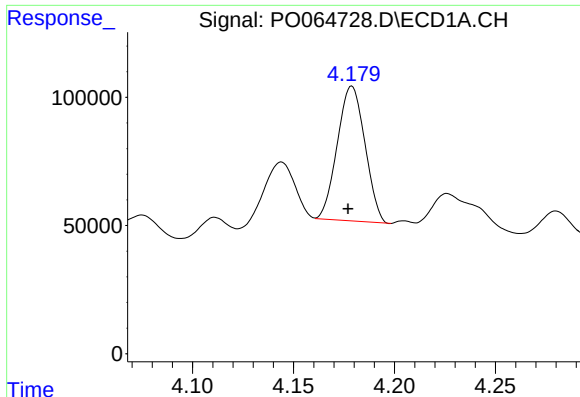


#1 Tetrachloro-m-xylene

R.T.: 4.179 min
Delta R.T.: 0.002 min
Response: 501149
Conc: 20.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
30789


Manual Integrations
APPROVED

Ankita
12/17/2019 10:46:07 AM

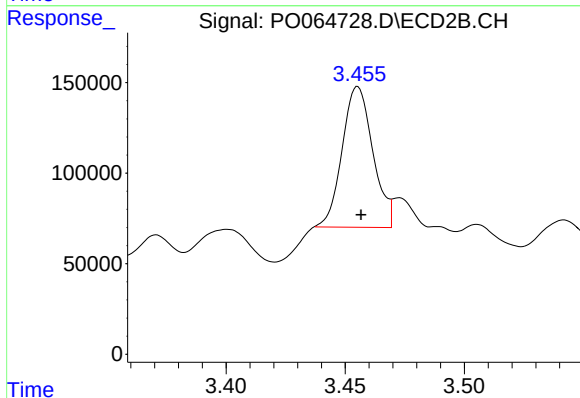


#1 Tetrachloro-m-xylene

R.T.: 3.455 min
Delta R.T.: -0.002 min
Response: 692198
Conc: 27.31 ng/ml m

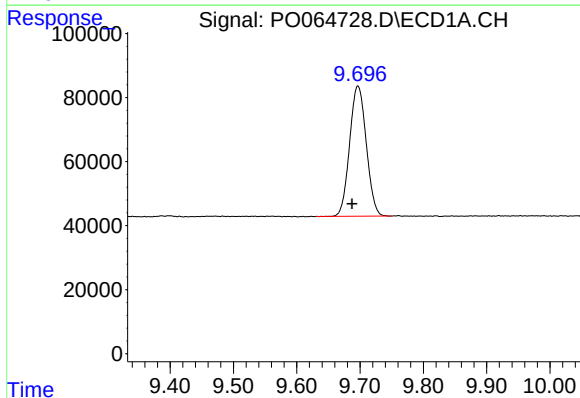

#2 Decachlorobiphenyl

R.T.: 9.697 min
Delta R.T.: 0.009 min
Response: 742181
Conc: 24.18 ng/ml

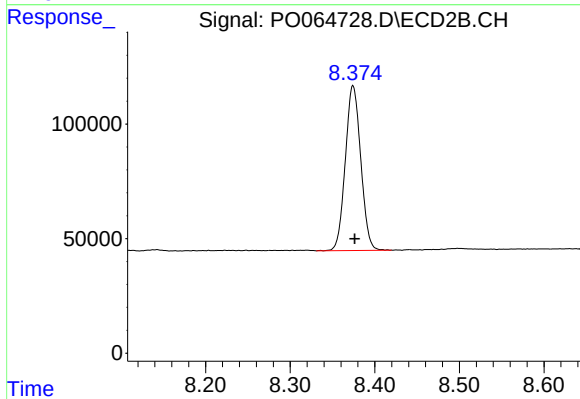

#2 Decachlorobiphenyl

R.T.: 8.374 min
Delta R.T.: -0.002 min
Response: 911439
Conc: 26.24 ng/ml