

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0121619\
 Data File : P0064730.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Dec 2019 21:57
 Operator : SM/AJ
 Sample : K6310-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 SP-01

Manual Integrations
 APPROVED

Ankita
 12/17/2019 10:46:09 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 00:43:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0121319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 13 08:19:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.180	3.455	894310	1078543	36.735	42.547
2) SA Decachlor...	9.699	8.375	855461	1012079	27.874	29.143
Target Compounds						
31) L7 AR-1260-1	6.916	5.984	37979	43734	24.721	23.685
32) L7 AR-1260-2	7.168	6.172	141536	51723	71.700	22.231 #
33) L7 AR-1260-3	7.526	6.323	38179	42603	25.409m	20.121
34) L7 AR-1260-4	7.750	6.790	43048	39676	23.304m	21.061m
35) L7 AR-1260-5	8.058	7.032	56135	85923	15.043	18.320

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121619\
Data File : PO064730.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Dec 2019 21:57
Operator : SM/AJ
Sample : K6310-03
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SP-01


Manual Integrations
APPROVED

Ankita
12/17/2019 10:46:09 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 00:43:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 13 08:19:24 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

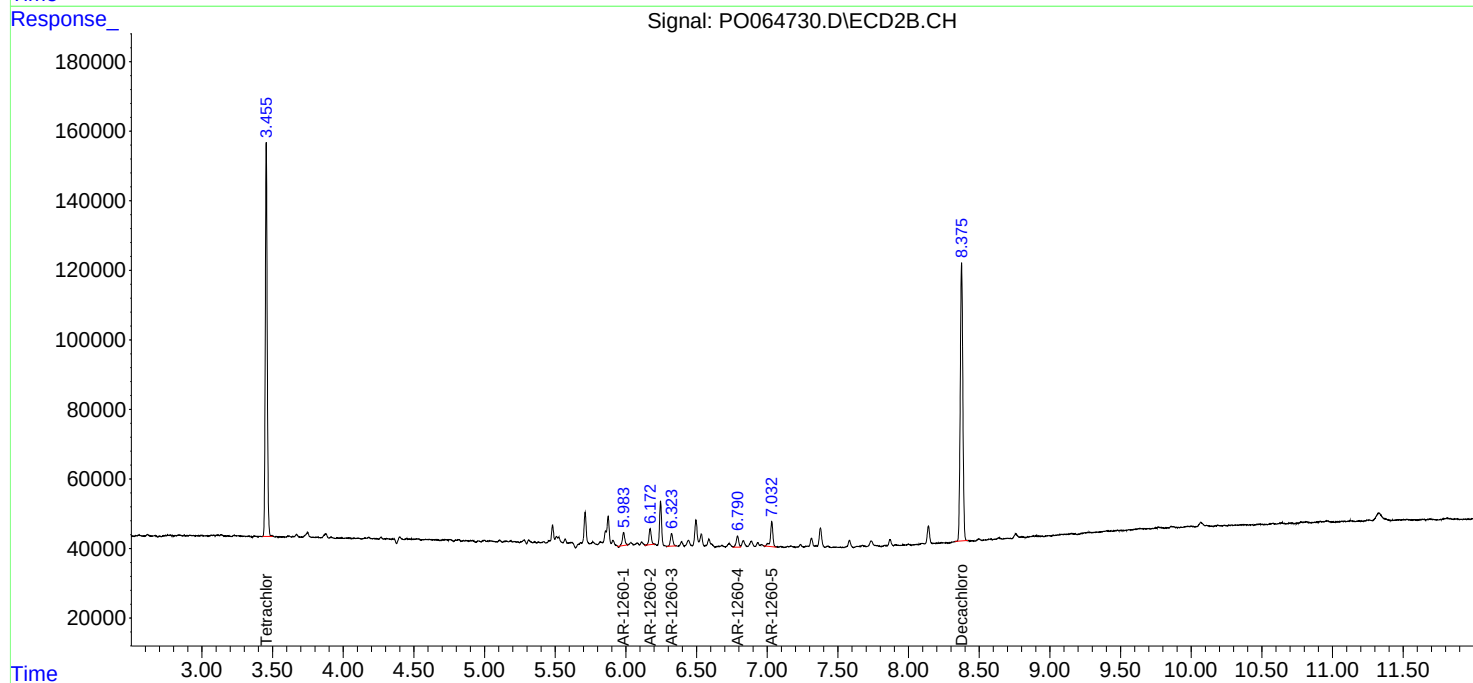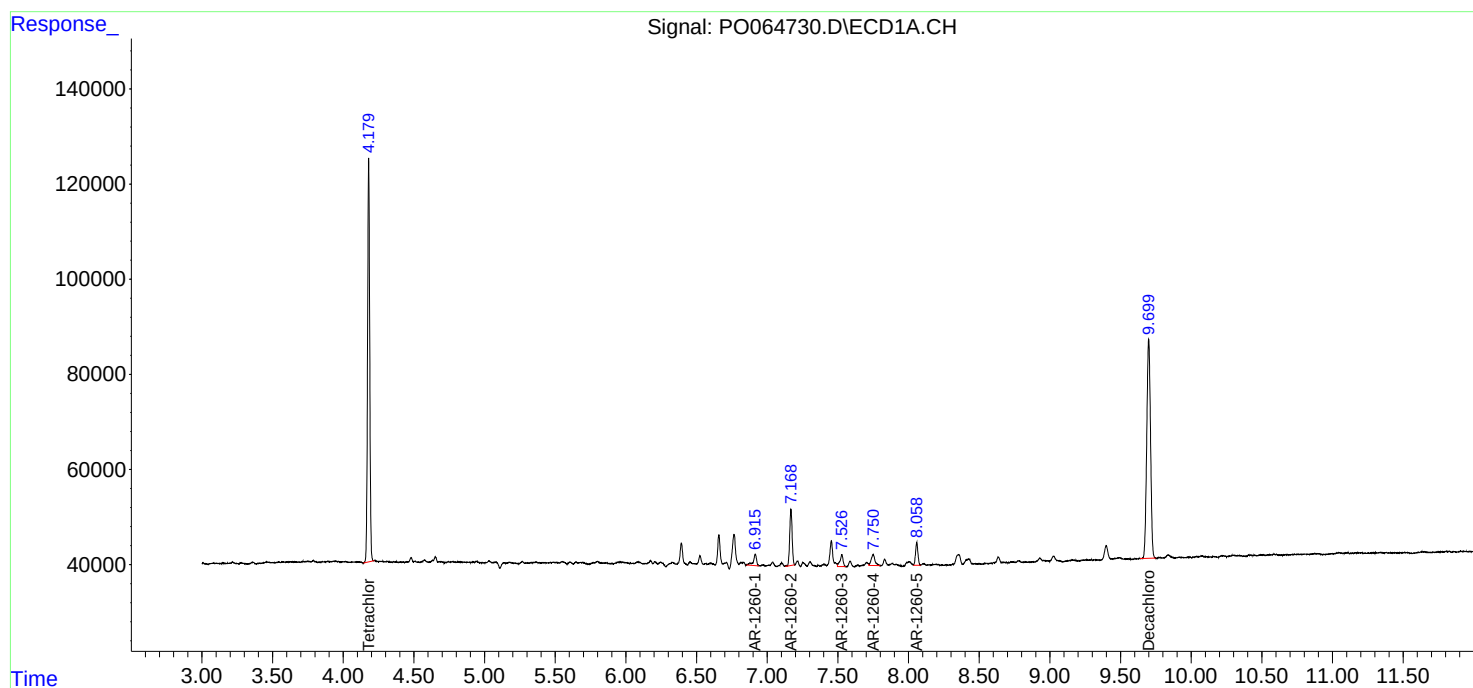

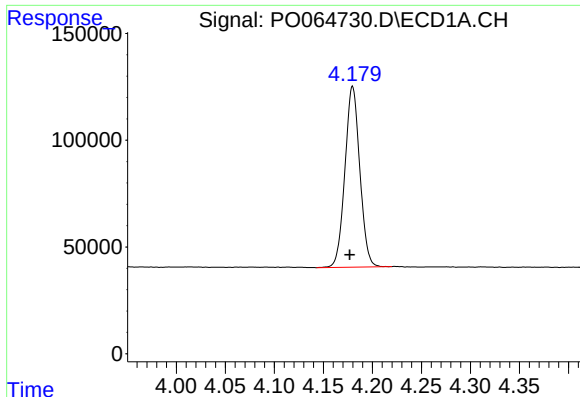


#1 Tetrachloro-m-xylene

R.T.: 4.180 min
Delta R.T.: 0.003 min
Response: 894310
Conc: 36.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-01


Manual Integrations
APPROVED

Ankita
12/17/2019 10:46:09 AM

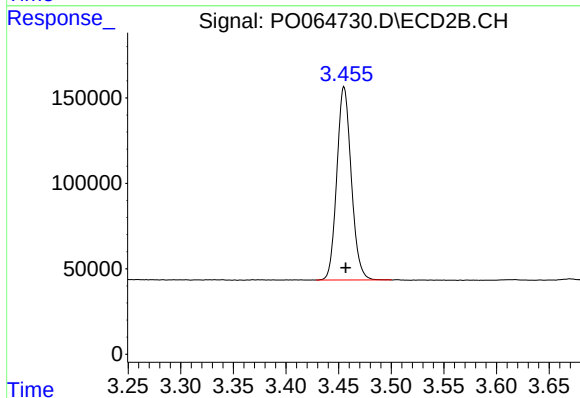


#1 Tetrachloro-m-xylene

R.T.: 3.455 min
Delta R.T.: -0.002 min
Response: 1078543
Conc: 42.55 ng/ml

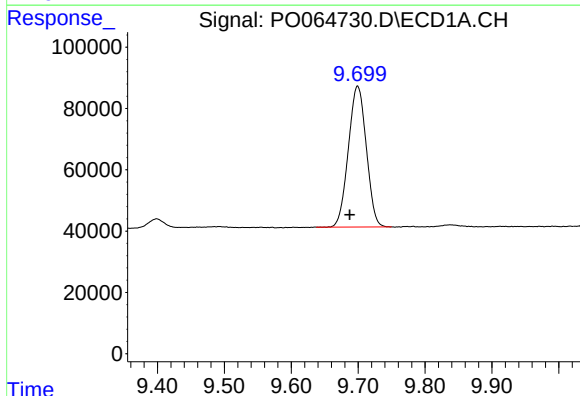


#2 Decachlorobiphenyl

R.T.: 9.699 min
Delta R.T.: 0.012 min
Response: 855461
Conc: 27.87 ng/ml

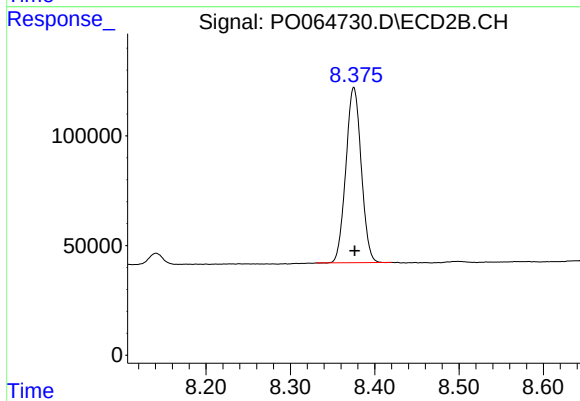

#2 Decachlorobiphenyl

R.T.: 8.375 min
Delta R.T.: 0.000 min
Response: 1012079
Conc: 29.14 ng/ml

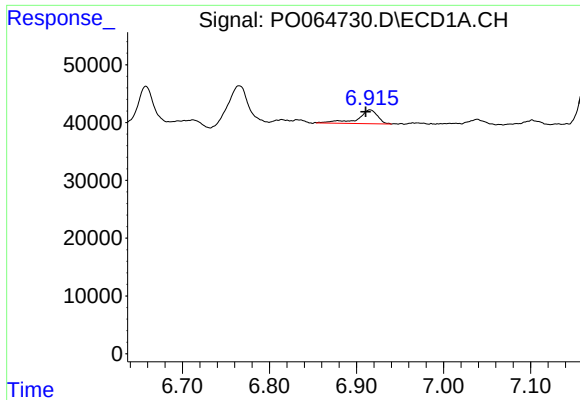


#31 AR-1260-1

R.T.: 6.916 min
Delta R.T.: 0.005 min
Response: 37979
Conc: 24.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-01


Manual Integrations
APPROVED

Ankita
12/17/2019 10:46:09 AM

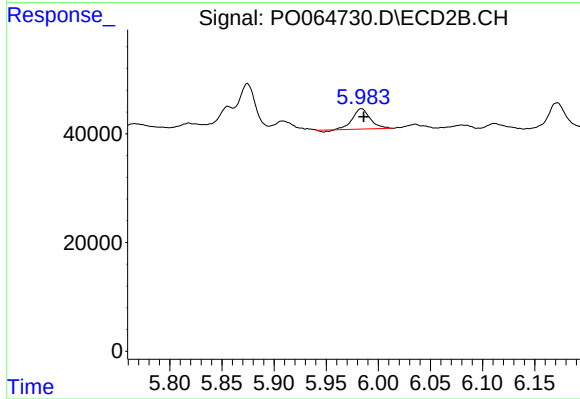


#31 AR-1260-1

R.T.: 5.984 min
Delta R.T.: -0.002 min
Response: 43734
Conc: 23.68 ng/ml

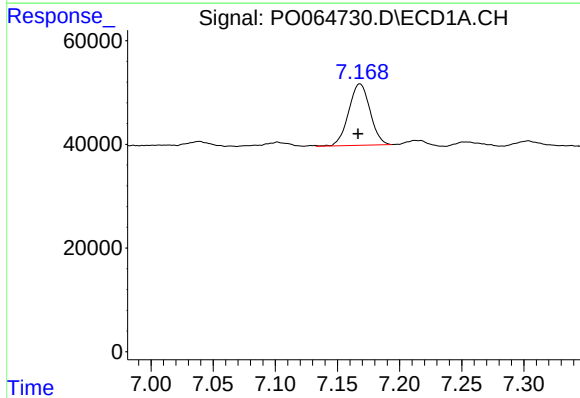


#32 AR-1260-2

R.T.: 7.168 min
Delta R.T.: 0.001 min
Response: 141536
Conc: 71.70 ng/ml

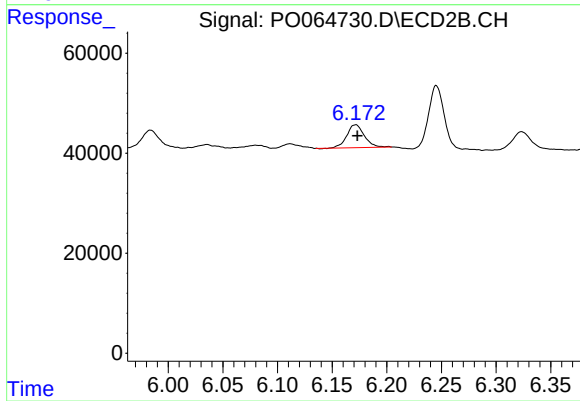

#32 AR-1260-2

R.T.: 6.172 min
Delta R.T.: -0.001 min
Response: 51723
Conc: 22.23 ng/ml

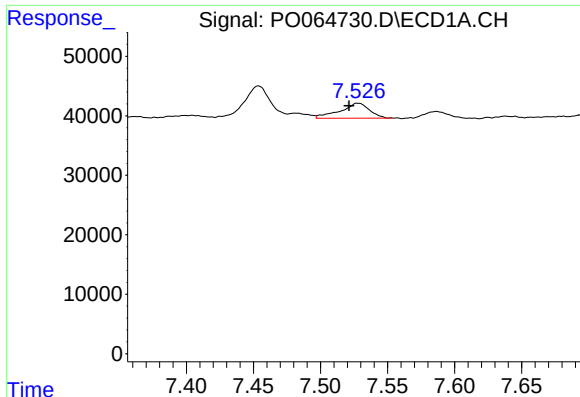


#33 AR-1260-3

R.T.: 7.526 min
Delta R.T.: 0.005 min
Response: 38179
Conc: 25.41 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SP-01


Manual Integrations
APPROVED

Ankita
12/17/2019 10:46:09 AM

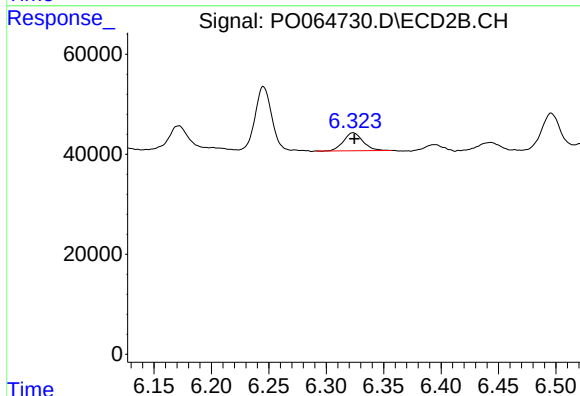


#33 AR-1260-3

R.T.: 6.323 min
Delta R.T.: -0.001 min
Response: 42603
Conc: 20.12 ng/ml

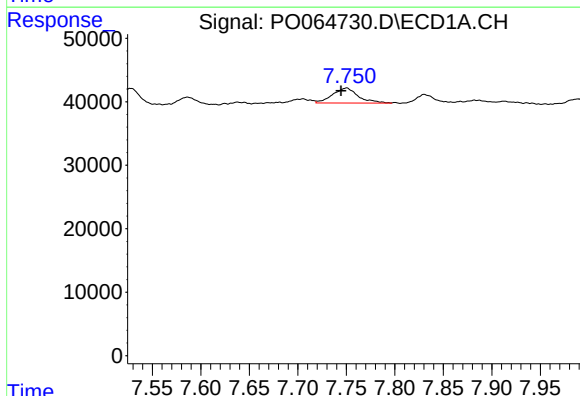


#34 AR-1260-4

R.T.: 7.750 min
Delta R.T.: 0.006 min
Response: 43048
Conc: 23.30 ng/ml m

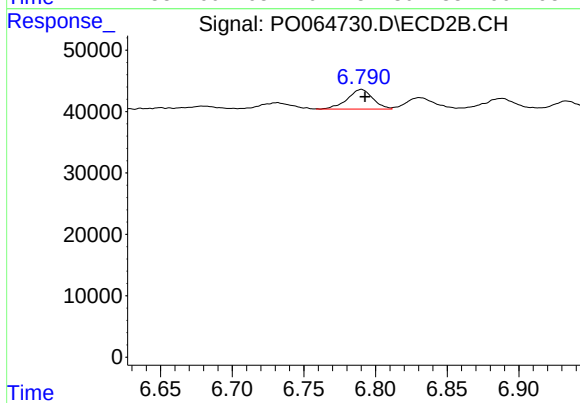

#34 AR-1260-4

R.T.: 6.790 min
Delta R.T.: -0.003 min
Response: 39676
Conc: 21.06 ng/ml m

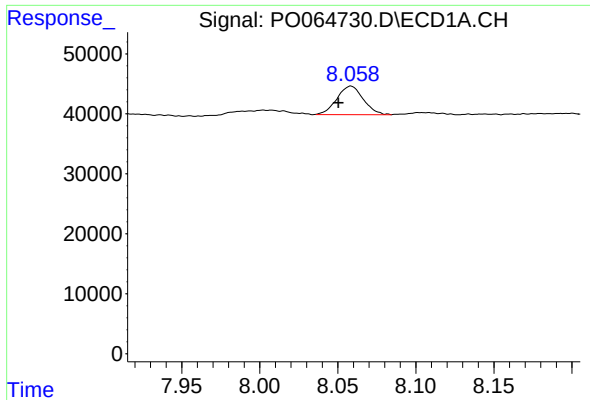


#35 AR-1260-5

R.T.: 8.058 min
Delta R.T.: 0.008 min
Response: 56135
Conc: 15.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-01

Manual Integrations
APPROVED

Ankita
12/17/2019 10:46:09 AM

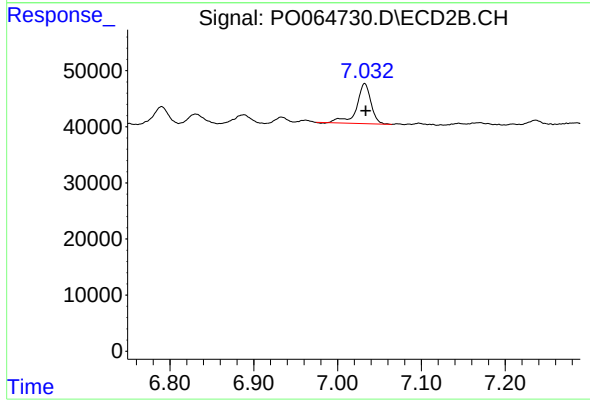

#35 AR-1260-5

R.T.: 7.032 min
Delta R.T.: -0.001 min
Response: 85923
Conc: 18.32 ng/ml