

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121719\
 Data File : P0064752.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Dec 2019 15:53
 Operator : SM/AJ
 Sample : K6299-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SHORE-RD-BH-04

Manual Integrations
 APPROVED

Ankita
 12/18/2019 9:25:24 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 16:09:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0121319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 13 08:19:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.179	3.453	631550	782915	25.942m	30.885m
2)	SA Decachlor...	9.704	8.379	572480	648268	18.653	18.667

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121719\
Data File : PO064752.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Dec 2019 15:53
Operator : SM/AJ
Sample : K6299-10
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
SHORE-RD-BH-04


Manual Integrations
APPROVED

Ankita
12/18/2019 9:25:24 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 16:09:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 13 08:19:24 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

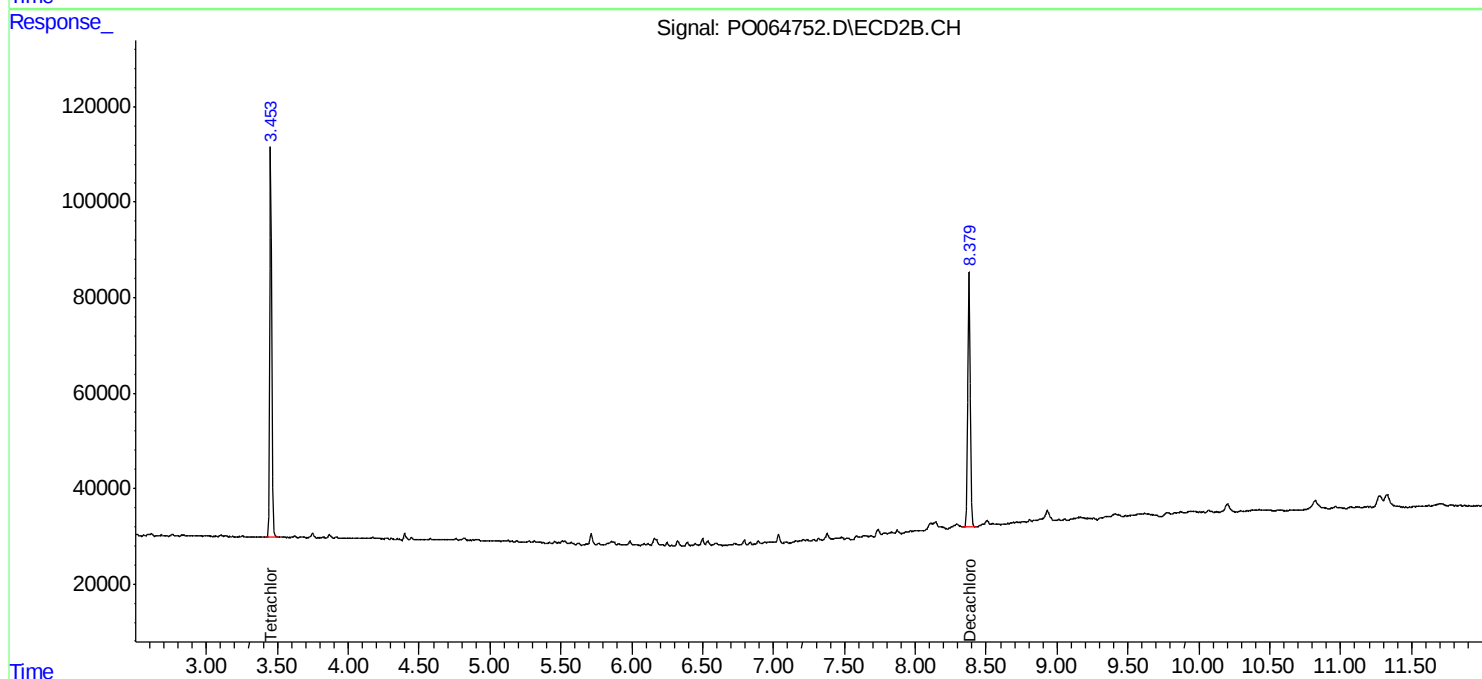

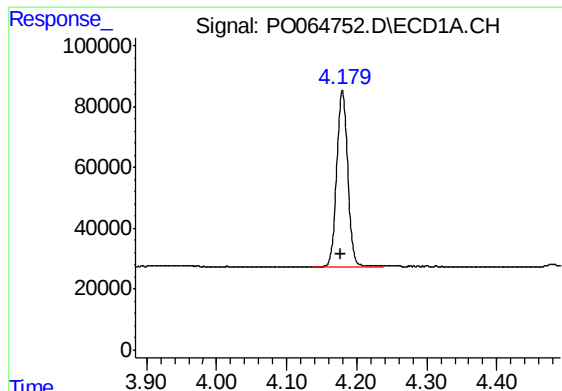


#1 Tetrachloro-m-xylene

R.T.: 4.179 min
Delta R.T.: 0.002 min
Response: 631550
Conc: 25.94 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SHORE-RD-BH-04


Manual Integrations
APPROVED

Ankita
12/18/2019 9:25:24 AM

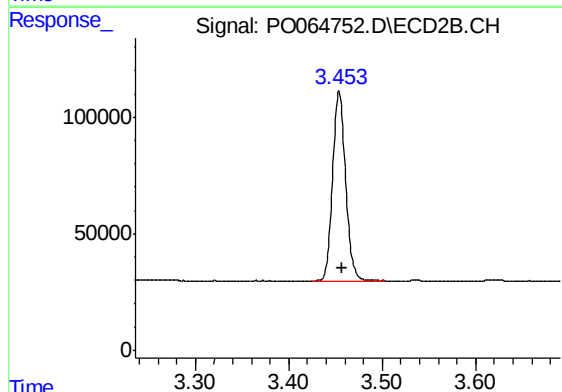


#1 Tetrachloro-m-xylene

R.T.: 3.453 min
Delta R.T.: -0.003 min
Response: 782915
Conc: 30.89 ng/ml m

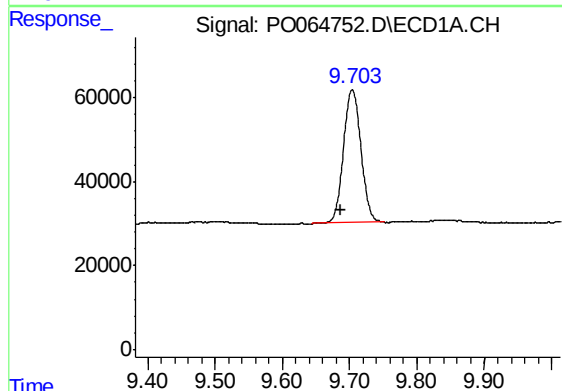

#2 Decachlorobiphenyl

R.T.: 9.704 min
Delta R.T.: 0.016 min
Response: 572480
Conc: 18.65 ng/ml

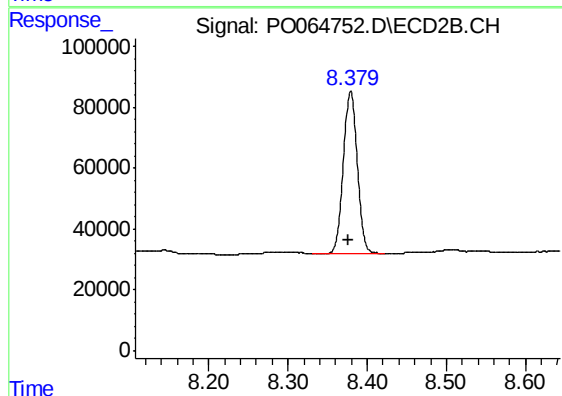

#2 Decachlorobiphenyl

R.T.: 8.379 min
Delta R.T.: 0.003 min
Response: 648268
Conc: 18.67 ng/ml