

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121719\
 Data File : P0064756.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Dec 2019 17:00
 Operator : SM/AJ
 Sample : K6318-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 X089-WC-2

Manual Integrations
 APPROVED

Ankita
 12/18/2019 9:25:31 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 17:23:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0121319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 13 08:19:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.180	3.454	797812	976179	32.771	38.509m
2) SA Decachlor...	9.704	8.378	826643	1006585	26.935	28.984

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121719\
Data File : PO064756.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Dec 2019 17:00
Operator : SM/AJ
Sample : K6318-08
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
X089-WC-2


Manual Integrations
APPROVED

Ankita
12/18/2019 9:25:31 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 17:23:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 13 08:19:24 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

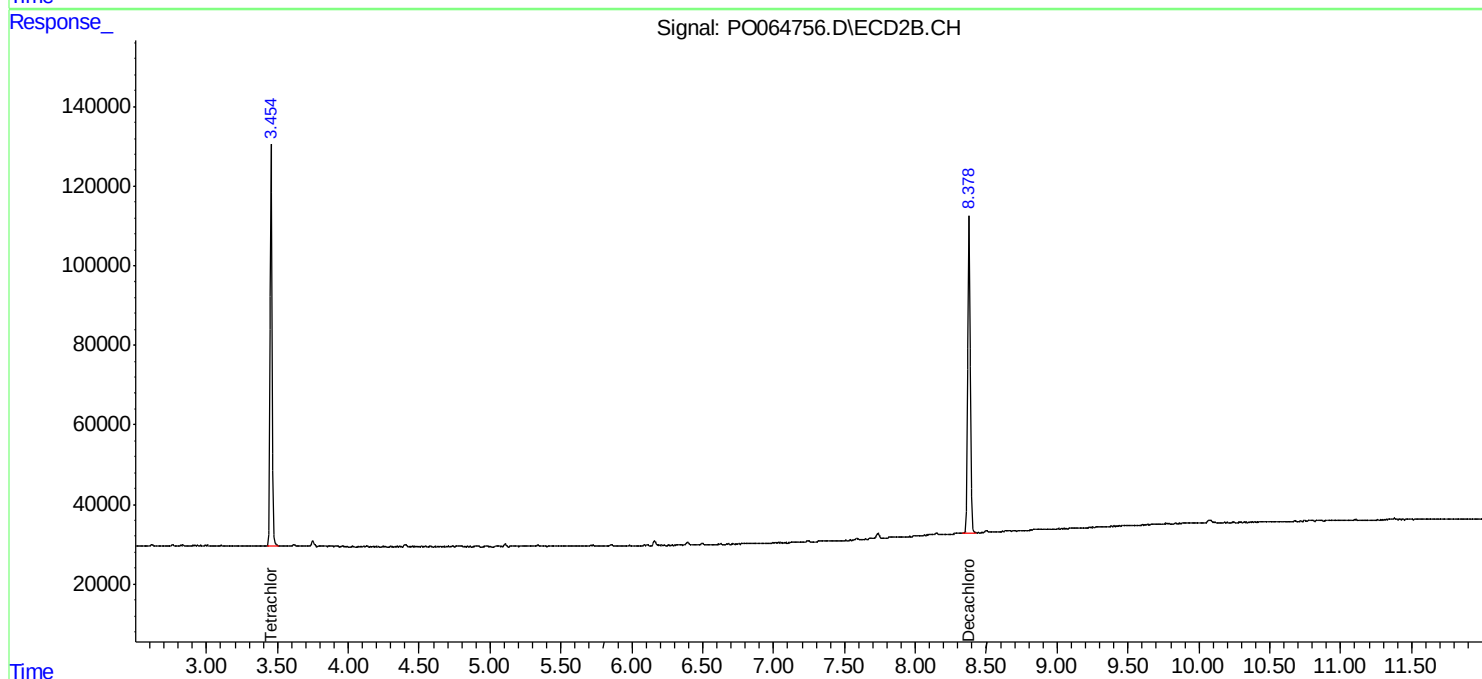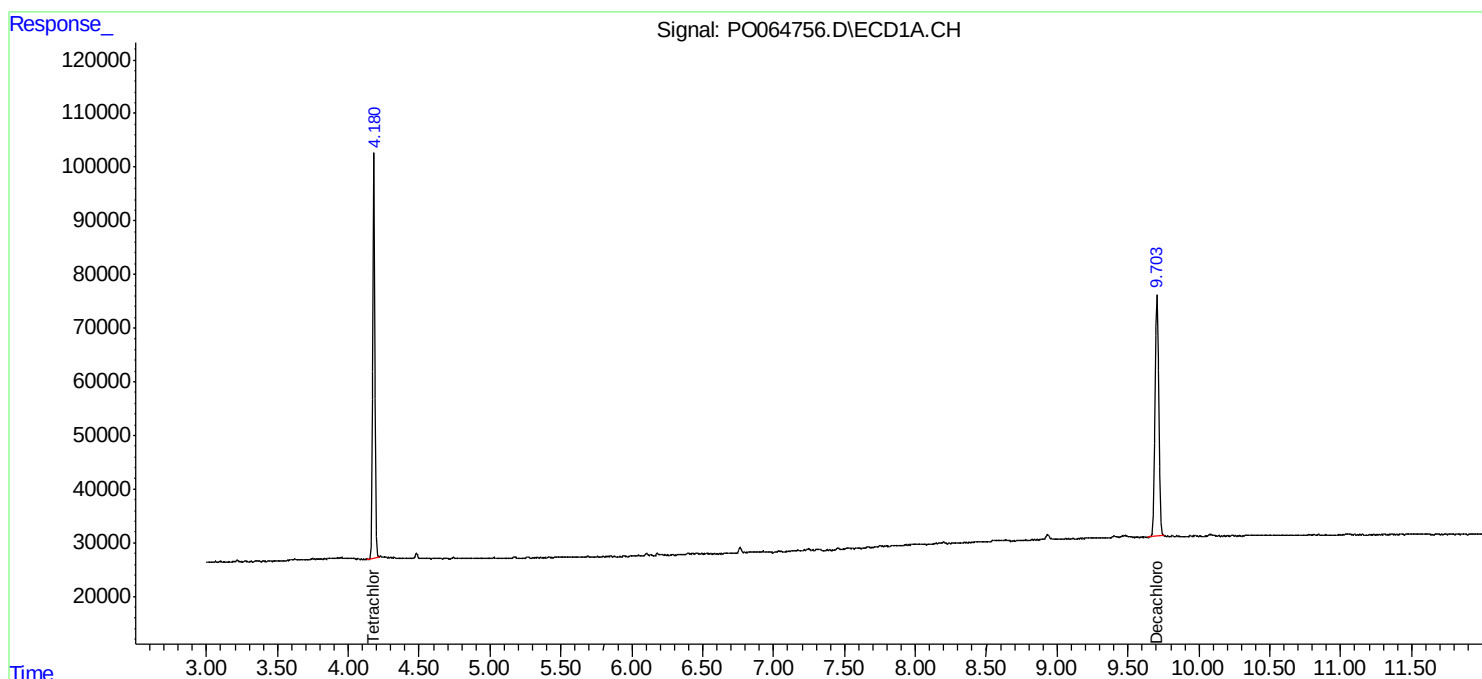

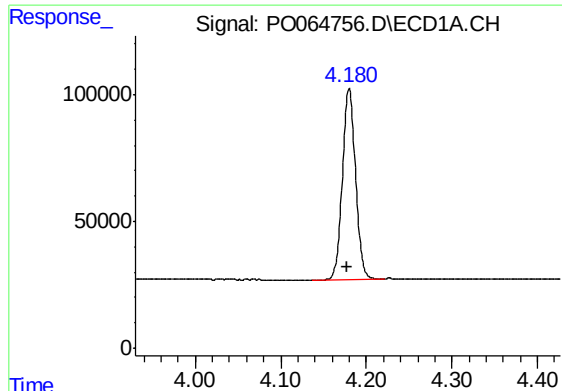


#1 Tetrachloro-m-xylene

R.T.: 4.180 min
Delta R.T.: 0.003 min
Response: 797812
Conc: 32.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
X089-WC-2


Manual Integrations
APPROVED

Ankita
12/18/2019 9:25:31 AM

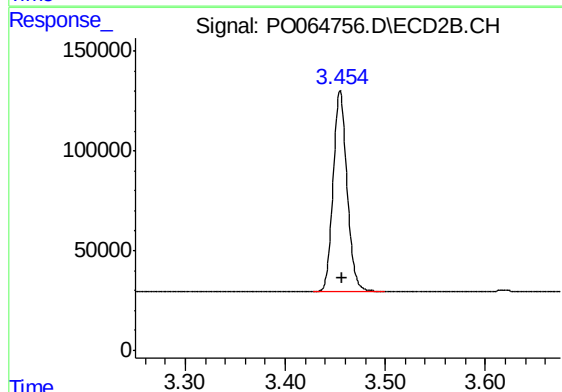


#1 Tetrachloro-m-xylene

R.T.: 3.454 min
Delta R.T.: -0.002 min
Response: 976179
Conc: 38.51 ng/ml m

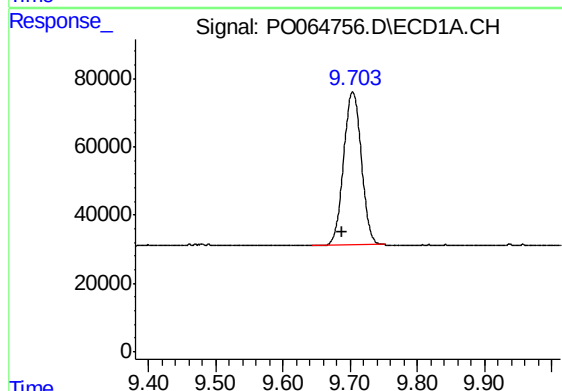

#2 Decachlorobiphenyl

R.T.: 9.704 min
Delta R.T.: 0.016 min
Response: 826643
Conc: 26.94 ng/ml

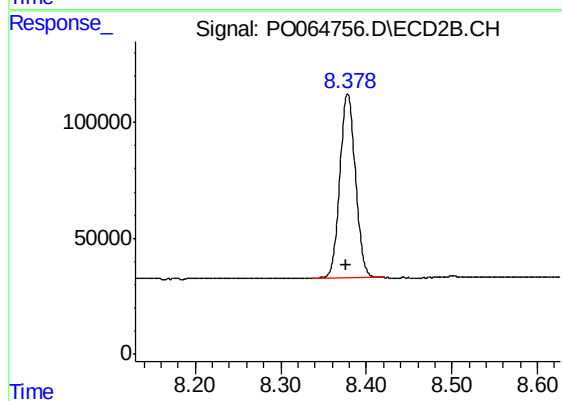

#2 Decachlorobiphenyl

R.T.: 8.378 min
Delta R.T.: 0.002 min
Response: 1006585
Conc: 28.98 ng/ml