

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121719\
 Data File : P0064764.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Dec 2019 19:13
 Operator : SM/AJ
 Sample : K6333-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-1A-COMP

Manual Integrations
 APPROVED

Ankita
 12/18/2019 9:25:49 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 01:03:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0121319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 13 08:19:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.179	3.454	614453	755718	25.239	29.812m
2)	SA Decachlor...	9.703	8.377	645632	810268	21.037	23.331

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121719\
Data File : PO064764.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Dec 2019 19:13
Operator : SM/AJ
Sample : K6333-04
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-1A-COMP


Manual Integrations
APPROVED

Ankita
12/18/2019 9:25:49 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 01:03:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 13 08:19:24 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

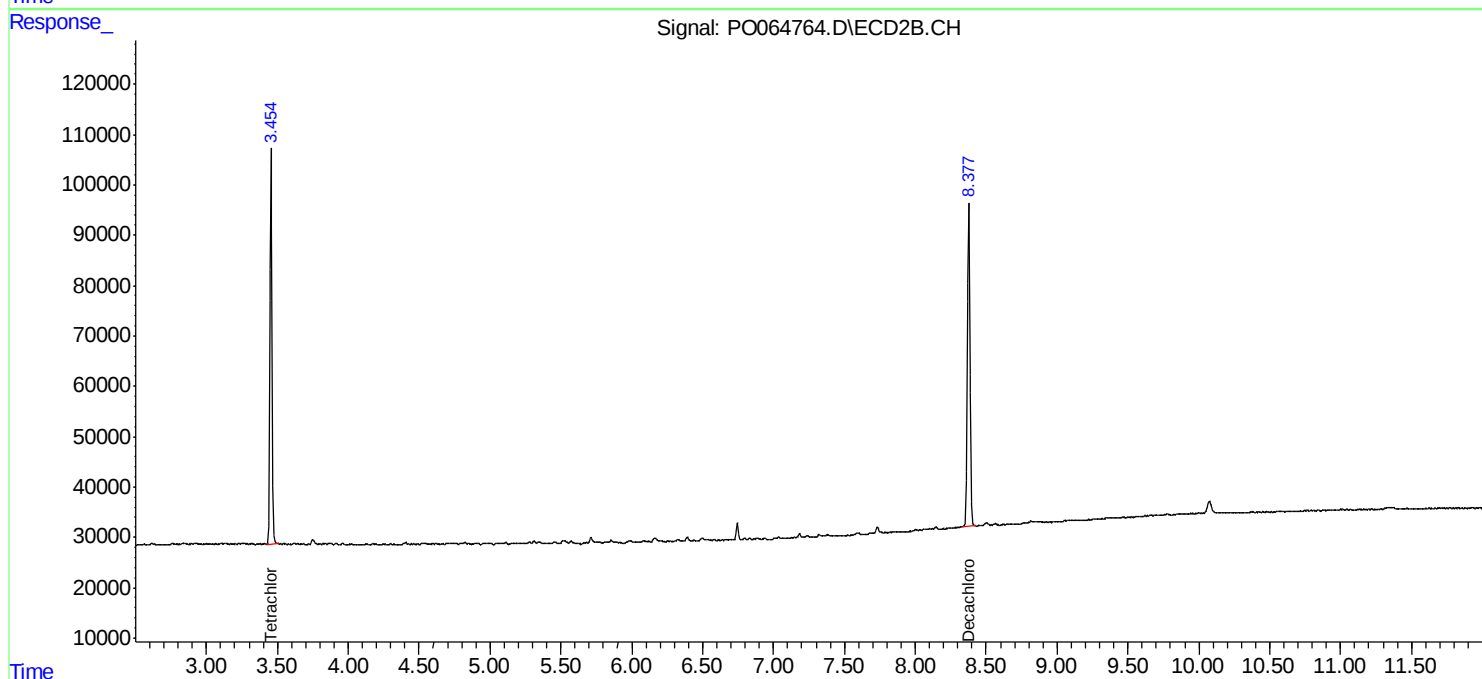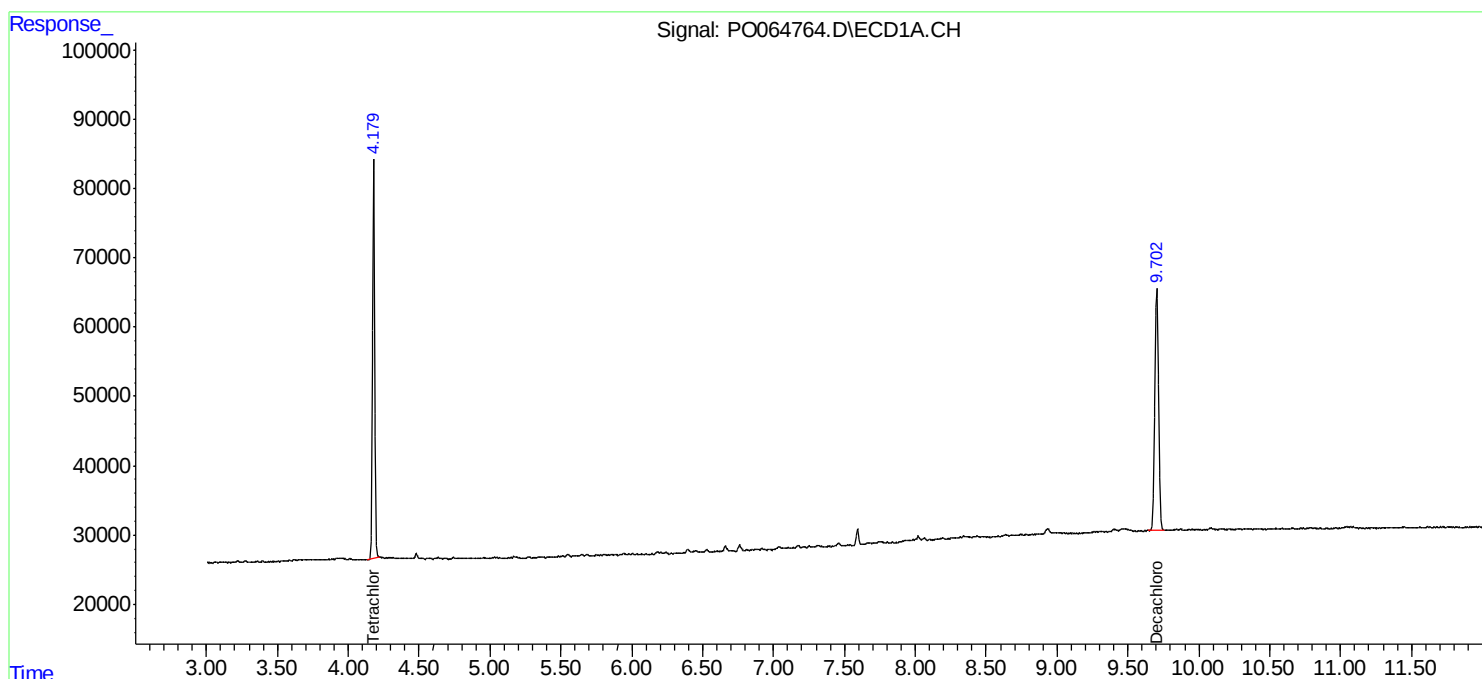

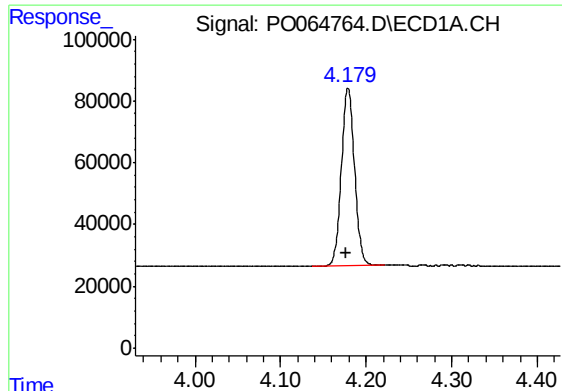


#1 Tetrachloro-m-xylene

R.T.: 4.179 min
Delta R.T.: 0.002 min
Response: 614453
Conc: 25.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-1A-COMP


Manual Integrations
APPROVED

Ankita
12/18/2019 9:25:49 AM

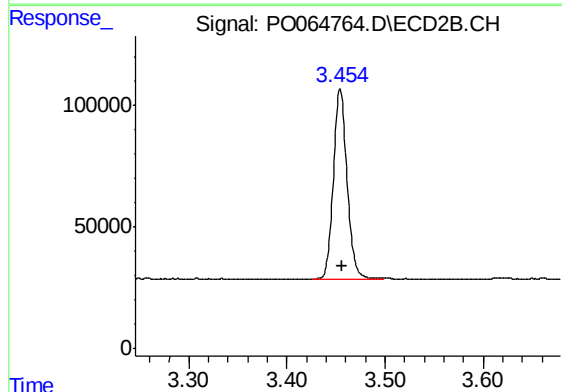


#1 Tetrachloro-m-xylene

R.T.: 3.454 min
Delta R.T.: -0.003 min
Response: 755718
Conc: 29.81 ng/ml m

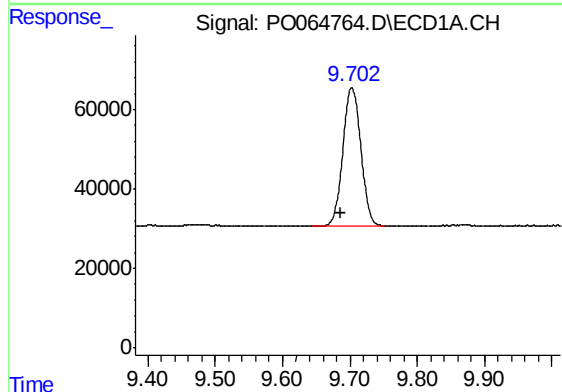

#2 Decachlorobiphenyl

R.T.: 9.703 min
Delta R.T.: 0.015 min
Response: 645632
Conc: 21.04 ng/ml

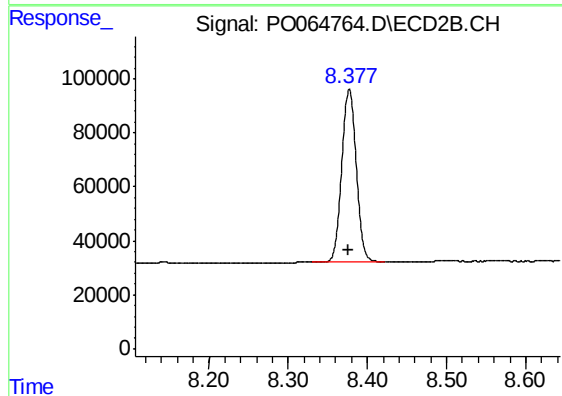

#2 Decachlorobiphenyl

R.T.: 8.377 min
Delta R.T.: 0.000 min
Response: 810268
Conc: 23.33 ng/ml