

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121719\
 Data File : P0064767.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Dec 2019 20:03
 Operator : SM/AJ
 Sample : PB125549BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB125549BL

Manual Integrations
 APPROVED

Ankita
 12/18/2019 9:25:55 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 01:04:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0121319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 13 08:19:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.180	3.454	613762	746516	25.211	29.449m
2)	SA Decachlor...	9.703	8.377	707027	899018	23.037	25.887

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121719\
Data File : PO064767.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Dec 2019 20:03
Operator : SM/AJ
Sample : PB125549BL
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB125549BL


Manual Integrations
APPROVED

Ankita
12/18/2019 9:25:55 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 01:04:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 13 08:19:24 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

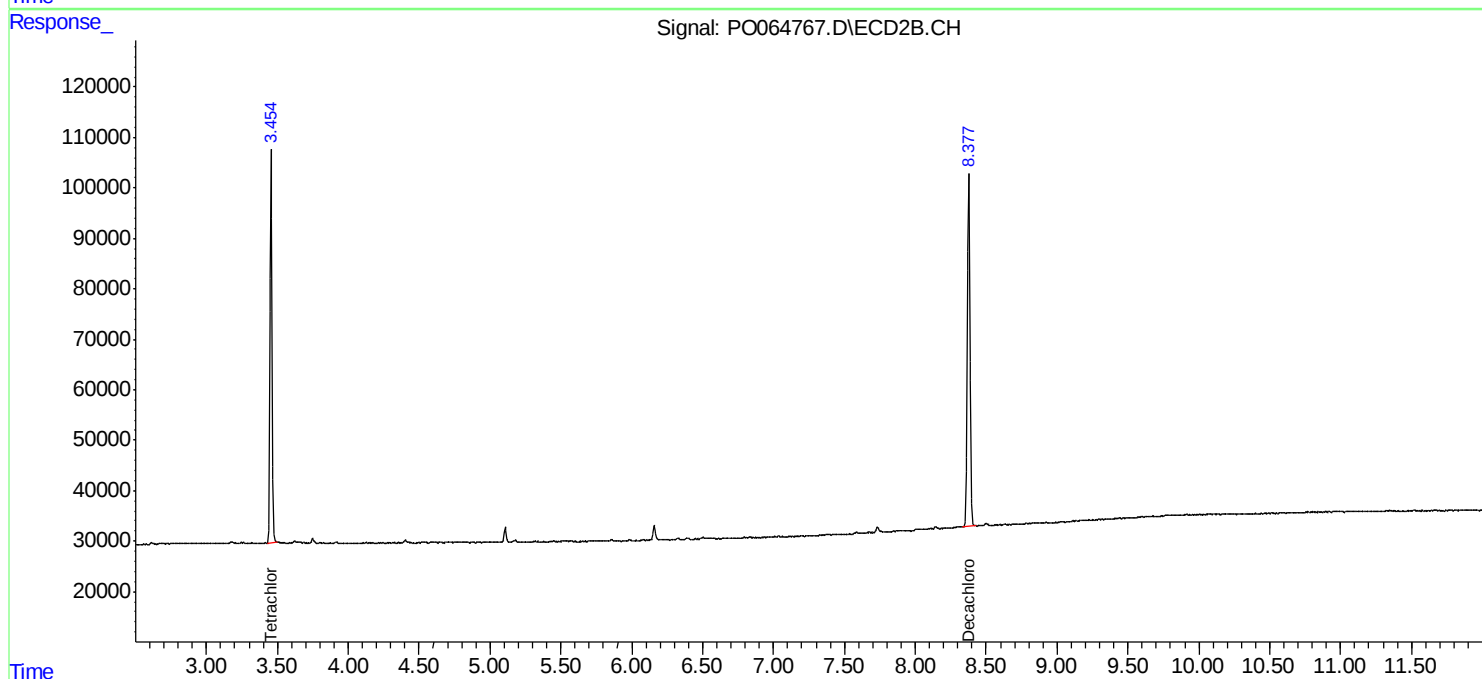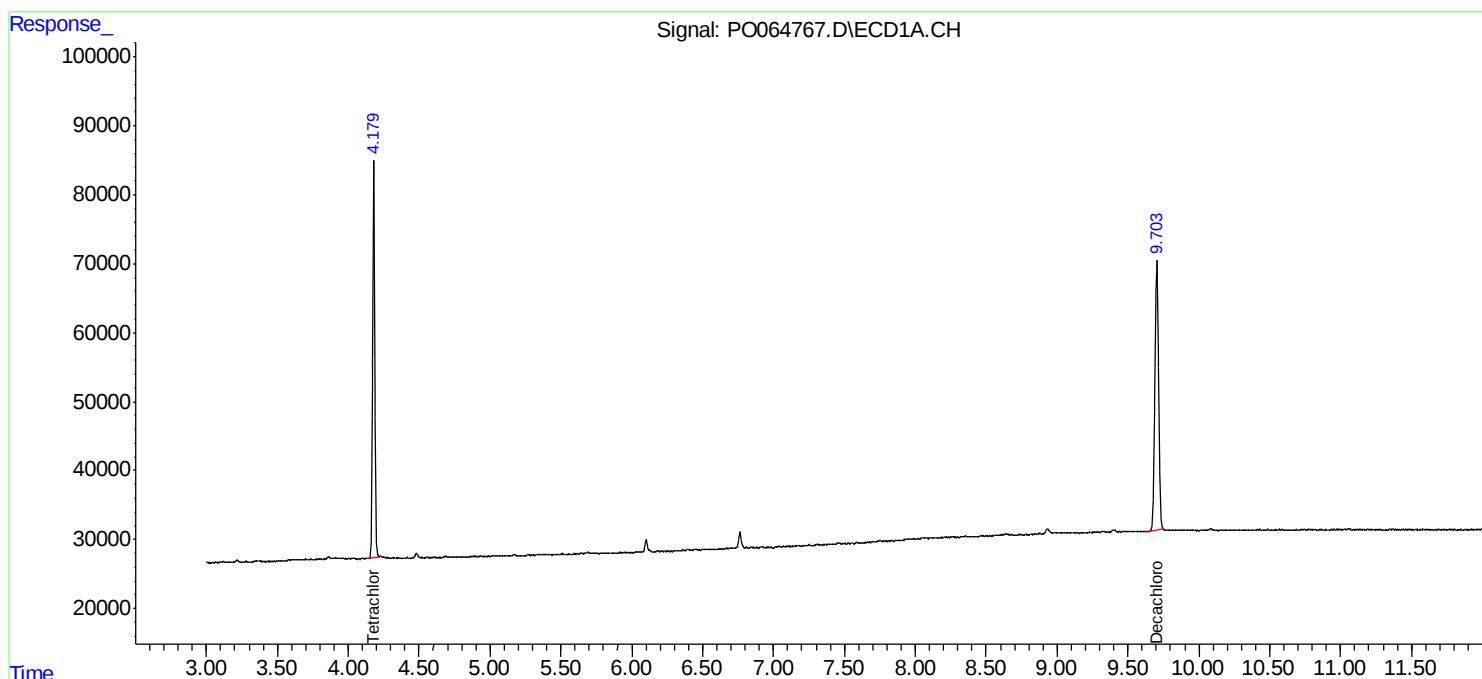

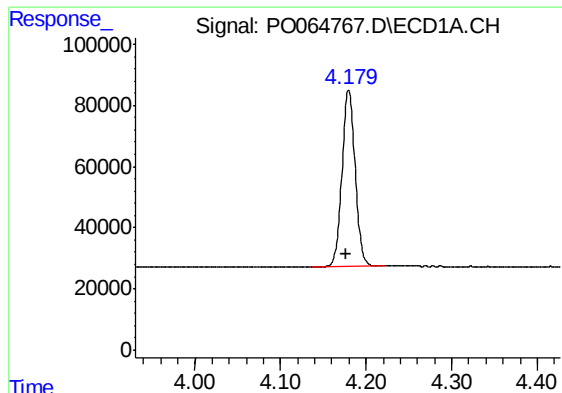


#1 Tetrachloro-m-xylene

R.T.: 4.180 min
Delta R.T.: 0.003 min
Response: 613762
Conc: 25.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB125549BL


Manual Integrations
APPROVED

Ankita
12/18/2019 9:25:55 AM

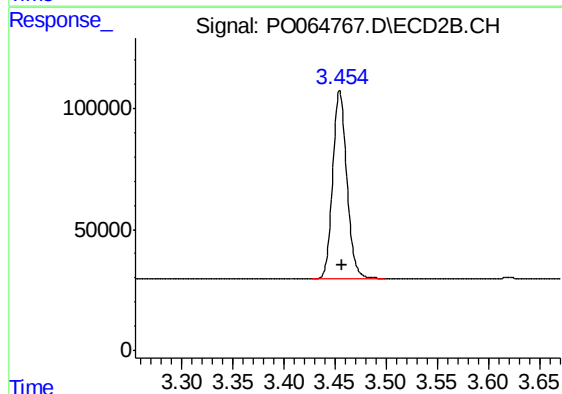


#1 Tetrachloro-m-xylene

R.T.: 3.454 min
Delta R.T.: -0.003 min
Response: 746516
Conc: 29.45 ng/ml m

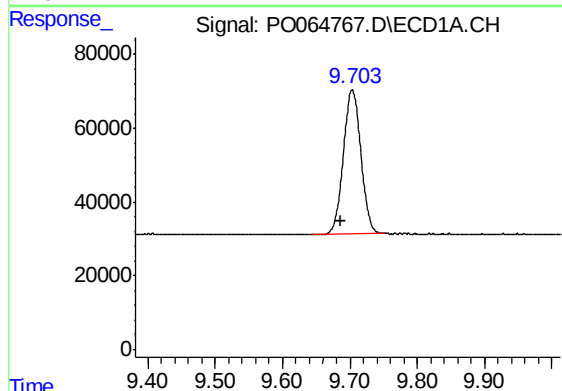

#2 Decachlorobiphenyl

R.T.: 9.703 min
Delta R.T.: 0.016 min
Response: 707027
Conc: 23.04 ng/ml

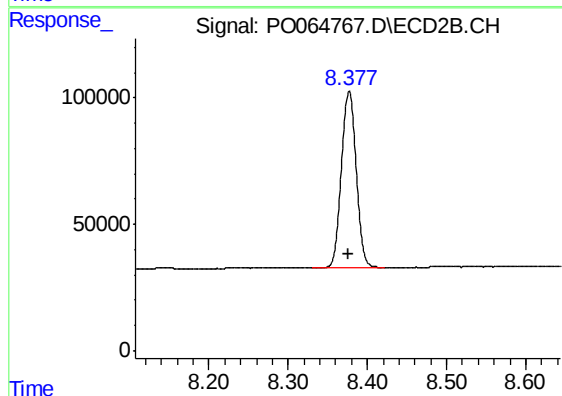

#2 Decachlorobiphenyl

R.T.: 8.377 min
Delta R.T.: 0.000 min
Response: 899018
Conc: 25.89 ng/ml