

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121818\
 Data File : PO052692.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Dec 2018 18:00
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 01:27:44 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Dec 16 03:01:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.251	3.274	19687733	4702798	25.105	22.193
2)	SA Decachlor...	9.803	7.959	10611916	4413376	21.061	20.004
Target Compounds							
7)	L1 AR-1016-5	0.000	4.705	0	321888	N.D.	50.007 #
15)	L3 AR-1232-5	0.000	4.705	0	321888	N.D.	120.756 #
20)	L4 AR-1242-5	6.277	0.000	2661185	0	188.924	N.D. #
24)	L5 AR-1248-4	6.277	4.705	2661185	321888	116.693	37.607 #
25)	L5 AR-1248-5	6.277	0.000	2661185	0	121.872	N.D. #
26)	L6 AR-1254-1	6.260	0.000	2044099	0	81.816	N.D. #
27)	L6 AR-1254-2	0.000	5.208	0	441746	N.D.	36.031 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121818\
Data File : PO052692.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Dec 2018 18:00
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 01:27:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121518.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Dec 16 03:01:24 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

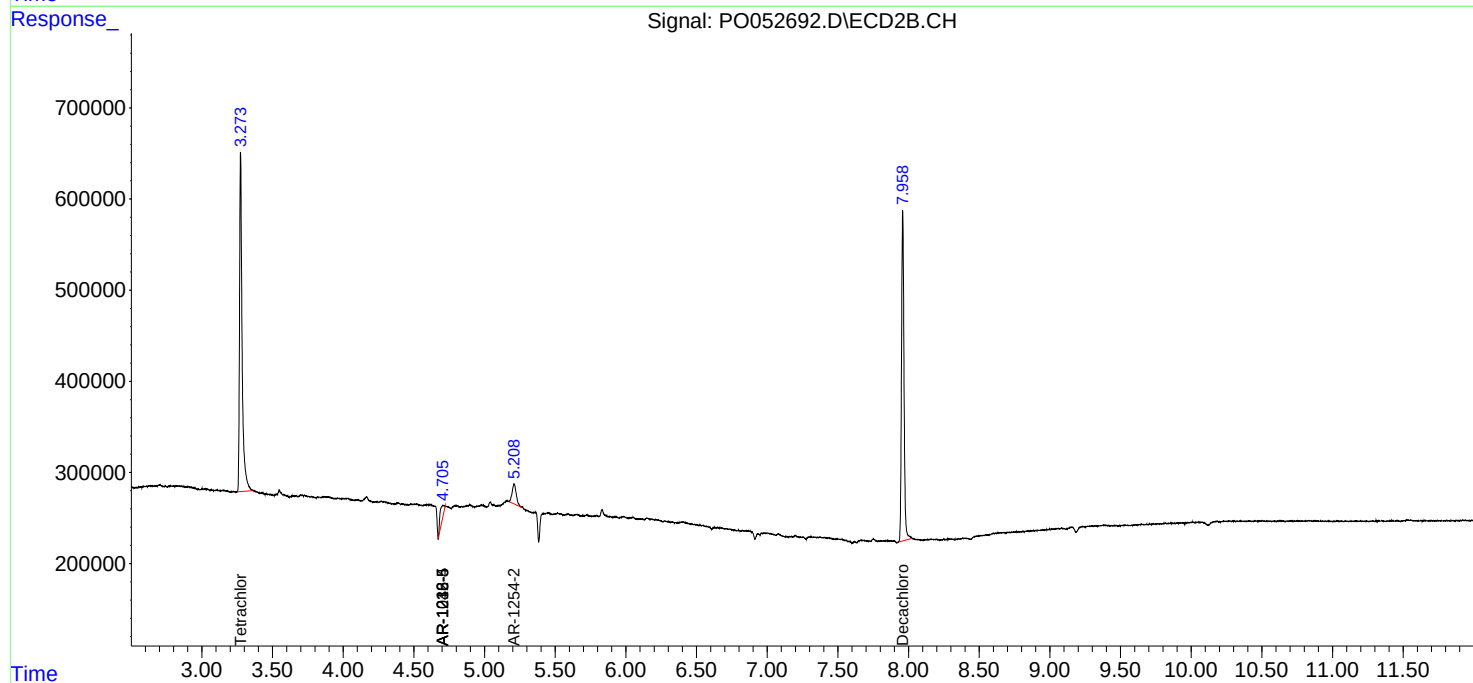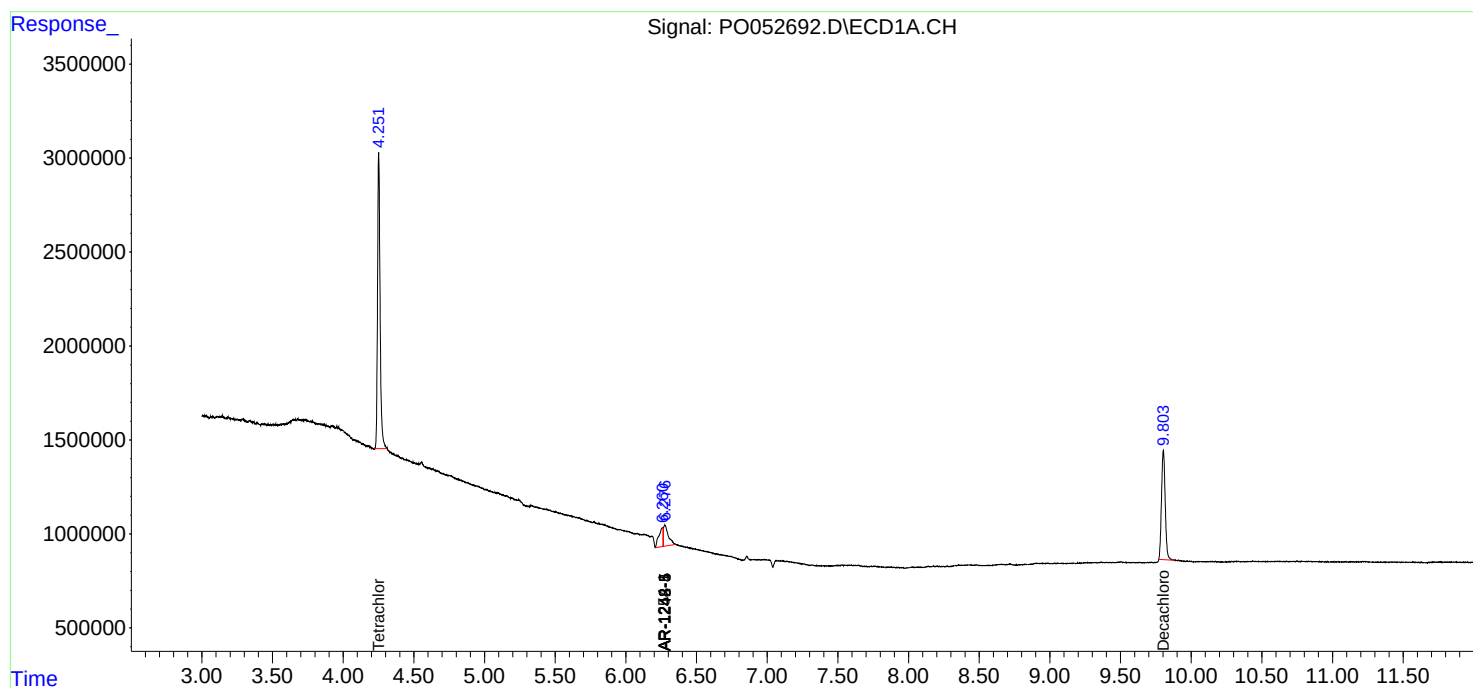


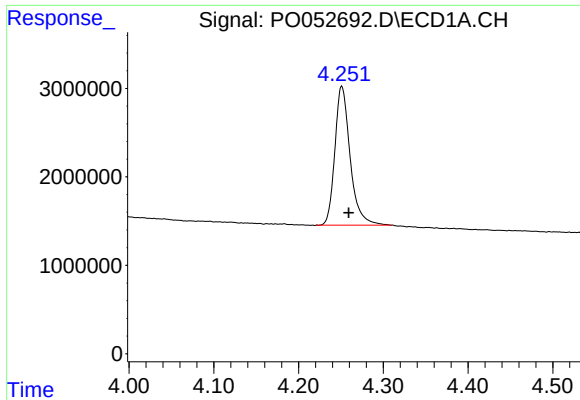

#1 Tetrachloro-m-xylene


R.T.: 4.251 min
Delta R.T.: -0.008 min
Response: 19687733
Conc: 25.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

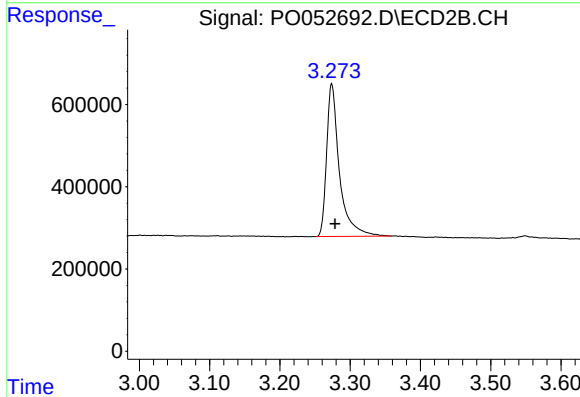


#1 Tetrachloro-m-xylene

R.T.: 3.274 min
Delta R.T.: -0.005 min
Response: 4702798
Conc: 22.19 ng/ml

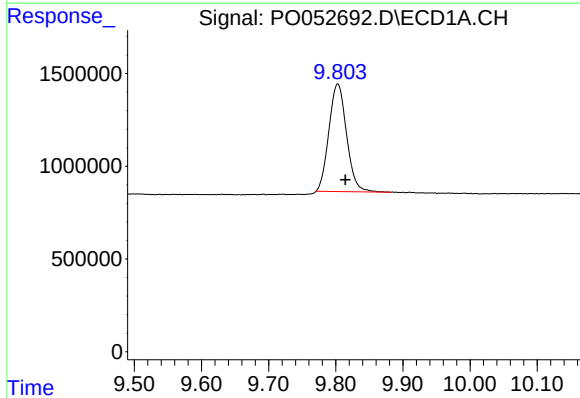


#2 Decachlorobiphenyl

R.T.: 9.803 min
Delta R.T.: -0.011 min
Response: 10611916
Conc: 21.06 ng/ml

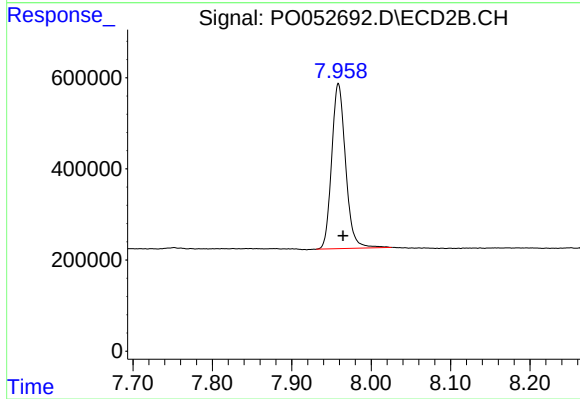

#2 Decachlorobiphenyl


R.T.: 7.959 min
Delta R.T.: -0.006 min
Response: 4413376
Conc: 20.00 ng/ml

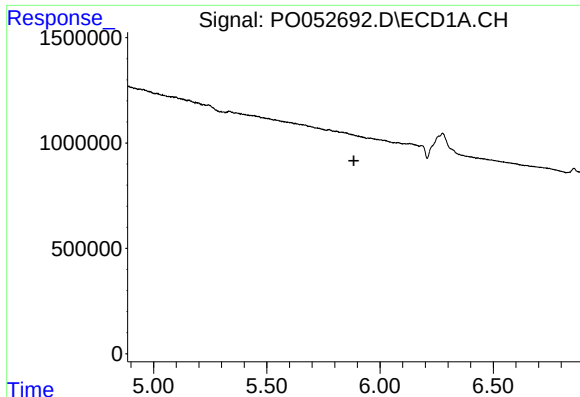

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.884 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

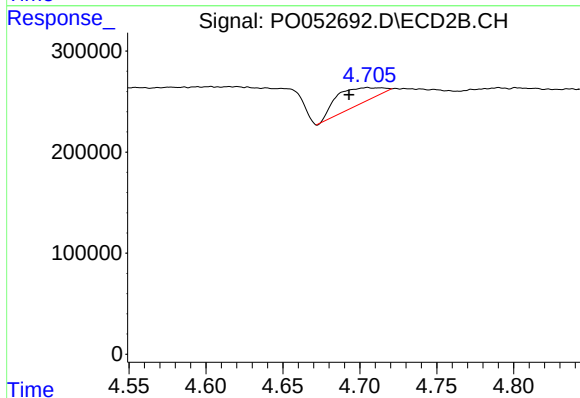


#7 AR-1016-5

R.T.: 4.705 min
Delta R.T.: 0.012 min
Response: 321888
Conc: 50.01 ng/ml

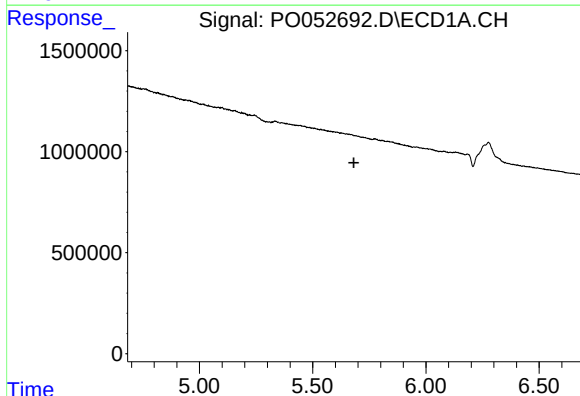


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T.: 5.682 min
Response: 0
Conc: N.D.

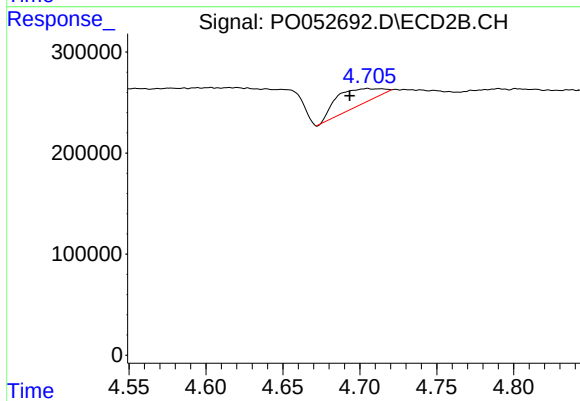

#15 AR-1232-5


R.T.: 4.705 min
Delta R.T.: 0.011 min
Response: 321888
Conc: 120.76 ng/ml

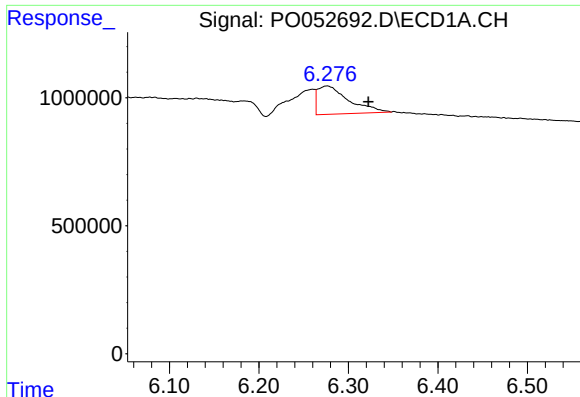

#20 AR-1242-5


R.T.: 6.277 min
Delta R.T.: -0.046 min
Response: 2661185
Conc: 188.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

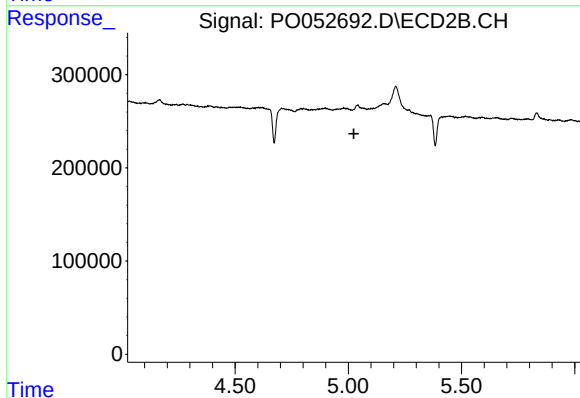


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 5.024 min
Response: 0
Conc: N.D.

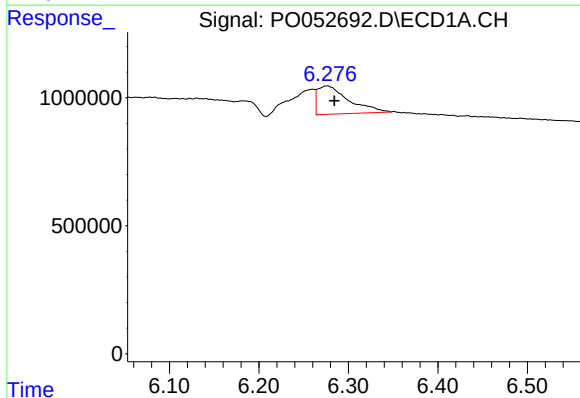


#24 AR-1248-4

R.T.: 6.277 min
Delta R.T.: -0.008 min
Response: 2661185
Conc: 116.69 ng/ml

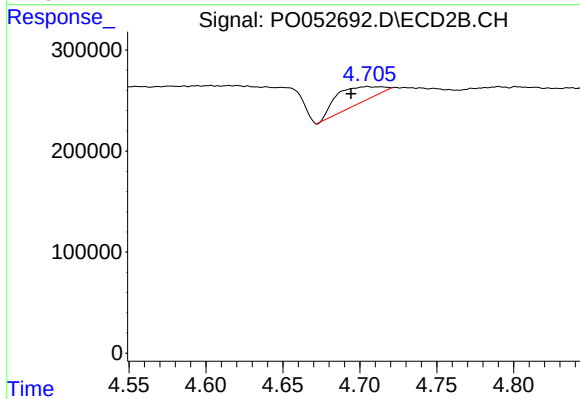

#24 AR-1248-4


R.T.: 4.705 min
Delta R.T.: 0.011 min
Response: 321888
Conc: 37.61 ng/ml

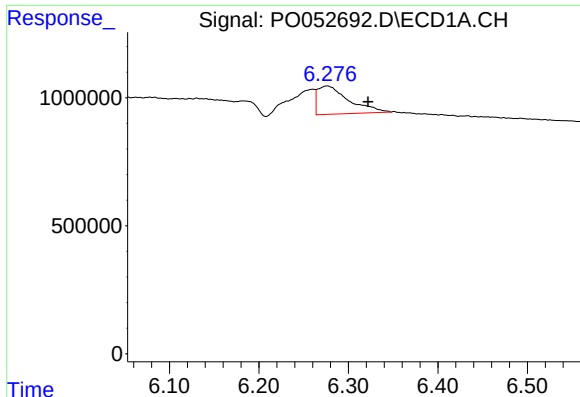

#25 AR-1248-5


R.T.: 6.277 min
Delta R.T.: -0.045 min
Response: 2661185
Conc: 121.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

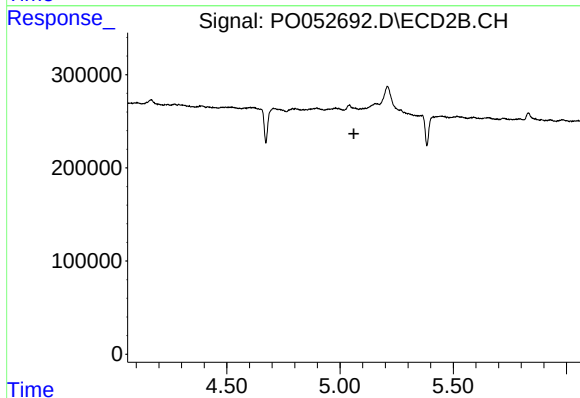


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 5.061 min
Response: 0
Conc: N.D.

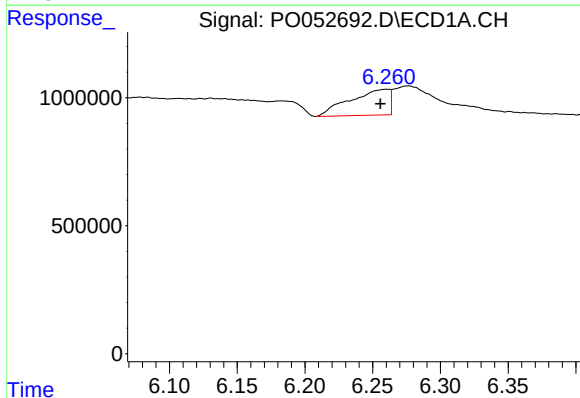


#26 AR-1254-1

R.T.: 6.260 min
Delta R.T.: 0.005 min
Response: 2044099
Conc: 81.82 ng/ml

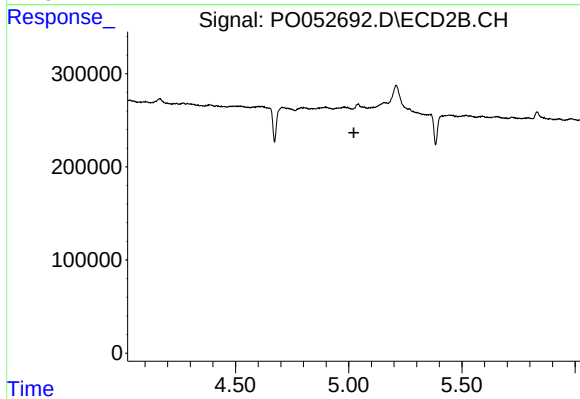

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 5.023 min
Response: 0
Conc: N.D.

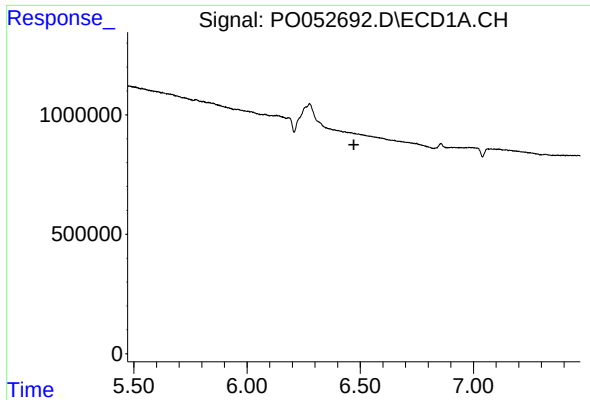

#27 AR-1254-2

R.T.: 0.000 min
Exp R.T.: 6.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

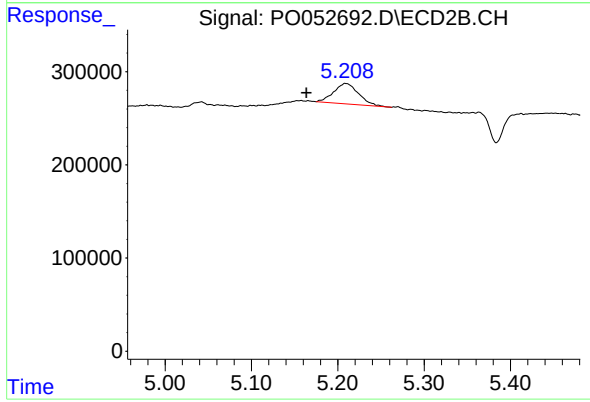

#27 AR-1254-2

R.T.: 5.208 min
Delta R.T.: 0.045 min
Response: 441746
Conc: 36.03 ng/ml