

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121818\
 Data File : PO052710.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Dec 2018 23:13
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 01:35:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Dec 16 03:01:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.251	3.273	20739698	4947456	26.447	23.347
2)	SA Decachlor...	9.801	7.958	10635460	5034530	21.108	22.819
Target Compounds							
7)	L1 AR-1016-5	0.000	4.708	0	670071	N.D.	104.100 #
15)	L3 AR-1232-5	0.000	4.708	0	670071	N.D.	251.377 #
20)	L4 AR-1242-5	6.282	0.000	53054	0	3.766	N.D. #
24)	L5 AR-1248-4	6.282	4.708	53054	670071	2.326	78.285 #
25)	L5 AR-1248-5	6.282	0.000	53054	0	2.430	N.D. #
26)	L6 AR-1254-1	6.253	0.000	1324793	0	53.026	N.D. #
28)	L6 AR-1254-3	6.854	0.000	321858	0	8.169	N.D. #
29)	L6 AR-1254-4	7.080	0.000	72652	0	2.646	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121818\
Data File : PO052710.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Dec 2018 23:13
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 01:35:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121518.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Dec 16 03:01:24 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

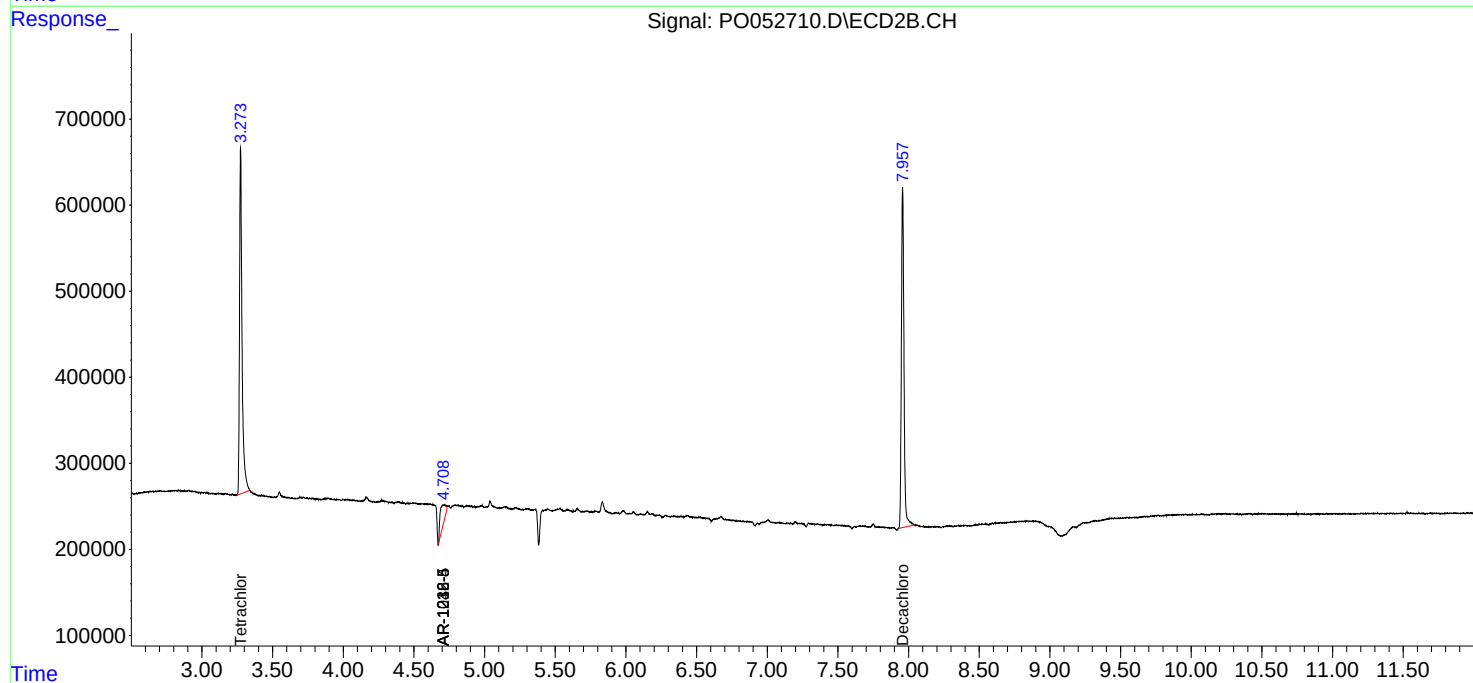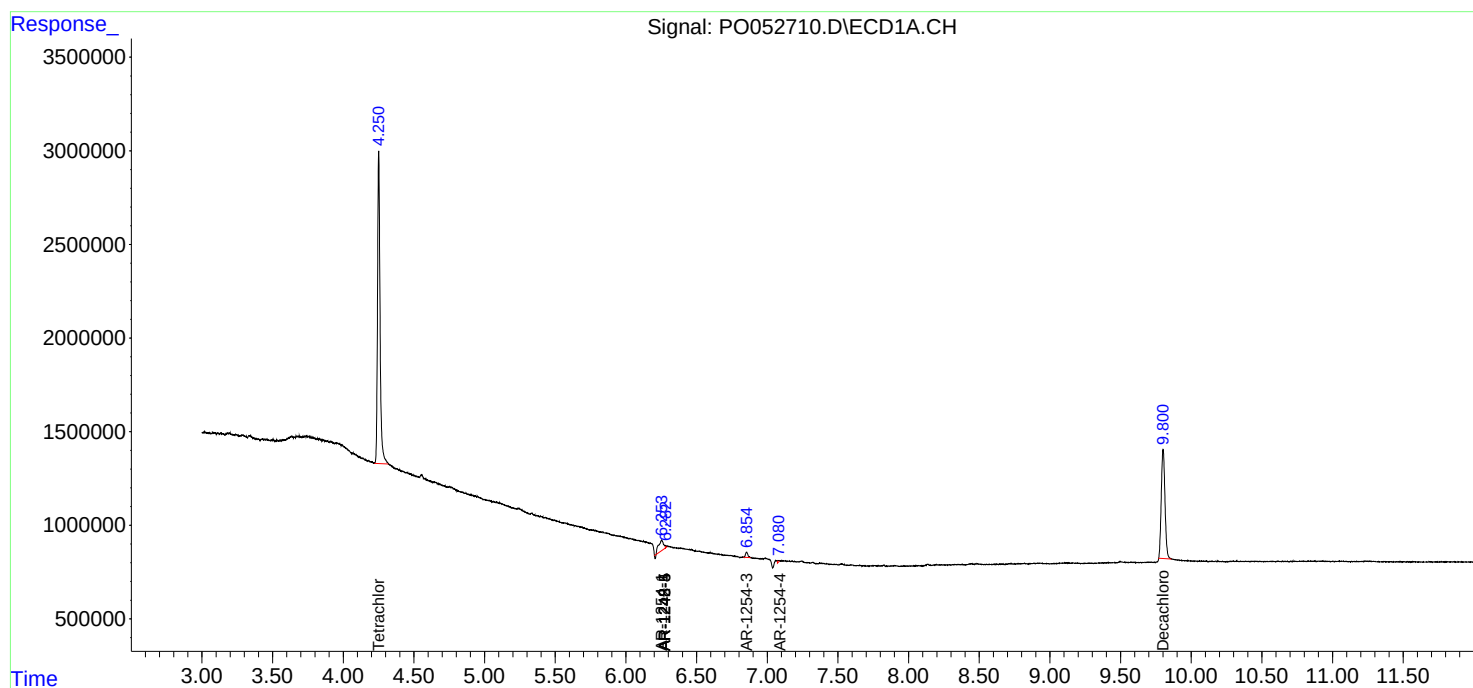


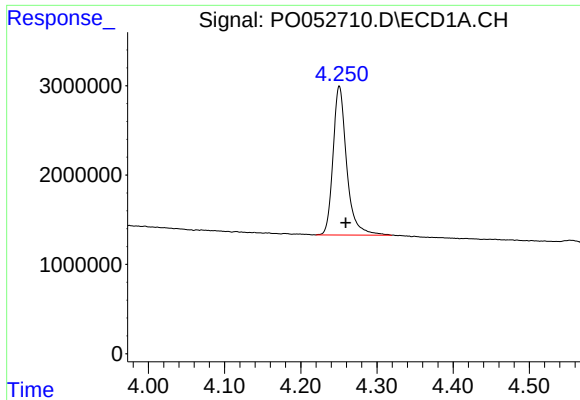

#1 Tetrachloro-m-xylene


R.T.: 4.251 min
Delta R.T.: -0.008 min
Response: 20739698
Conc: 26.45 ng/ml

Instrument :
ECD_O
ClientSampleId :

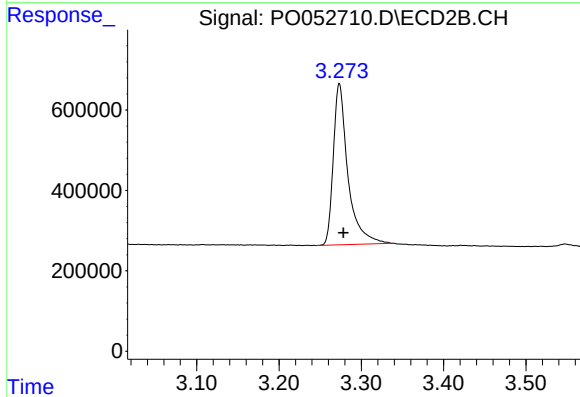


#1 Tetrachloro-m-xylene

R.T.: 3.273 min
Delta R.T.: -0.005 min
Response: 4947456
Conc: 23.35 ng/ml

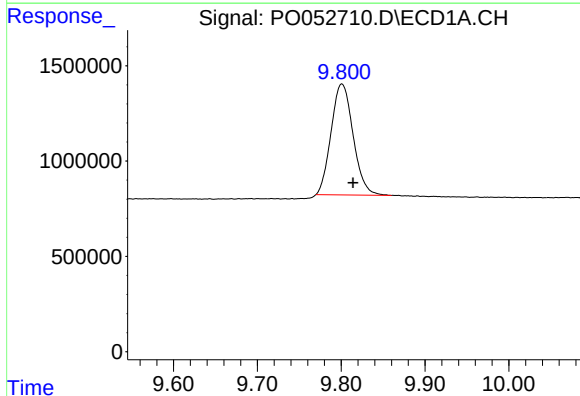


#2 Decachlorobiphenyl

R.T.: 9.801 min
Delta R.T.: -0.013 min
Response: 10635460
Conc: 21.11 ng/ml

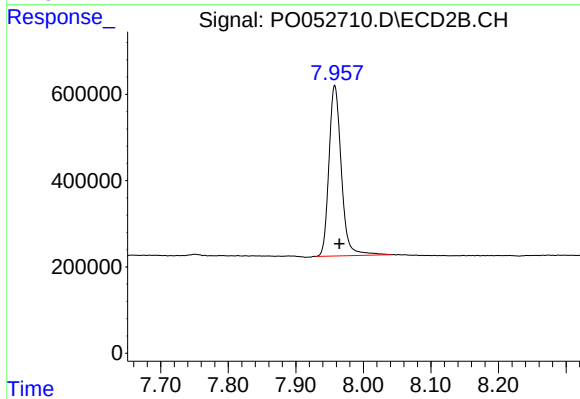

#2 Decachlorobiphenyl


R.T.: 7.958 min
Delta R.T.: -0.007 min
Response: 5034530
Conc: 22.82 ng/ml

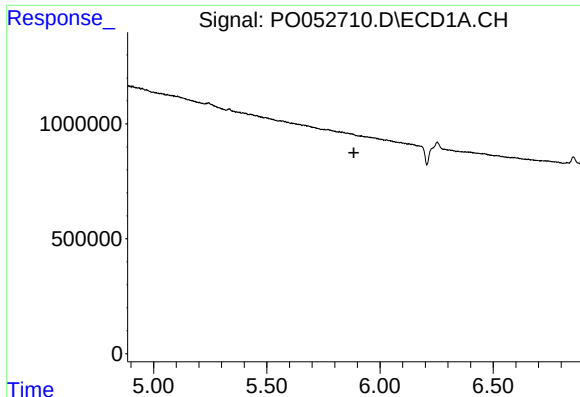

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 5.884 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

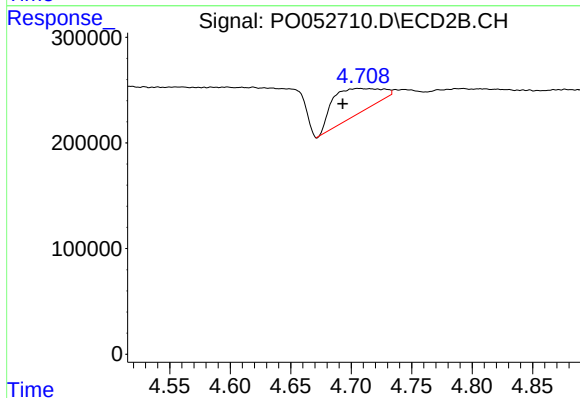


#7 AR-1016-5

R.T.: 4.708 min
Delta R.T.: 0.015 min
Response: 670071
Conc: 104.10 ng/ml

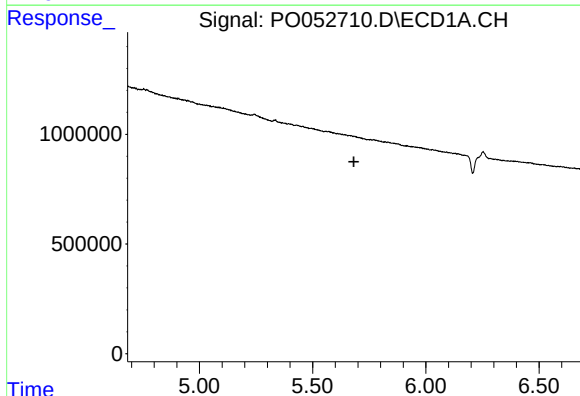


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.682 min
Response: 0
Conc: N.D.

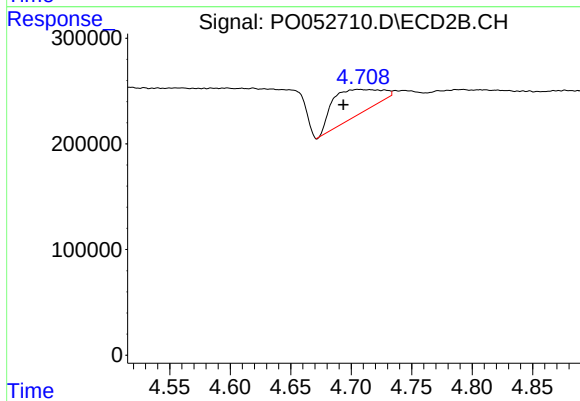

#15 AR-1232-5


R.T.: 4.708 min
Delta R.T.: 0.015 min
Response: 670071
Conc: 251.38 ng/ml

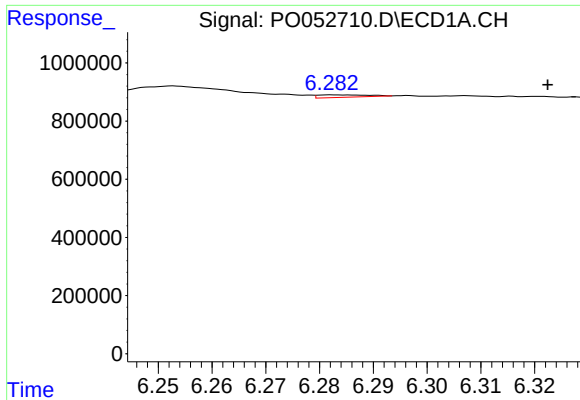

#20 AR-1242-5


R.T.: 6.282 min
Delta R.T.: -0.040 min
Response: 53054
Conc: 3.77 ng/ml

Instrument :
ECD_O
ClientSampleId :

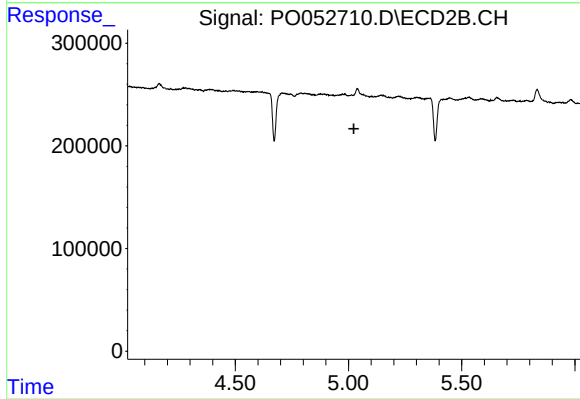


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 5.024 min
Response: 0
Conc: N.D.

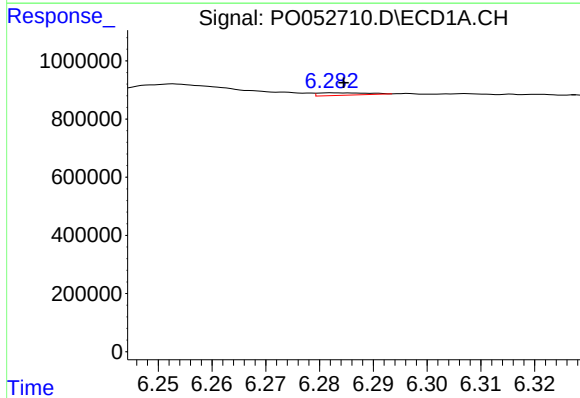


#24 AR-1248-4

R.T.: 6.282 min
Delta R.T.: -0.002 min
Response: 53054
Conc: 2.33 ng/ml

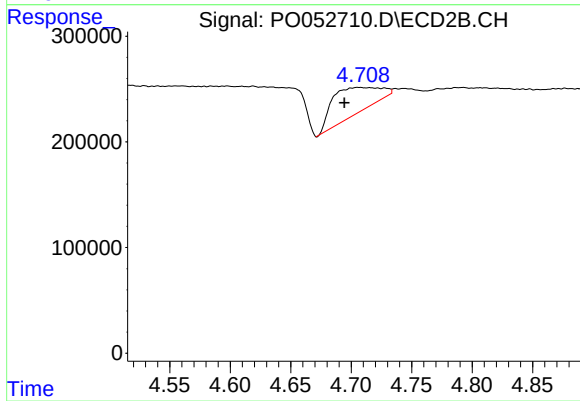

#24 AR-1248-4


R.T.: 4.708 min
Delta R.T.: 0.014 min
Response: 670071
Conc: 78.29 ng/ml

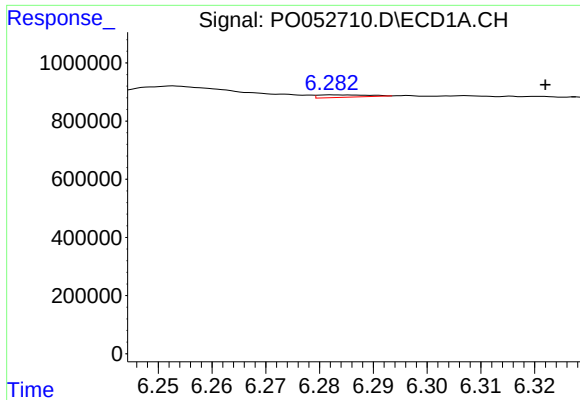

#25 AR-1248-5


R.T.: 6.282 min
Delta R.T.: -0.040 min
Response: 53054
Conc: 2.43 ng/ml

Instrument :
ECD_O
ClientSampleId :

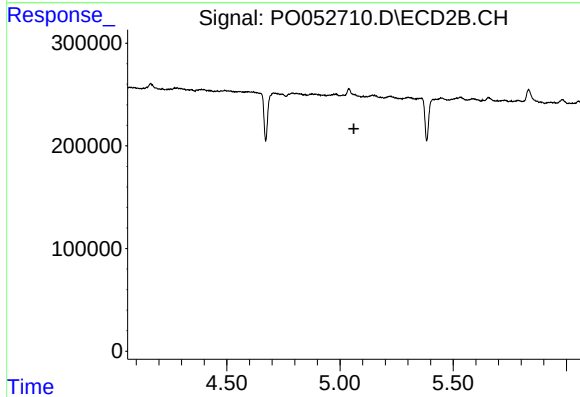


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.061 min
Response: 0
Conc: N.D.

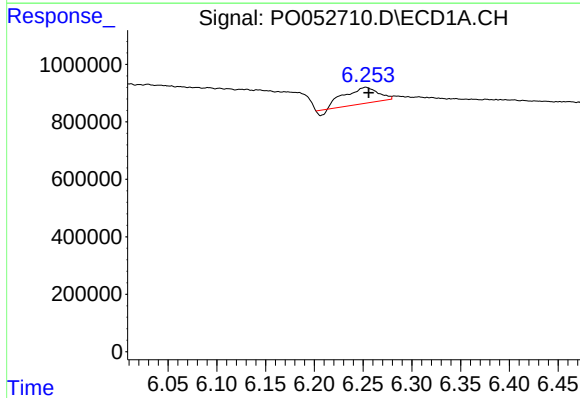


#26 AR-1254-1

R.T.: 6.253 min
Delta R.T.: -0.003 min
Response: 1324793
Conc: 53.03 ng/ml

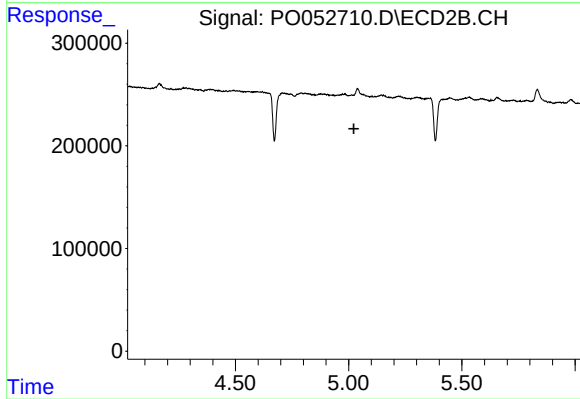

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.023 min
Response: 0
Conc: N.D.

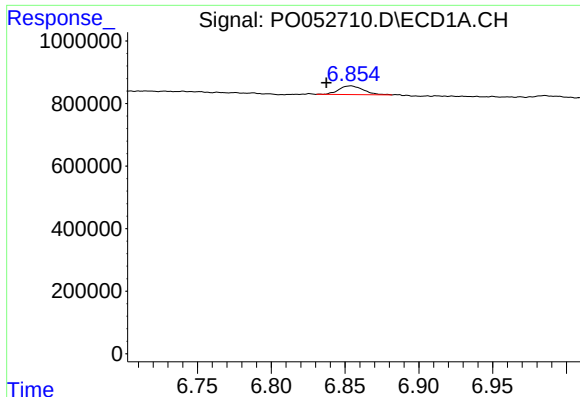

#28 AR-1254-3


R.T.: 6.854 min
Delta R.T.: 0.017 min
Response: 321858
Conc: 8.17 ng/ml

Instrument :
ECD_O
ClientSampleId :

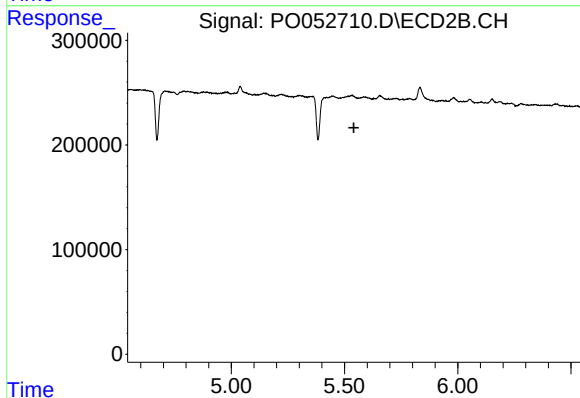


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 5.541 min
Response: 0
Conc: N.D.

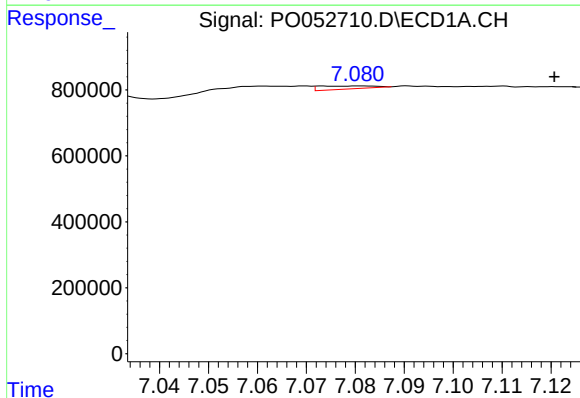

#29 AR-1254-4

R.T.: 7.080 min
Delta R.T.: -0.040 min
Response: 72652
Conc: 2.65 ng/ml

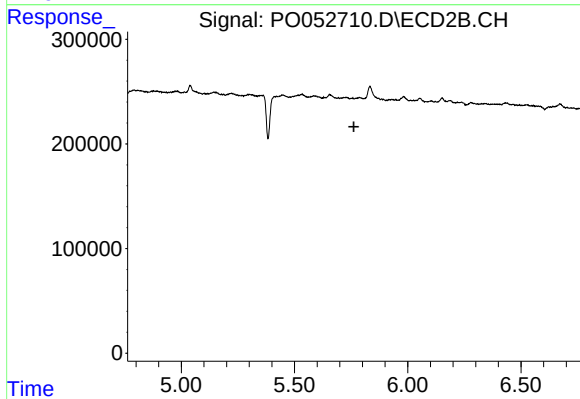

#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 5.763 min
Response: 0
Conc: N.D.