

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121818\
 Data File : PO052688.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Dec 2018 16:52
 Operator : SM/SJ
 Sample : J6437-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 23573

Manual Integrations
 APPROVED

Sohil
 12/19/2018 4:09:11 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 01:25:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Dec 16 03:01:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.252	3.273	18575804	7063415	23.687m	33.333 #
2) SA Decachlor...	9.804	7.959	11190186	4220763	22.209m	19.131

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121818\
Data File : PO052688.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Dec 2018 16:52
Operator : SM/SJ
Sample : J6437-04
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
23573


Manual Integrations
APPROVED

Sohil
12/19/2018 4:09:11 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 01:25:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121518.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Dec 16 03:01:24 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

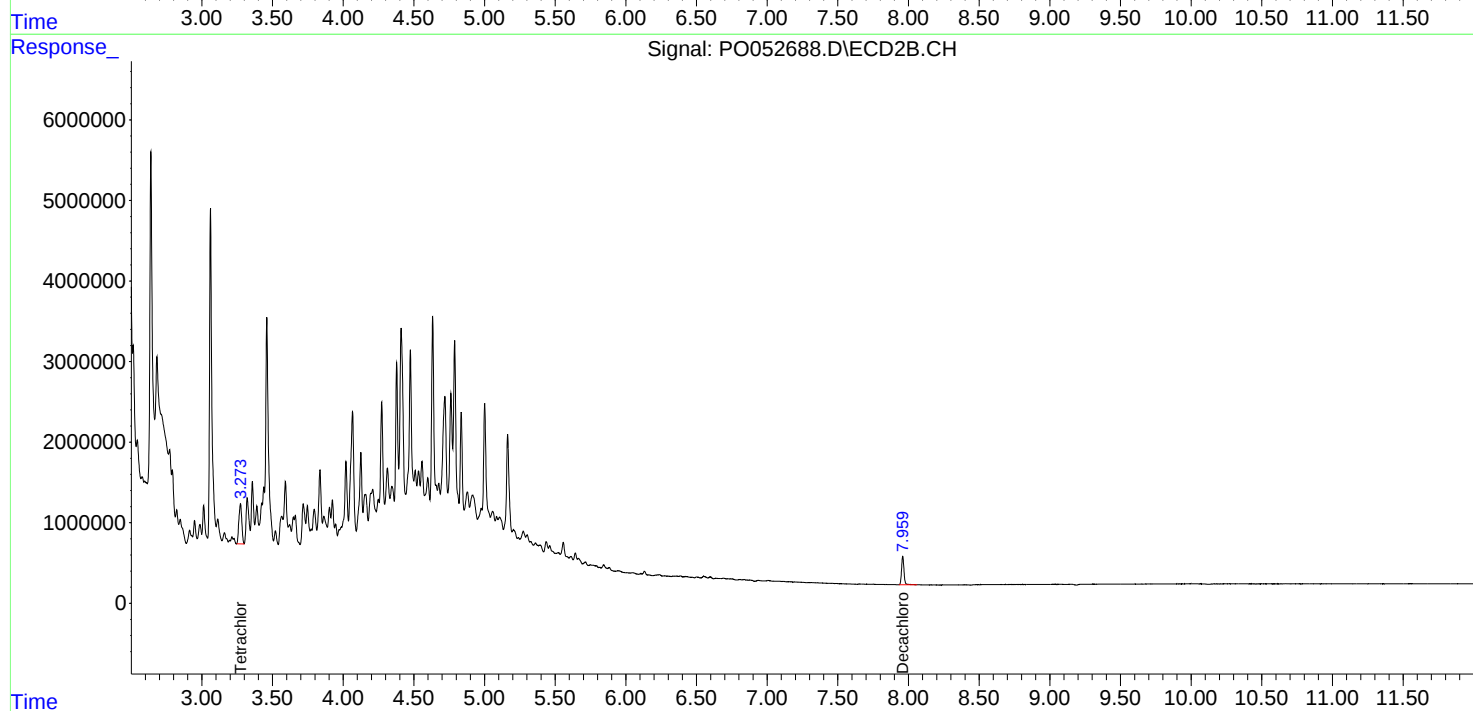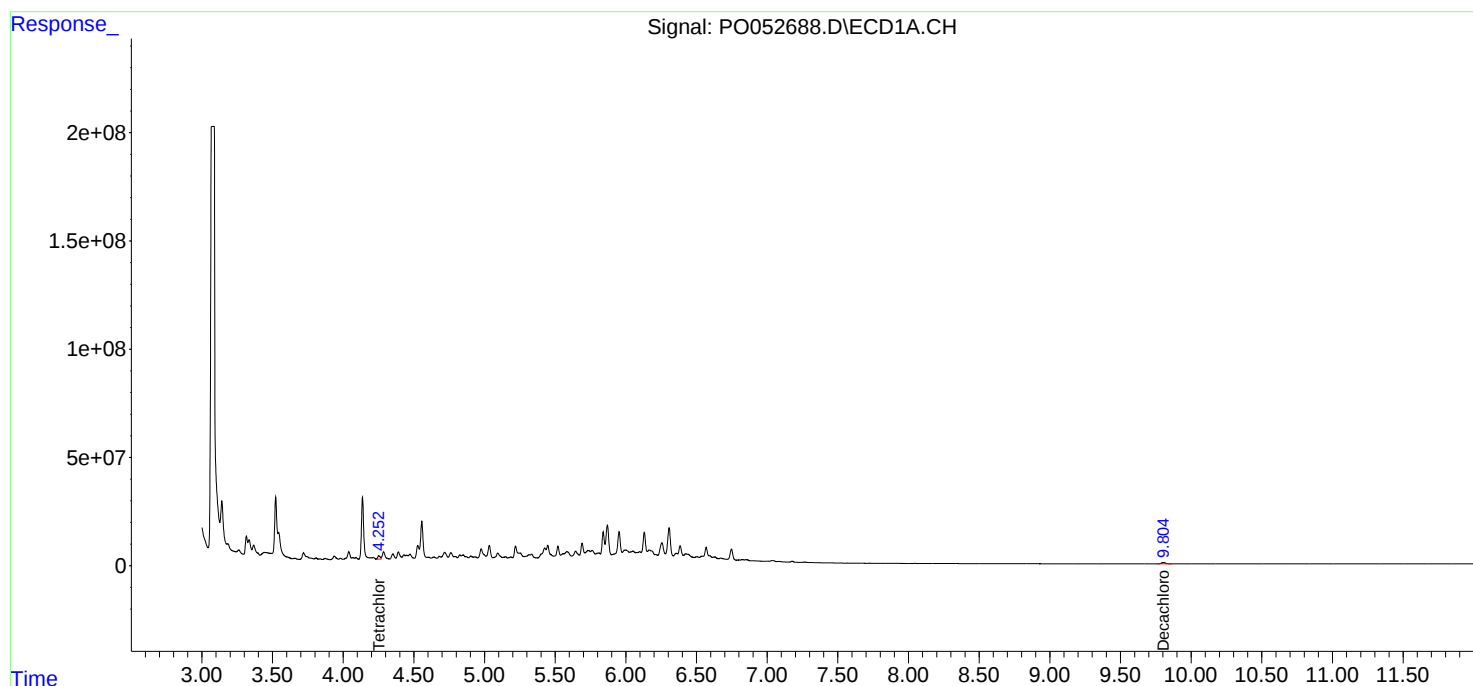

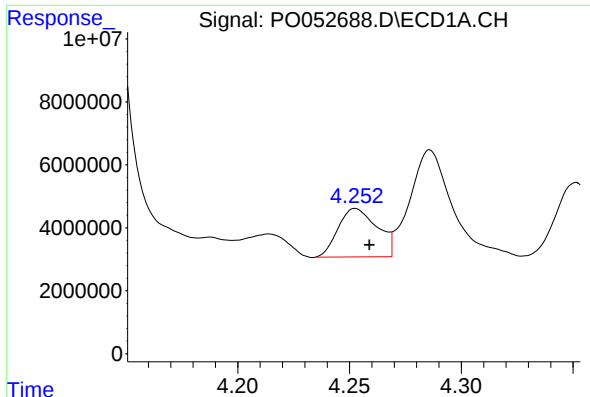


#1 Tetrachloro-m-xylene

R.T.: 4.252 min
Delta R.T.: -0.007 min
Response: 18575804
Conc: 23.69 ng/ml m

Instrument :
ECD_O
ClientSampleId :
23573


Manual Integrations
APPROVED

Sohil
12/19/2018 4:09:11 PM

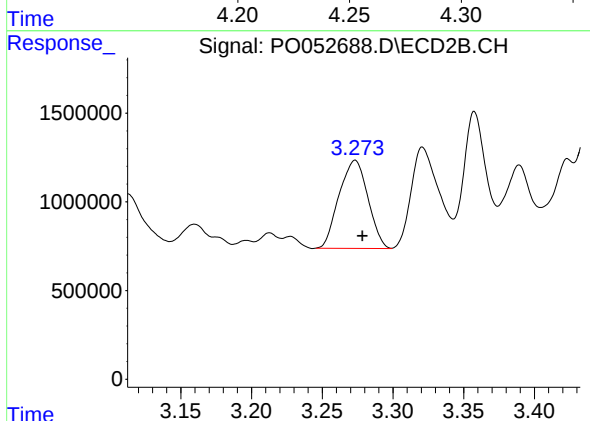


#1 Tetrachloro-m-xylene

R.T.: 3.273 min
Delta R.T.: -0.005 min
Response: 7063415
Conc: 33.33 ng/ml

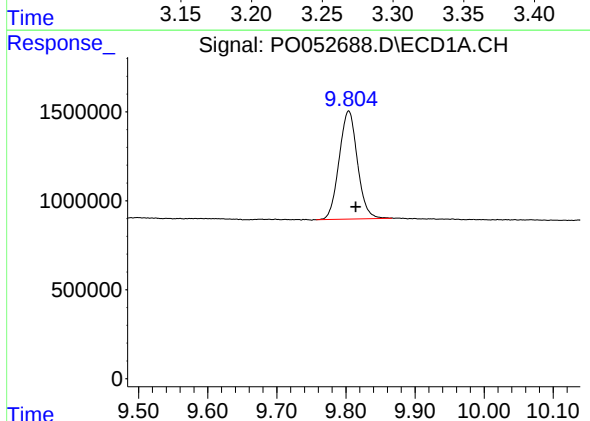

#2 Decachlorobiphenyl

R.T.: 9.804 min
Delta R.T.: -0.011 min
Response: 11190186
Conc: 22.21 ng/ml m

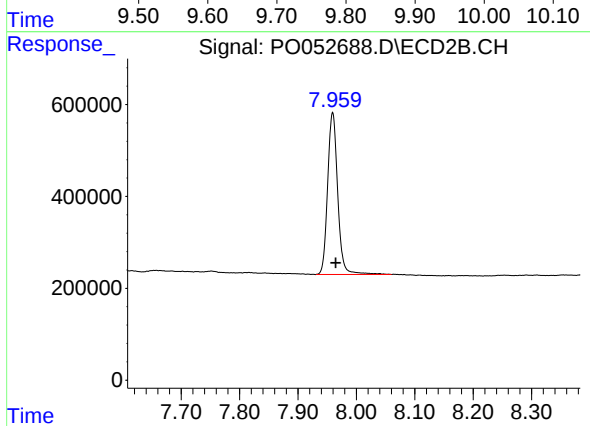

#2 Decachlorobiphenyl

R.T.: 7.959 min
Delta R.T.: -0.005 min
Response: 4220763
Conc: 19.13 ng/ml