

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121818\
 Data File : P0052726.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Dec 2018 4:17
 Operator : SM/SJ
 Sample : J6438-13
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-3

Manual Integrations
 APPROVED

Sohil
 12/19/2018 4:10:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 05:40:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Dec 16 03:01:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.249	3.272	383037	76402	0.488m	0.361m#
2) SA Decachlor...	9.800	7.960	138790	50787	0.275m	0.230m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121818\
Data File : P0052726.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Dec 2018 4:17
Operator : SM/SJ
Sample : J6438-13
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Sohil
12/19/2018 4:10:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 05:40:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121518.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Dec 16 03:01:24 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

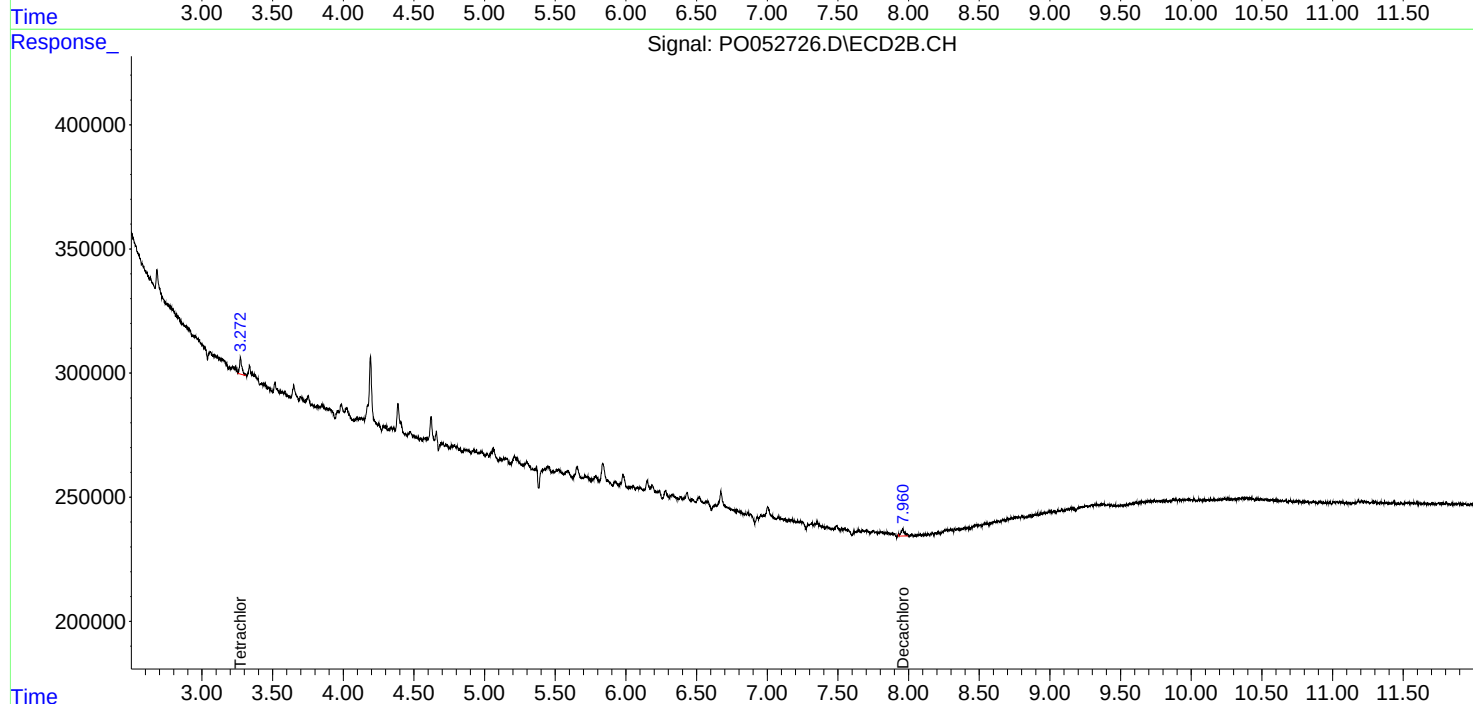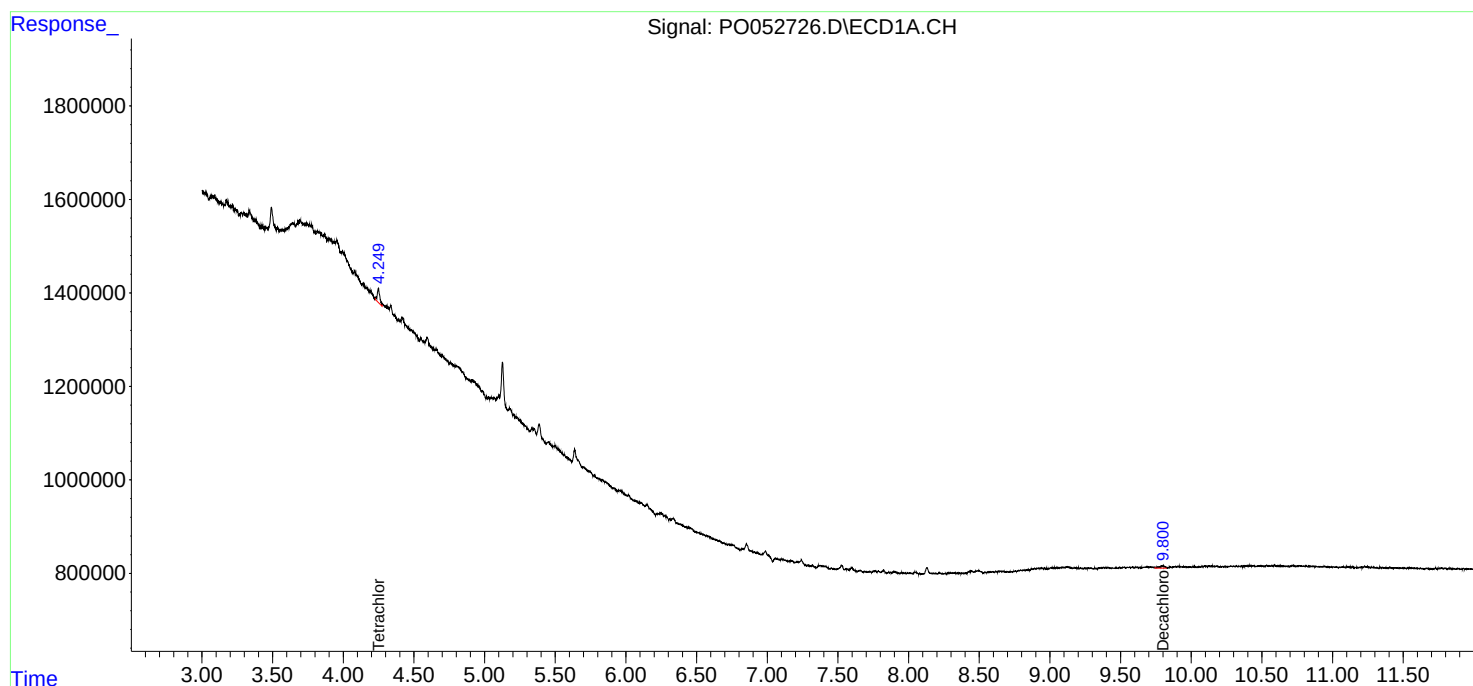

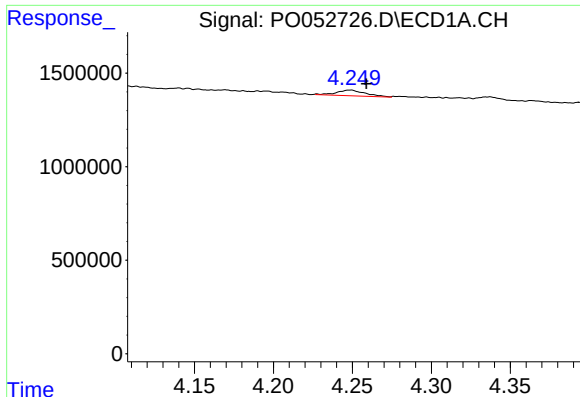


#1 Tetrachloro-m-xylene

R.T.: 4.249 min
Delta R.T.: -0.010 min
Response: 383037
Conc: 0.49 ng/ml m

Instrument :
ECD_O
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Sohil
12/19/2018 4:10:17 PM

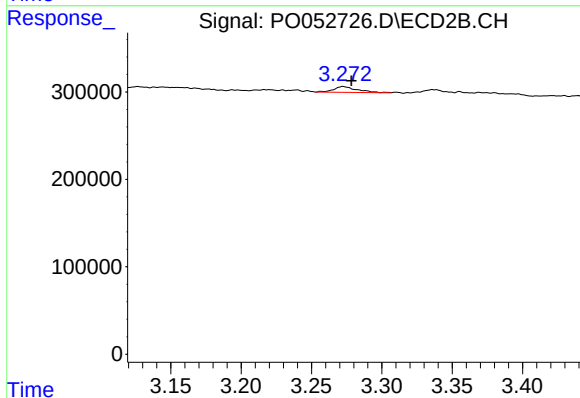


#1 Tetrachloro-m-xylene

R.T.: 3.272 min
Delta R.T.: -0.006 min
Response: 76402
Conc: 0.36 ng/ml m

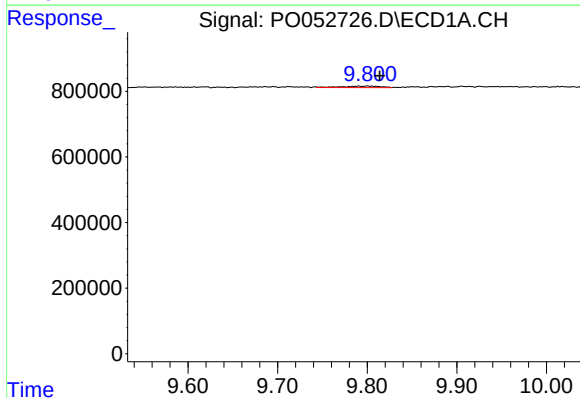

#2 Decachlorobiphenyl

R.T.: 9.800 min
Delta R.T.: -0.014 min
Response: 138790
Conc: 0.28 ng/ml m

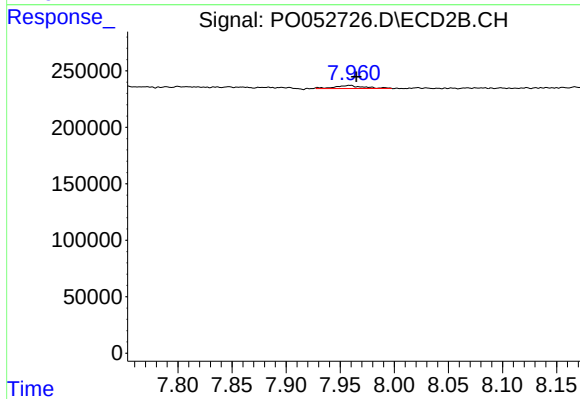

#2 Decachlorobiphenyl

R.T.: 7.960 min
Delta R.T.: -0.005 min
Response: 50787
Conc: 0.23 ng/ml m