

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0121919\
 Data File : P0064788.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Dec 2019 9:15
 Operator : SM/AJ
 Sample : K6325-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 RT-3860

Manual Integrations
 APPROVED

Ankita
 12/20/2019 8:28:21 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 10:52:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0121319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 13 08:19:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.186	3.458	419478	531804	17.230m	20.979m
2) SA Decachlor...	9.708	8.378	548326	697466	17.866	20.083
Target Compounds						
31) L7 AR-1260-1	6.923	5.988	27559	35503	17.938m	19.227m
32) L7 AR-1260-2	7.177	6.175	43760	52278	22.168	22.470m
33) L7 AR-1260-3	7.459	6.328	64470	43200	42.905m	20.403m#
34) L7 AR-1260-4	7.755	6.794	34303	30989	18.570m	16.449m
35) L7 AR-1260-5	8.063	7.035	43094	77167	11.548m	16.453m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121919\
Data File : PO064788.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Dec 2019 9:15
Operator : SM/AJ
Sample : K6325-01
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
RT-3860


Manual Integrations
APPROVED

Ankita
12/20/2019 8:28:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 10:52:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 13 08:19:24 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

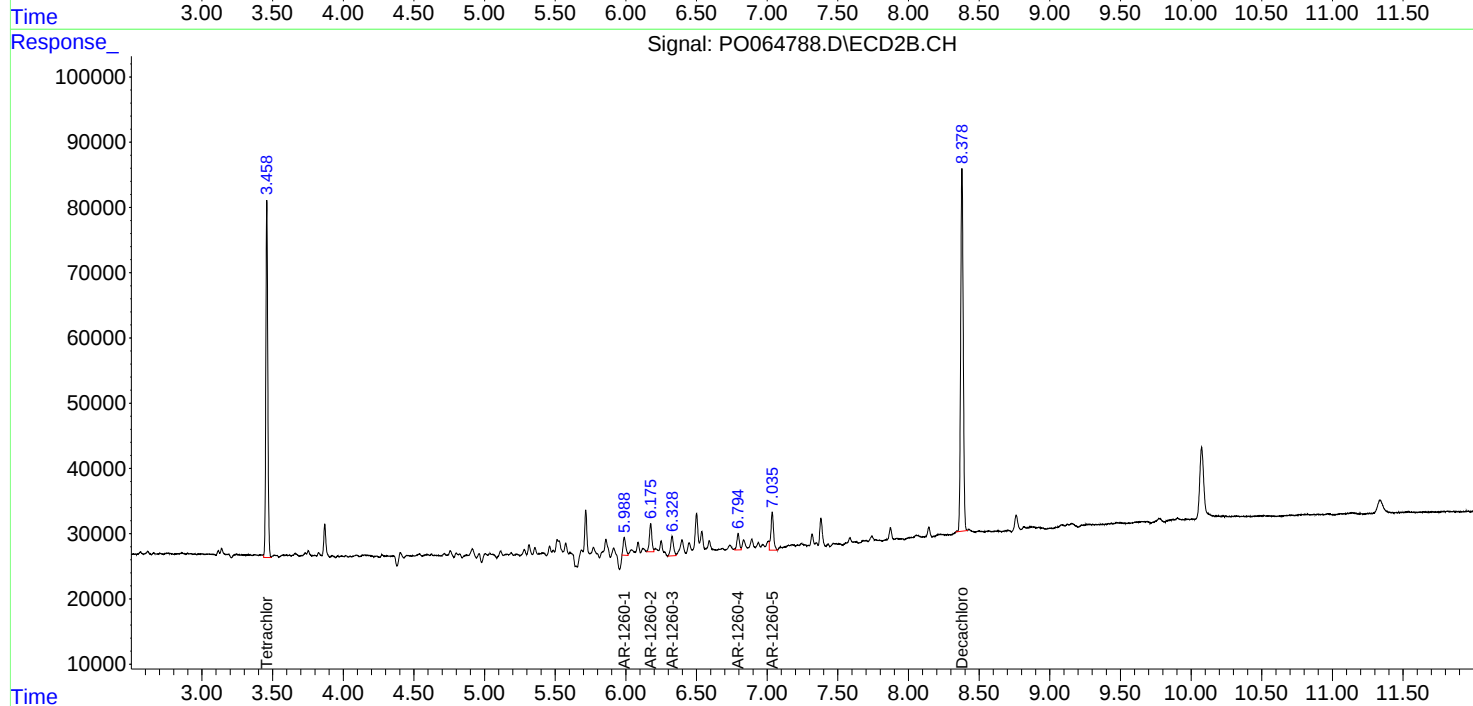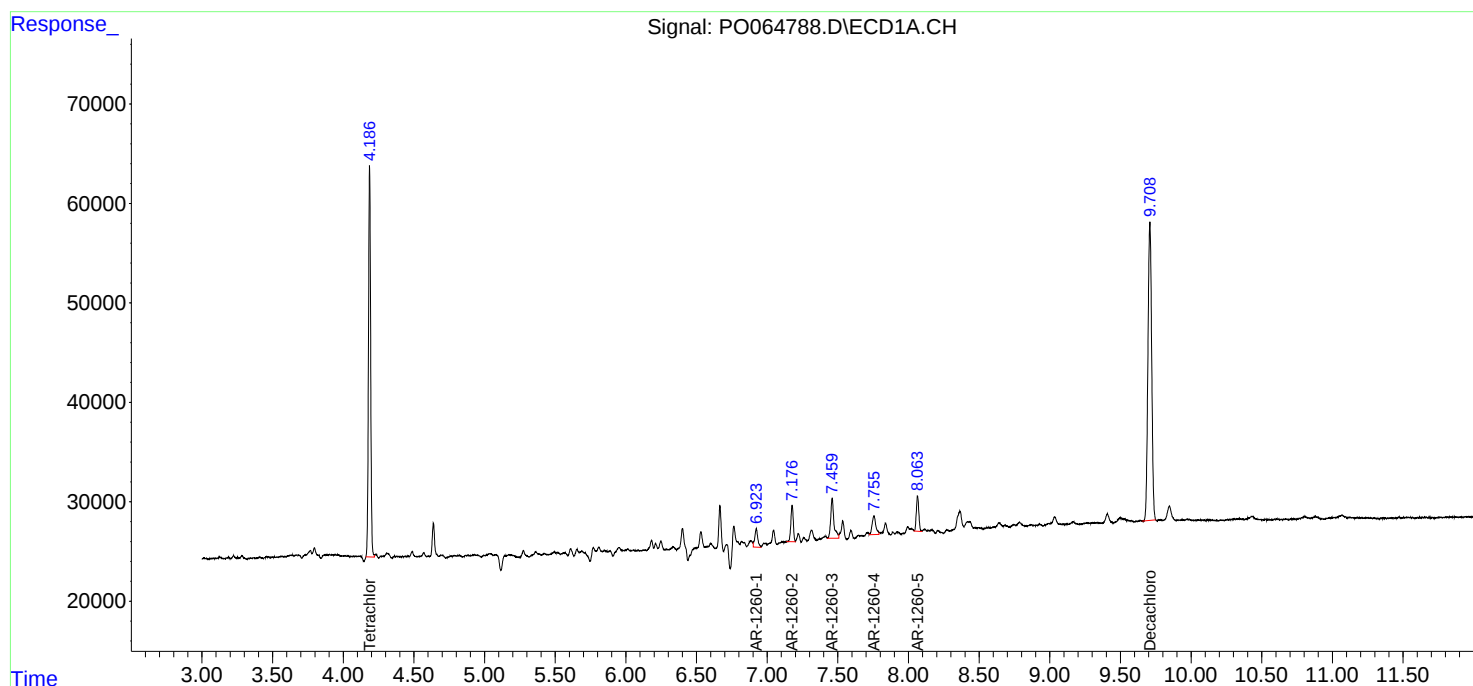

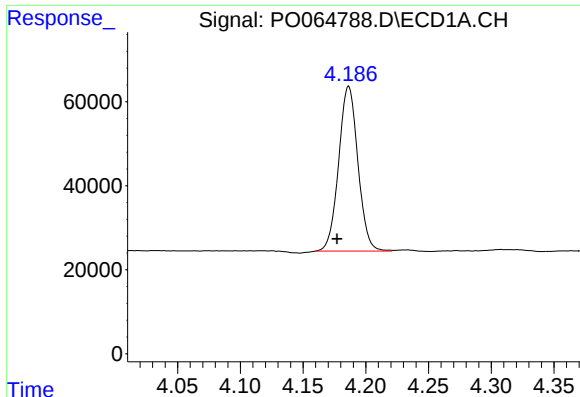


#1 Tetrachloro-m-xylene

R.T.: 4.186 min
Delta R.T.: 0.009 min
Response: 419478
Conc: 17.23 ng/ml m

Instrument :
ECD_O
ClientSampleId :
RT-3860


Manual Integrations
APPROVED

Ankita
12/20/2019 8:28:21 AM

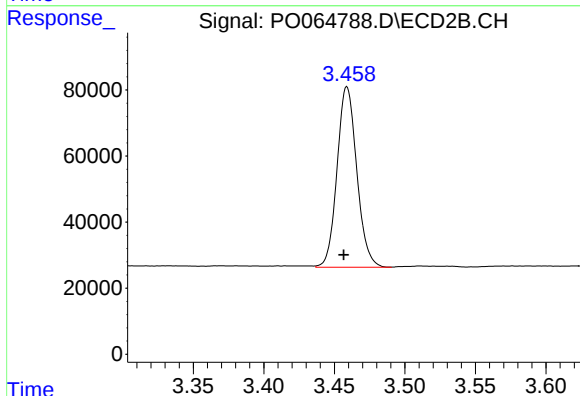


#1 Tetrachloro-m-xylene

R.T.: 3.458 min
Delta R.T.: 0.002 min
Response: 531804
Conc: 20.98 ng/ml m

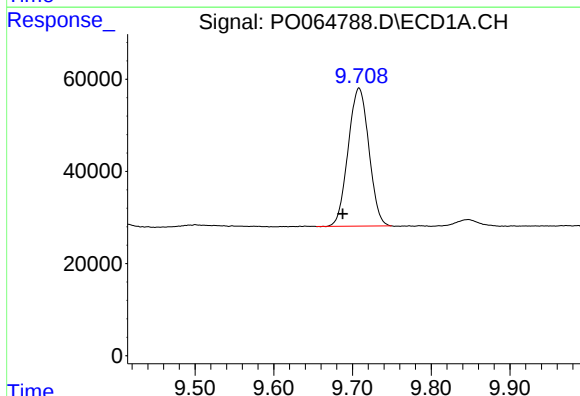


#2 Decachlorobiphenyl

R.T.: 9.708 min
Delta R.T.: 0.021 min
Response: 548326
Conc: 17.87 ng/ml

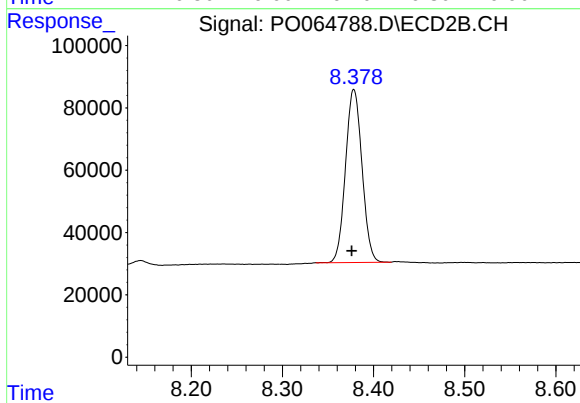

#2 Decachlorobiphenyl

R.T.: 8.378 min
Delta R.T.: 0.002 min
Response: 697466
Conc: 20.08 ng/ml

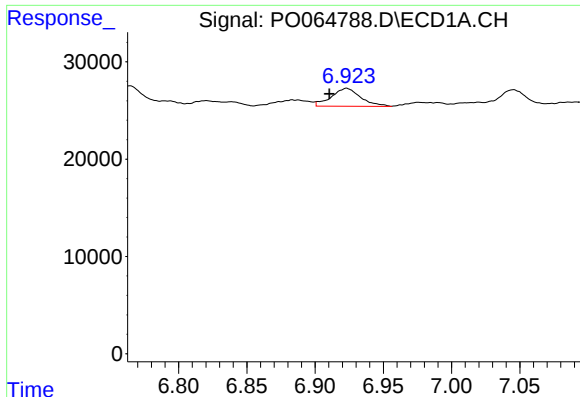


#31 AR-1260-1

R.T.: 6.923 min
Delta R.T.: 0.012 min
Response: 27559
Conc: 17.94 ng/ml m

Instrument :
ECD_O
ClientSampleId :
RT-3860


Manual Integrations
APPROVED

Ankita
12/20/2019 8:28:21 AM

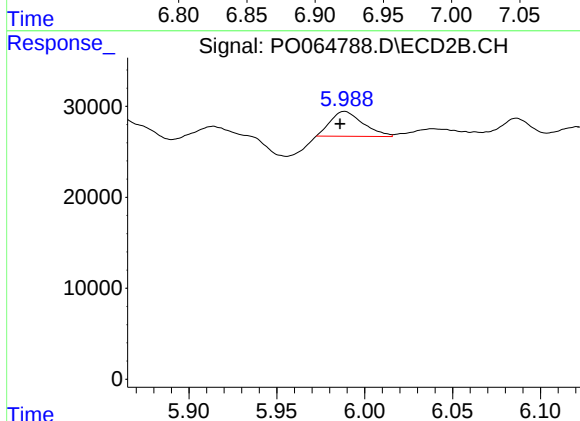


#31 AR-1260-1

R.T.: 5.988 min
Delta R.T.: 0.002 min
Response: 35503
Conc: 19.23 ng/ml m

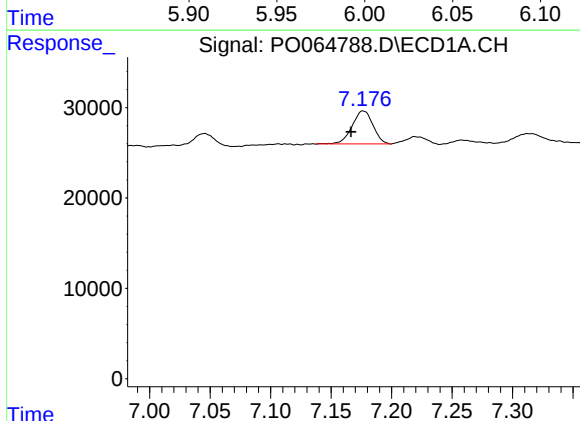


#32 AR-1260-2

R.T.: 7.177 min
Delta R.T.: 0.010 min
Response: 43760
Conc: 22.17 ng/ml

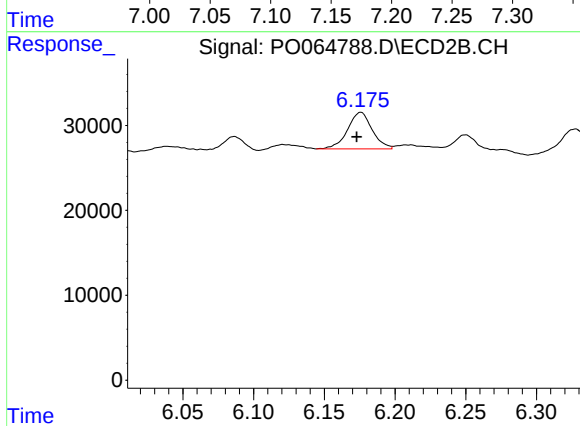

#32 AR-1260-2

R.T.: 6.175 min
Delta R.T.: 0.002 min
Response: 52278
Conc: 22.47 ng/ml m

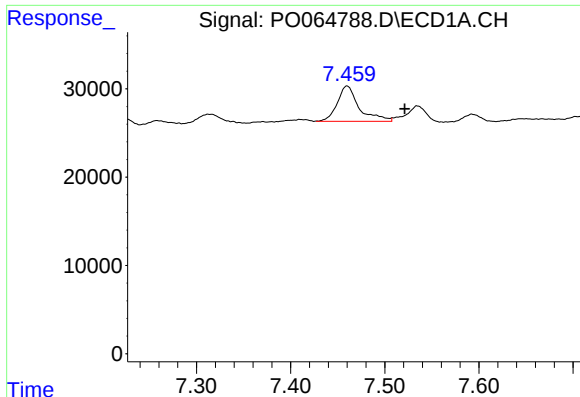


#33 AR-1260-3

R.T.: 7.459 min
Delta R.T.: -0.062 min
Response: 64470
Conc: 42.91 ng/ml m

Instrument :
ECD_O
ClientSampleId :
RT-3860


Manual Integrations
APPROVED

Ankita
12/20/2019 8:28:21 AM

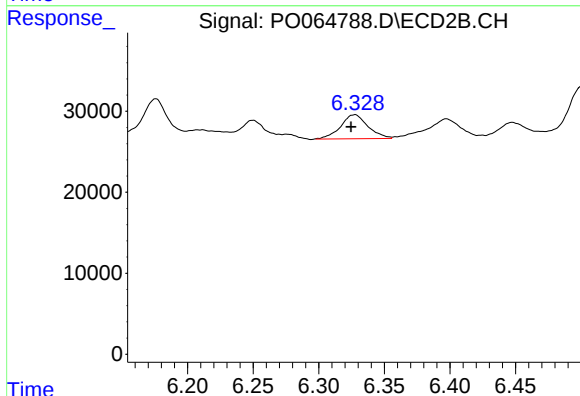


#33 AR-1260-3

R.T.: 6.328 min
Delta R.T.: 0.003 min
Response: 43200
Conc: 20.40 ng/ml m

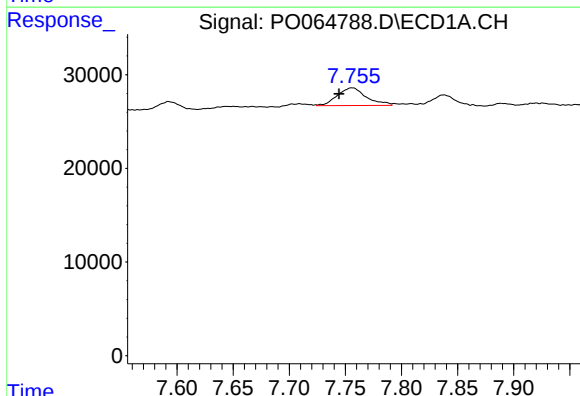


#34 AR-1260-4

R.T.: 7.755 min
Delta R.T.: 0.011 min
Response: 34303
Conc: 18.57 ng/ml m

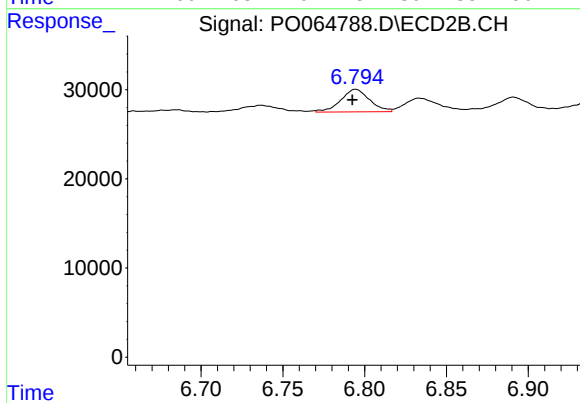

#34 AR-1260-4

R.T.: 6.794 min
Delta R.T.: 0.001 min
Response: 30989
Conc: 16.45 ng/ml m

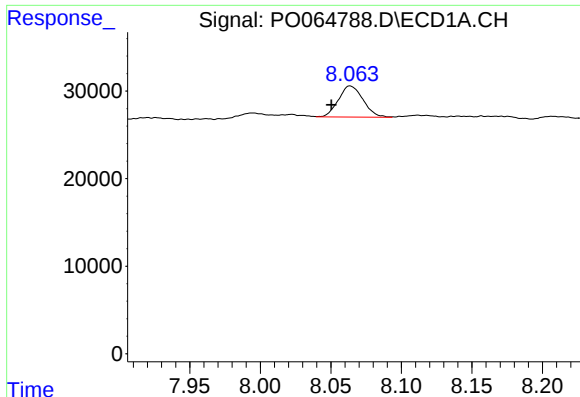


#35 AR-1260-5

R.T.: 8.063 min
Delta R.T.: 0.013 min
Response: 43094
Conc: 11.55 ng/ml m

Instrument :
ECD_O
ClientSampleId :
RT-3860

Manual Integrations
APPROVED

Ankita
12/20/2019 8:28:21 AM

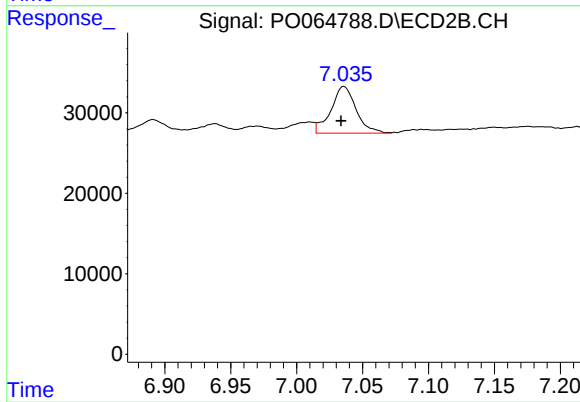

#35 AR-1260-5

R.T.: 7.035 min
Delta R.T.: 0.002 min
Response: 77167
Conc: 16.45 ng/ml m