

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122419\
 Data File : P0064913.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Dec 2019 12:26
 Operator : SM/AJ
 Sample : K6117-07
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TR-04-121919

Manual Integrations
 APPROVED

Ankita
 12/26/2019 1:39:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 13:06:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 13 08:19:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.191	3.456	542985	717732	22.304	28.314 #
2) SA Decachlor...	9.713	8.375	612129	756874	19.945m	21.794

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122419\
Data File : P0064913.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Dec 2019 12:26
Operator : SM/AJ
Sample : K6117-07
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TR-04-121919


Manual Integrations
APPROVED

Ankita
12/26/2019 1:39:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 13:06:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 13 08:19:24 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

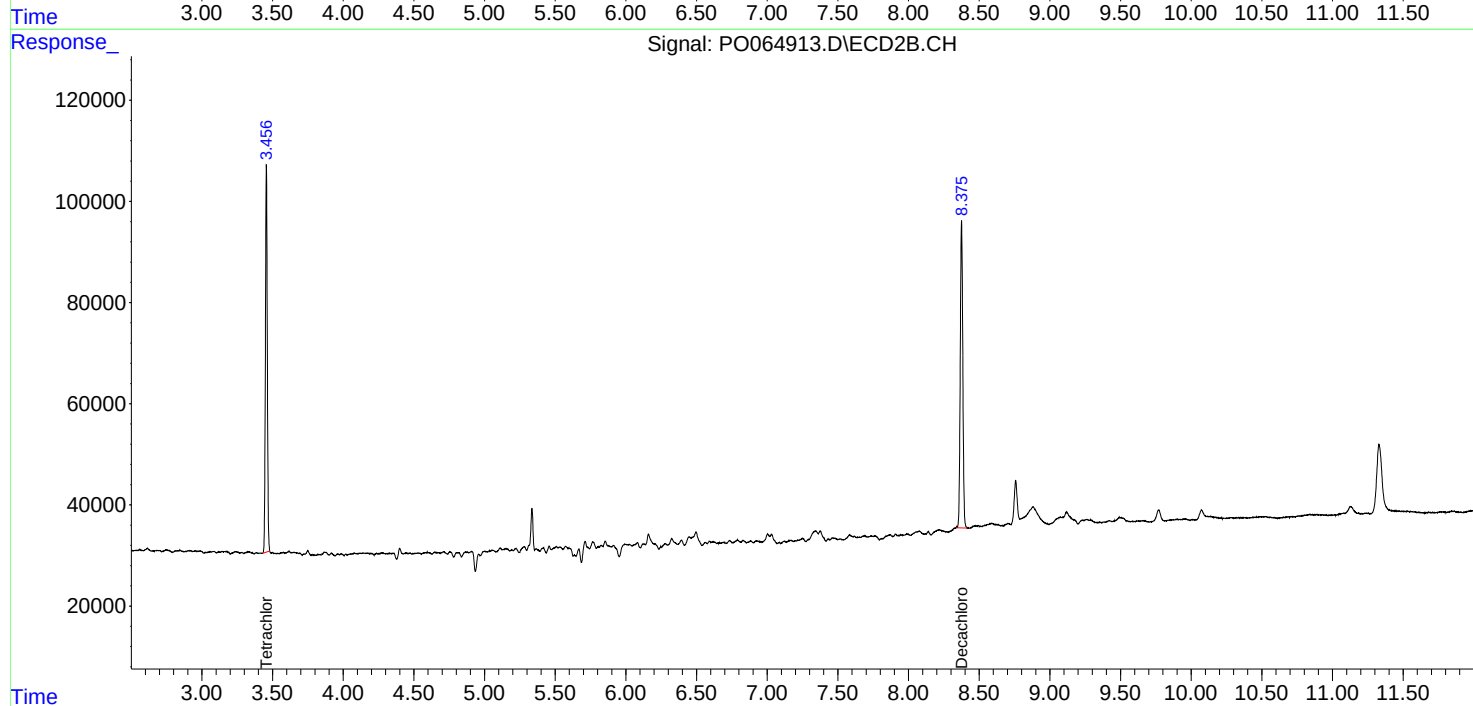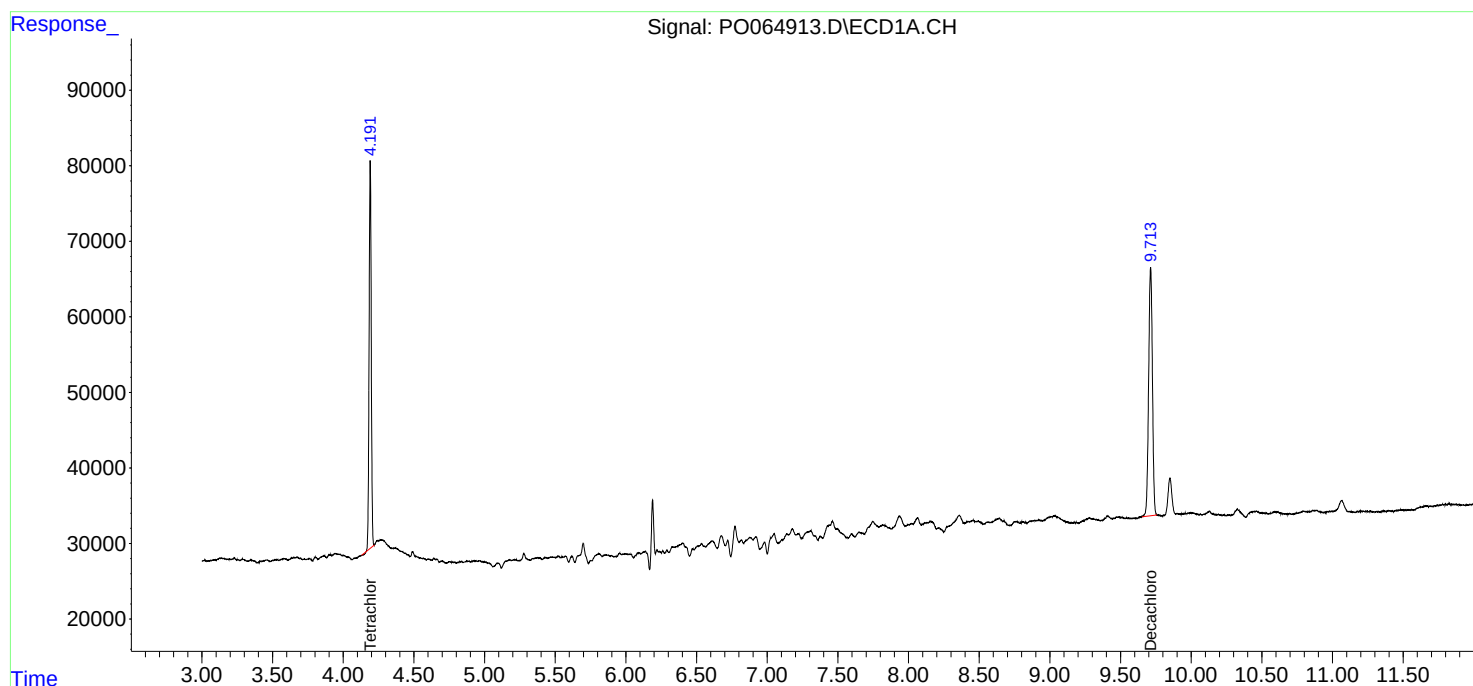

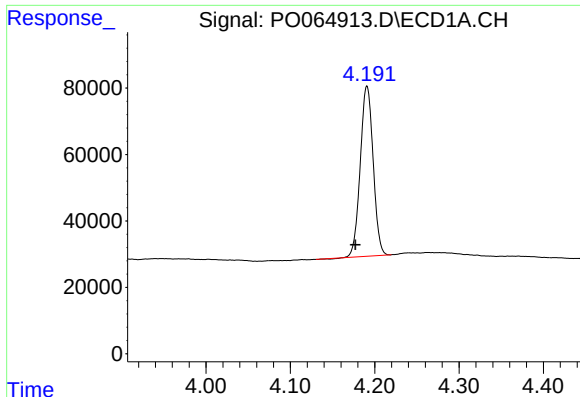


#1 Tetrachloro-m-xylene

R.T.: 4.191 min
Delta R.T.: 0.014 min
Response: 542985
Conc: 22.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
TR-04-121919


Manual Integrations
APPROVED

Ankita
12/26/2019 1:39:36 PM

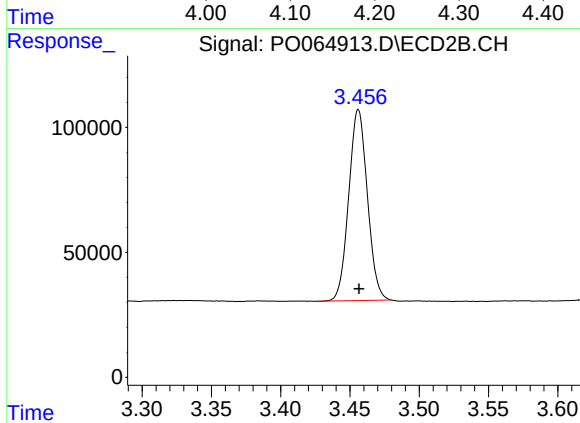


#1 Tetrachloro-m-xylene

R.T.: 3.456 min
Delta R.T.: 0.000 min
Response: 717732
Conc: 28.31 ng/ml

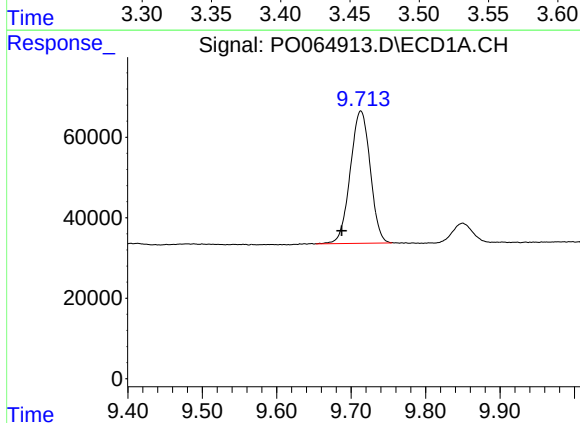

#2 Decachlorobiphenyl

R.T.: 9.713 min
Delta R.T.: 0.025 min
Response: 612129
Conc: 19.95 ng/ml m

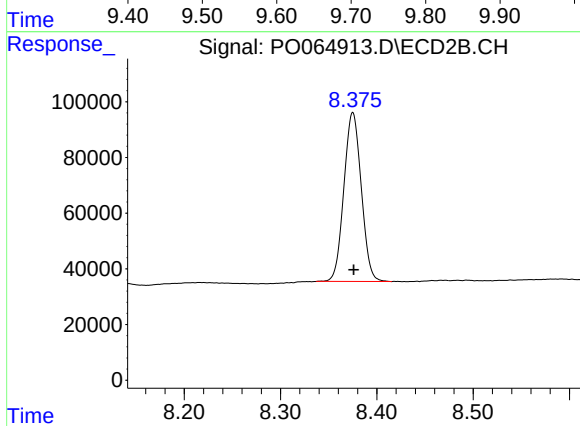

#2 Decachlorobiphenyl

R.T.: 8.375 min
Delta R.T.: -0.001 min
Response: 756874
Conc: 21.79 ng/ml