

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122419\
 Data File : P0064939.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Dec 2019 23:06
 Operator : SM/AJ
 Sample : K6396-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-2-(4-5)

Manual Integrations
 APPROVED

Ankita
 12/26/2019 1:41:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 04:20:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 13 08:19:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.182	3.456	593319	771611	24.371	30.439m
2) SA Decachlor...	9.700	8.371	456803	579636	14.884	16.691

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122419\
Data File : P0064939.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Dec 2019 23:06
Operator : SM/AJ
Sample : K6396-03
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-2-(4-5)


Manual Integrations
APPROVED

Ankita
12/26/2019 1:41:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 04:20:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 13 08:19:24 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

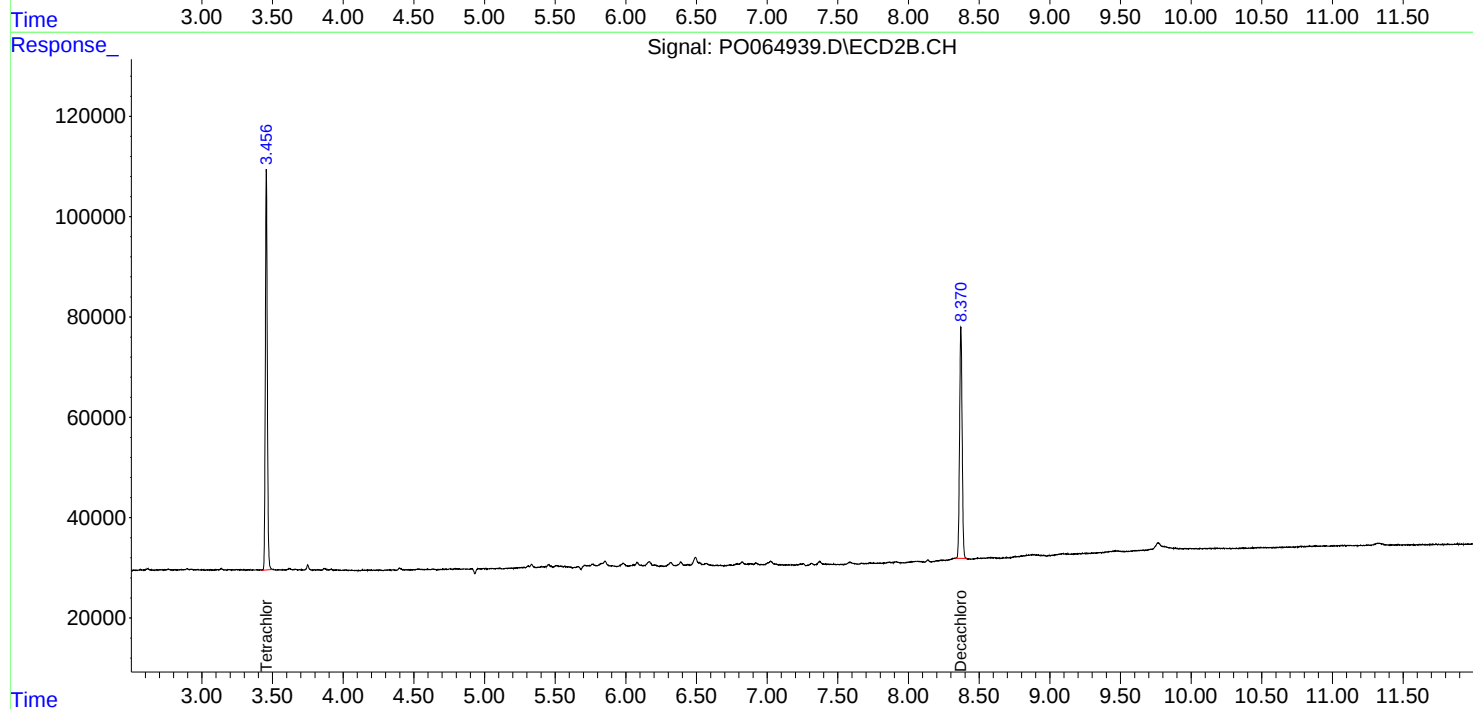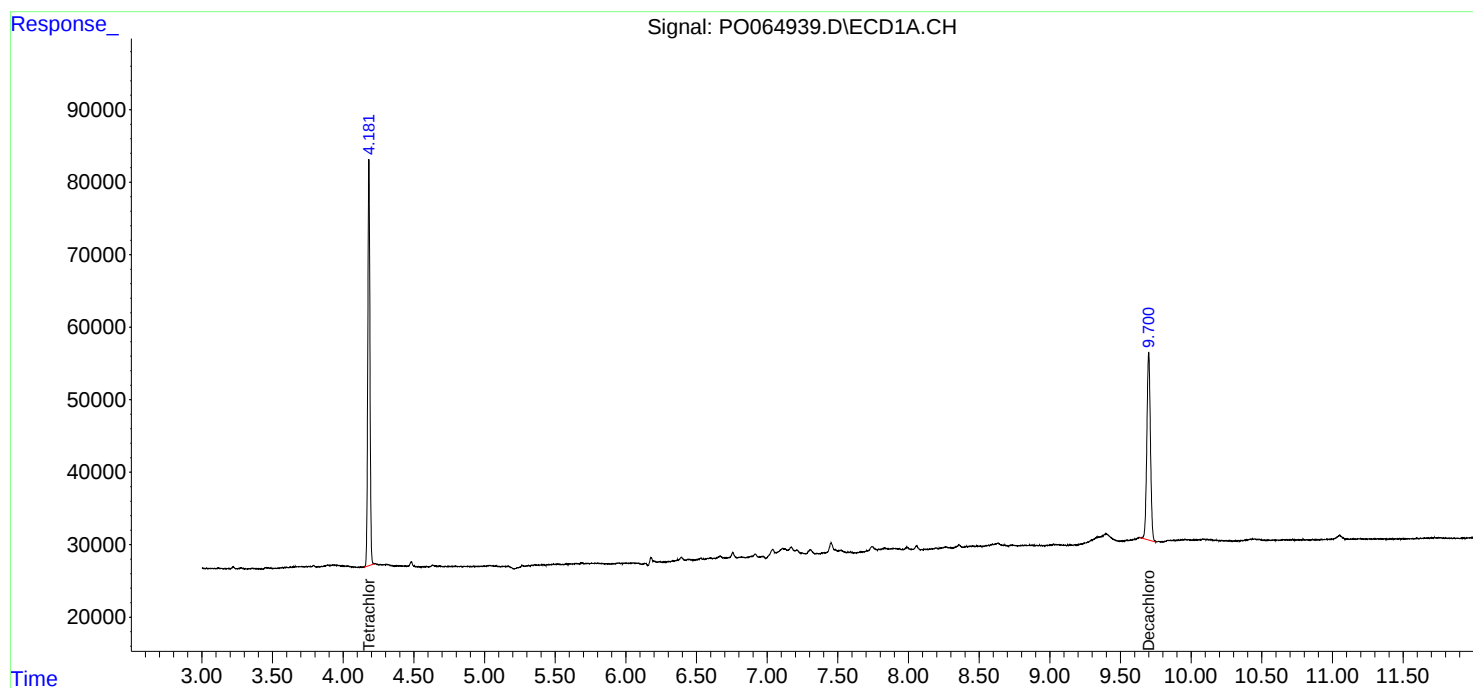

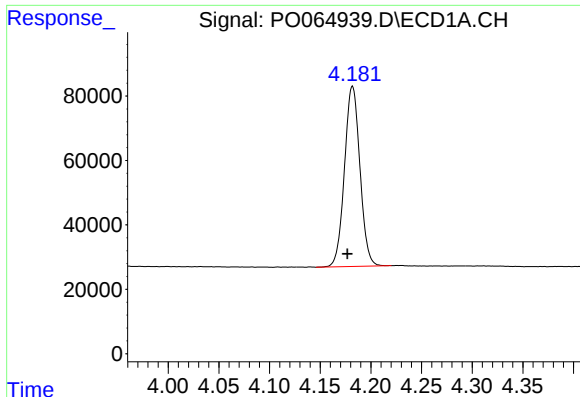


#1 Tetrachloro-m-xylene

R.T.: 4.182 min
Delta R.T.: 0.005 min
Response: 593319
Conc: 24.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-2-(4-5)


Manual Integrations
APPROVED

Ankita
12/26/2019 1:41:22 PM

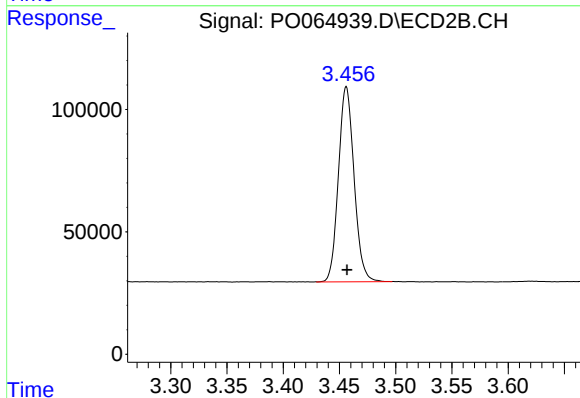


#1 Tetrachloro-m-xylene

R.T.: 3.456 min
Delta R.T.: 0.000 min
Response: 771611
Conc: 30.44 ng/ml m

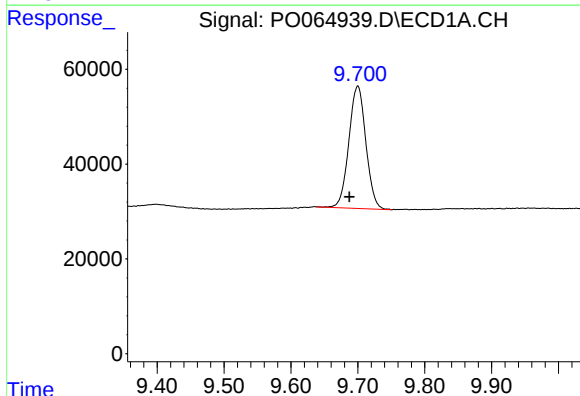

#2 Decachlorobiphenyl

R.T.: 9.700 min
Delta R.T.: 0.013 min
Response: 456803
Conc: 14.88 ng/ml

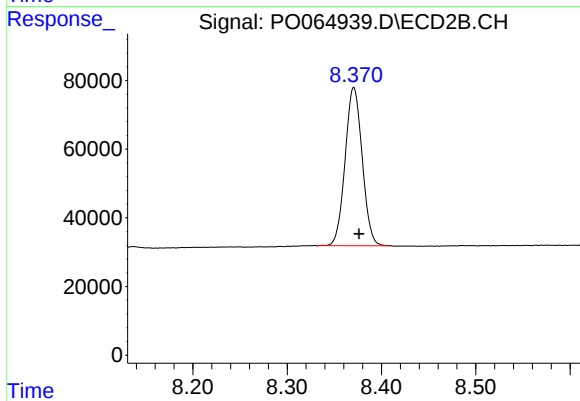

#2 Decachlorobiphenyl

R.T.: 8.371 min
Delta R.T.: -0.005 min
Response: 579636
Conc: 16.69 ng/ml