

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122419\
 Data File : P0064942.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Dec 2019 23:56
 Operator : SM/AJ
 Sample : K6396-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-2-(8-10)

Manual Integrations
 APPROVED

Ankita
 12/26/2019 1:41:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 04:21:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 13 08:19:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.183	3.459	700828	679852	28.787	26.819m
2) SA Decachlor...	9.699	8.371	391565	489685	12.759	14.100

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122419\
Data File : P0064942.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Dec 2019 23:56
Operator : SM/AJ
Sample : K6396-06
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-2-(8-10)


Manual Integrations
APPROVED

Ankita
12/26/2019 1:41:28 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 04:21:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 13 08:19:24 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

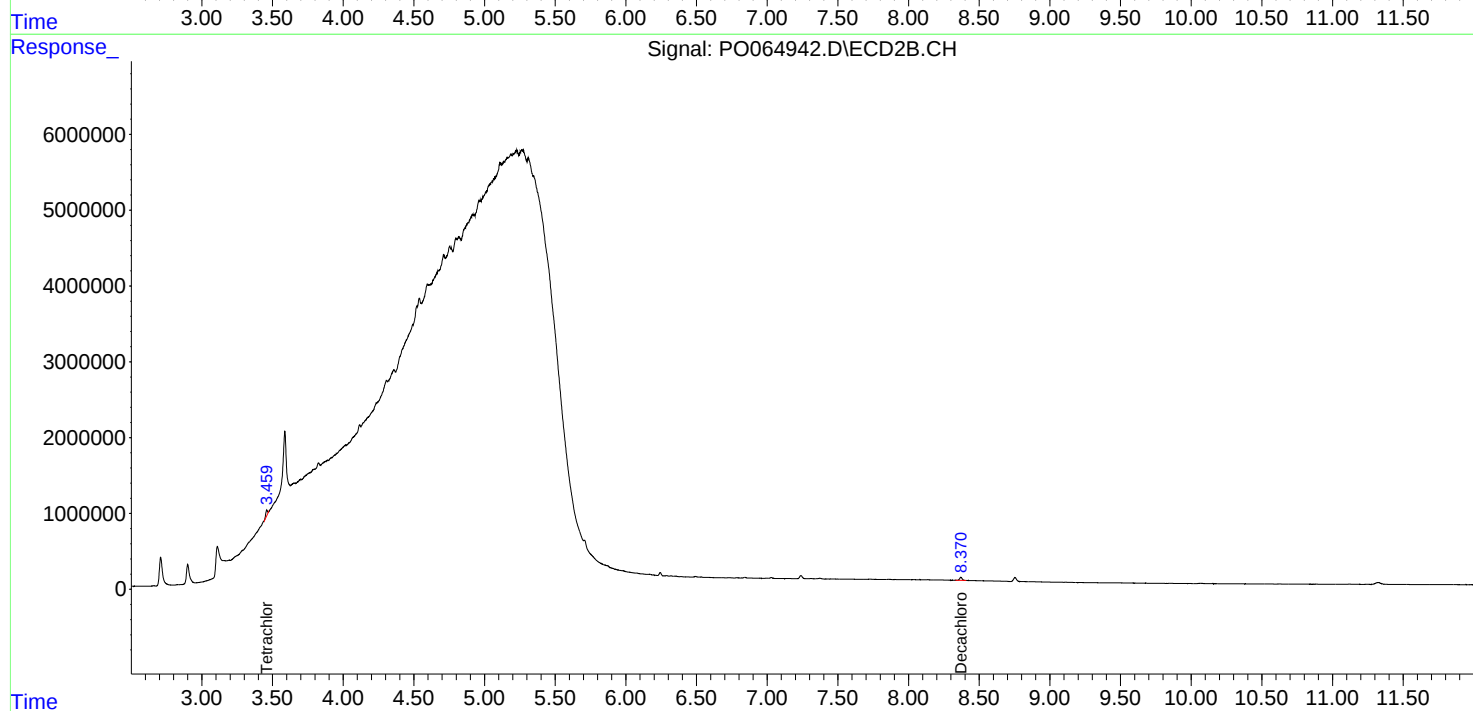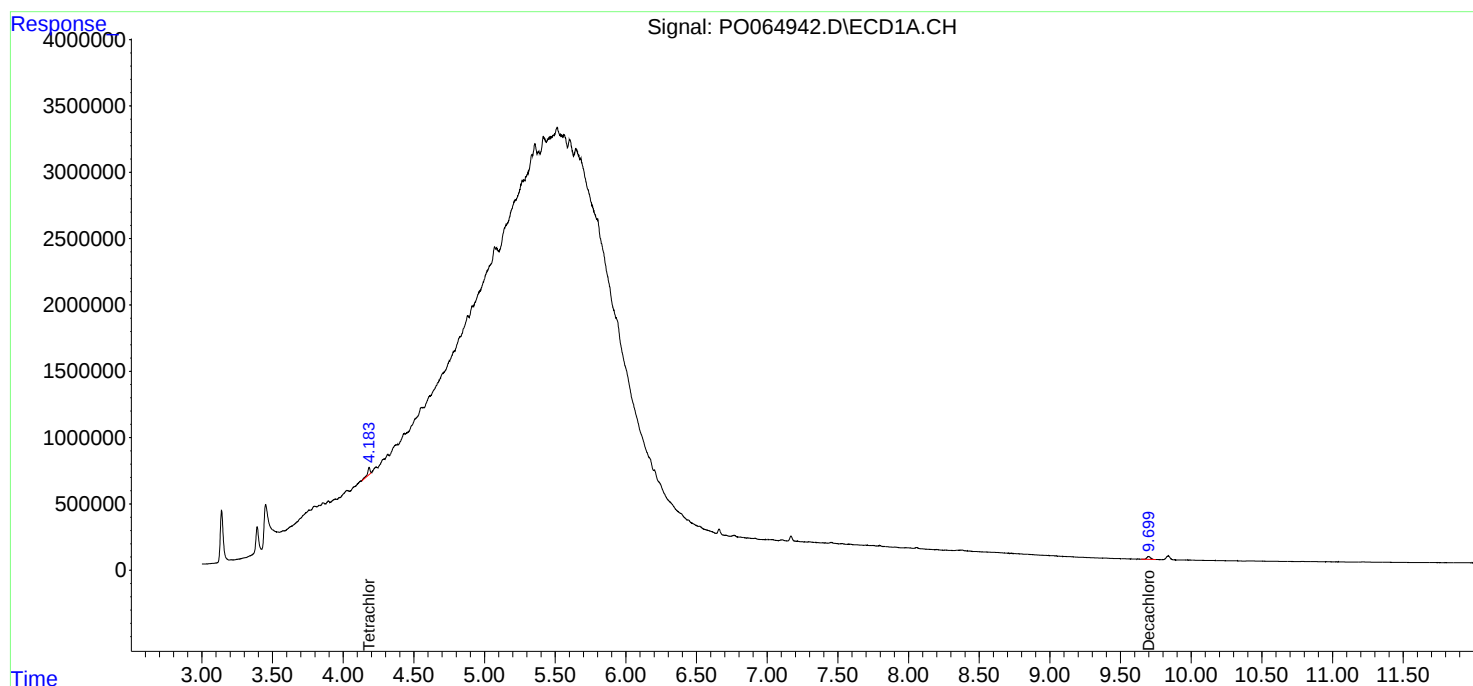

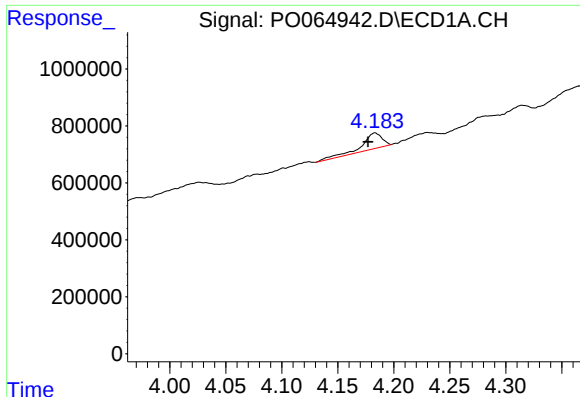


#1 Tetrachloro-m-xylene

R.T.: 4.183 min
Delta R.T.: 0.006 min
Response: 700828
Conc: 28.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-2-(8-10)


Manual Integrations
APPROVED

Ankita
12/26/2019 1:41:28 PM

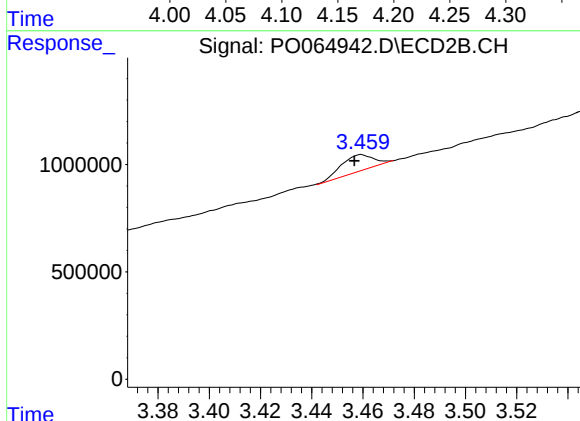


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: 0.002 min
Response: 679852
Conc: 26.82 ng/ml m

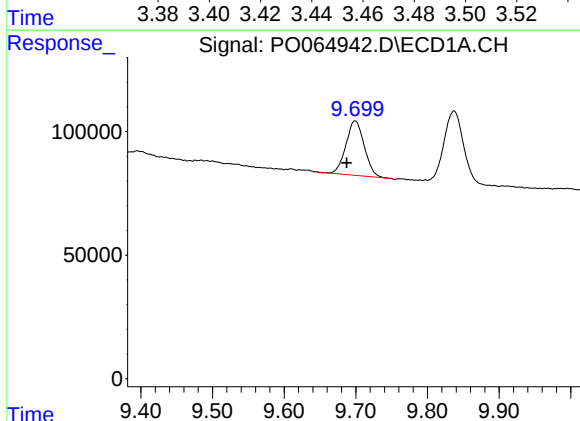

#2 Decachlorobiphenyl

R.T.: 9.699 min
Delta R.T.: 0.011 min
Response: 391565
Conc: 12.76 ng/ml

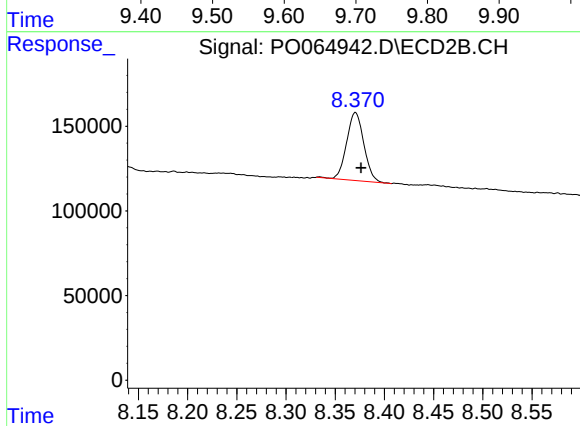

#2 Decachlorobiphenyl

R.T.: 8.371 min
Delta R.T.: -0.006 min
Response: 489685
Conc: 14.10 ng/ml