

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122419\
 Data File : P0064944.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Dec 2019 00:30
 Operator : SM/AJ
 Sample : K6396-08
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-3-(3-4)

Manual Integrations
 APPROVED

Ankita
 12/26/2019 1:41:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 04:22:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 13 08:19:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.181	3.456	580593	779270	23.848m	30.741 #
2) SA Decachlor...	9.699	8.370	385531	481471	12.562	13.864

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122419\
Data File : P0064944.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Dec 2019 00:30
Operator : SM/AJ
Sample : K6396-08
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-3-(3-4)


Manual Integrations
APPROVED

Ankita
12/26/2019 1:41:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 04:22:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 13 08:19:24 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

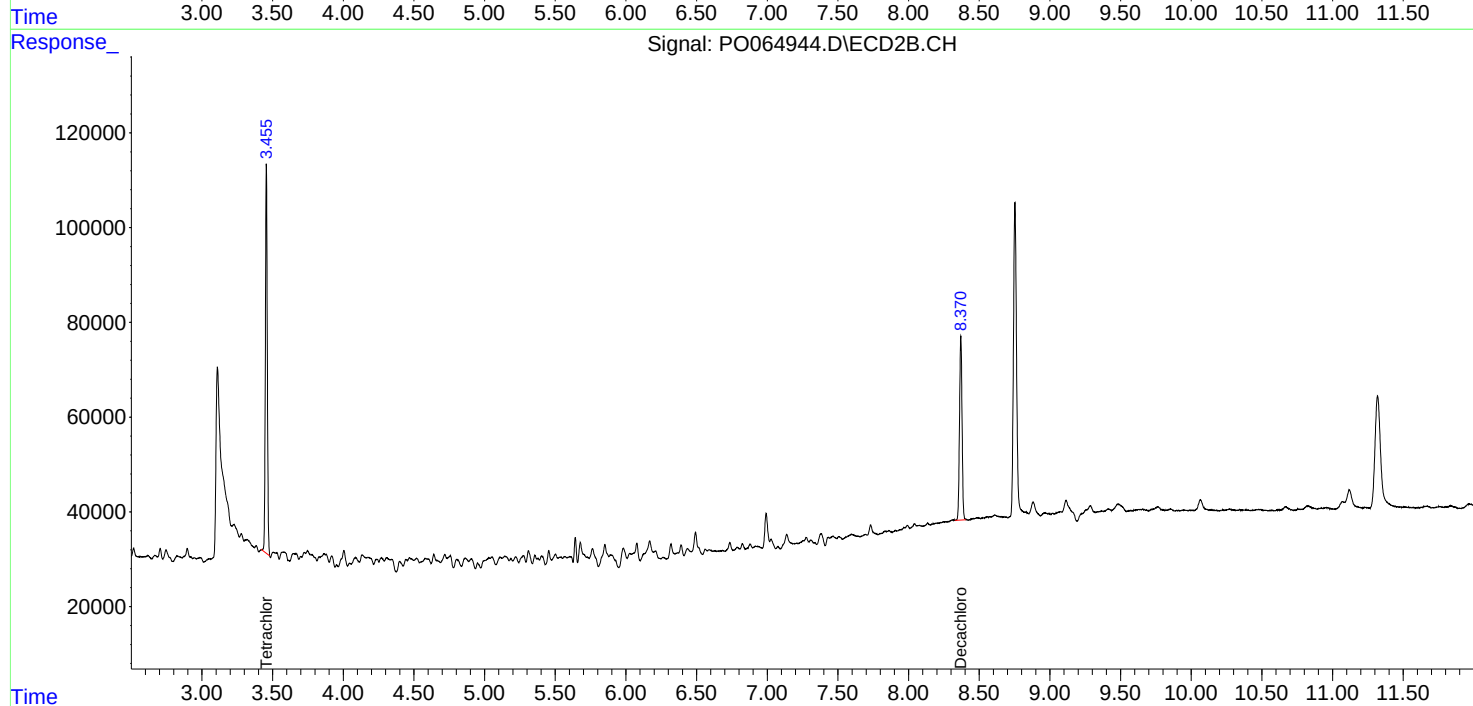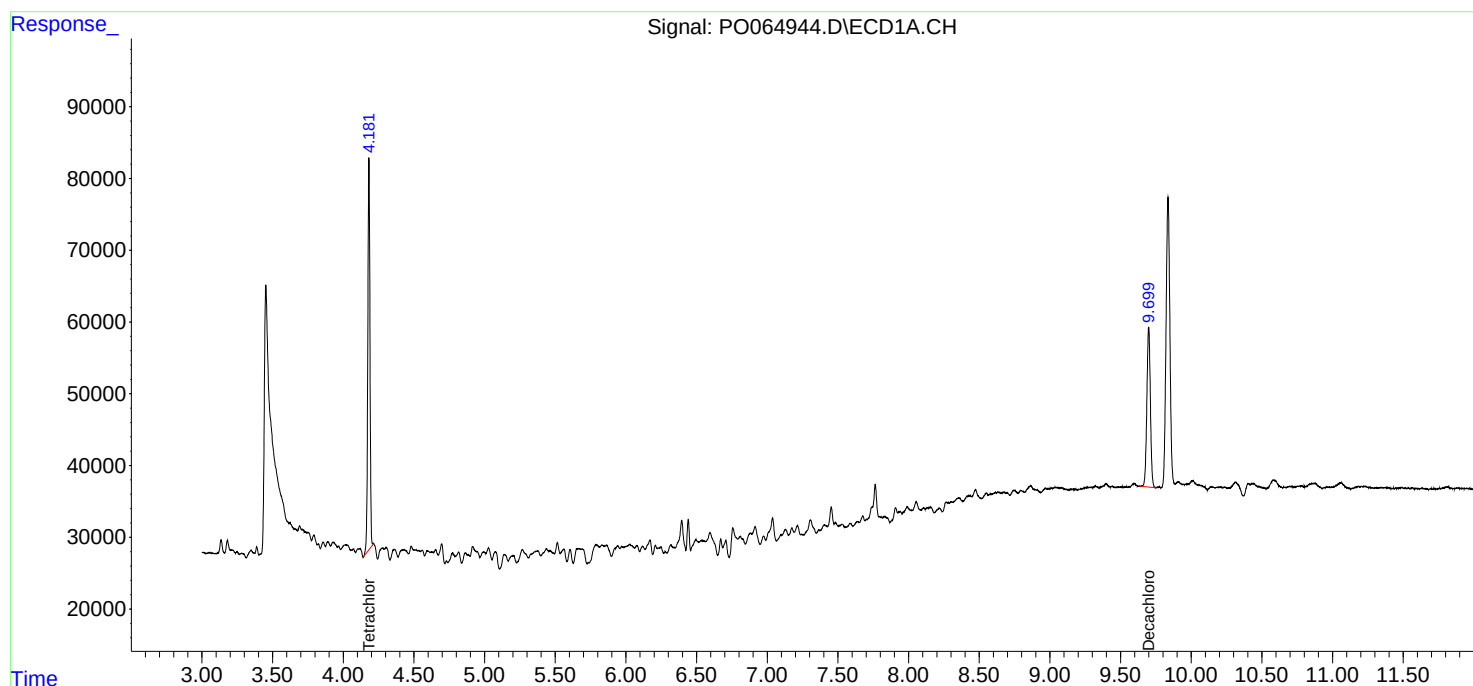

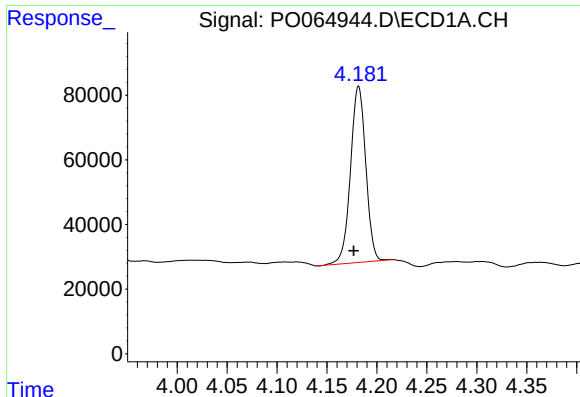


#1 Tetrachloro-m-xylene

R.T.: 4.181 min
Delta R.T.: 0.004 min
Response: 580593
Conc: 23.85 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-3-(3-4)


Manual Integrations
APPROVED

Ankita
12/26/2019 1:41:32 PM

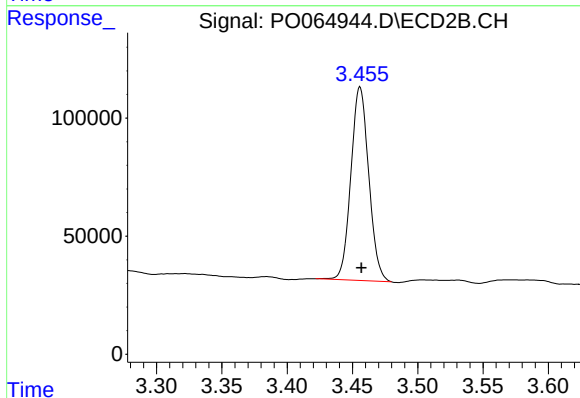


#1 Tetrachloro-m-xylene

R.T.: 3.456 min
Delta R.T.: 0.000 min
Response: 779270
Conc: 30.74 ng/ml

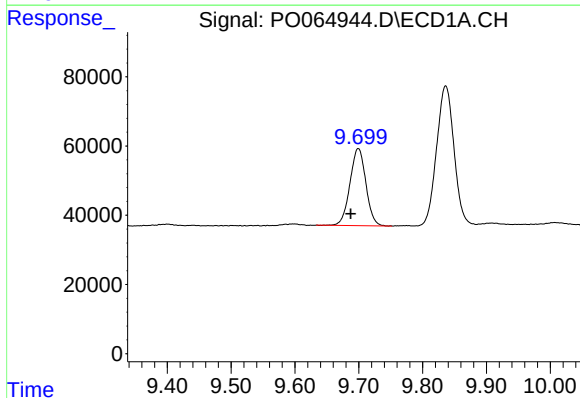

#2 Decachlorobiphenyl

R.T.: 9.699 min
Delta R.T.: 0.012 min
Response: 385531
Conc: 12.56 ng/ml

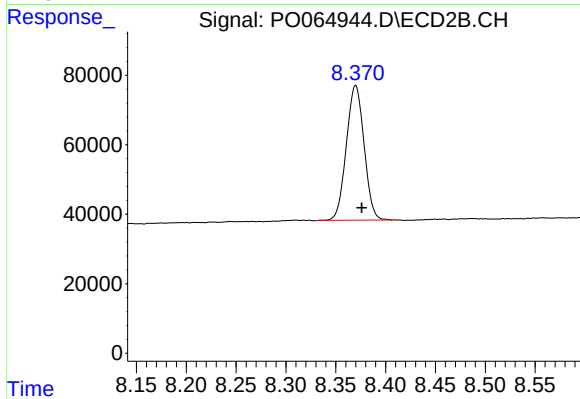

#2 Decachlorobiphenyl

R.T.: 8.370 min
Delta R.T.: -0.006 min
Response: 481471
Conc: 13.86 ng/ml