

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122419\
 Data File : P0064945.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Dec 2019 00:47
 Operator : SM/AJ
 Sample : K6396-09
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-4-(0-2)

Manual Integrations
 APPROVED

Ankita
 12/26/2019 1:41:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 04:23:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 13 08:19:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.182	3.458	679742	2041798	27.921m	80.547 #
2) SA Decachlor...	9.699	8.371	458765	569005	14.948	16.384

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122419\
Data File : P0064945.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Dec 2019 00:47
Operator : SM/AJ
Sample : K6396-09
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-4-(0-2)


Manual Integrations
APPROVED

Ankita
12/26/2019 1:41:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 04:23:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 13 08:19:24 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

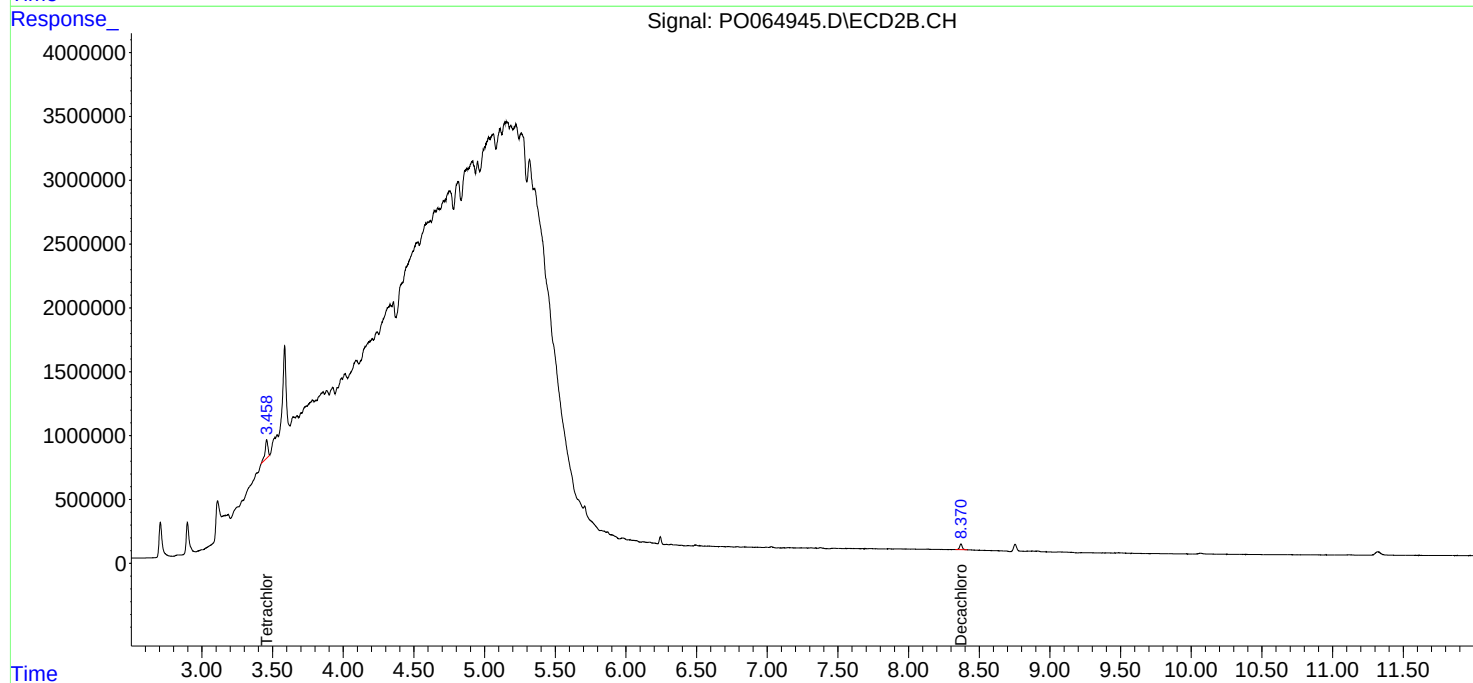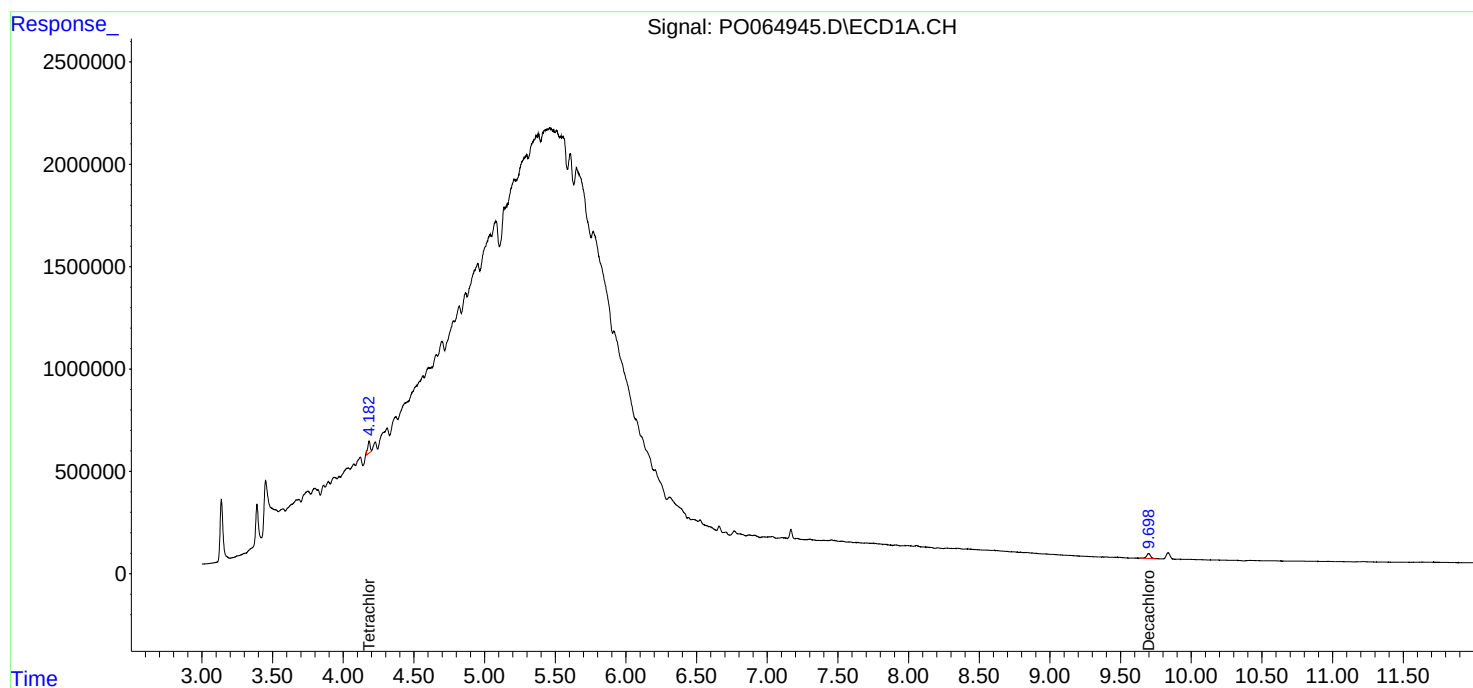

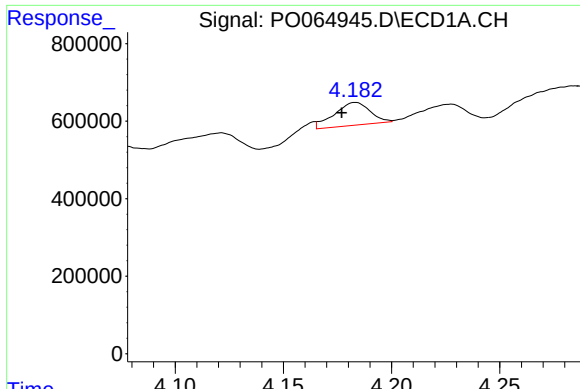


#1 Tetrachloro-m-xylene

R.T.: 4.182 min
Delta R.T.: 0.005 min
Response: 679742
Conc: 27.92 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB-4-(0-2)


Manual Integrations
APPROVED

Ankita
12/26/2019 1:41:34 PM

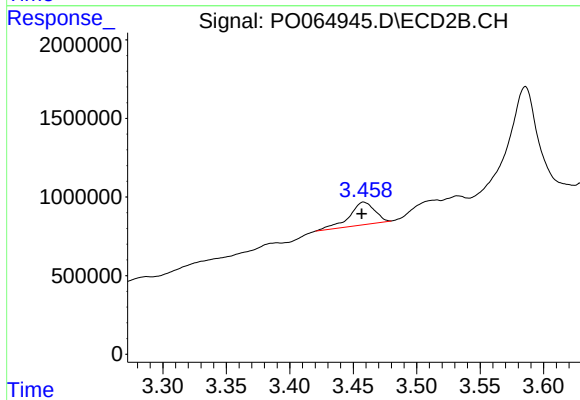


#1 Tetrachloro-m-xylene

R.T.: 3.458 min
Delta R.T.: 0.002 min
Response: 2041798
Conc: 80.55 ng/ml

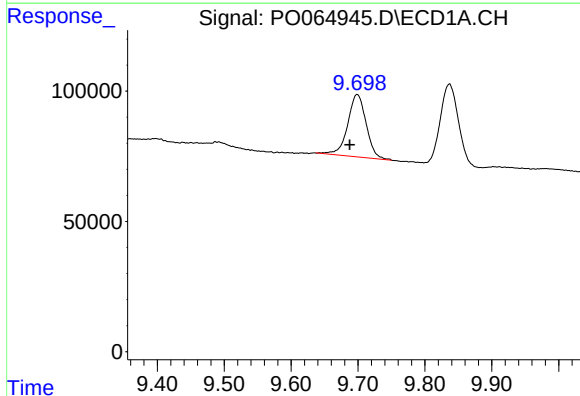

#2 Decachlorobiphenyl

R.T.: 9.699 min
Delta R.T.: 0.011 min
Response: 458765
Conc: 14.95 ng/ml

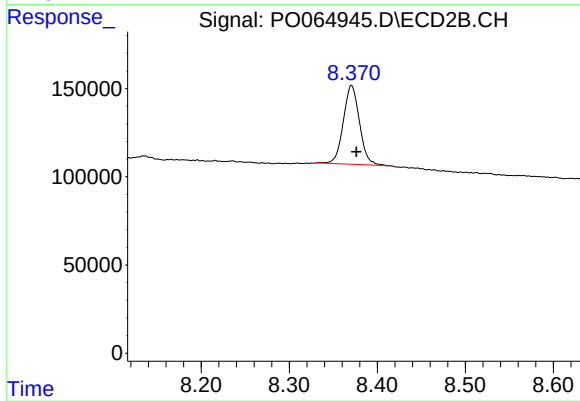

#2 Decachlorobiphenyl

R.T.: 8.371 min
Delta R.T.: -0.005 min
Response: 569005
Conc: 16.38 ng/ml