

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122618\
 Data File : PO052968.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Dec 2018 16:49
 Operator : SM/SJ
 Sample : J6498-02RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SSSI-1218-S-DH-9-TRE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 00:18:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Dec 24 02:43:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.247	3.267	14872216	2966744	10.807	10.025
2) SA Decachlor...	9.779	7.941	4827291	1841215	6.886	6.542

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122618\
Data File : PO052968.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Dec 2018 16:49
Operator : SM/SJ
Sample : J6498-02RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SSSI-1218-S-DH-9-TRE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 00:18:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Dec 24 02:43:03 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

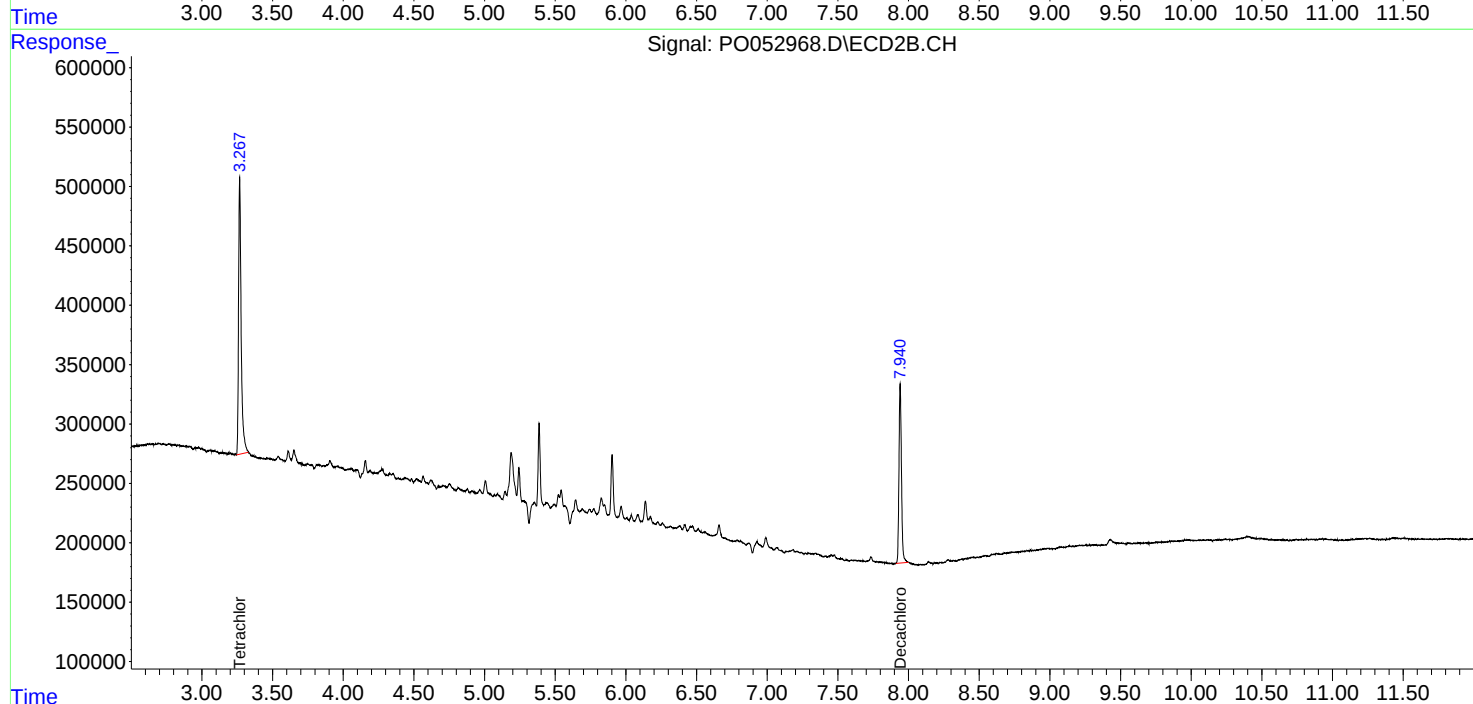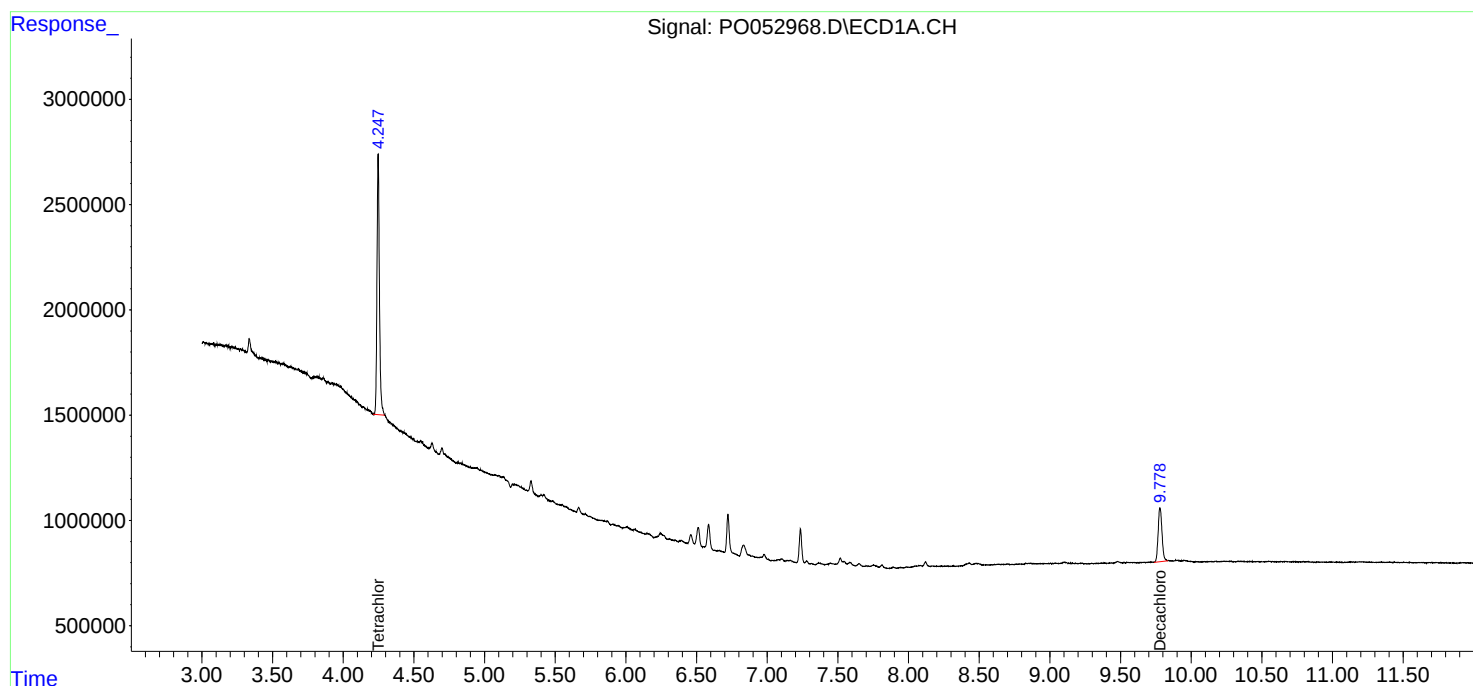


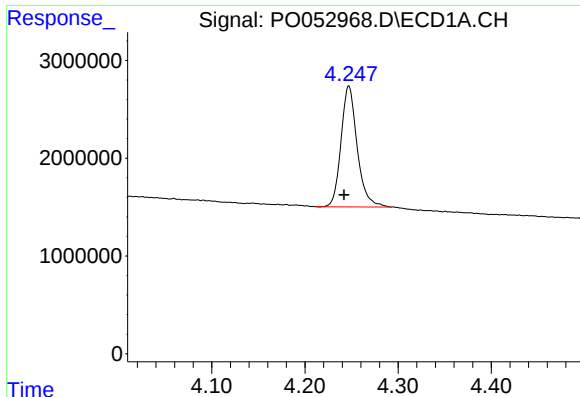

#1 Tetrachloro-m-xylene


R.T.: 4.247 min
Delta R.T.: 0.005 min
Response: 14872216
Conc: 10.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
SSSI-1218-S-DH-9-TRE

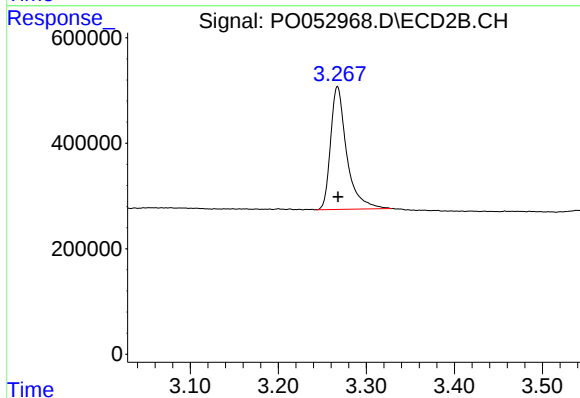


#1 Tetrachloro-m-xylene

R.T.: 3.267 min
Delta R.T.: 0.000 min
Response: 2966744
Conc: 10.02 ng/ml

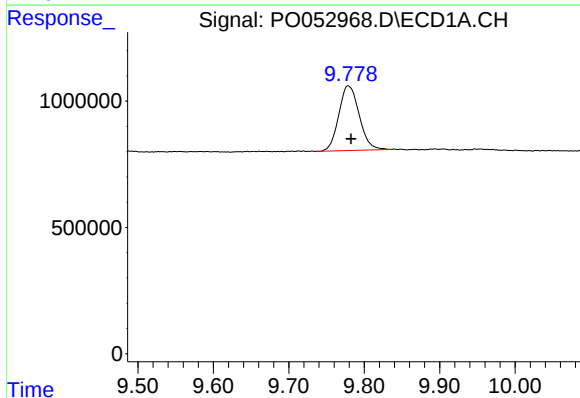

#2 Decachlorobiphenyl

R.T.: 9.779 min
Delta R.T.: -0.004 min
Response: 4827291
Conc: 6.89 ng/ml

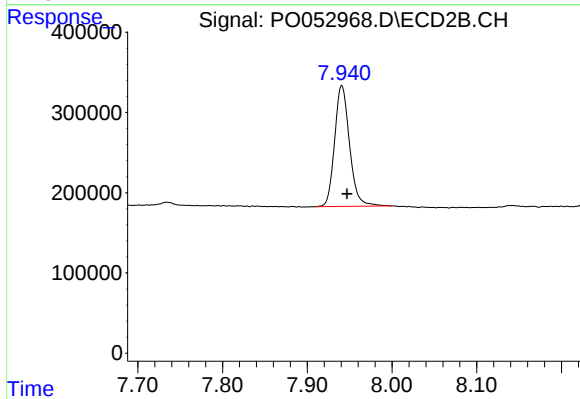

#2 Decachlorobiphenyl

R.T.: 7.941 min
Delta R.T.: -0.006 min
Response: 1841215
Conc: 6.54 ng/ml