

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122618\
 Data File : PO052970.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Dec 2018 17:23
 Operator : SM/SJ
 Sample : J6498-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SSSI-1218-S-AB-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 00:19:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Dec 24 02:43:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.236	3.266	11722848	2456441	8.519	8.300
2) SA Decachlor...	9.764	7.936	3750523	1514977	5.350	5.383

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122618\
Data File : PO052970.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Dec 2018 17:23
Operator : SM/SJ
Sample : J6498-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SSSI-1218-S-AB-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 00:19:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Dec 24 02:43:03 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

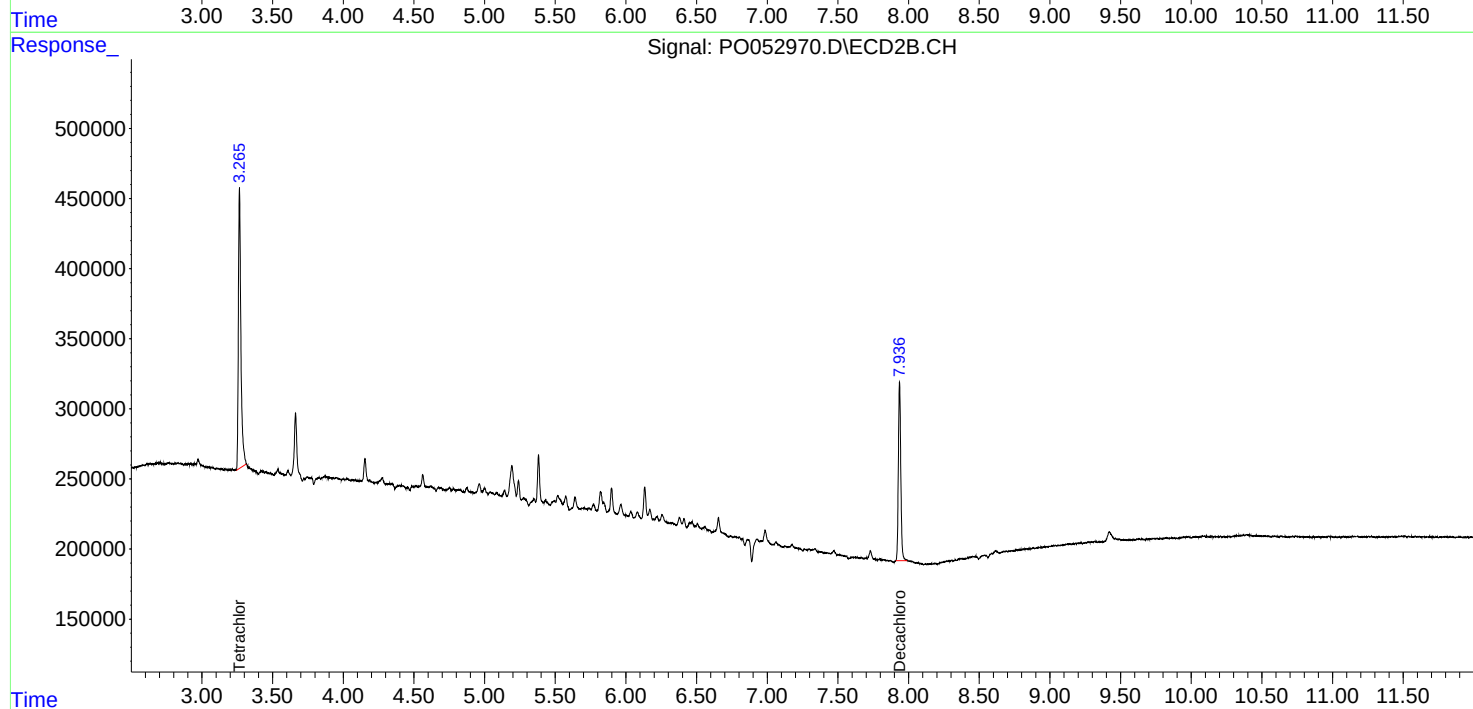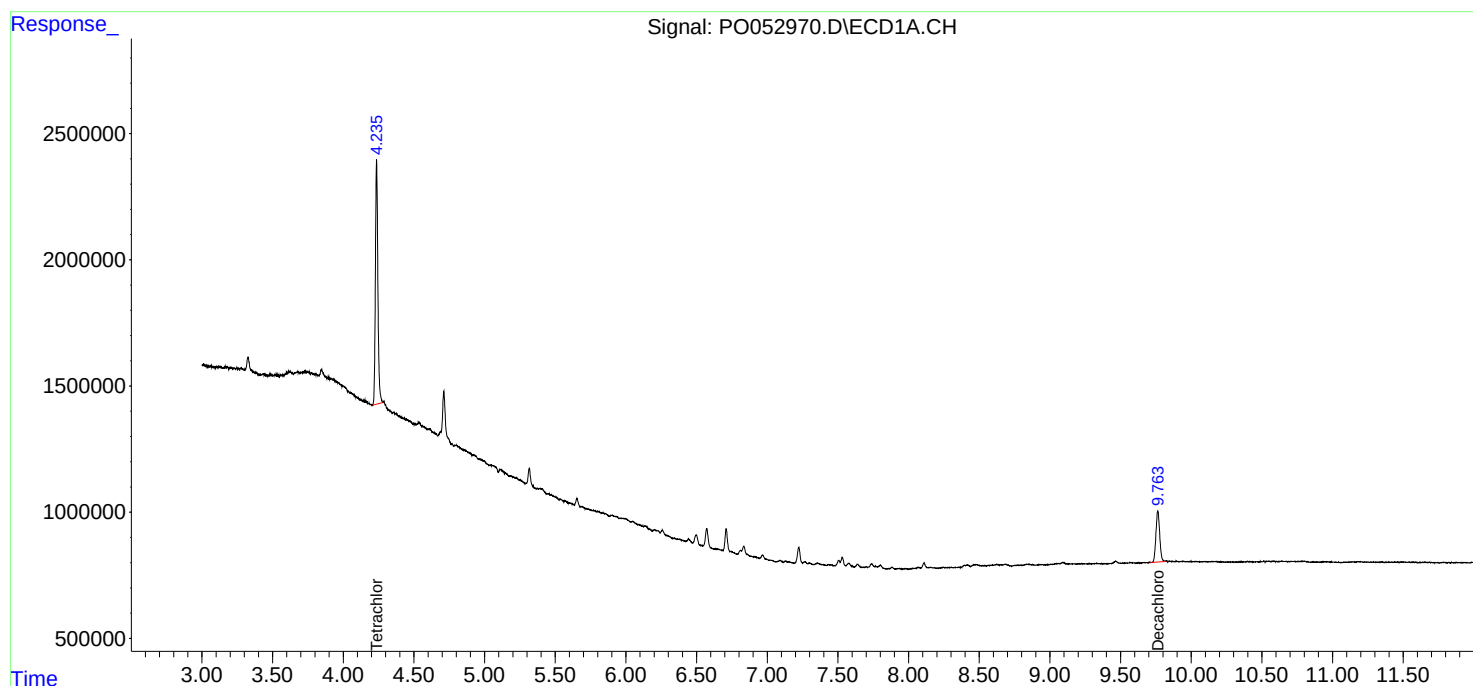


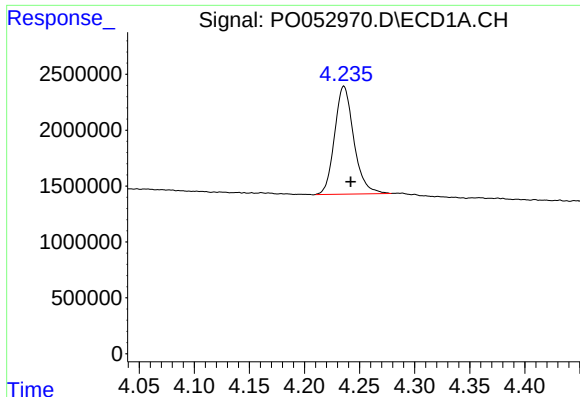

#1 Tetrachloro-m-xylene


R.T.: 4.236 min
Delta R.T.: -0.006 min
Response: 11722848
Conc: 8.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
SSSI-1218-S-AB-6

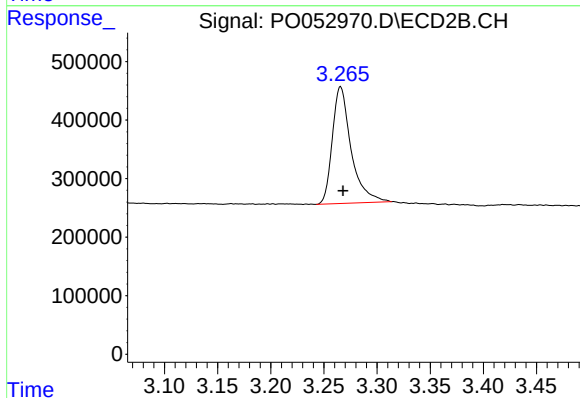


#1 Tetrachloro-m-xylene

R.T.: 3.266 min
Delta R.T.: -0.002 min
Response: 2456441
Conc: 8.30 ng/ml

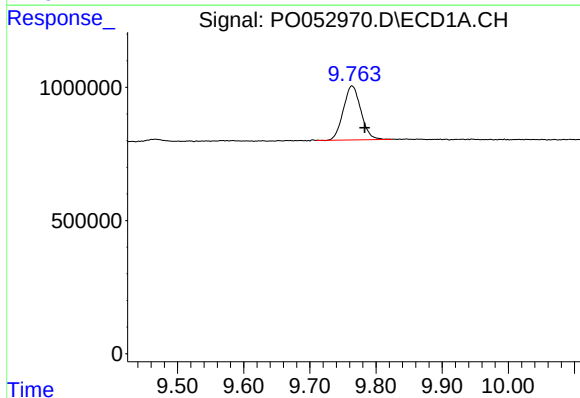

#2 Decachlorobiphenyl

R.T.: 9.764 min
Delta R.T.: -0.019 min
Response: 3750523
Conc: 5.35 ng/ml

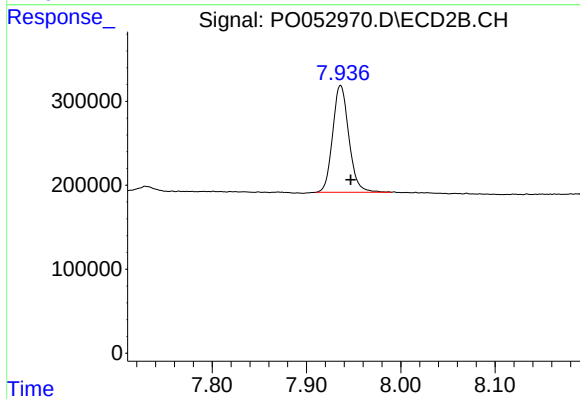

#2 Decachlorobiphenyl

R.T.: 7.936 min
Delta R.T.: -0.011 min
Response: 1514977
Conc: 5.38 ng/ml