

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122619\
 Data File : P0064963.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Dec 2019 13:18
 Operator : SM/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 26 13:33:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122619.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 26 13:32:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.178	3.451	448625	559626	19.100	19.868
2)	SA Decachlor...	9.692	8.365	580354	749821	22.860	22.888
Target Compounds							
28)	L6 AR-1254-3	6.758	0.000	156428	0	69.966	N.D. #
30)	L6 AR-1254-5	7.448	0.000	6506	0	3.329	N.D. #
35)	L7 AR-1260-5	8.056	0.000	20749	0	6.421	N.D. #
37)	L8 AR-1262-2	8.056	0.000	20749	0	5.390	N.D. #
40)	L8 AR-1262-5	9.029	0.000	16559	0	12.408	N.D. #
43)	L9 AR-1268-3	8.626	0.000	42927	0	13.183	N.D. #
44)	L9 AR-1268-4	9.029	0.000	16559	0	12.346	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122619\
Data File : P0064963.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Dec 2019 13:18
Operator : SM/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 26 13:33:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122619.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 26 13:32:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

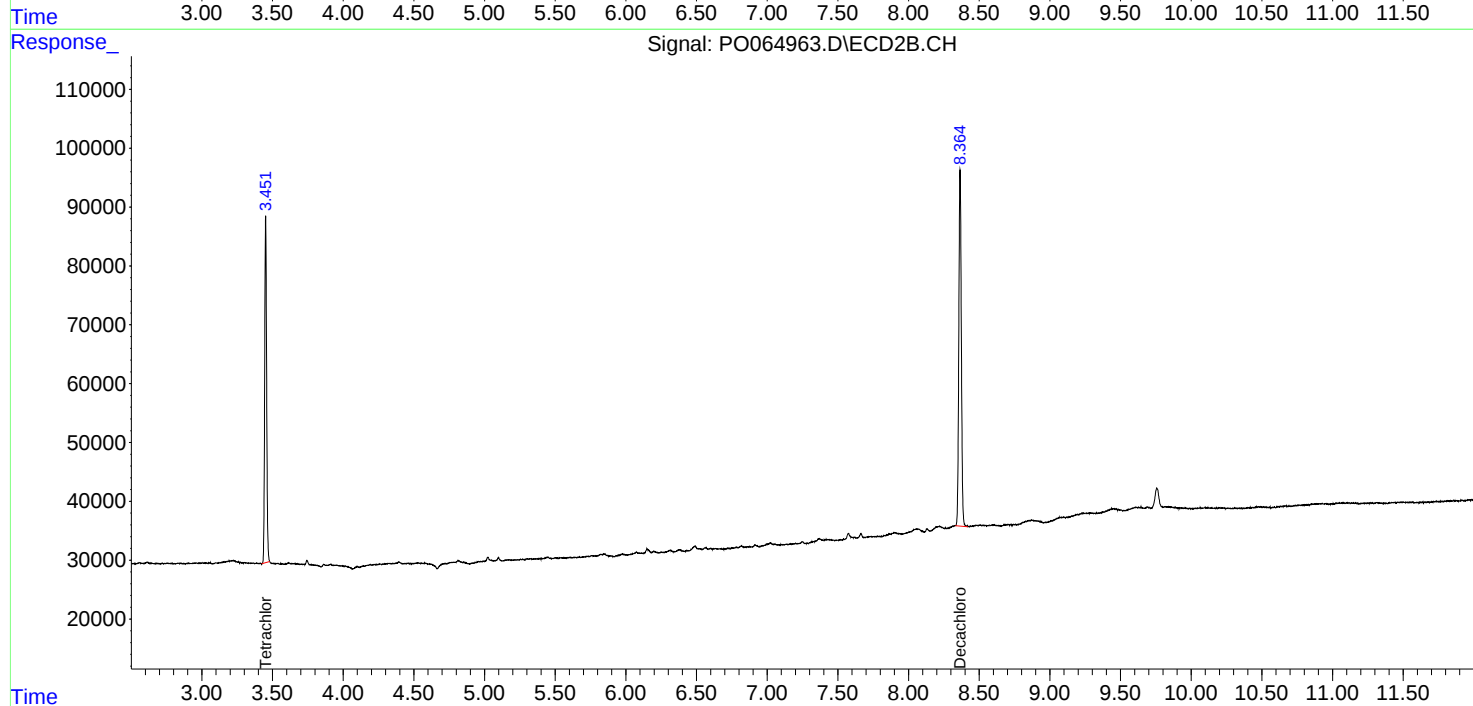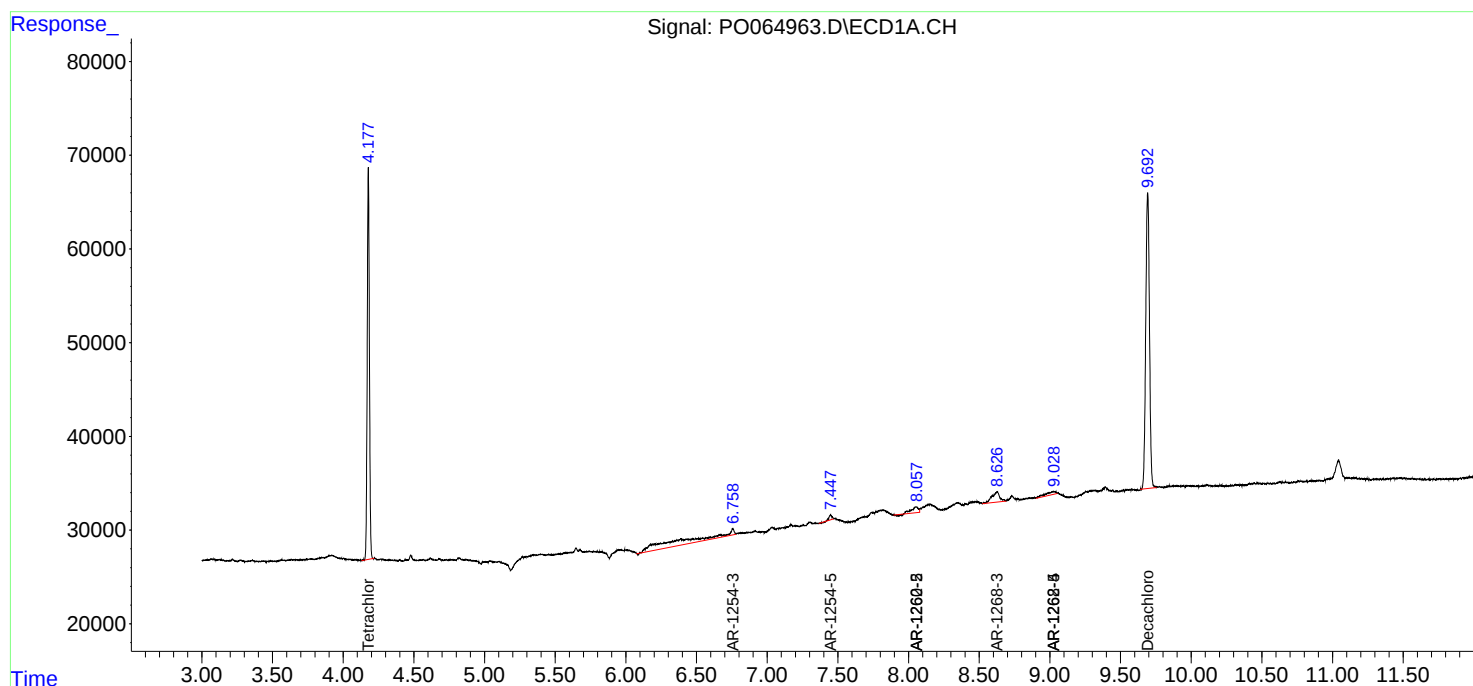


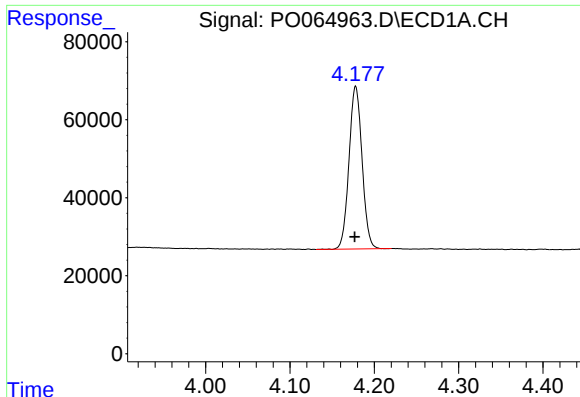

#1 Tetrachloro-m-xylene


R.T.: 4.178 min
Delta R.T.: 0.000 min
Response: 448625
Conc: 19.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

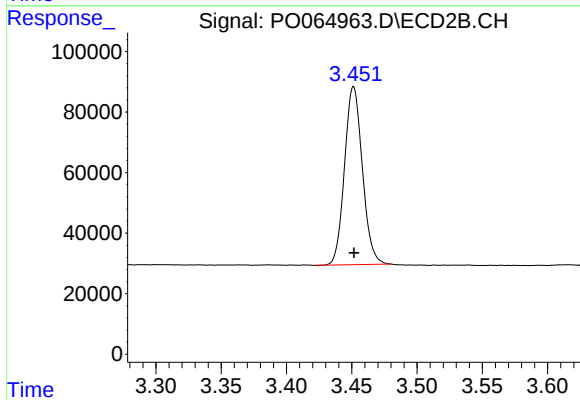


#1 Tetrachloro-m-xylene

R.T.: 3.451 min
Delta R.T.: 0.000 min
Response: 559626
Conc: 19.87 ng/ml

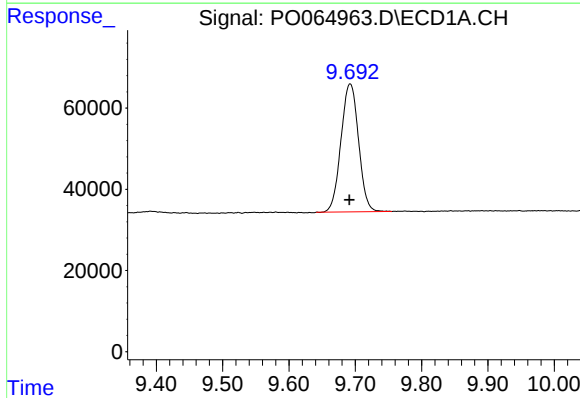


#2 Decachlorobiphenyl

R.T.: 9.692 min
Delta R.T.: 0.000 min
Response: 580354
Conc: 22.86 ng/ml

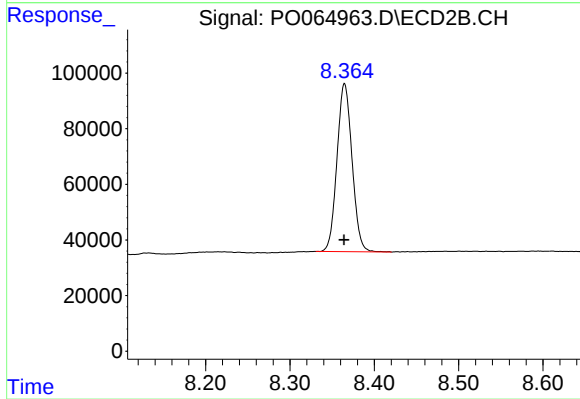

#2 Decachlorobiphenyl


R.T.: 8.365 min
Delta R.T.: 0.000 min
Response: 749821
Conc: 22.89 ng/ml

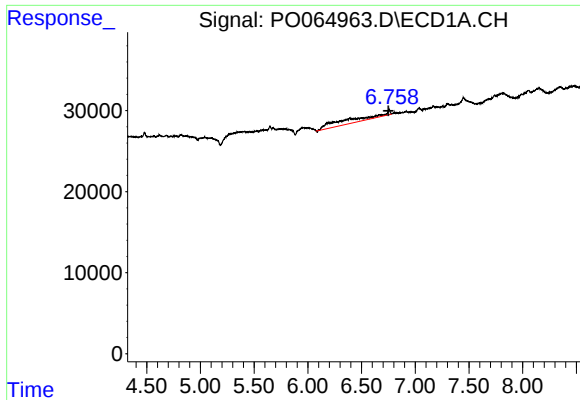

#28 AR-1254-3


R.T.: 6.758 min
Delta R.T.: 0.008 min
Response: 156428
Conc: 69.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

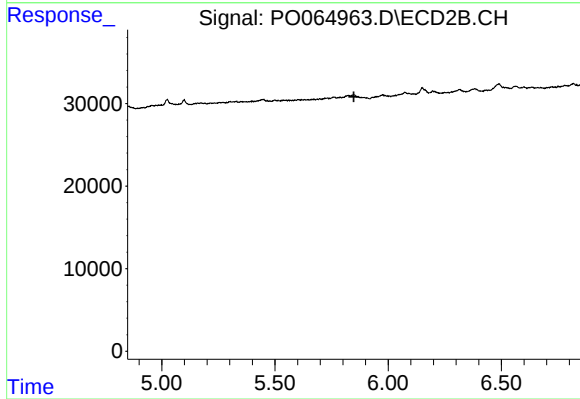


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 5.848 min
Response: 0
Conc: N.D.

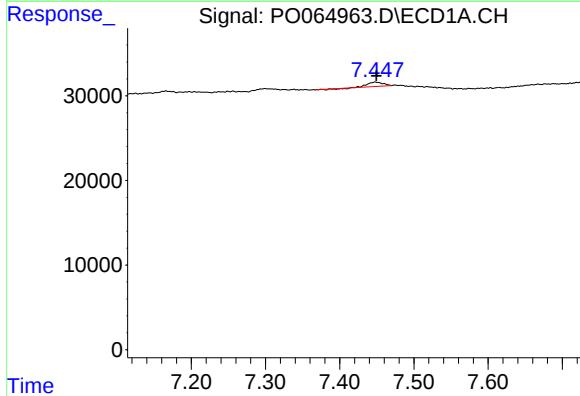


#30 AR-1254-5

R.T.: 7.448 min
Delta R.T.: -0.002 min
Response: 6506
Conc: 3.33 ng/ml

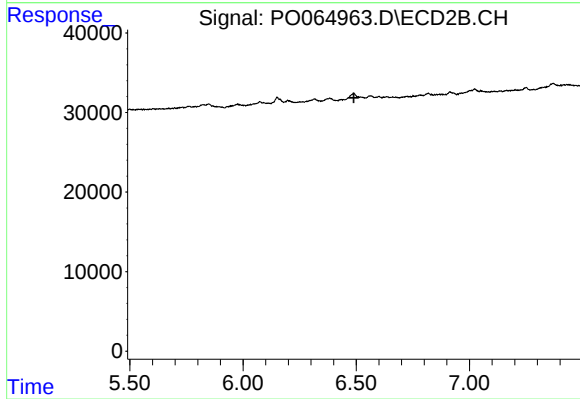

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 6.489 min
Response: 0
Conc: N.D.

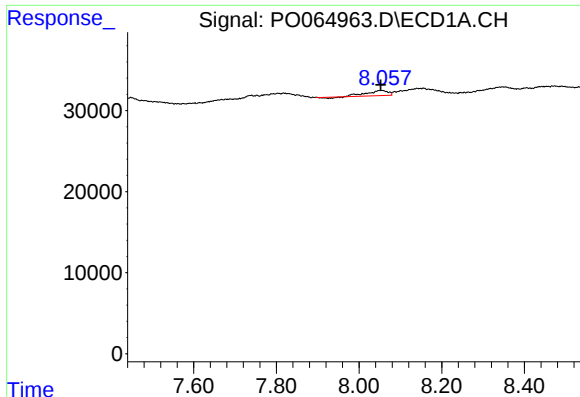

#35 AR-1260-5


R.T.: 8.056 min
Delta R.T.: 0.003 min
Response: 20749
Conc: 6.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

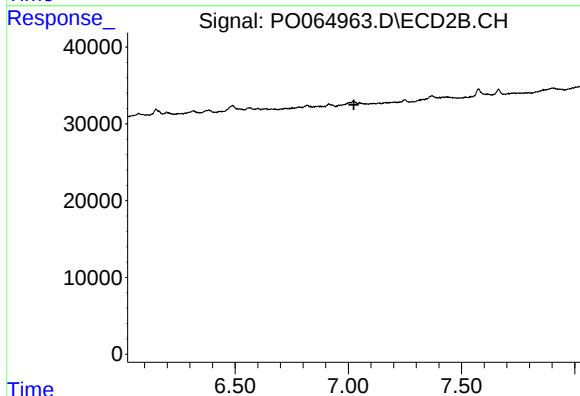


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.024 min
Response: 0
Conc: N.D.

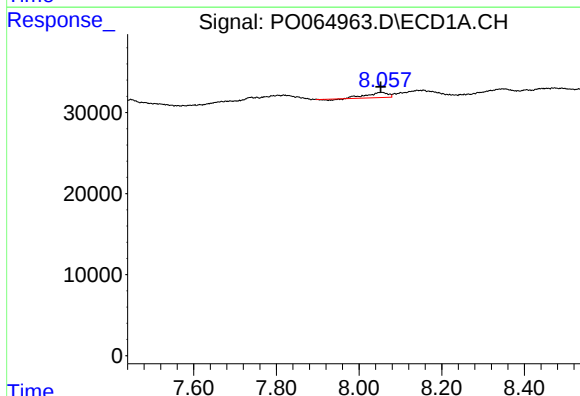


#37 AR-1262-2

R.T.: 8.056 min
Delta R.T.: 0.003 min
Response: 20749
Conc: 5.39 ng/ml

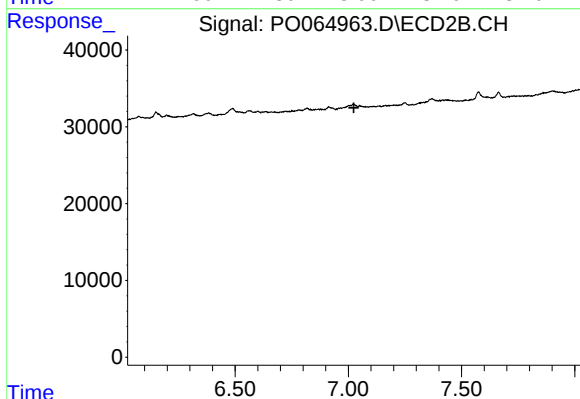

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.025 min
Response: 0
Conc: N.D.

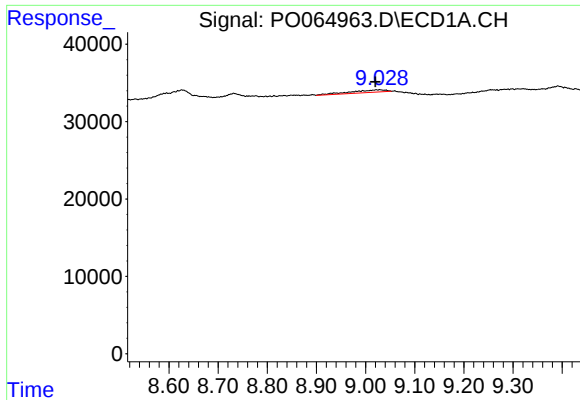

#40 AR-1262-5


R.T.: 9.029 min
Delta R.T.: 0.009 min
Response: 16559
Conc: 12.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

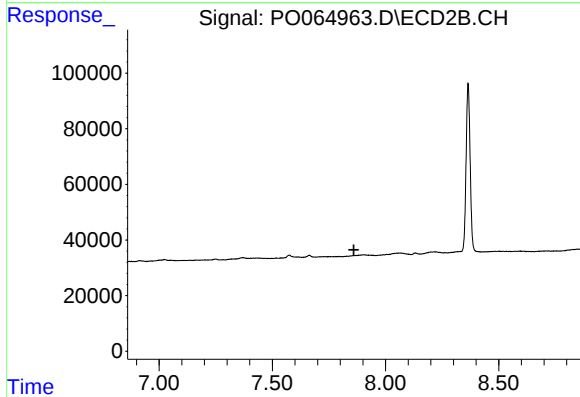


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 7.861 min
Response: 0
Conc: N.D.

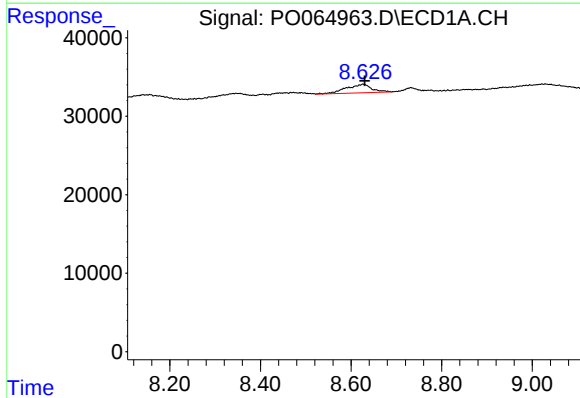


#43 AR-1268-3

R.T.: 8.626 min
Delta R.T.: -0.004 min
Response: 42927
Conc: 13.18 ng/ml

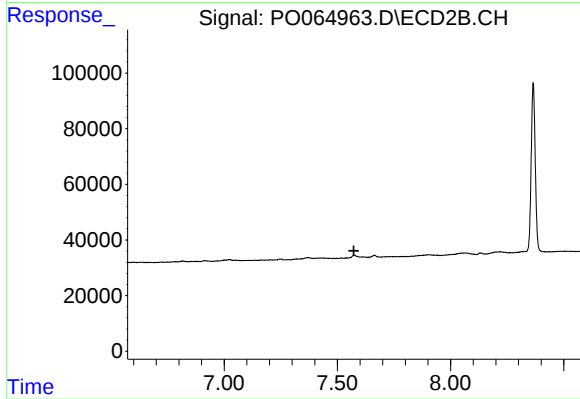

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 7.573 min
Response: 0
Conc: N.D.

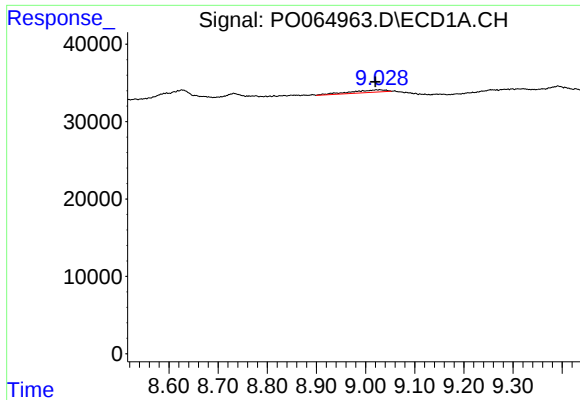

#44 AR-1268-4

R.T.: 9.029 min
Delta R.T.: 0.008 min
Response: 16559
Conc: 12.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

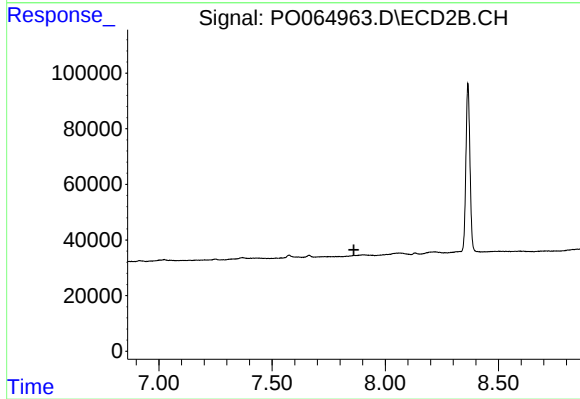

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 7.861 min
Response: 0
Conc: N.D.