

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0122619\
 Data File : P0064968.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Dec 2019 14:41
 Operator : SM/AJ
 Sample : K6376-08 2X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-121719-08

Manual Integrations
 APPROVED

Ankita
 12/27/2019 9:32:57 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 26 15:37:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0122619.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 26 13:32:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.179	3.455	358401	460916	15.259	16.364
2) SA Decachlor...	9.693	8.366	257987	303208	10.162m	9.255
Target Compounds						
26) L6 AR-1254-1	6.173	5.304	1108560	1657486	870.406	732.239m
27) L6 AR-1254-2	6.390	5.451	993389	912301	496.408	452.621
28) L6 AR-1254-3	6.752	5.849	860436	1234470	384.849	365.369
29) L6 AR-1254-4	7.035	6.077	356109	349991	211.271	162.054
30) L6 AR-1254-5	7.451	6.490	344349	439048	176.222	145.886

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122619\
Data File : P0064968.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Dec 2019 14:41
Operator : SM/AJ
Sample : K6376-08 2X
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PCB-121719-08


Manual Integrations
APPROVED

Ankita
12/27/2019 9:32:57 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 26 15:37:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122619.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 26 13:32:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

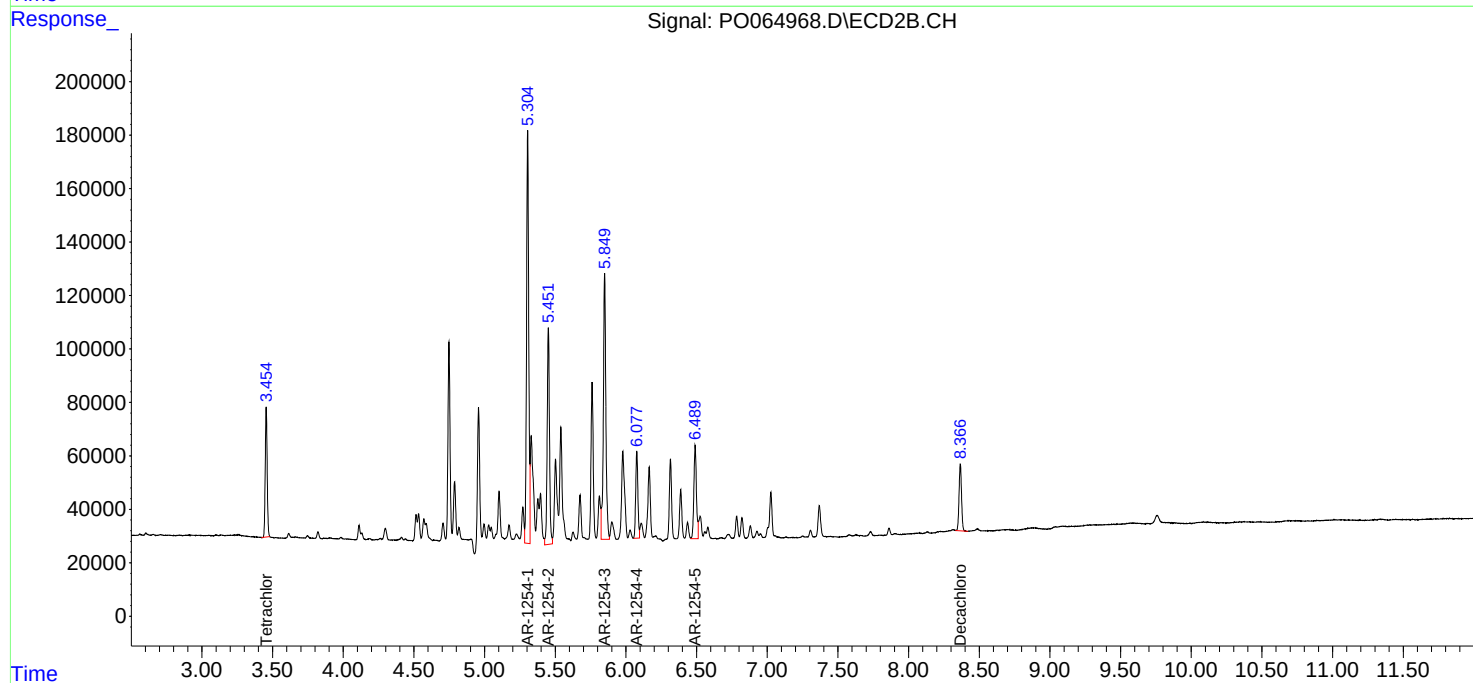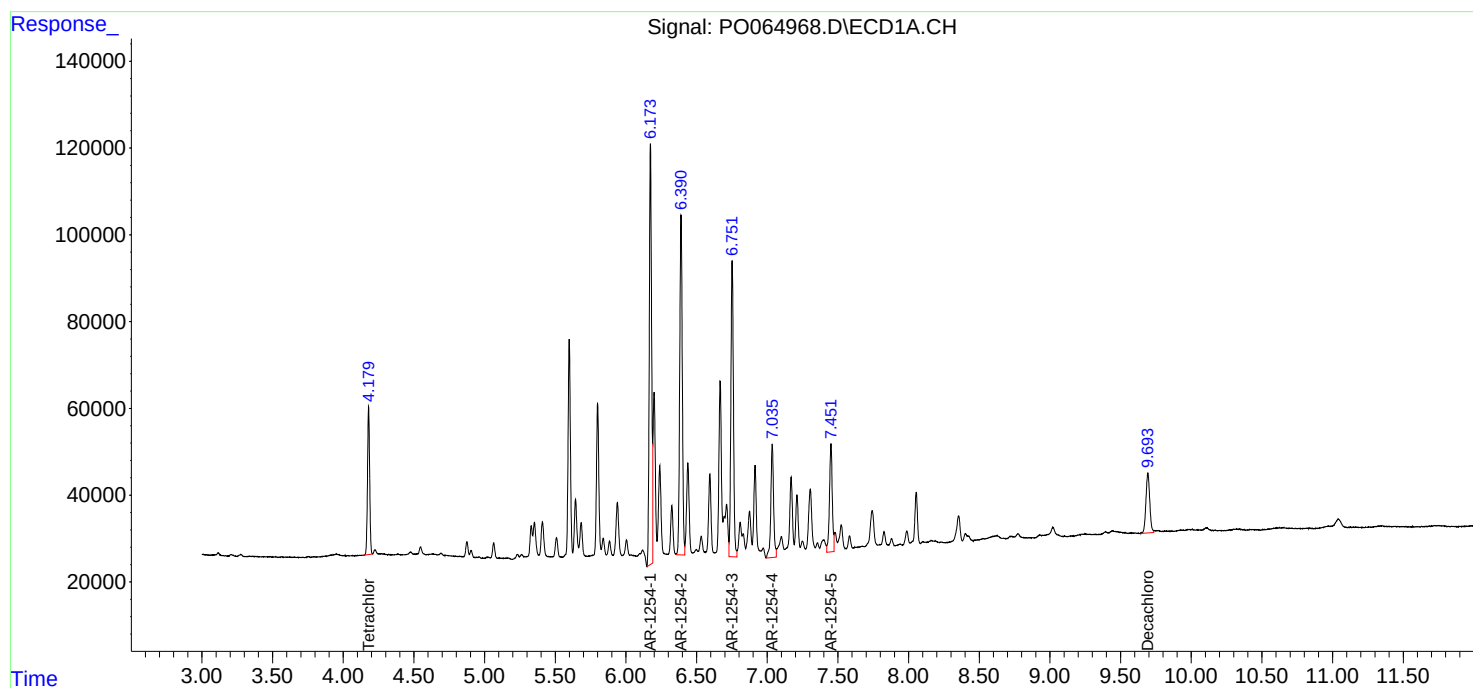

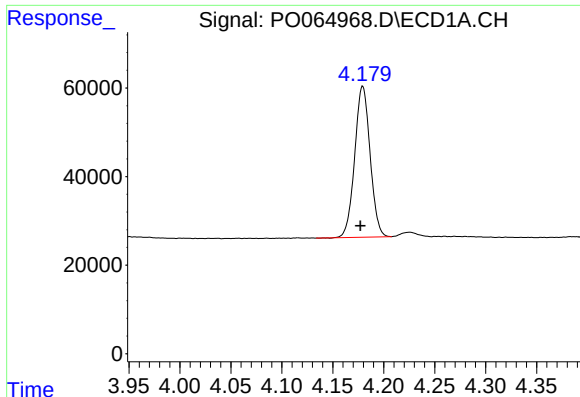


#1 Tetrachloro-m-xylene

R.T.: 4.179 min
Delta R.T.: 0.002 min
Response: 358401
Conc: 15.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-121719-08


Manual Integrations
APPROVED

Ankita
12/27/2019 9:32:57 AM

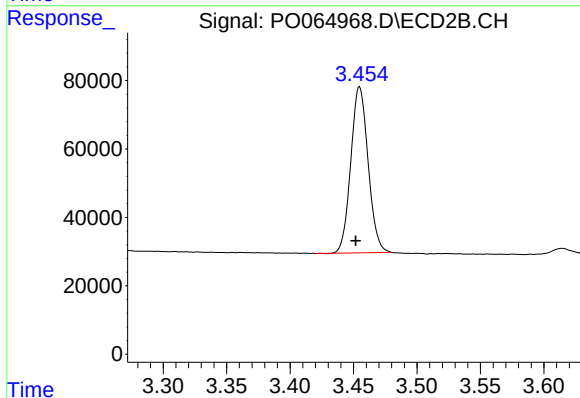


#1 Tetrachloro-m-xylene

R.T.: 3.455 min
Delta R.T.: 0.003 min
Response: 460916
Conc: 16.36 ng/ml

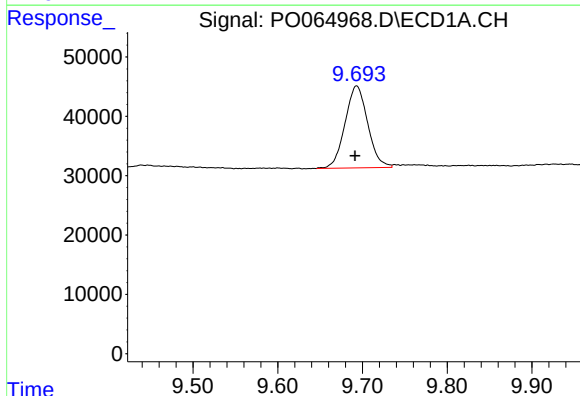


#2 Decachlorobiphenyl

R.T.: 9.693 min
Delta R.T.: 0.001 min
Response: 257987
Conc: 10.16 ng/ml m

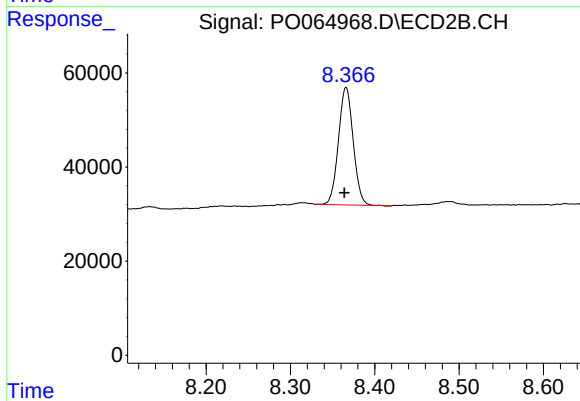

#2 Decachlorobiphenyl

R.T.: 8.366 min
Delta R.T.: 0.002 min
Response: 303208
Conc: 9.26 ng/ml

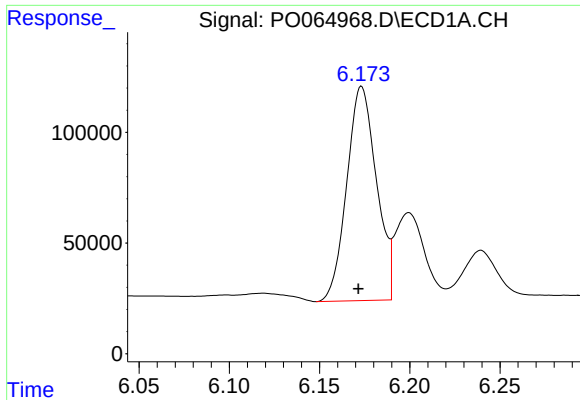


#26 AR-1254-1

R.T.: 6.173 min
Delta R.T.: 0.002 min
Response: 1108560
Conc: 870.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-121719-08


Manual Integrations
APPROVED

Ankita
12/27/2019 9:32:57 AM

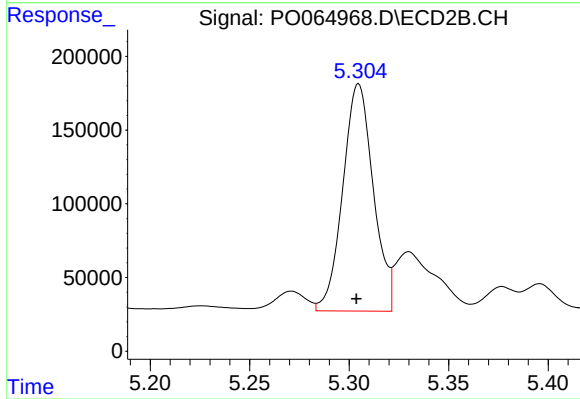


#26 AR-1254-1

R.T.: 5.304 min
Delta R.T.: 0.000 min
Response: 1657486
Conc: 732.24 ng/ml m

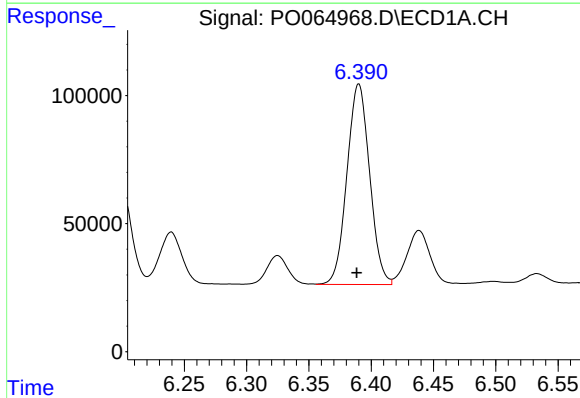


#27 AR-1254-2

R.T.: 6.390 min
Delta R.T.: 0.002 min
Response: 993389
Conc: 496.41 ng/ml

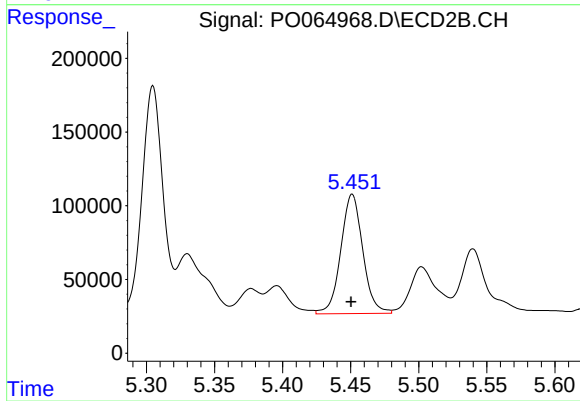

#27 AR-1254-2

R.T.: 5.451 min
Delta R.T.: 0.000 min
Response: 912301
Conc: 452.62 ng/ml

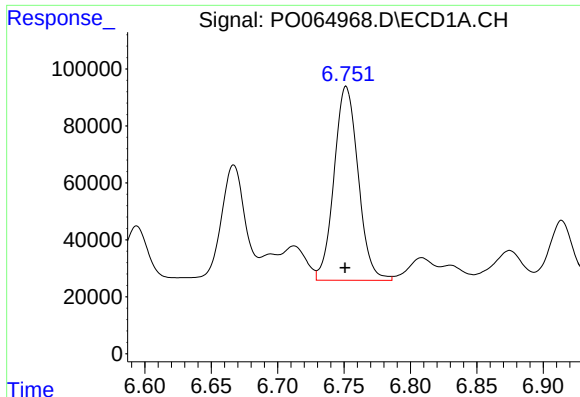


#28 AR-1254-3

R.T.: 6.752 min
Delta R.T.: 0.000 min
Response: 860436
Conc: 384.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-121719-08


Manual Integrations
APPROVED

Ankita
12/27/2019 9:32:57 AM

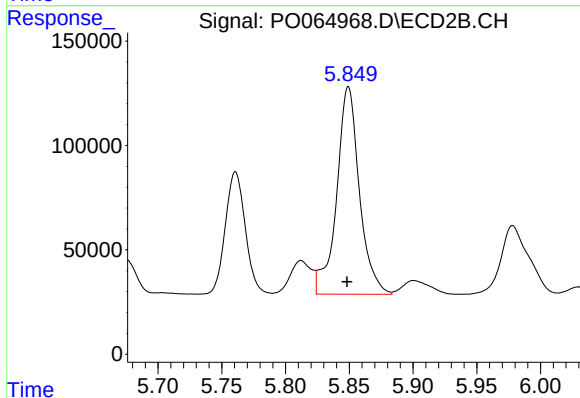


#28 AR-1254-3

R.T.: 5.849 min
Delta R.T.: 0.000 min
Response: 1234470
Conc: 365.37 ng/ml

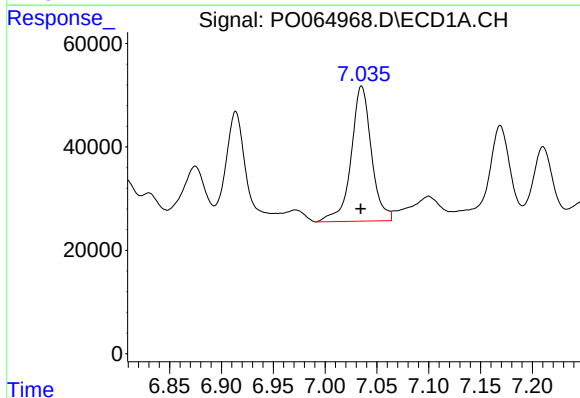


#29 AR-1254-4

R.T.: 7.035 min
Delta R.T.: 0.000 min
Response: 356109
Conc: 211.27 ng/ml

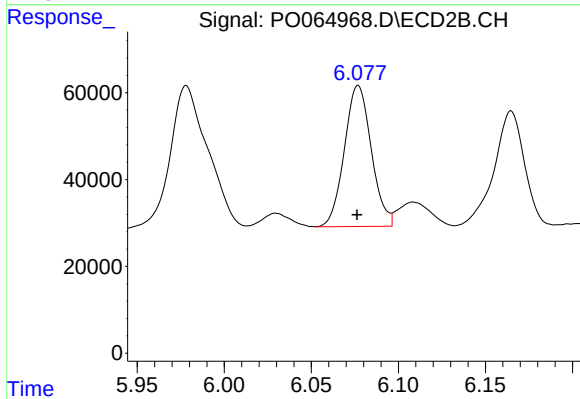

#29 AR-1254-4

R.T.: 6.077 min
Delta R.T.: 0.000 min
Response: 349991
Conc: 162.05 ng/ml

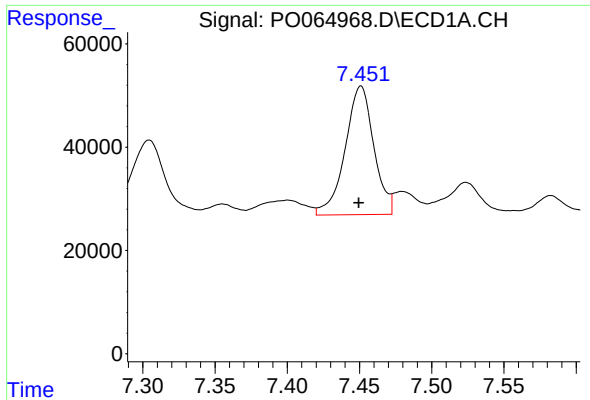


#30 AR-1254-5

R.T.: 7.451 min
Delta R.T.: 0.002 min
Response: 344349
Conc: 176.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-121719-08

Manual Integrations
APPROVED

Ankita
12/27/2019 9:32:57 AM

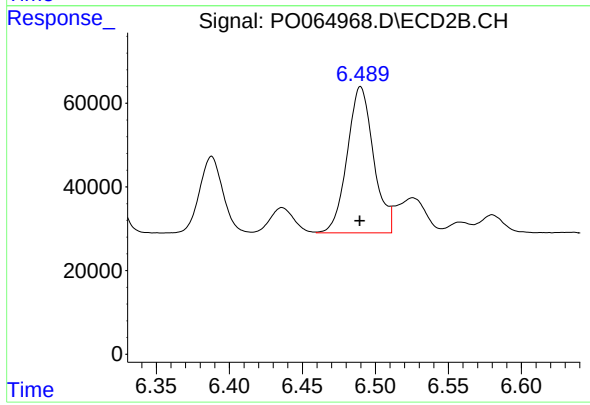

#30 AR-1254-5

R.T.: 6.490 min
Delta R.T.: 0.000 min
Response: 439048
Conc: 145.89 ng/ml