

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0122619\
 Data File : P0064990.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Dec 2019 3:28
 Operator : SM/AJ
 Sample : K6417-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 TP-2

Manual Integrations
 APPROVED

Ankita
 12/27/2019 9:33:00 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 27 06:59:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0122619.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 26 13:32:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.171	3.446	563981	737047	24.012	26.167
2)	SA Decachlor...	9.681	8.357	682264	883635	26.874	26.972
Target Compounds							
26)	L6 AR-1254-1	6.164	5.298	32833	63051	25.780m	27.854
27)	L6 AR-1254-2	6.382	5.443	95890	63818	47.917	31.662 #
28)	L6 AR-1254-3	6.744	5.841	97531	167725	43.623m	49.642m
29)	L6 AR-1254-4	7.027	6.068	89957	100041	53.369m	46.322m
30)	L6 AR-1254-5	7.443	6.482	149686	244393	76.602m	81.206m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122619\
Data File : P0064990.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Dec 2019 3:28
Operator : SM/AJ
Sample : K6417-02
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-2


Manual Integrations
APPROVED

Ankita
12/27/2019 9:33:00 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 27 06:59:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122619.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 26 13:32:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

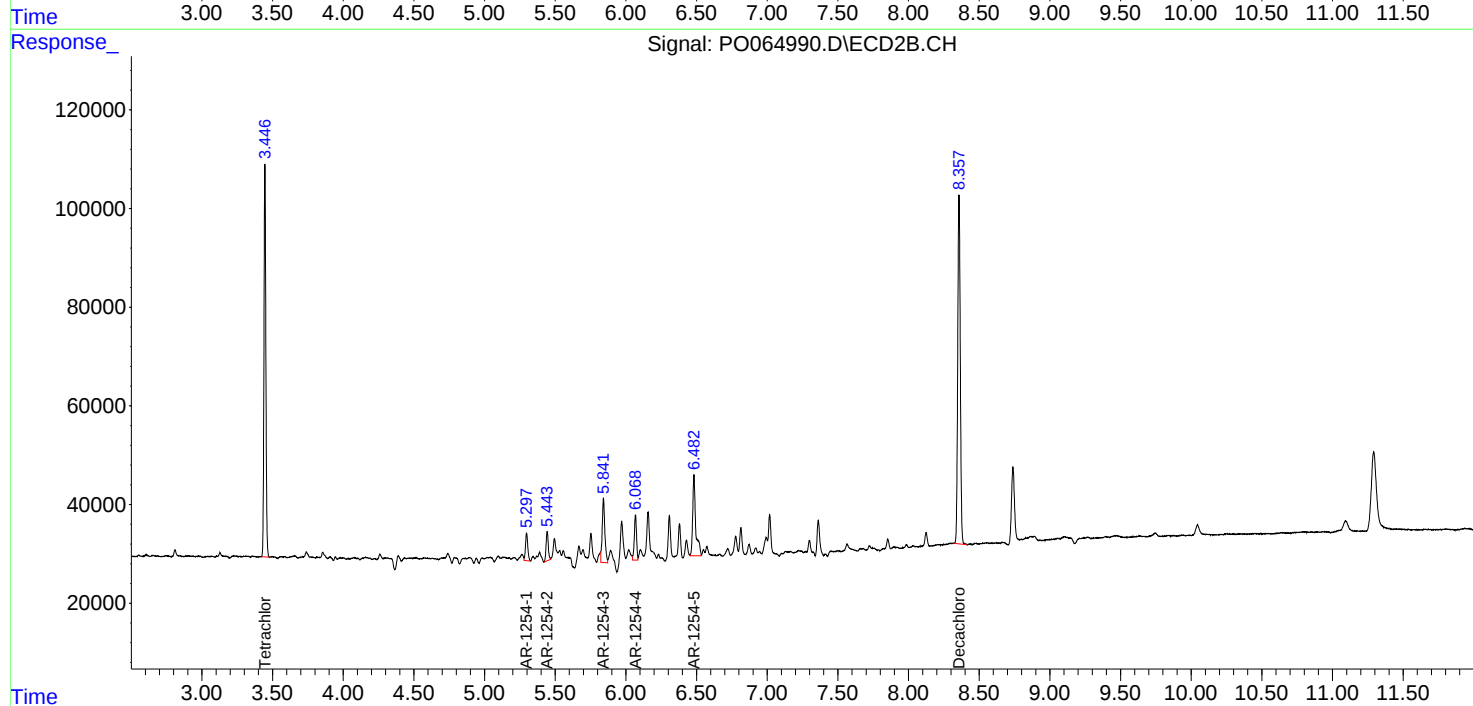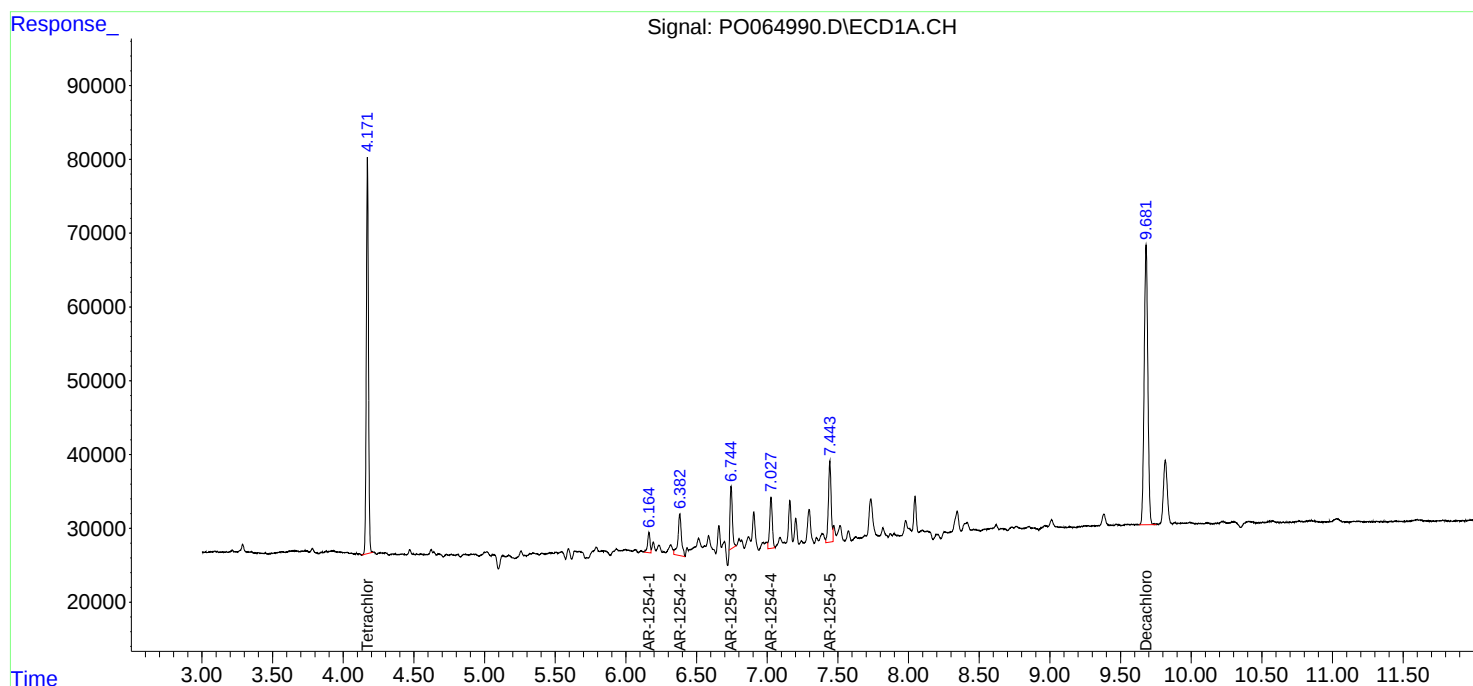

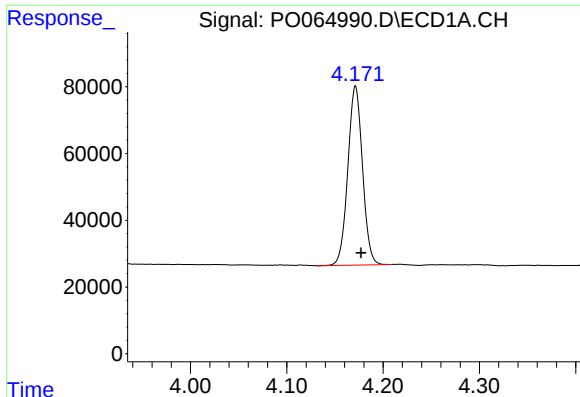


#1 Tetrachloro-m-xylene

R.T.: 4.171 min
Delta R.T.: -0.006 min
Response: 563981
Conc: 24.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
12/27/2019 9:33:00 AM

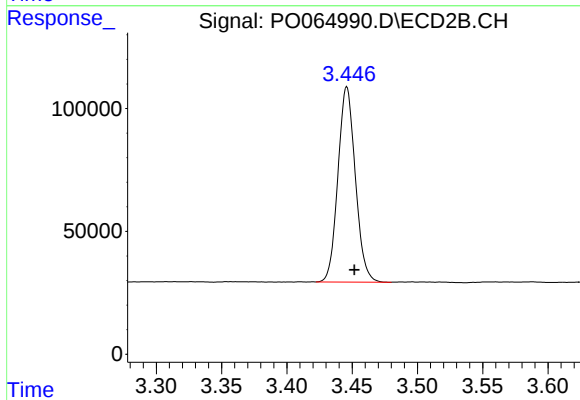


#1 Tetrachloro-m-xylene

R.T.: 3.446 min
Delta R.T.: -0.006 min
Response: 737047
Conc: 26.17 ng/ml

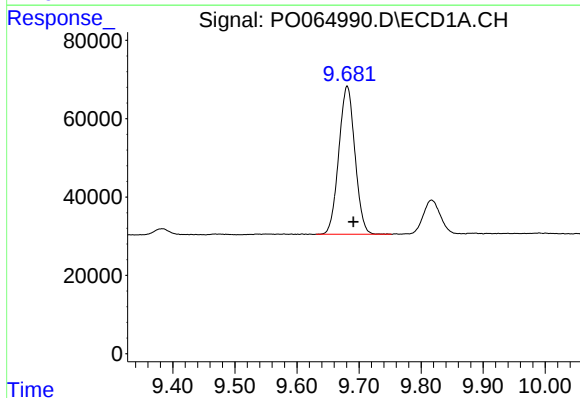


#2 Decachlorobiphenyl

R.T.: 9.681 min
Delta R.T.: -0.010 min
Response: 682264
Conc: 26.87 ng/ml

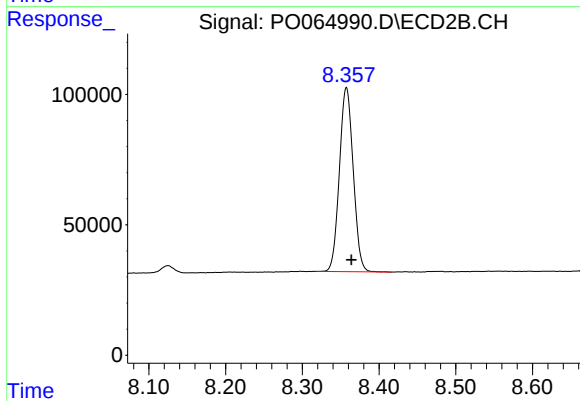

#2 Decachlorobiphenyl

R.T.: 8.357 min
Delta R.T.: -0.007 min
Response: 883635
Conc: 26.97 ng/ml

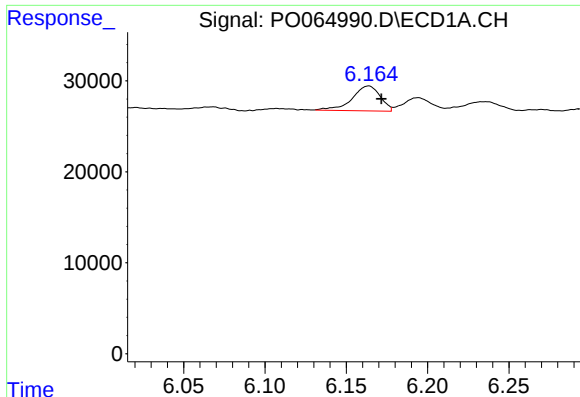


#26 AR-1254-1

R.T.: 6.164 min
Delta R.T.: -0.008 min
Response: 32833
Conc: 25.78 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
12/27/2019 9:33:00 AM

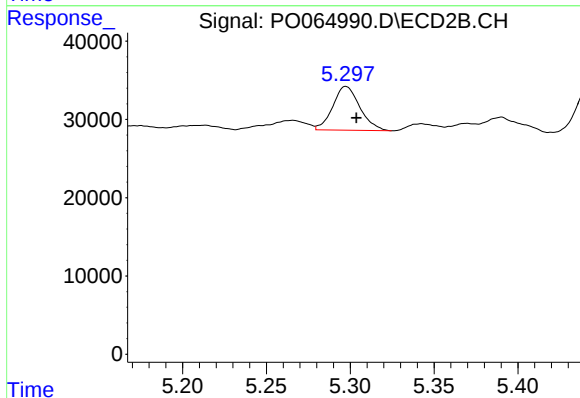


#26 AR-1254-1

R.T.: 5.298 min
Delta R.T.: -0.006 min
Response: 63051
Conc: 27.85 ng/ml

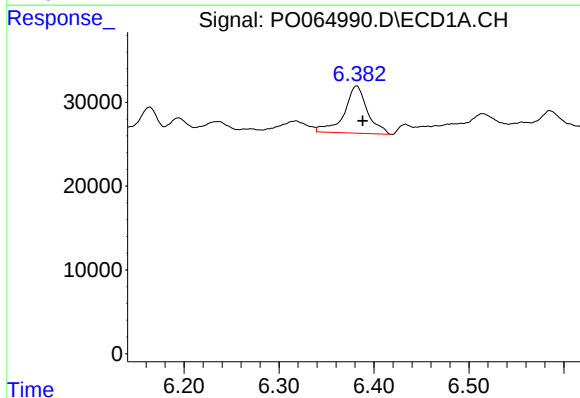


#27 AR-1254-2

R.T.: 6.382 min
Delta R.T.: -0.007 min
Response: 95890
Conc: 47.92 ng/ml

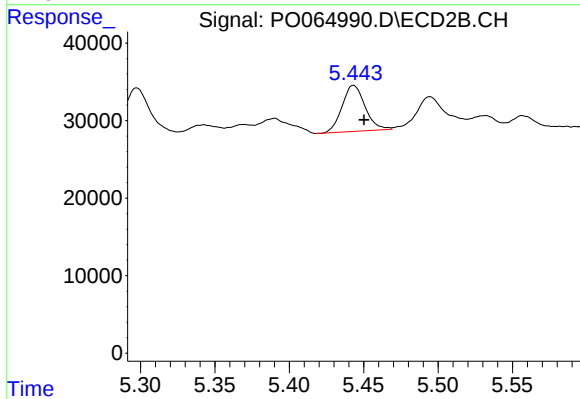

#27 AR-1254-2

R.T.: 5.443 min
Delta R.T.: -0.007 min
Response: 63818
Conc: 31.66 ng/ml

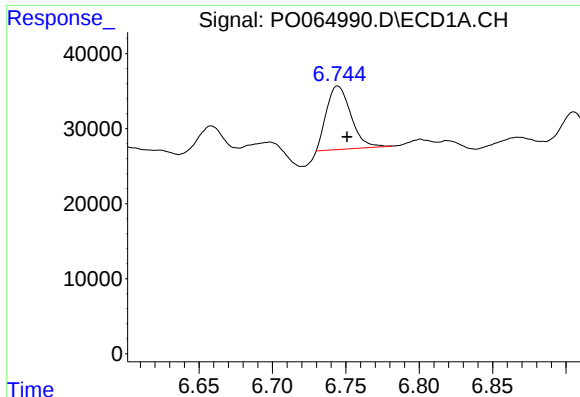


#28 AR-1254-3

R.T.: 6.744 min
Delta R.T.: -0.007 min
Response: 97531
Conc: 43.62 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
12/27/2019 9:33:00 AM

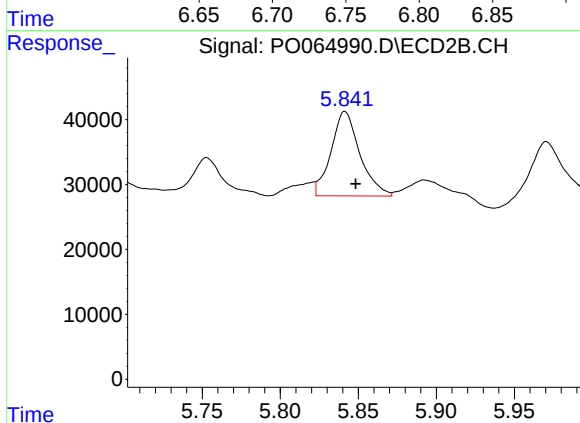


#28 AR-1254-3

R.T.: 5.841 min
Delta R.T.: -0.007 min
Response: 167725
Conc: 49.64 ng/ml m

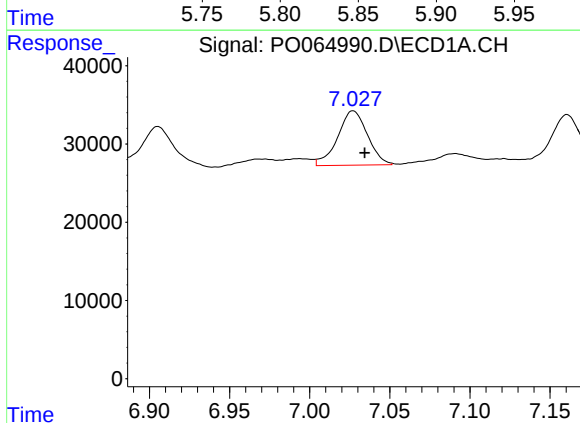


#29 AR-1254-4

R.T.: 7.027 min
Delta R.T.: -0.008 min
Response: 89957
Conc: 53.37 ng/ml m

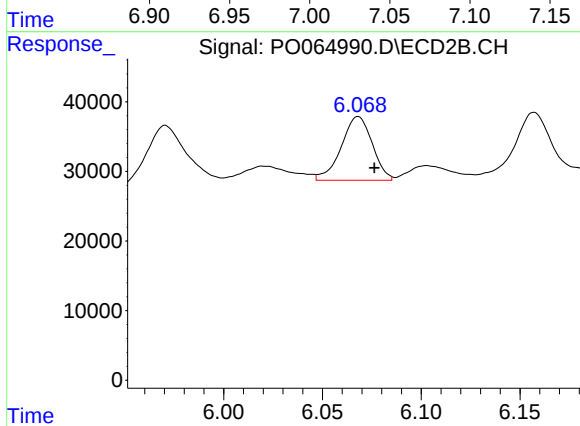

#29 AR-1254-4

R.T.: 6.068 min
Delta R.T.: -0.009 min
Response: 100041
Conc: 46.32 ng/ml m

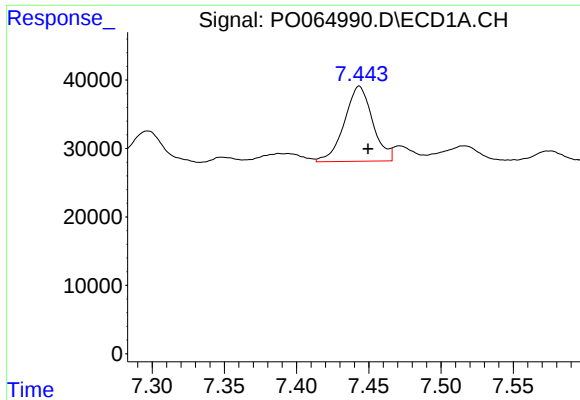


#30 AR-1254-5

R.T.: 7.443 min
Delta R.T.: -0.006 min
Response: 149686
Conc: 76.60 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-2

Manual Integrations
APPROVED

Ankita
12/27/2019 9:33:00 AM

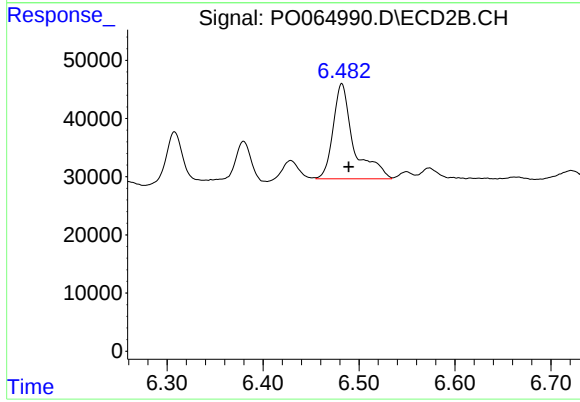

#30 AR-1254-5

R.T.: 6.482 min
Delta R.T.: -0.008 min
Response: 244393
Conc: 81.21 ng/ml m