

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122818\
 Data File : PO053030.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Dec 2018 10:18
 Operator : SM/SJ
 Sample : J6505-15
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-64(0-23)-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 10:54:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 28 04:30:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.185	3.215	17051630	3480844	17.576	17.927
2) SA Decachlor...	9.663	7.865	6696069	2610593	10.856	12.105

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122818\
Data File : P0053030.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Dec 2018 10:18
Operator : SM/SJ
Sample : J6505-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB-64(0-23)-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 10:54:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122818.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 28 04:30:51 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

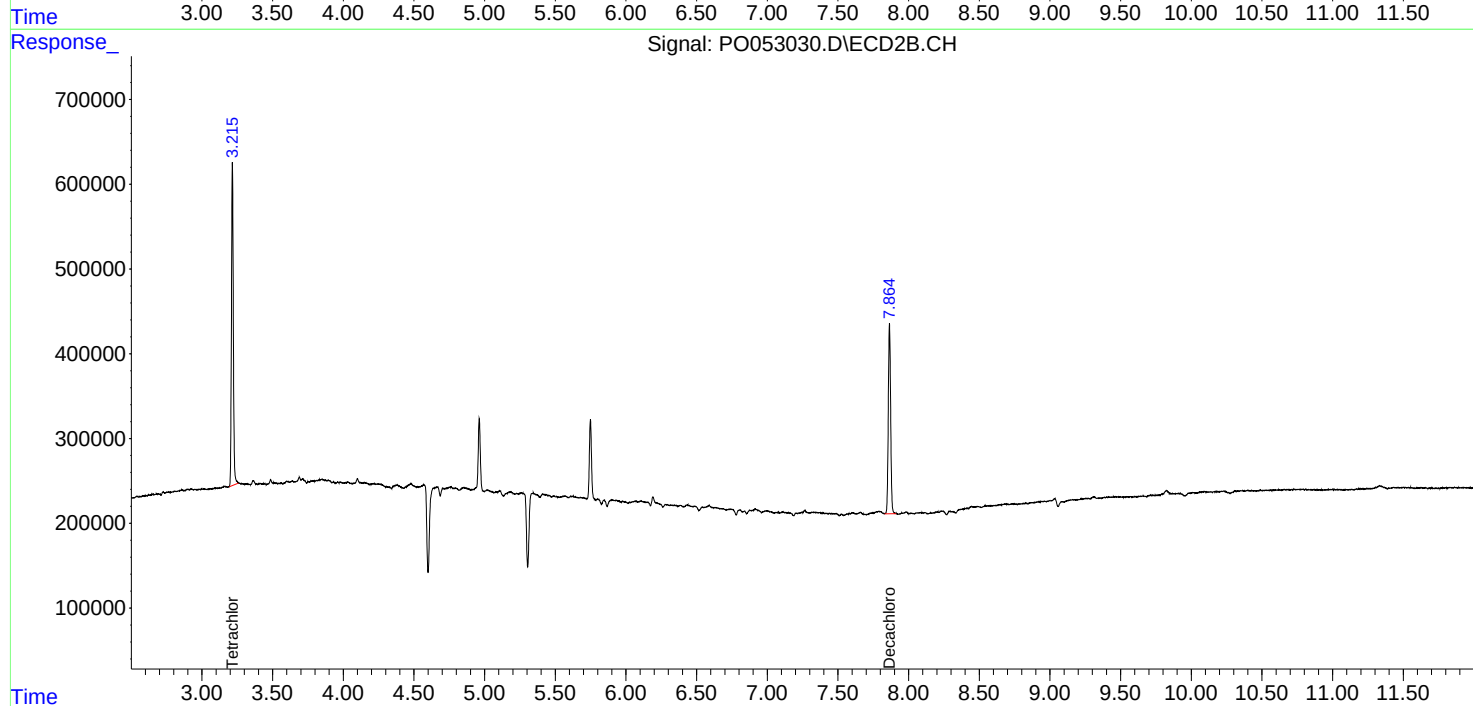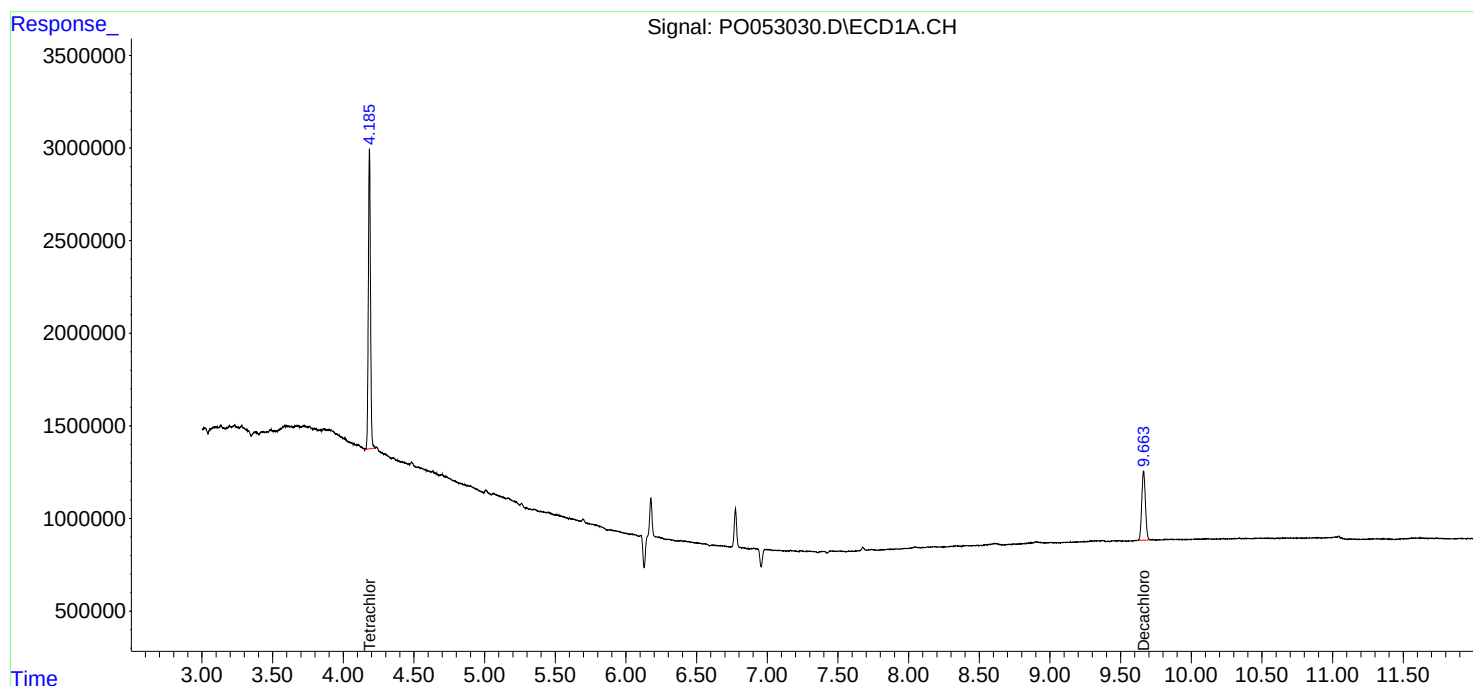


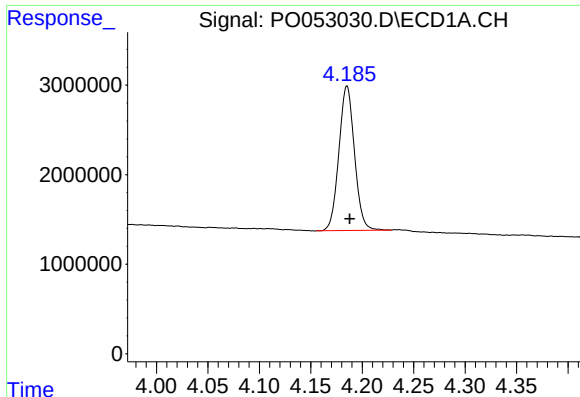

#1 Tetrachloro-m-xylene


R.T.: 4.185 min
Delta R.T.: -0.003 min
Response: 17051630
Conc: 17.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-64(0-23)-COMP

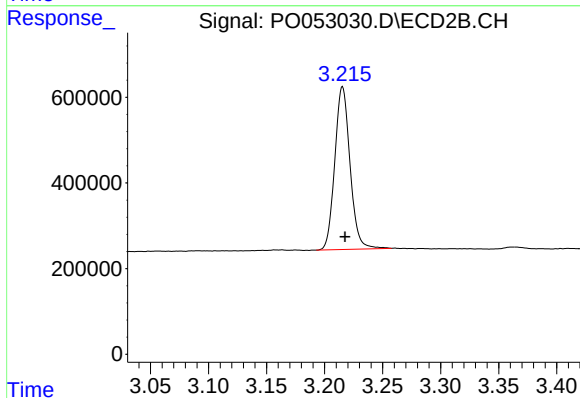


#1 Tetrachloro-m-xylene

R.T.: 3.215 min
Delta R.T.: -0.002 min
Response: 3480844
Conc: 17.93 ng/ml

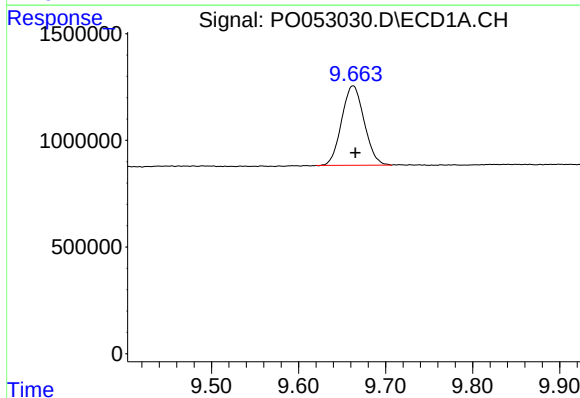

#2 Decachlorobiphenyl

R.T.: 9.663 min
Delta R.T.: -0.002 min
Response: 6696069
Conc: 10.86 ng/ml

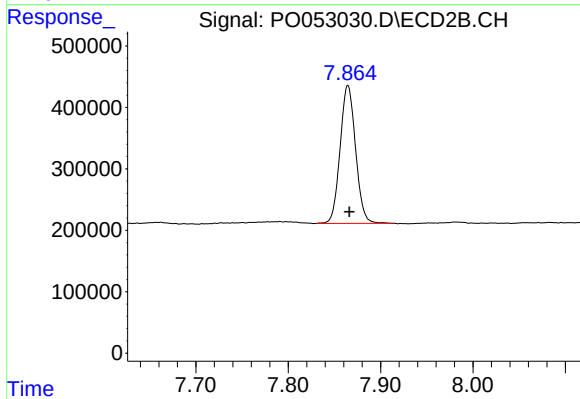

#2 Decachlorobiphenyl

R.T.: 7.865 min
Delta R.T.: -0.002 min
Response: 2610593
Conc: 12.11 ng/ml