

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010224\
 Data File : PP062694.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jan 2024 08:11
 Operator : YP\AJ
 Sample : 06038-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 T-401

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/04/2024
 Supervised By :Ankita Jodhani 01/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 23:19:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 22 03:29:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.402	3.695	32976528	49598850	15.168m	16.620m
2) SA Decachlor...	10.154	8.789	32800789	97773061	22.747m	38.407m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010224\
Data File : PP062694.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jan 2024 08:11
Operator : YP\AJ
Sample : 06038-03
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
T-401


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/04/2024
Supervised By :Ankita Jodhani 01/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 23:19:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122123.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 22 03:29:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

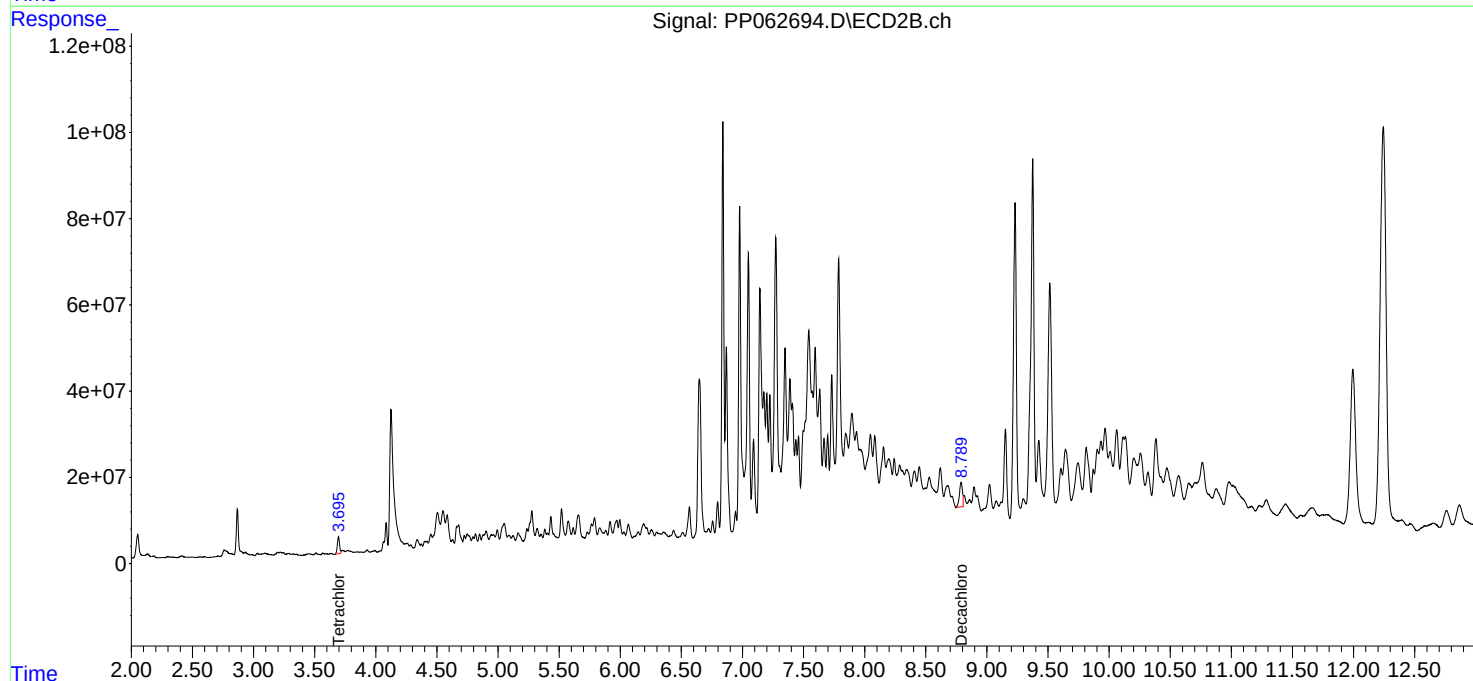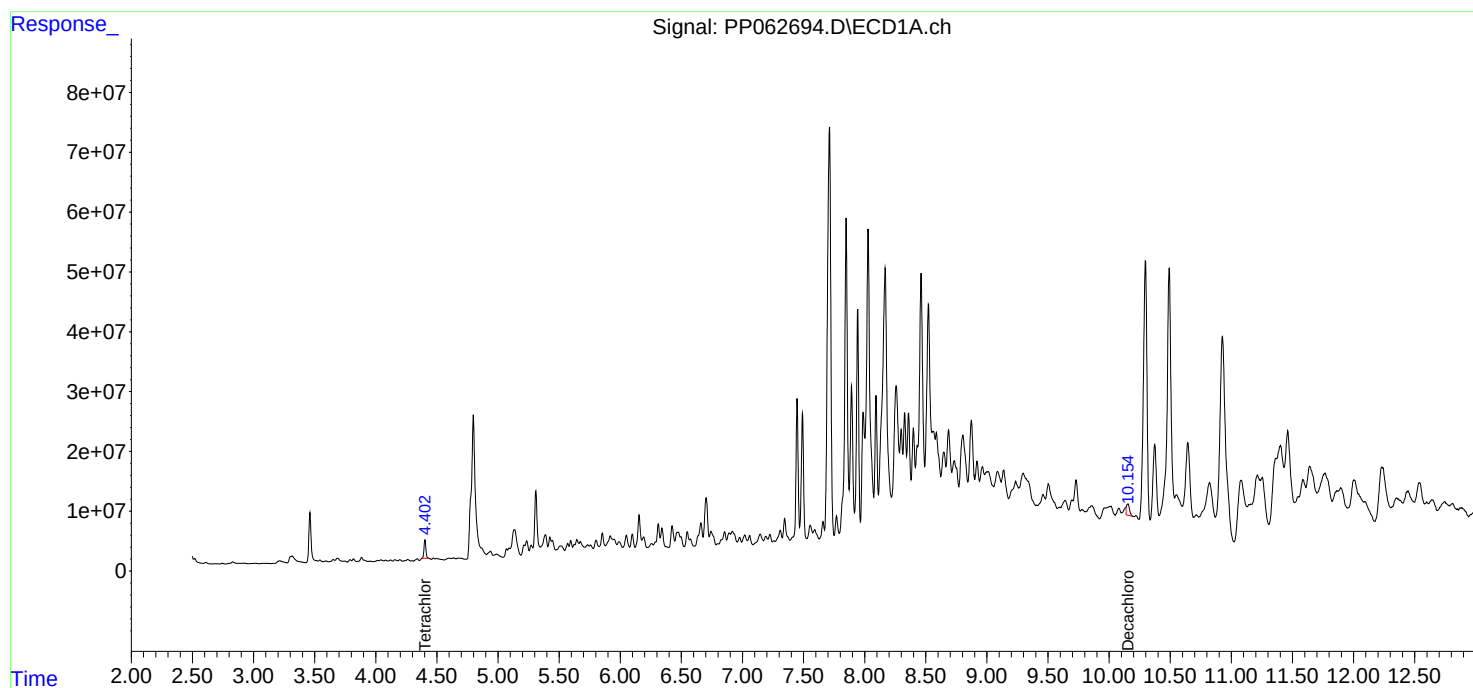

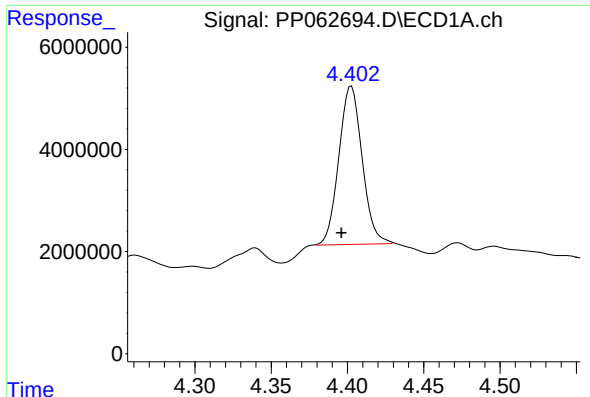


#1 Tetrachloro-m-xylene

R.T.: 4.402 min
Delta R.T.: 0.006 min
Response: 32976528
Conc: 15.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
T-401


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/04/2024
Supervised By :Ankita Jodhani 01/04/2024

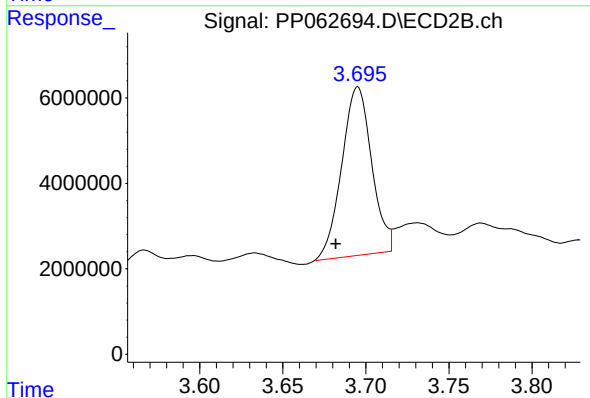


#1 Tetrachloro-m-xylene

R.T.: 3.695 min
Delta R.T.: 0.013 min
Response: 49598850
Conc: 16.62 ng/ml m

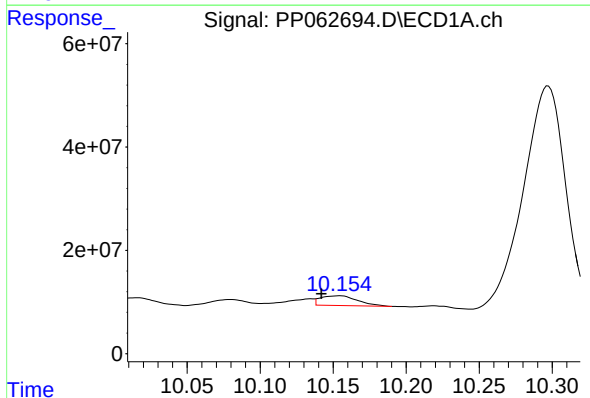

#2 Decachlorobiphenyl

R.T.: 10.154 min
Delta R.T.: 0.012 min
Response: 32800789
Conc: 22.75 ng/ml m

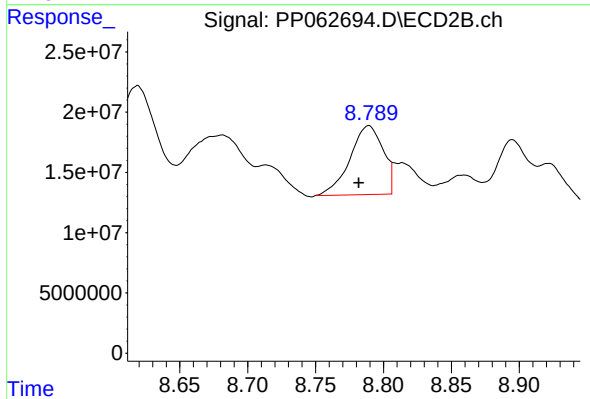

#2 Decachlorobiphenyl

R.T.: 8.789 min
Delta R.T.: 0.007 min
Response: 97773061
Conc: 38.41 ng/ml m