

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010522\
 Data File : PP042589.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jan 2022 4:54
 Operator : AJ\MA
 Sample : N1013-12 10X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 06 04:54:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 05 12:01:35 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.880	4.048	23035	40080	1.189	1.531 #
2)	SA Decachlor...	10.818	9.390	32718	31910	2.789	1.624 #
Target Compounds							
5)	L1 AR-1016-3	6.298f	0.000	9510	0	17.859	N.D. #
18)	L4 AR-1242-3	6.298f	0.000	9510	0	23.857	N.D. #
20)	L4 AR-1242-5	7.135f	6.183	27578	15885	83.683	21.657 #
24)	L5 AR-1248-4	7.135f	0.000	27578	0	49.314	N.D. #
25)	L5 AR-1248-5	7.135f	0.000	27578	0	50.335	N.D. #
26)	L6 AR-1254-1	0.000	6.183	0	15885	N.D.	10.316 #
27)	L6 AR-1254-2	7.303	0.000	3307	0	3.602	N.D. #
28)	L6 AR-1254-3	7.696	6.765	6733	34128	7.350	16.340 #
30)	L6 AR-1254-5	8.424	0.000	3254	0	5.146	N.D. #
32)	L7 AR-1260-2	0.000	7.090f	0	10956	N.D.	7.207 #
33)	L7 AR-1260-3	8.500	0.000	4338	0	7.829	N.D. #
34)	L7 AR-1260-4	8.720	0.000	2906	0	4.405	N.D. #
35)	L7 AR-1260-5	9.053	0.000	6841	0	5.671	N.D. #
36)	L8 AR-1262-1	8.500	0.000	4338	0	5.541	N.D. #
37)	L8 AR-1262-2	9.053	0.000	6841	0	5.116	N.D. #
38)	L8 AR-1262-3	9.352	0.000	506	0	0.768	N.D. #
39)	L8 AR-1262-4	9.436	0.000	2089	0	4.322	N.D. #
40)	L8 AR-1262-5	10.081	0.000	6022	0	12.342	N.D. #
41)	L9 AR-1268-1	9.352	0.000	506	0	0.309	N.D. #
42)	L9 AR-1268-2	9.447	0.000	2188	0	1.446	N.D. #
43)	L9 AR-1268-3	9.660	0.000	7466	0	5.547	N.D. #
44)	L9 AR-1268-4	10.081	0.000	6022	0	11.000	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010522\
Data File : PP042589.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jan 2022 4:54
Operator : AJ\MA
Sample : N1013-12 10X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 06 04:54:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 05 12:01:35 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

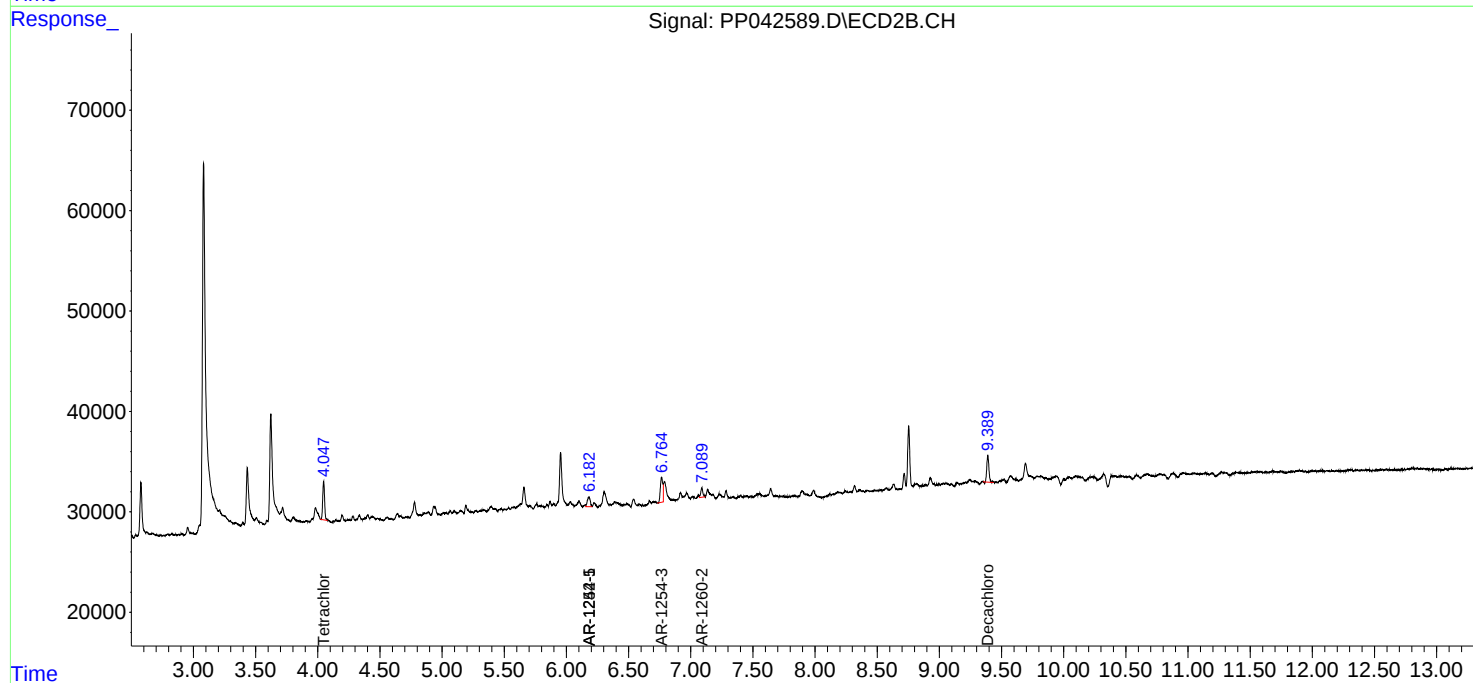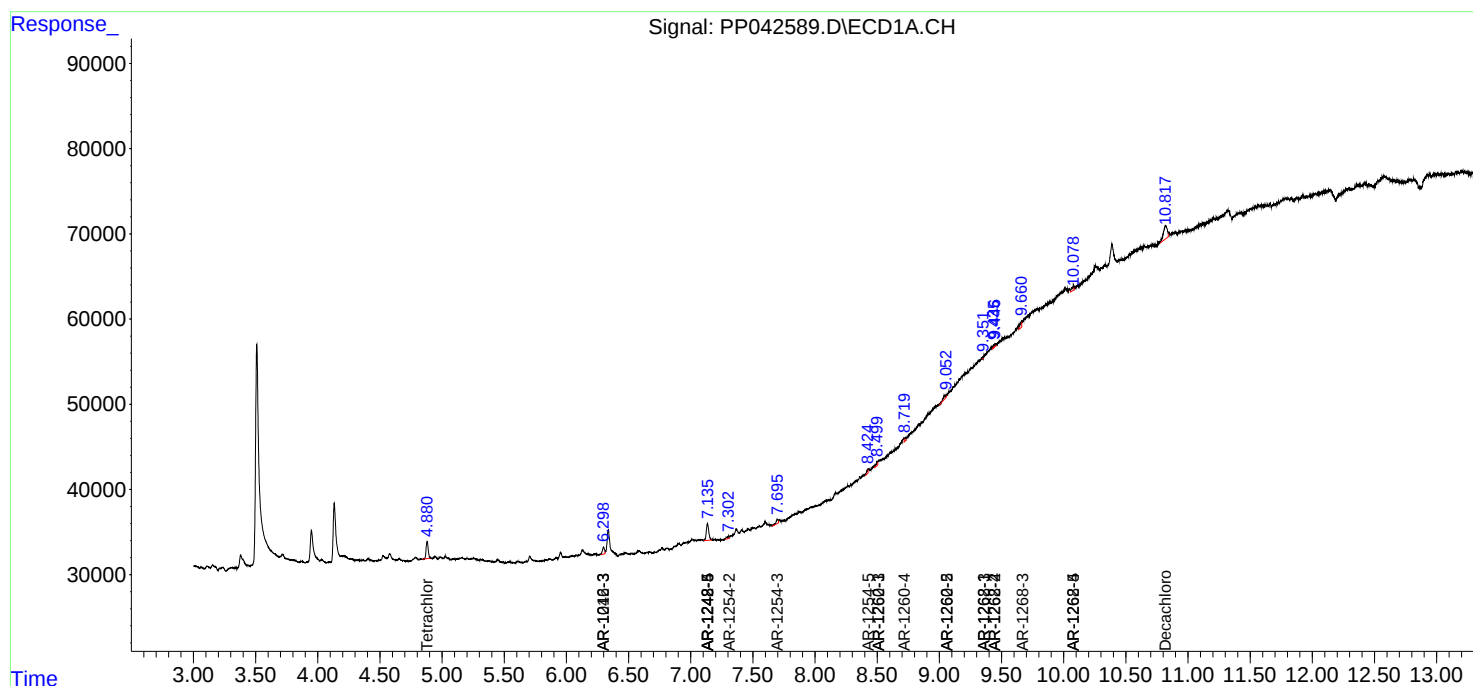


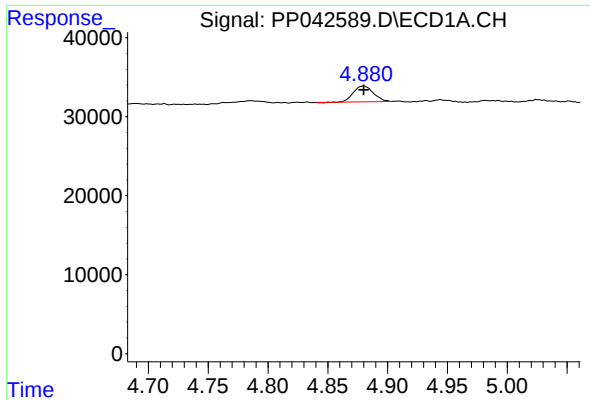

#1 Tetrachloro-m-xylene


R.T.: 4.880 min
Delta R.T.: 0.000 min
Response: 23035
Conc: 1.19 ng/ml

Instrument :
ECD_P
ClientSampleId :

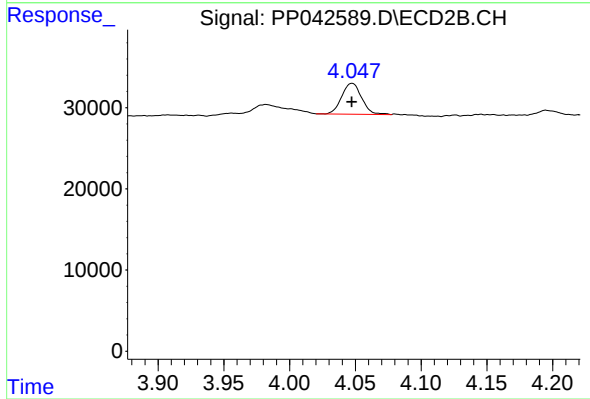


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.000 min
Response: 40080
Conc: 1.53 ng/ml

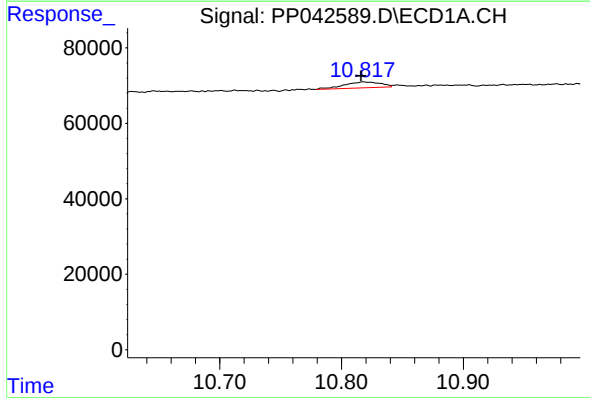


#2 Decachlorobiphenyl

R.T.: 10.818 min
Delta R.T.: 0.002 min
Response: 32718
Conc: 2.79 ng/ml

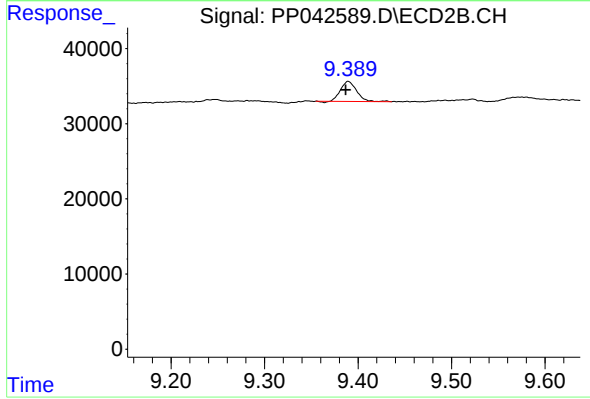

#2 Decachlorobiphenyl


R.T.: 9.390 min
Delta R.T.: 0.003 min
Response: 31910
Conc: 1.62 ng/ml

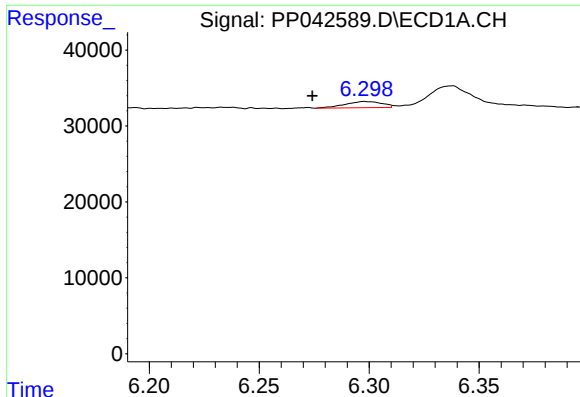

#5 AR-1016-3


R.T.: 6.298 min
Delta R.T.: 0.024 min
Response: 9510
Conc: 17.86 ng/ml

Instrument :
ECD_P
ClientSampleId :

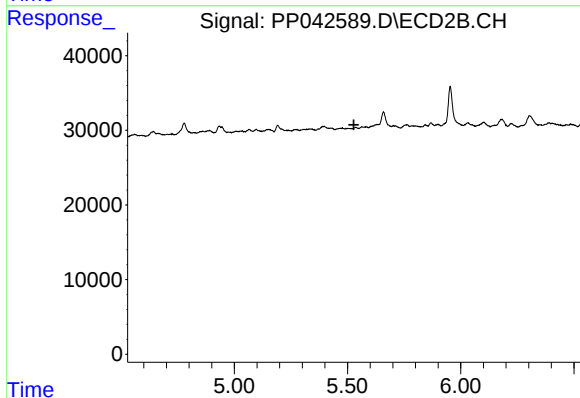


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 5.528 min
Response: 0
Conc: N.D.

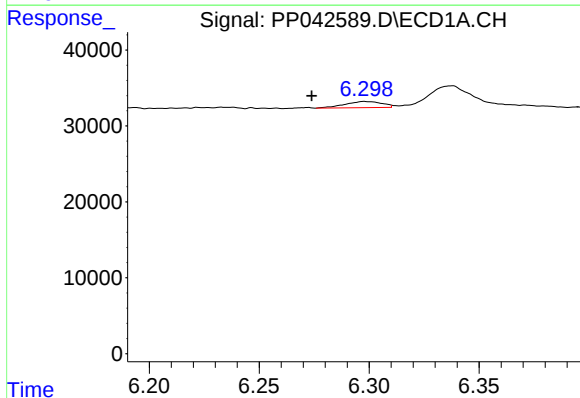


#18 AR-1242-3

R.T.: 6.298 min
Delta R.T.: 0.024 min
Response: 9510
Conc: 23.86 ng/ml

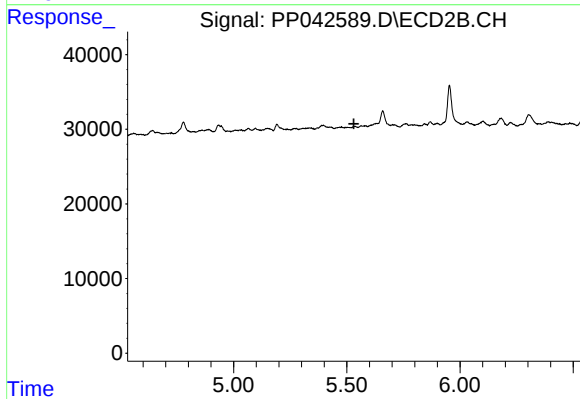

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 5.531 min
Response: 0
Conc: N.D.

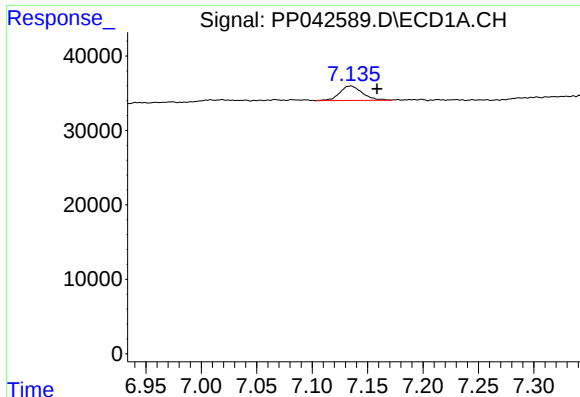

#20 AR-1242-5


R.T.: 7.135 min
Delta R.T.: -0.023 min
Response: 27578
Conc: 83.68 ng/ml

Instrument :
ECD_P
ClientSampleId :

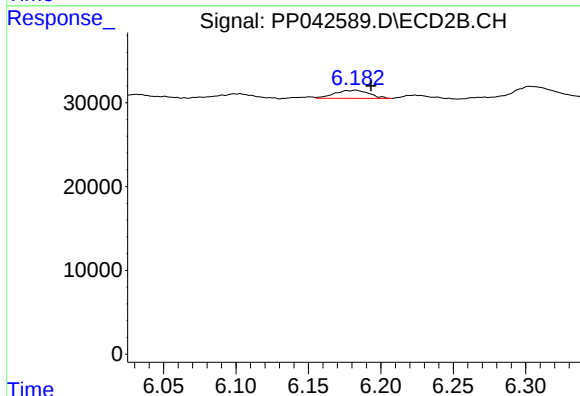


#20 AR-1242-5

R.T.: 6.183 min
Delta R.T.: -0.011 min
Response: 15885
Conc: 21.66 ng/ml

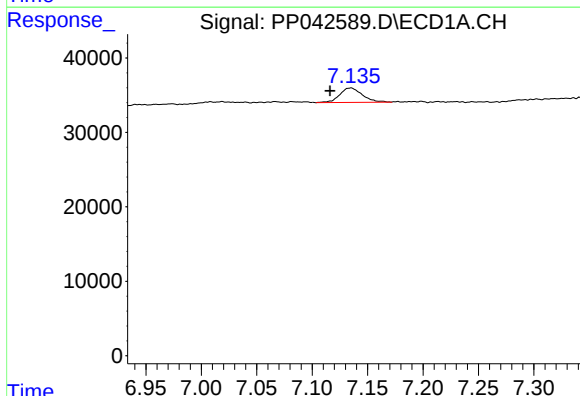


#24 AR-1248-4

R.T.: 7.135 min
Delta R.T.: 0.019 min
Response: 27578
Conc: 49.31 ng/ml

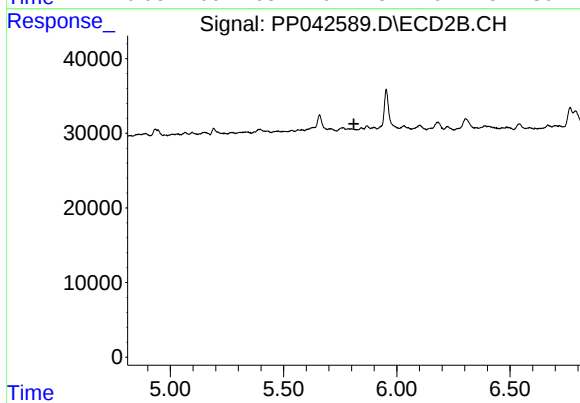

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.810 min
Response: 0
Conc: N.D.

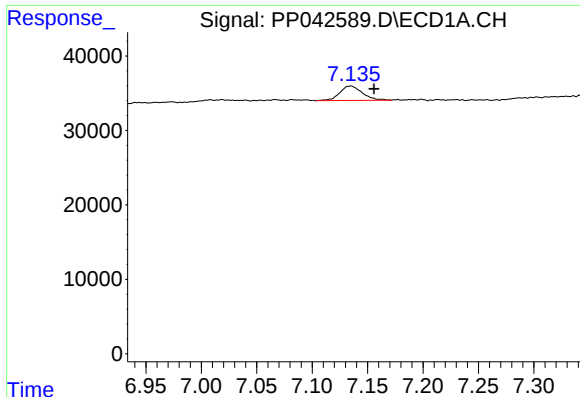

#25 AR-1248-5


R.T.: 7.135 min
Delta R.T.: -0.021 min
Response: 27578
Conc: 50.33 ng/ml

Instrument :
ECD_P
ClientSampleId :

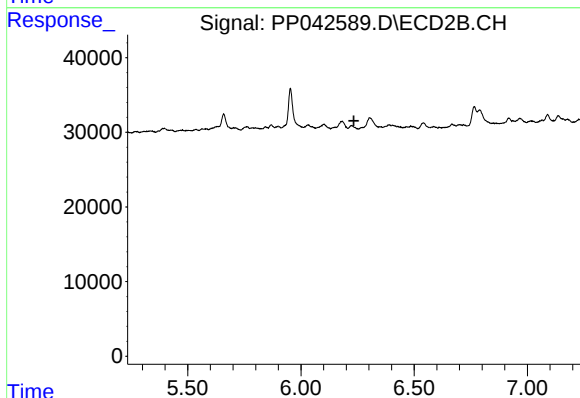


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.

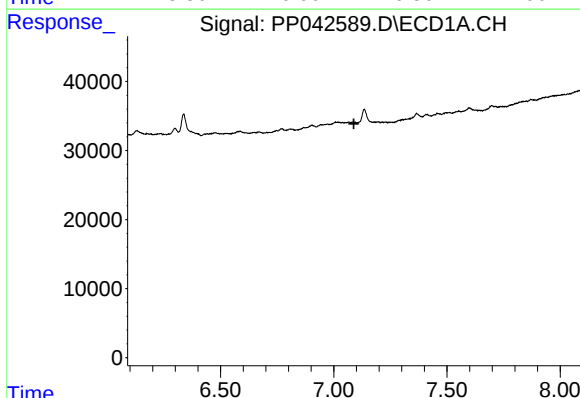


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 7.089 min
Response: 0
Conc: N.D.

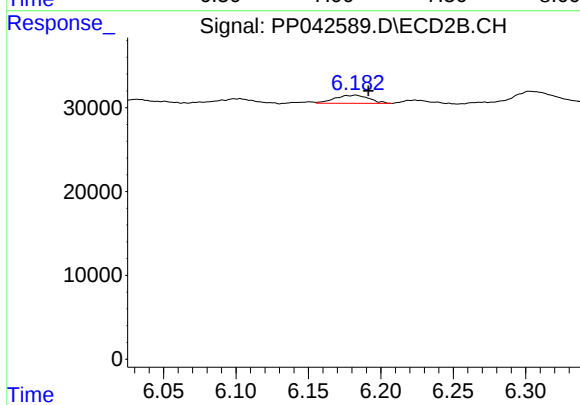

#26 AR-1254-1


R.T.: 6.183 min
Delta R.T.: -0.009 min
Response: 15885
Conc: 10.32 ng/ml

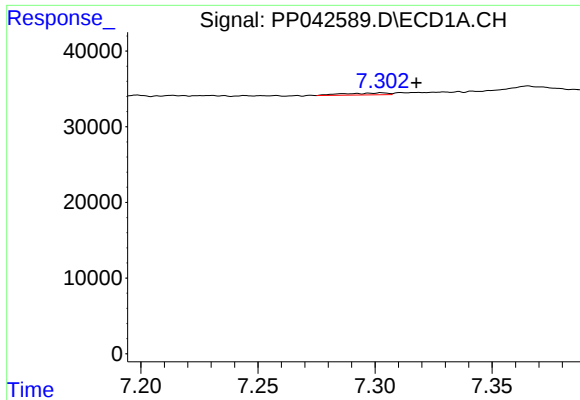

#27 AR-1254-2


R.T.: 7.303 min
Delta R.T.: -0.015 min
Response: 3307
Conc: 3.60 ng/ml

Instrument :
ECD_P
ClientSampleId :

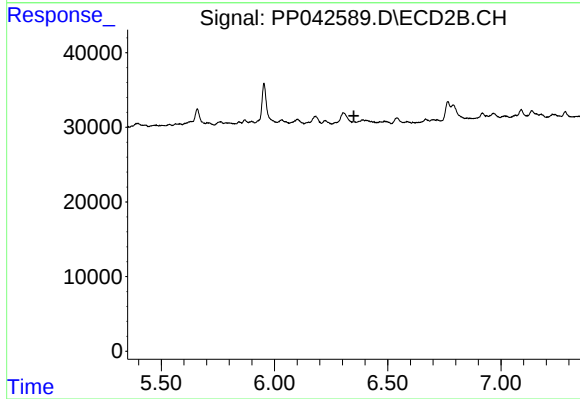


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.350 min
Response: 0
Conc: N.D.

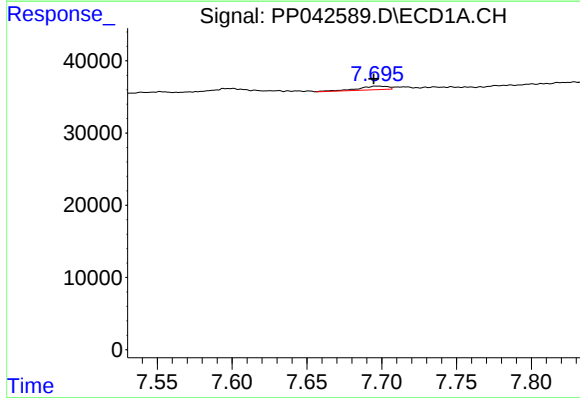


#28 AR-1254-3

R.T.: 7.696 min
Delta R.T.: 0.001 min
Response: 6733
Conc: 7.35 ng/ml

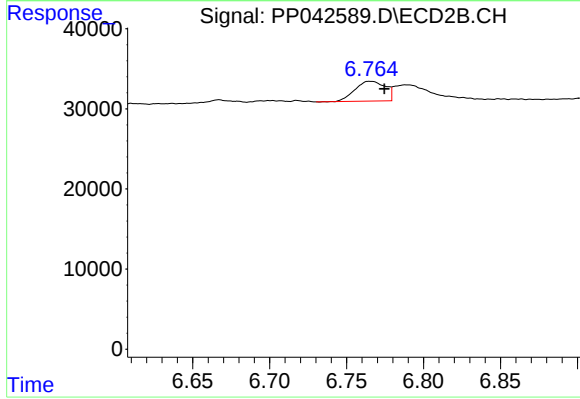

#28 AR-1254-3


R.T.: 6.765 min
Delta R.T.: -0.010 min
Response: 34128
Conc: 16.34 ng/ml

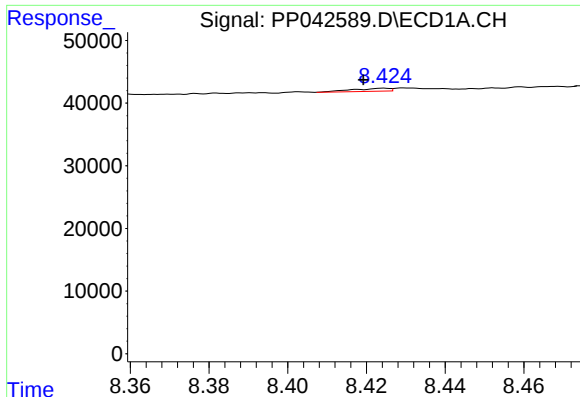

#30 AR-1254-5


R.T.: 8.424 min
Delta R.T.: 0.005 min
Response: 3254
Conc: 5.15 ng/ml

Instrument :
ECD_P
ClientSampleId :

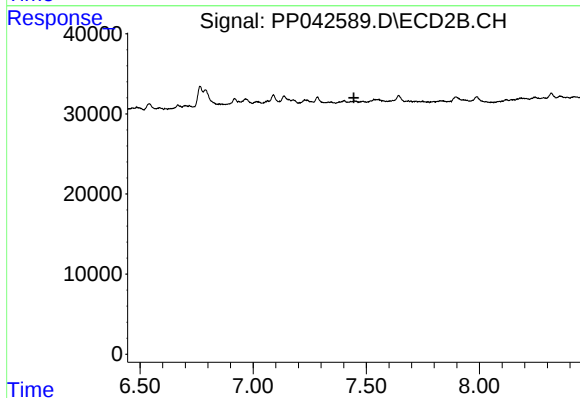


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.445 min
Response: 0
Conc: N.D.

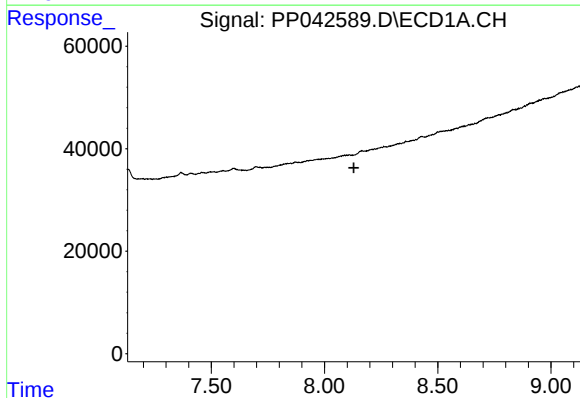


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 8.130 min
Response: 0
Conc: N.D.

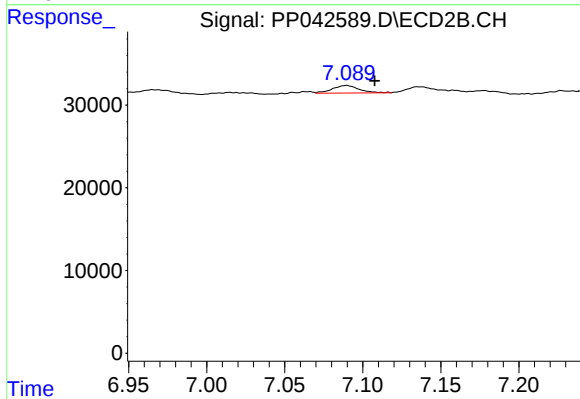

#32 AR-1260-2


R.T.: 7.090 min
Delta R.T.: -0.018 min
Response: 10956
Conc: 7.21 ng/ml

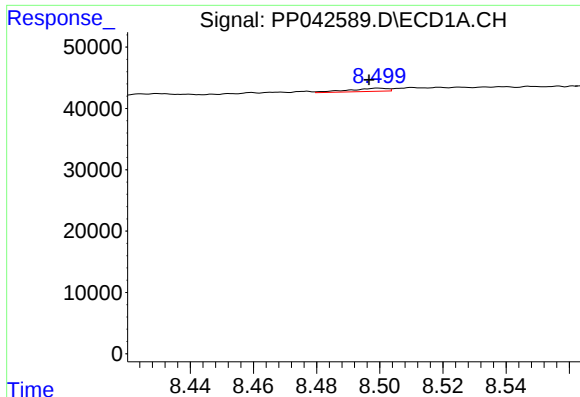

#33 AR-1260-3


R.T.: 8.500 min
Delta R.T.: 0.003 min
Response: 4338
Conc: 7.83 ng/ml

Instrument :
ECD_P
ClientSampleId :

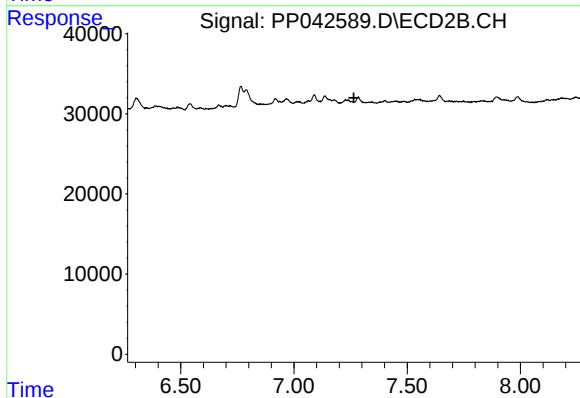


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.264 min
Response: 0
Conc: N.D.

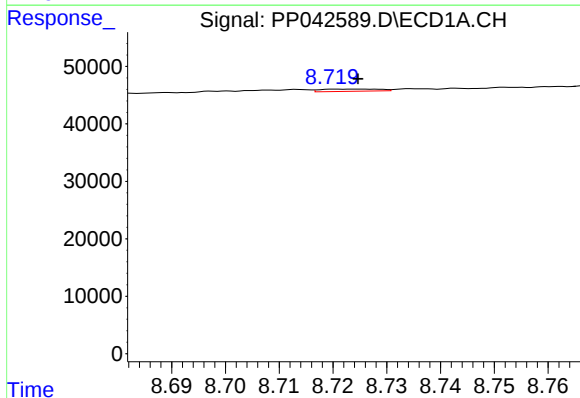


#34 AR-1260-4

R.T.: 8.720 min
Delta R.T.: -0.004 min
Response: 2906
Conc: 4.40 ng/ml

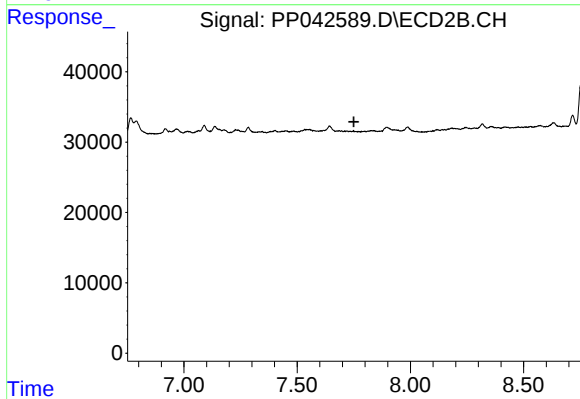

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.750 min
Response: 0
Conc: N.D.

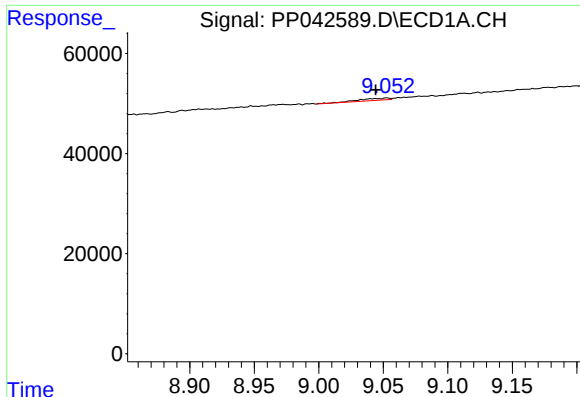

#35 AR-1260-5


R.T.: 9.053 min
Delta R.T.: 0.009 min
Response: 6841
Conc: 5.67 ng/ml

Instrument :
ECD_P
ClientSampleId :

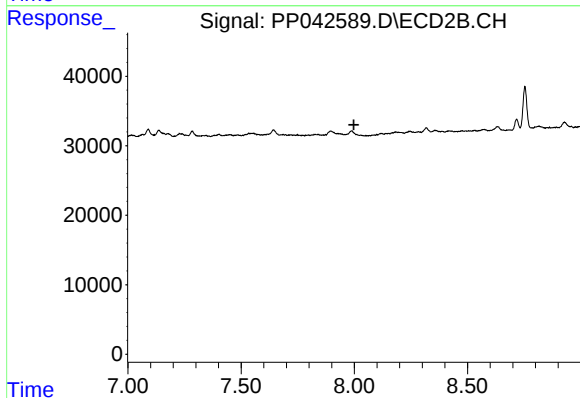


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.998 min
Response: 0
Conc: N.D.

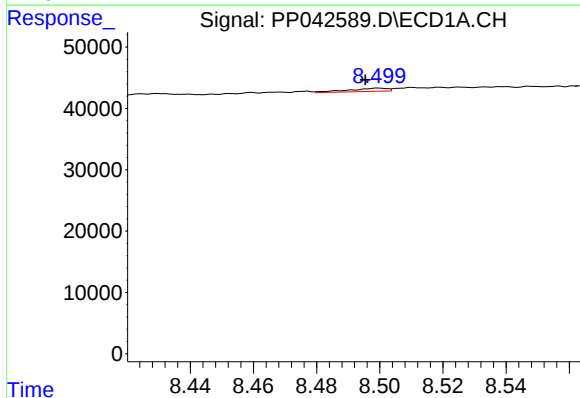


#36 AR-1262-1

R.T.: 8.500 min
Delta R.T.: 0.004 min
Response: 4338
Conc: 5.54 ng/ml

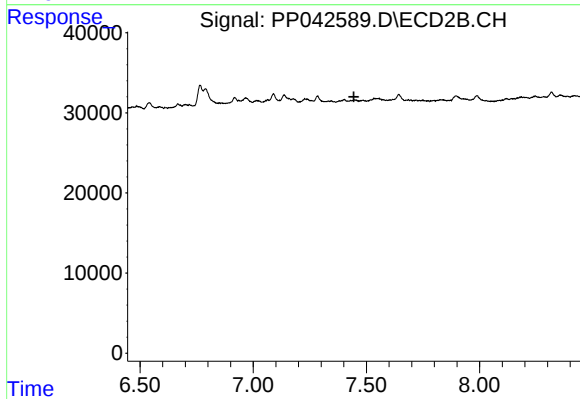

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 7.444 min
Response: 0
Conc: N.D.

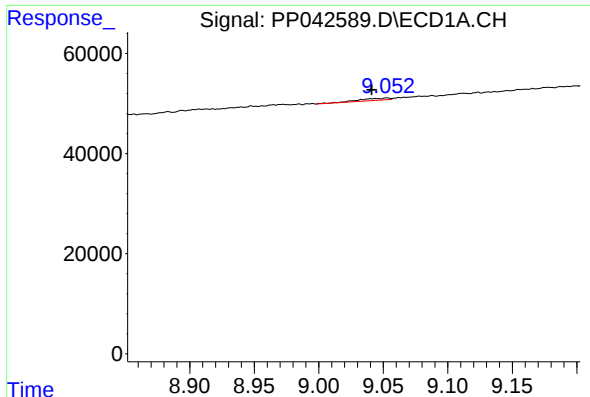

#37 AR-1262-2


R.T.: 9.053 min
Delta R.T.: 0.012 min
Response: 6841
Conc: 5.12 ng/ml

Instrument :
ECD_P
ClientSampleId :

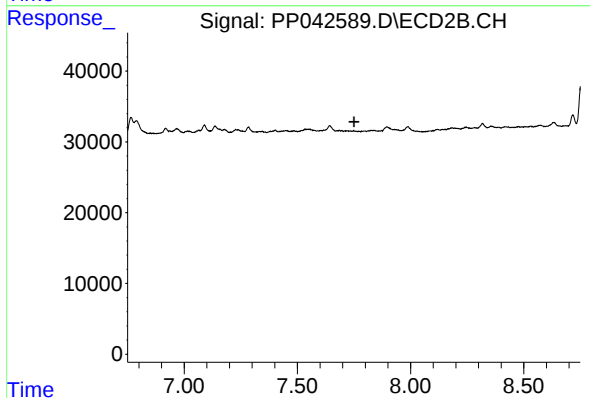


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.750 min
Response: 0
Conc: N.D.

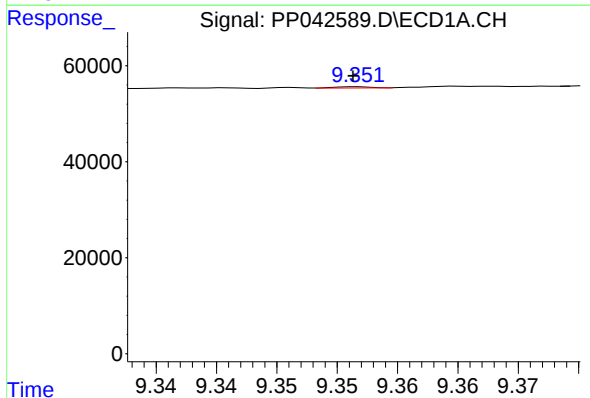


#38 AR-1262-3

R.T.: 9.352 min
Delta R.T.: 0.000 min
Response: 506
Conc: 0.77 ng/ml

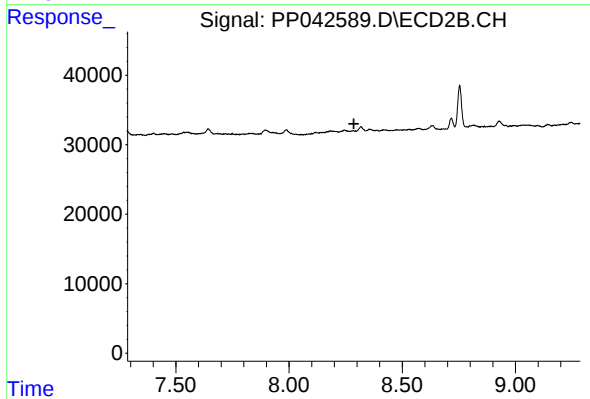

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 8.286 min
Response: 0
Conc: N.D.

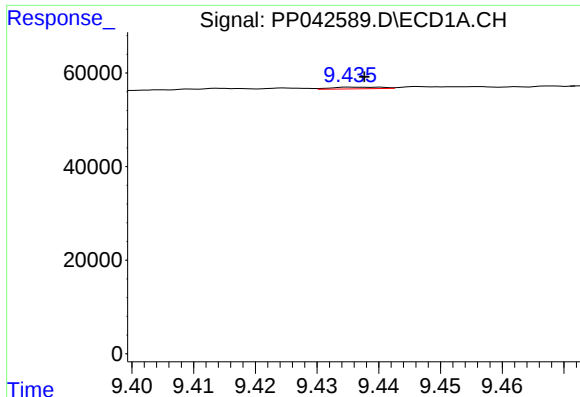

#39 AR-1262-4


R.T.: 9.436 min
Delta R.T.: -0.002 min
Response: 2089
Conc: 4.32 ng/ml

Instrument :
ECD_P
ClientSampleId :

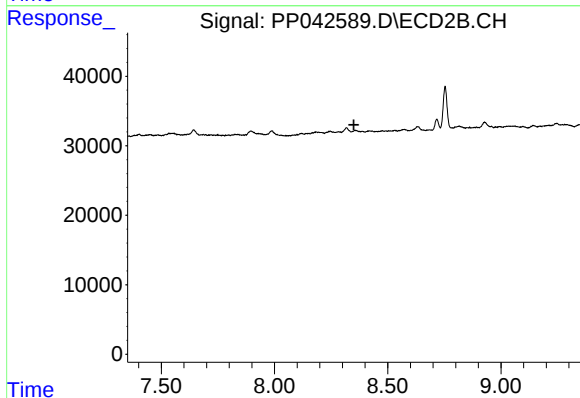


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.350 min
Response: 0
Conc: N.D.

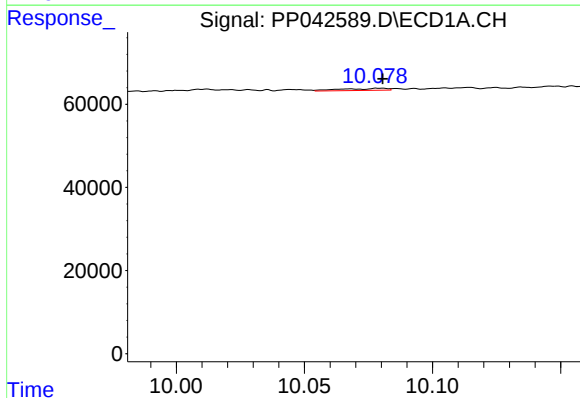


#40 AR-1262-5

R.T.: 10.081 min
Delta R.T.: 0.000 min
Response: 6022
Conc: 12.34 ng/ml

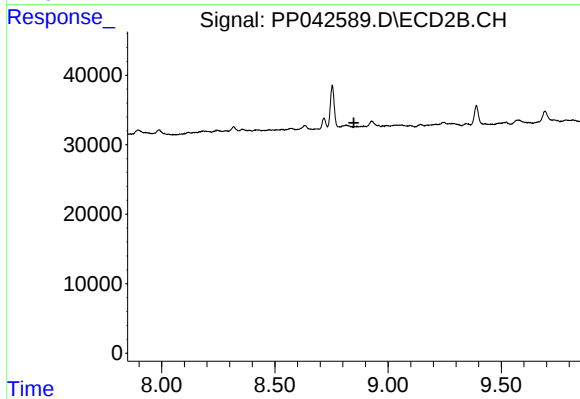

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 8.849 min
Response: 0
Conc: N.D.

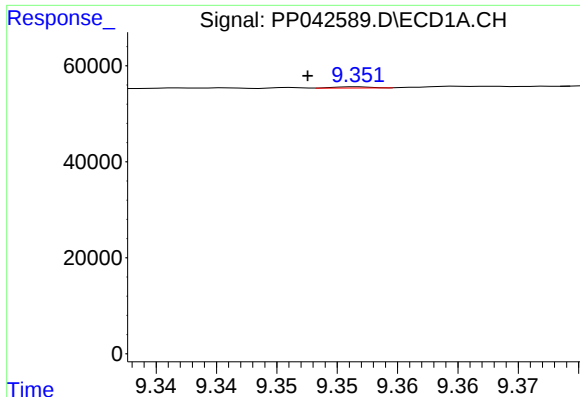

#41 AR-1268-1


R.T.: 9.352 min
Delta R.T.: 0.004 min
Response: 506
Conc: 0.31 ng/ml

Instrument :
ECD_P
ClientSampleId :

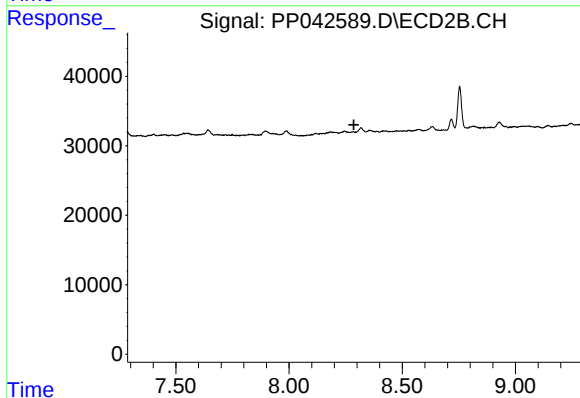


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.286 min
Response: 0
Conc: N.D.

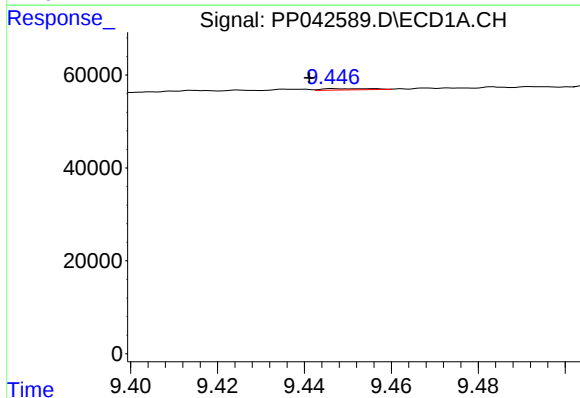


#42 AR-1268-2

R.T.: 9.447 min
Delta R.T.: 0.005 min
Response: 2188
Conc: 1.45 ng/ml

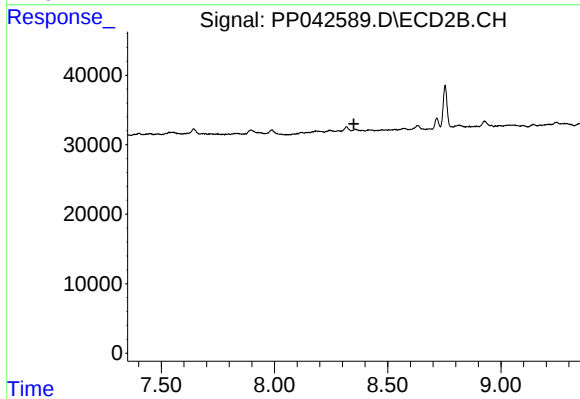

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.351 min
Response: 0
Conc: N.D.

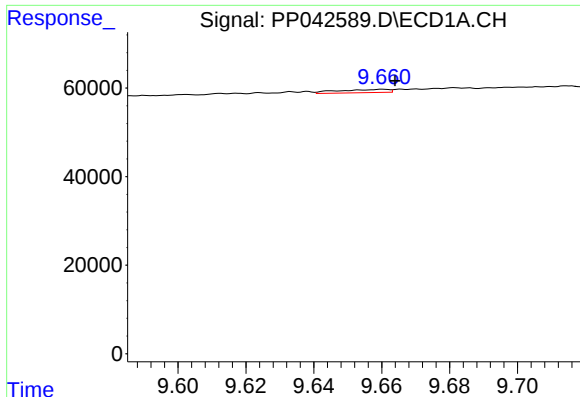

#43 AR-1268-3


R.T.: 9.660 min
Delta R.T.: -0.003 min
Response: 7466
Conc: 5.55 ng/ml

Instrument :
ECD_P
ClientSampleId :

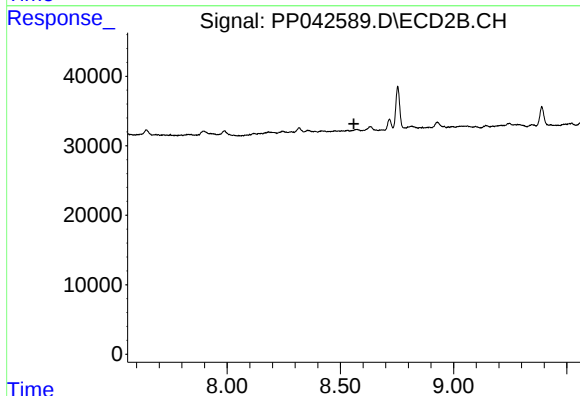


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.560 min
Response: 0
Conc: N.D.

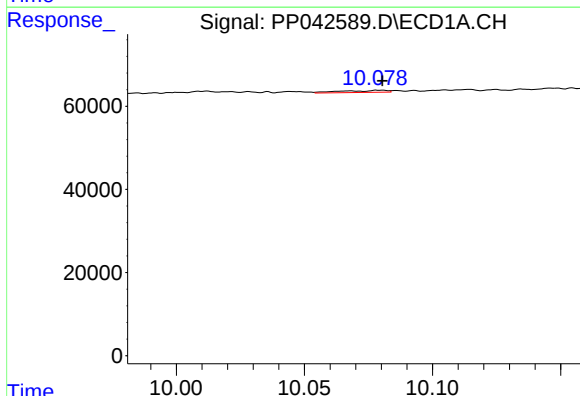

#44 AR-1268-4

R.T.: 10.081 min
Delta R.T.: 0.000 min
Response: 6022
Conc: 11.00 ng/ml

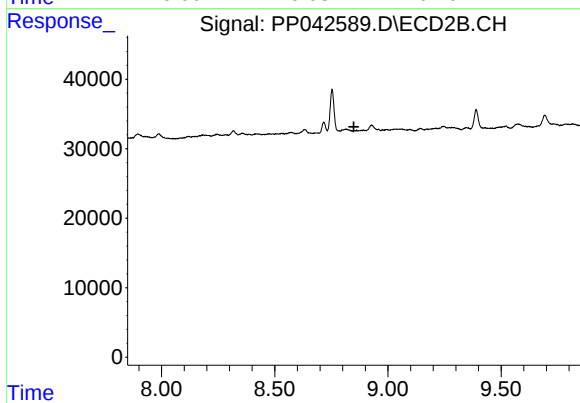

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.849 min
Response: 0
Conc: N.D.