

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010522\
 Data File : PP042595.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jan 2022 7:01
 Operator : AJ\MA
 Sample : N1013-13 10X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 06 13:50:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 05 12:01:35 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.879	4.047	32038	51848	1.654	1.981
2)	SA Decachlor...	10.821	9.389	34084	39661	2.905	2.018 #
Target Compounds							
28)	L6 AR-1254-3	7.701	0.000	5157	0	5.630	N.D. #
29)	L6 AR-1254-4	7.988	0.000	1441	0	2.406	N.D. #
30)	L6 AR-1254-5	8.417	0.000	2699	0	4.268	N.D. #
32)	L7 AR-1260-2	8.136	0.000	1743	0	2.477	N.D. #
33)	L7 AR-1260-3	8.506	0.000	3198	0	5.772	N.D. #
34)	L7 AR-1260-4	8.717	0.000	1919	0	2.909	N.D. #
35)	L7 AR-1260-5	9.039	0.000	7007	0	5.808	N.D. #
36)	L8 AR-1262-1	8.506	0.000	3198	0	4.085	N.D. #
37)	L8 AR-1262-2	9.039	0.000	7007	0	5.239	N.D. #
39)	L8 AR-1262-4	9.443	0.000	2813	0	5.821	N.D. #
40)	L8 AR-1262-5	10.086	0.000	4783	0	9.803	N.D. #
42)	L9 AR-1268-2	9.443	0.000	2813	0	1.860	N.D. #
43)	L9 AR-1268-3	9.666	0.000	5362	0	3.984	N.D. #
44)	L9 AR-1268-4	10.086	0.000	4783	0	8.737	N.D. #
45)	L9 AR-1268-5	10.503f	0.000	10151	0	2.275	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010522\
Data File : PP042595.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jan 2022 7:01
Operator : AJ\MA
Sample : N1013-13 10X
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 06 13:50:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 05 12:01:35 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

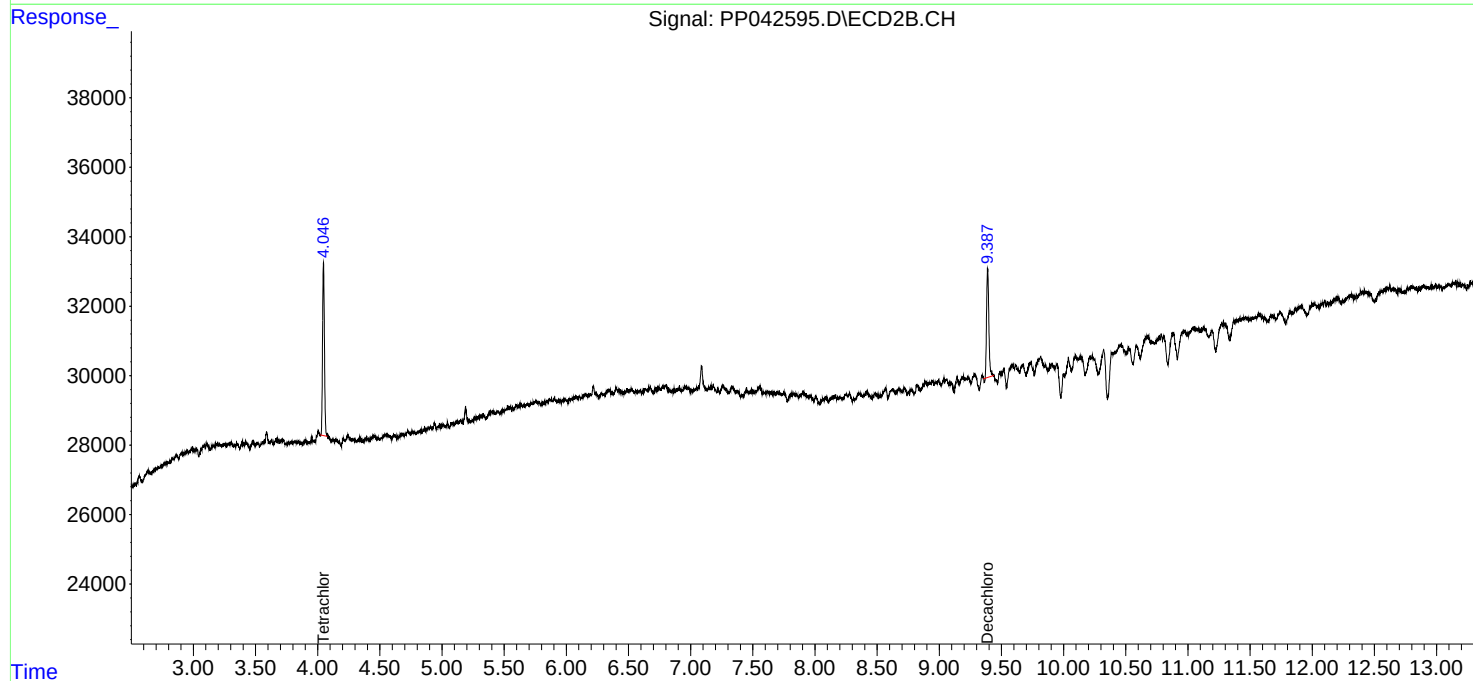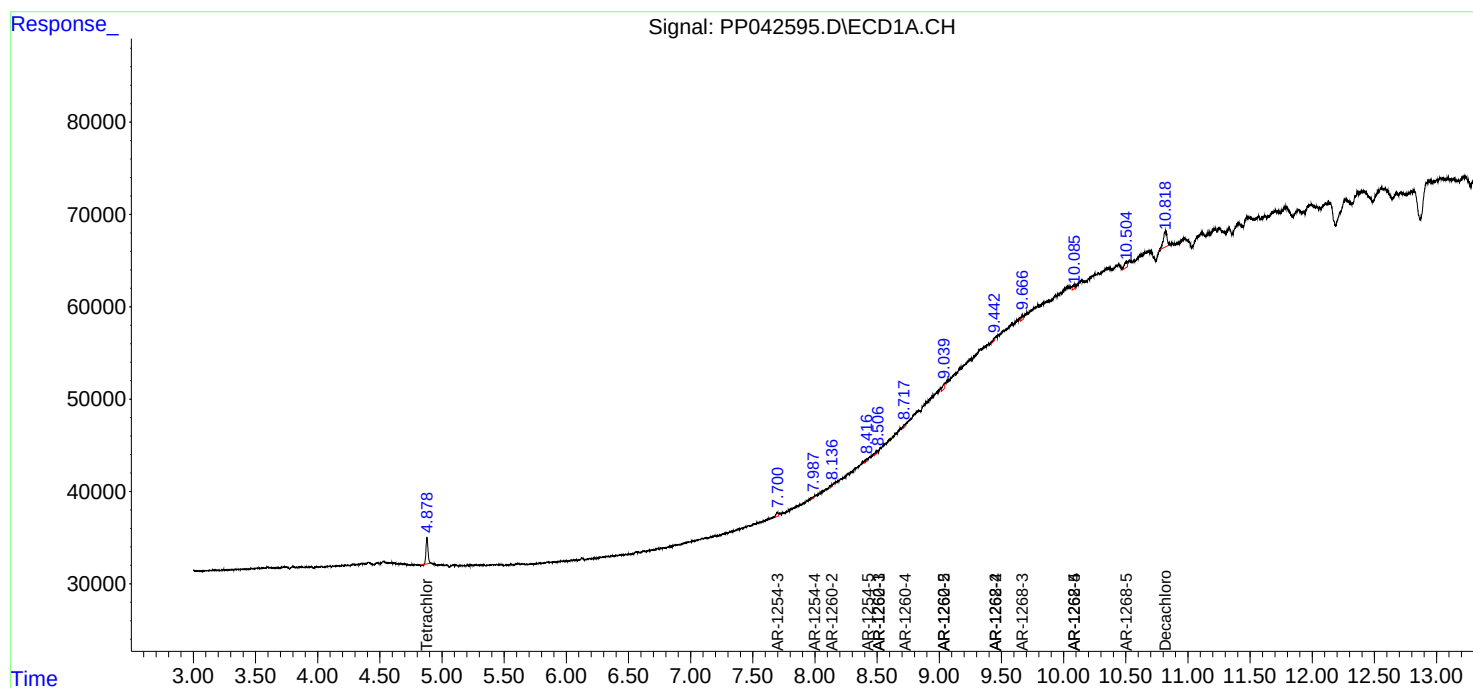


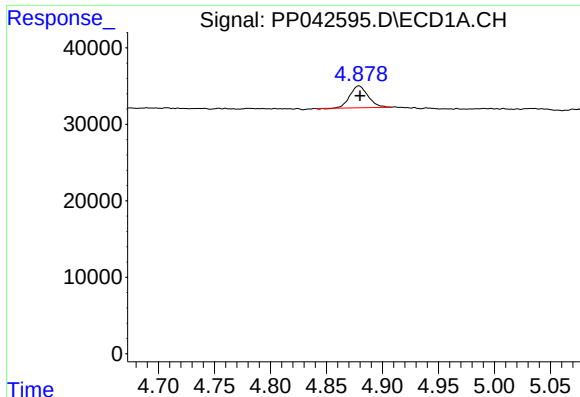

#1 Tetrachloro-m-xylene


R.T.: 4.879 min
Delta R.T.: -0.001 min
Response: 32038
Conc: 1.65 ng/ml

Instrument :
ECD_P
ClientSampleId :

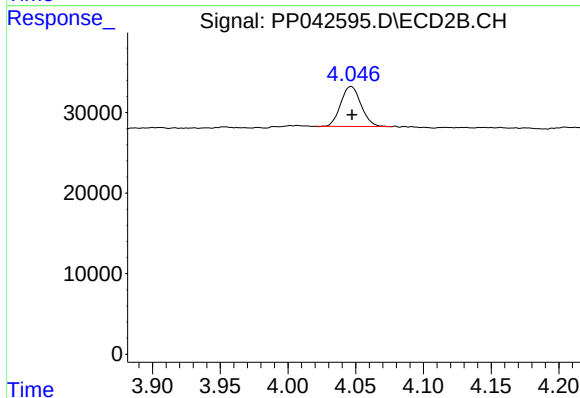


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 51848
Conc: 1.98 ng/ml

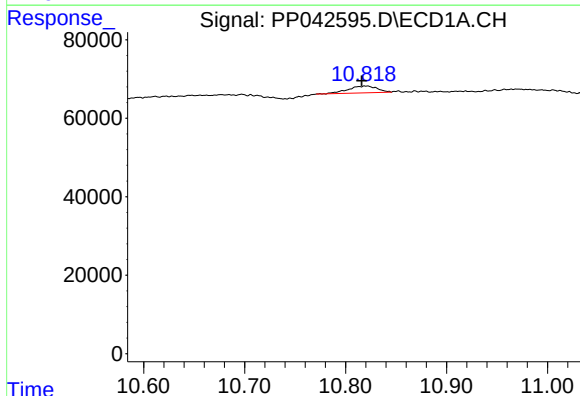


#2 Decachlorobiphenyl

R.T.: 10.821 min
Delta R.T.: 0.005 min
Response: 34084
Conc: 2.91 ng/ml

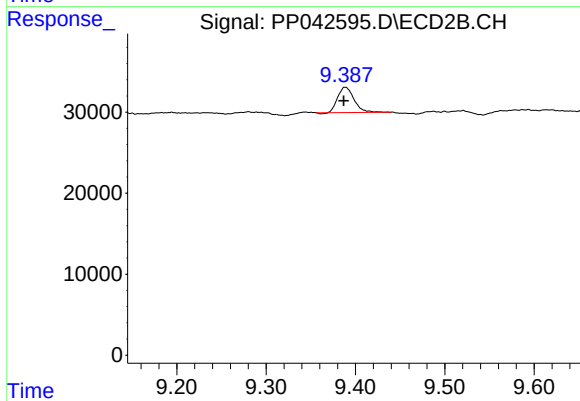

#2 Decachlorobiphenyl


R.T.: 9.389 min
Delta R.T.: 0.002 min
Response: 39661
Conc: 2.02 ng/ml

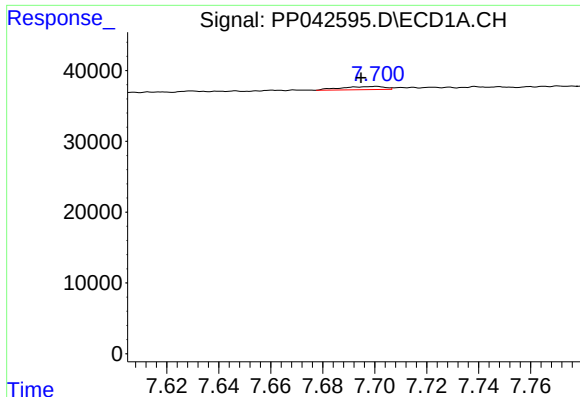

#28 AR-1254-3


R.T.: 7.701 min
Delta R.T.: 0.006 min
Response: 5157
Conc: 5.63 ng/ml

Instrument :
ECD_P
ClientSampleId :

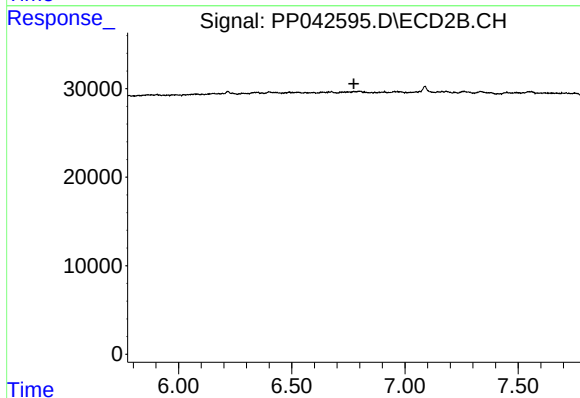


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.774 min
Response: 0
Conc: N.D.

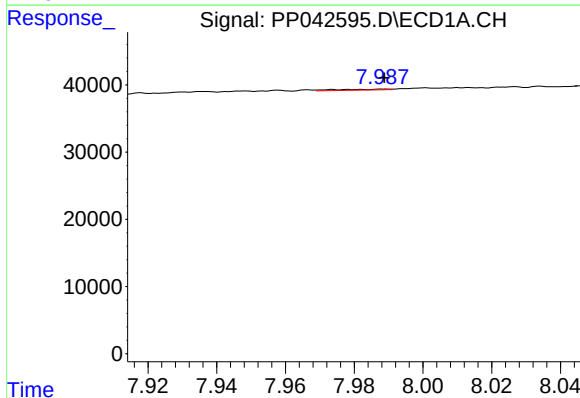


#29 AR-1254-4

R.T.: 7.988 min
Delta R.T.: 0.000 min
Response: 1441
Conc: 2.41 ng/ml

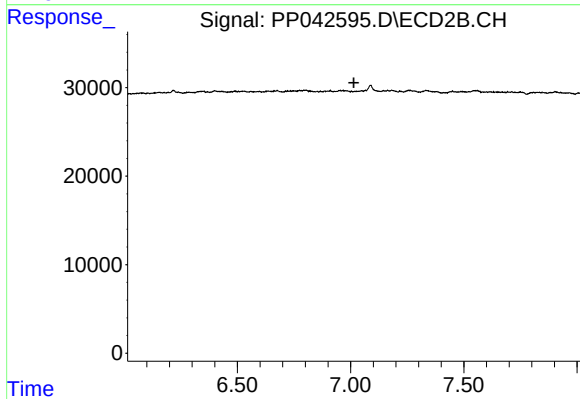

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 7.014 min
Response: 0
Conc: N.D.

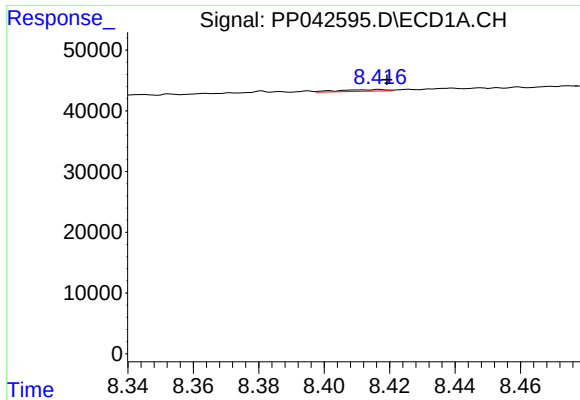

#30 AR-1254-5


R.T.: 8.417 min
Delta R.T.: -0.002 min
Response: 2699
Conc: 4.27 ng/ml

Instrument :
ECD_P
ClientSampleId :

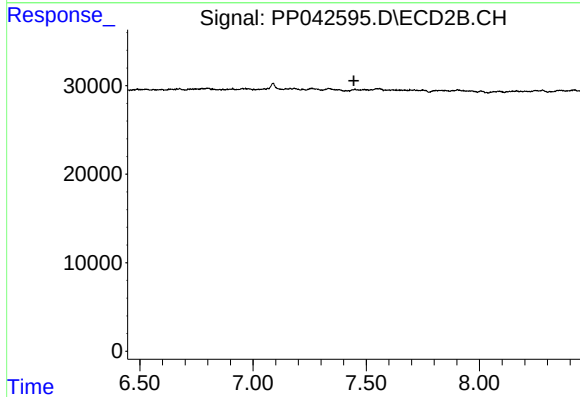


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.445 min
Response: 0
Conc: N.D.

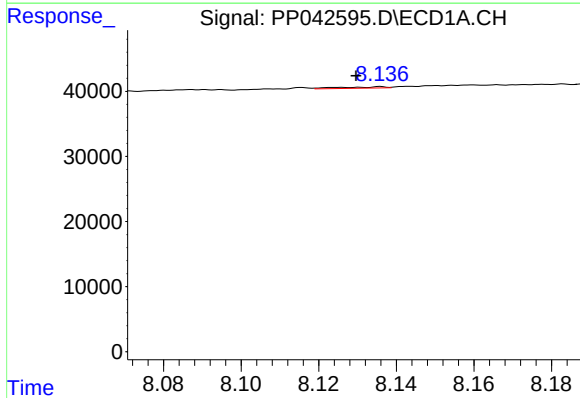


#32 AR-1260-2

R.T.: 8.136 min
Delta R.T.: 0.006 min
Response: 1743
Conc: 2.48 ng/ml

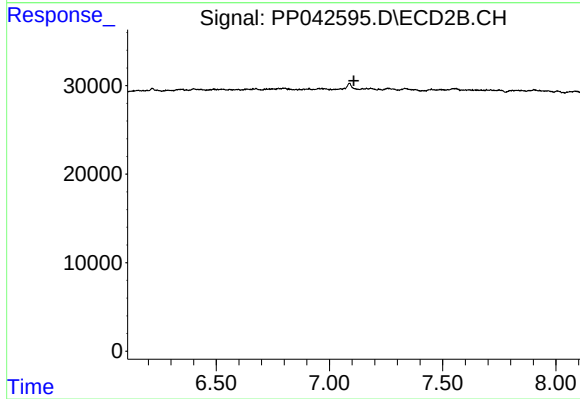

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.108 min
Response: 0
Conc: N.D.

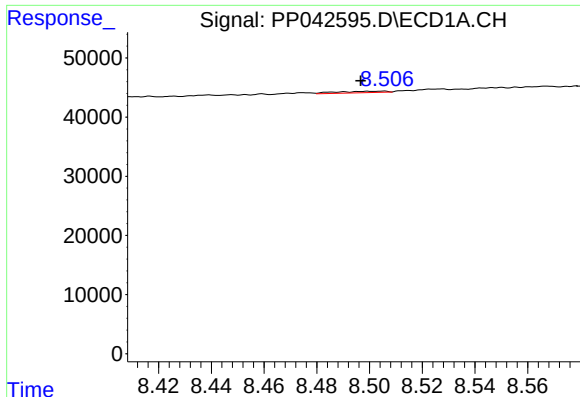

#33 AR-1260-3


R.T.: 8.506 min
Delta R.T.: 0.009 min
Response: 3198
Conc: 5.77 ng/ml

Instrument :
ECD_P
ClientSampleId :

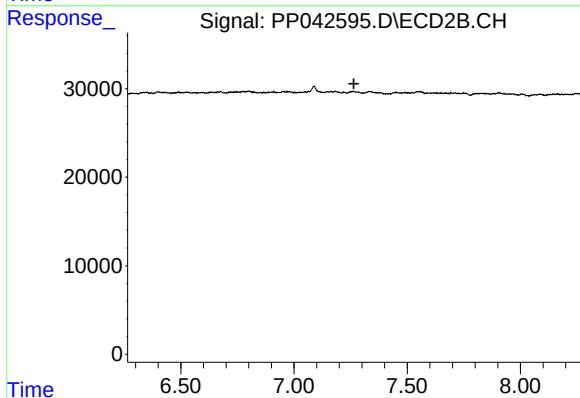


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.264 min
Response: 0
Conc: N.D.

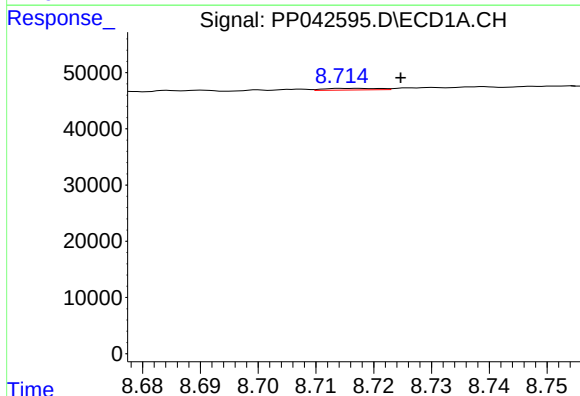


#34 AR-1260-4

R.T.: 8.717 min
Delta R.T.: -0.007 min
Response: 1919
Conc: 2.91 ng/ml

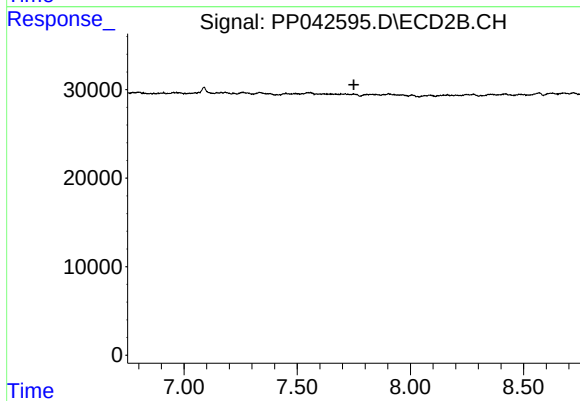

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.750 min
Response: 0
Conc: N.D.

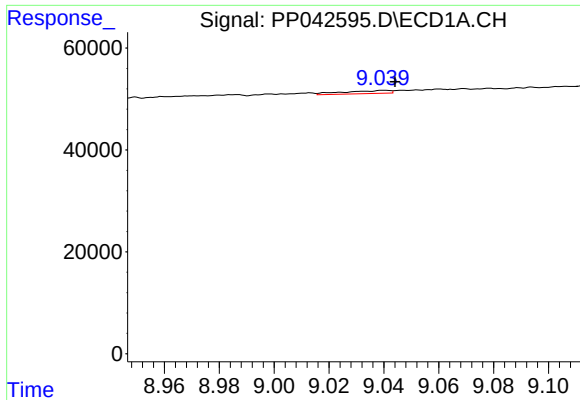

#35 AR-1260-5


R.T.: 9.039 min
Delta R.T.: -0.005 min
Response: 7007
Conc: 5.81 ng/ml

Instrument :
ECD_P
ClientSampleId :

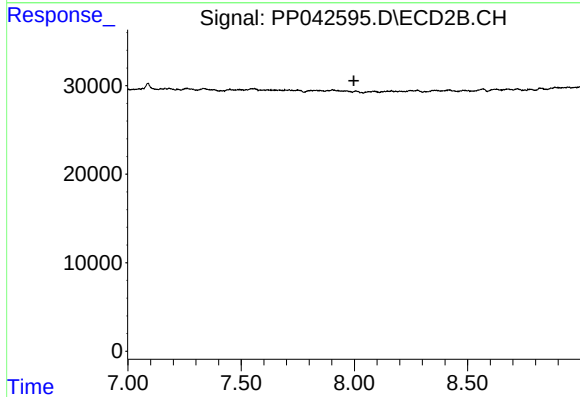


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.998 min
Response: 0
Conc: N.D.

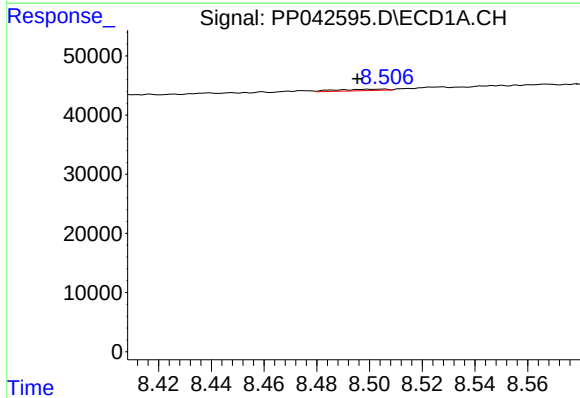


#36 AR-1262-1

R.T.: 8.506 min
Delta R.T.: 0.010 min
Response: 3198
Conc: 4.09 ng/ml

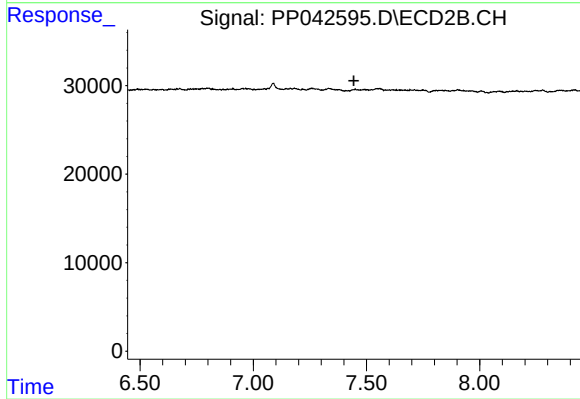

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 7.444 min
Response: 0
Conc: N.D.

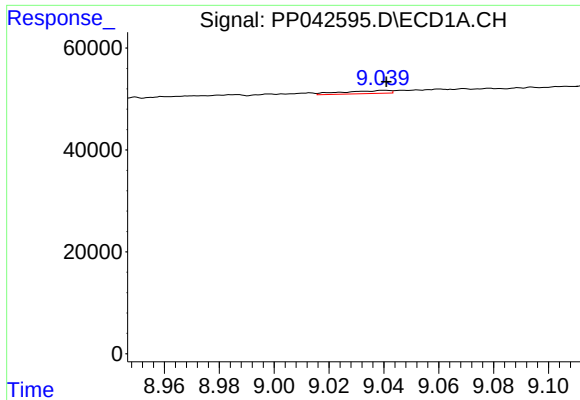

#37 AR-1262-2


R.T.: 9.039 min
Delta R.T.: -0.002 min
Response: 7007
Conc: 5.24 ng/ml

Instrument :
ECD_P
ClientSampleId :

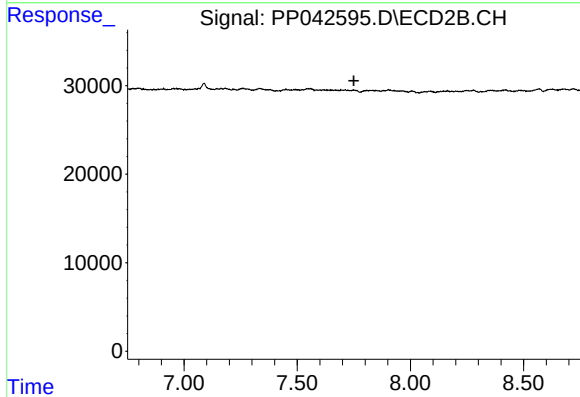


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.750 min
Response: 0
Conc: N.D.

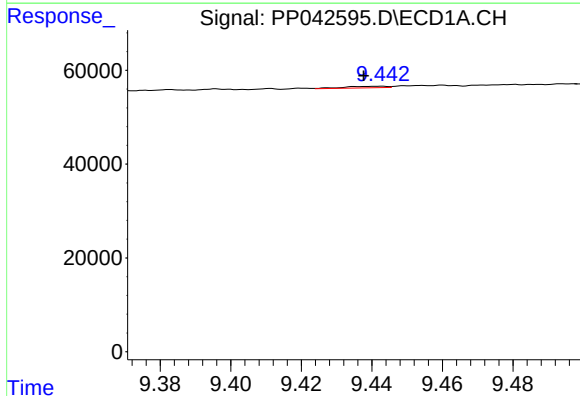


#39 AR-1262-4

R.T.: 9.443 min
Delta R.T.: 0.005 min
Response: 2813
Conc: 5.82 ng/ml

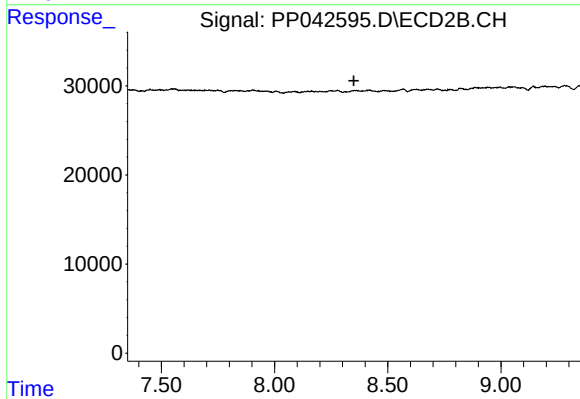

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.350 min
Response: 0
Conc: N.D.

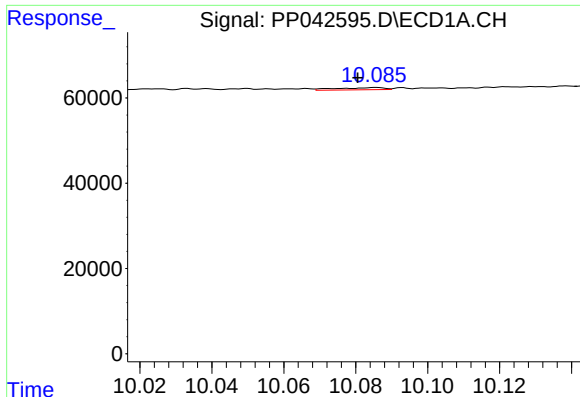

#40 AR-1262-5


R.T.: 10.086 min
Delta R.T.: 0.005 min
Response: 4783
Conc: 9.80 ng/ml

Instrument :
ECD_P
ClientSampleId :

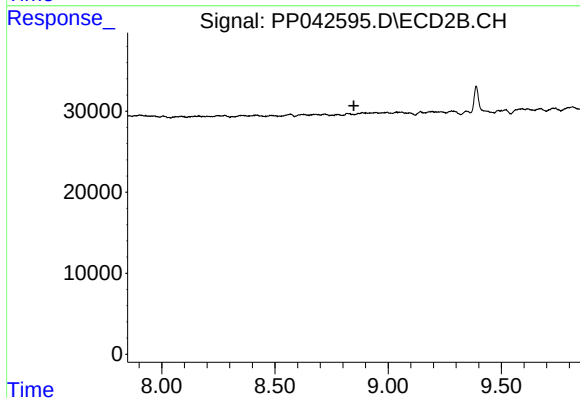


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 8.849 min
Response: 0
Conc: N.D.

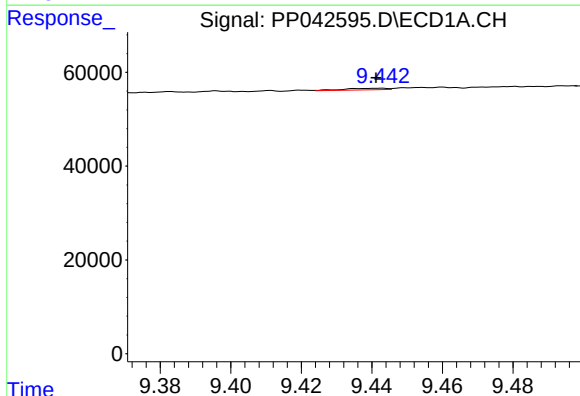


#42 AR-1268-2

R.T.: 9.443 min
Delta R.T.: 0.002 min
Response: 2813
Conc: 1.86 ng/ml

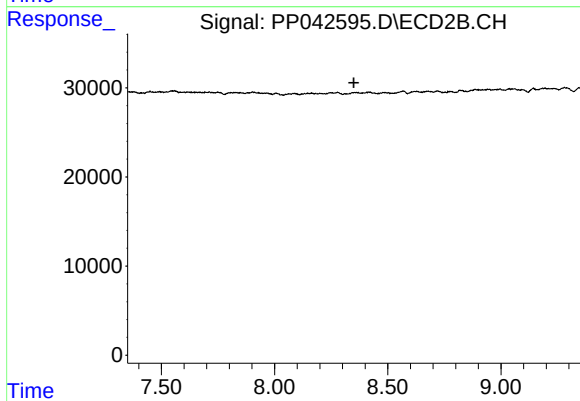

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.351 min
Response: 0
Conc: N.D.

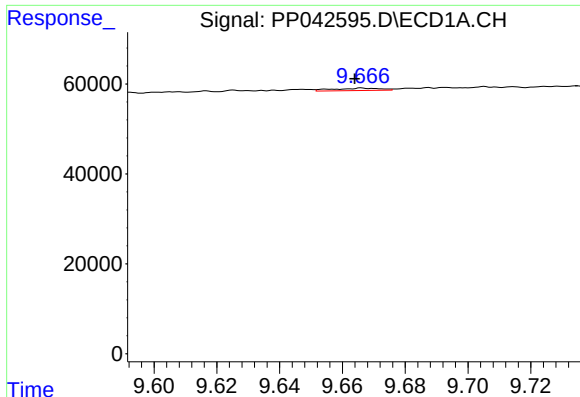

#43 AR-1268-3


R.T.: 9.666 min
Delta R.T.: 0.002 min
Response: 5362
Conc: 3.98 ng/ml

Instrument :
ECD_P
ClientSampleId :

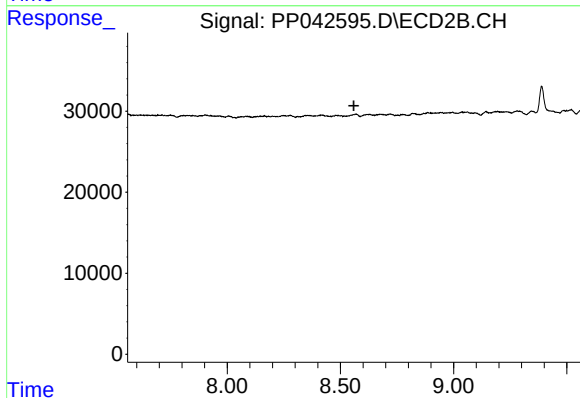


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.560 min
Response: 0
Conc: N.D.

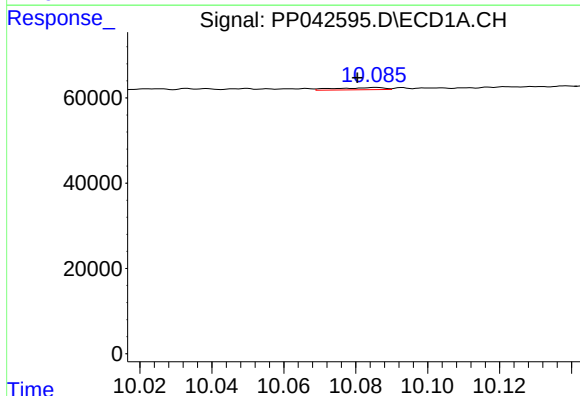


#44 AR-1268-4

R.T.: 10.086 min
Delta R.T.: 0.005 min
Response: 4783
Conc: 8.74 ng/ml

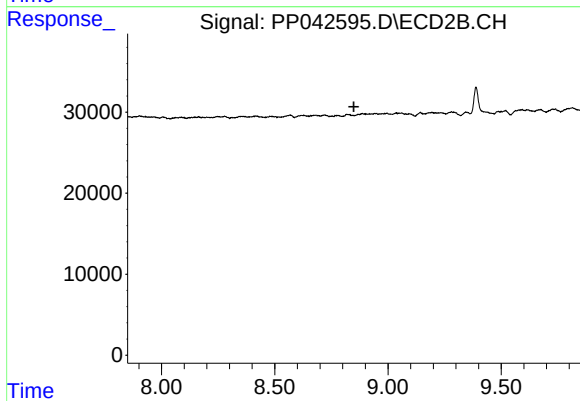

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 8.849 min
Response: 0
Conc: N.D.

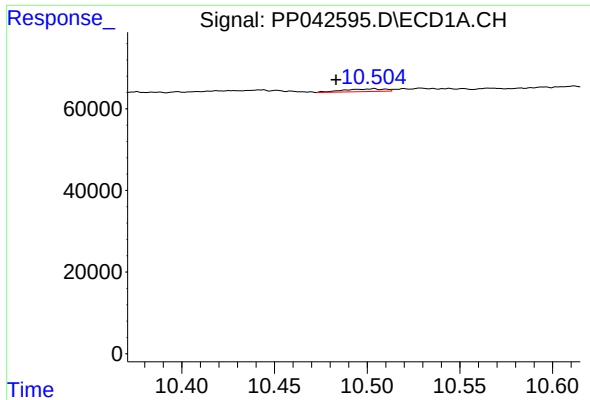

#45 AR-1268-5

R.T.: 10.503 min
Delta R.T.: 0.020 min
Response: 10151
Conc: 2.27 ng/ml

Instrument :
ECD_P
ClientSampleId :

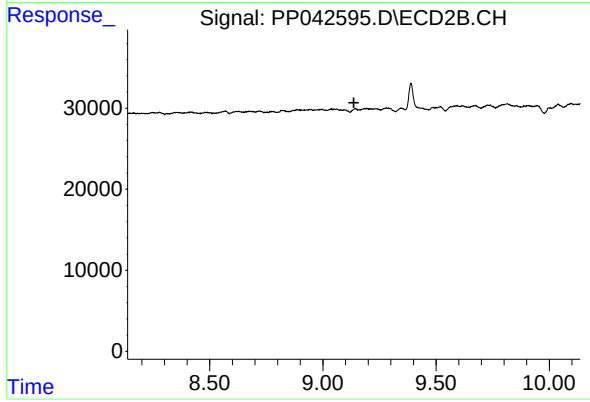

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.137 min
Response: 0
Conc: N.D.