

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010522\
 Data File : PP042598.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jan 2022 7:51
 Operator : AJ\MA
 Sample : N1013-16 10X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 06 13:50:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 05 12:01:35 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.878	4.047	29417	46101	1.518	1.761
2)	SA Decachlor...	10.814	9.389	22772	33908	1.941	1.725
Target Compounds							
29)	L6 AR-1254-4	7.990	0.000	12466	0	20.812	N.D. #
30)	L6 AR-1254-5	8.418	0.000	975	0	1.541	N.D. #
33)	L7 AR-1260-3	8.493	0.000	5211	0	9.406	N.D. #
34)	L7 AR-1260-4	8.723	0.000	3948	0	5.984	N.D. #
35)	L7 AR-1260-5	9.017f	0.000	1803	0	1.495	N.D. #
36)	L8 AR-1262-1	8.493	0.000	5211	0	6.656	N.D. #
37)	L8 AR-1262-2	9.017f	0.000	1803	0	1.349	N.D. #
38)	L8 AR-1262-3	9.362	0.000	1026	0	1.557	N.D. #
39)	L8 AR-1262-4	9.438	0.000	1416	0	2.930	N.D. #
40)	L8 AR-1262-5	10.074	0.000	2953	0	6.053	N.D. #
41)	L9 AR-1268-1	9.362	0.000	1026	0	0.627	N.D. #
42)	L9 AR-1268-2	9.444	0.000	362	0	0.239	N.D. #
43)	L9 AR-1268-3	9.669	0.000	3708	0	2.755	N.D. #
44)	L9 AR-1268-4	10.074	0.000	2953	0	5.395	N.D. #
45)	L9 AR-1268-5	10.481	0.000	1019	0	0.228	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010522\
Data File : PP042598.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jan 2022 7:51
Operator : AJ\MA
Sample : N1013-16 10X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 06 13:50:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 05 12:01:35 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

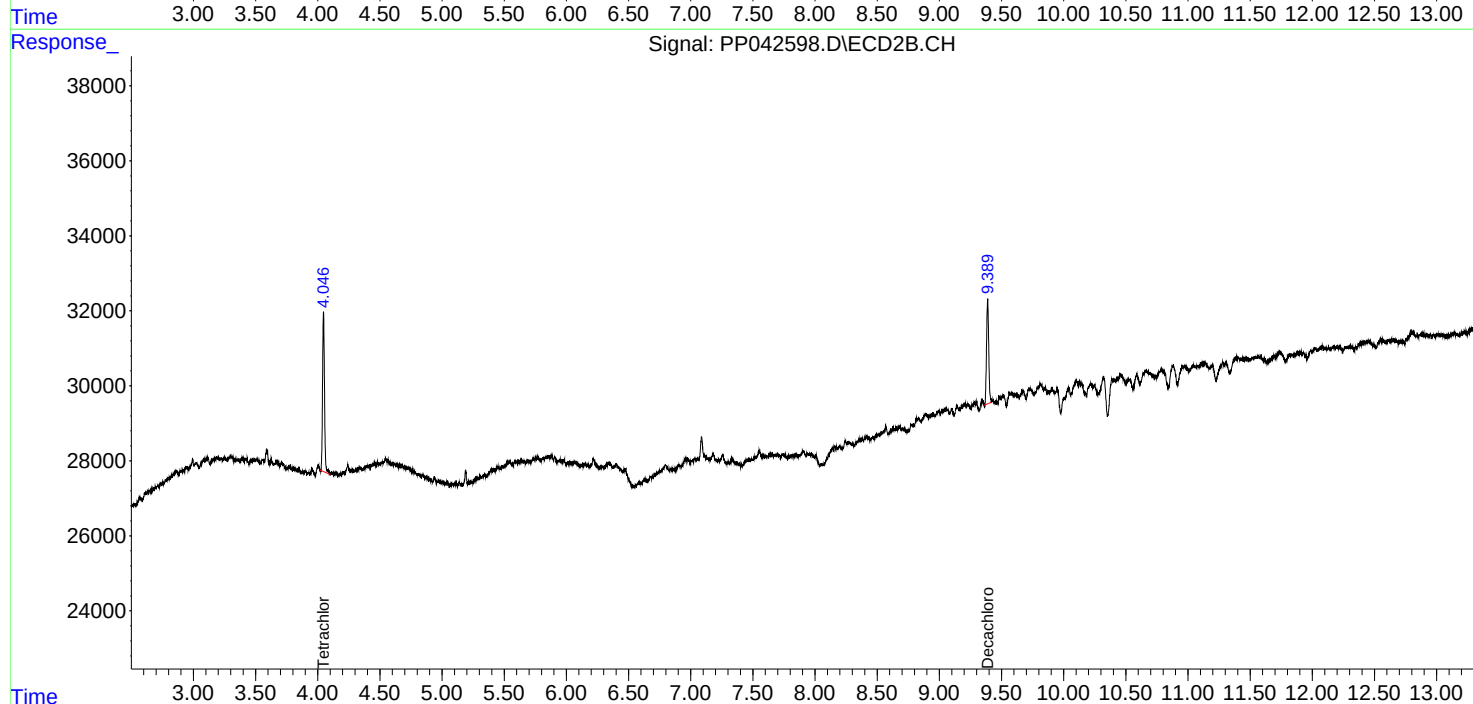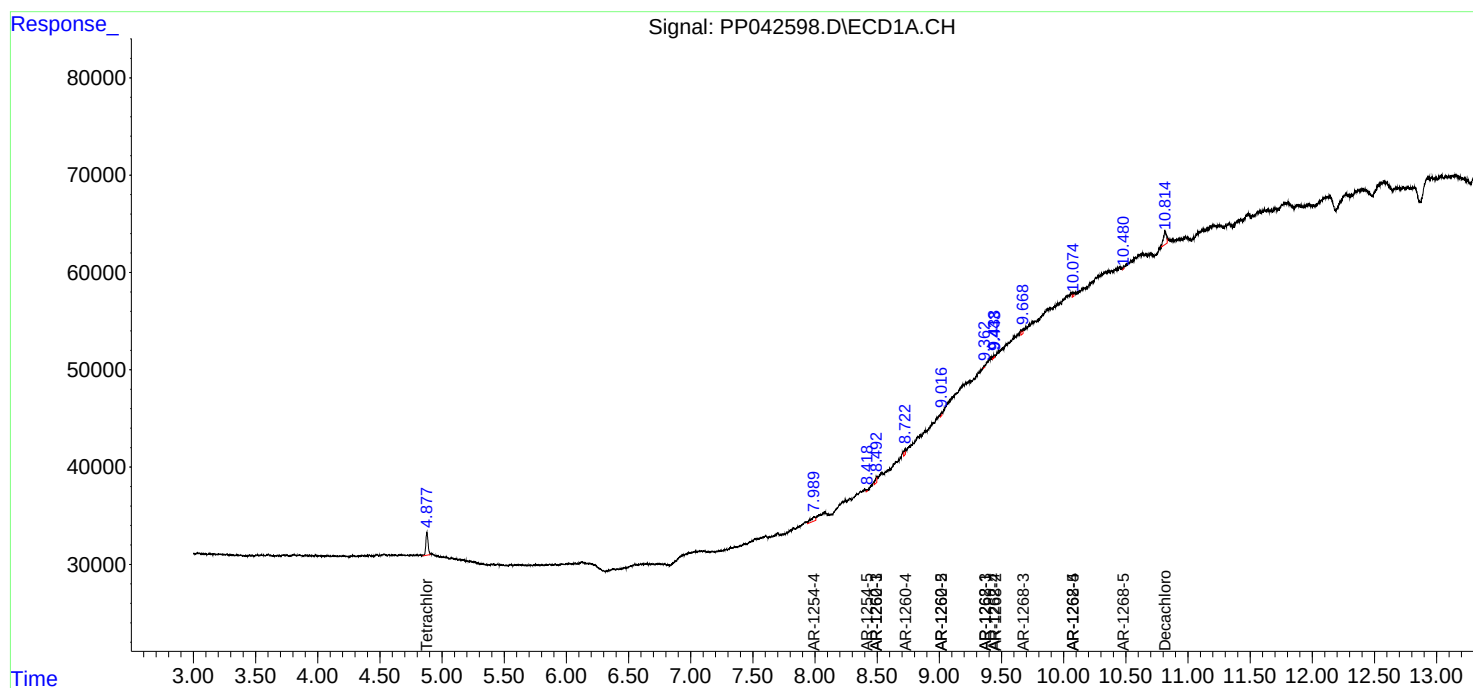


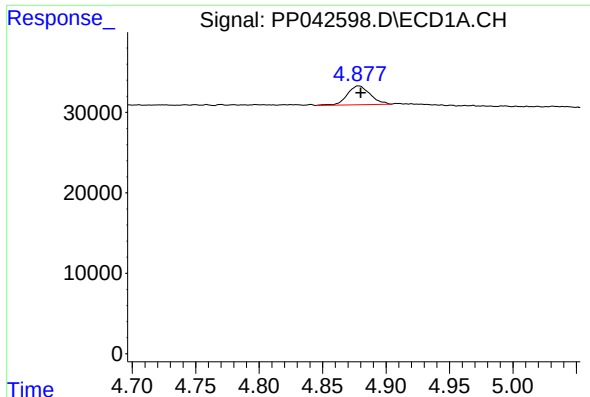

#1 Tetrachloro-m-xylene


R.T.: 4.878 min
Delta R.T.: -0.002 min
Response: 29417
Conc: 1.52 ng/ml

Instrument :
ECD_P
ClientSampleId :

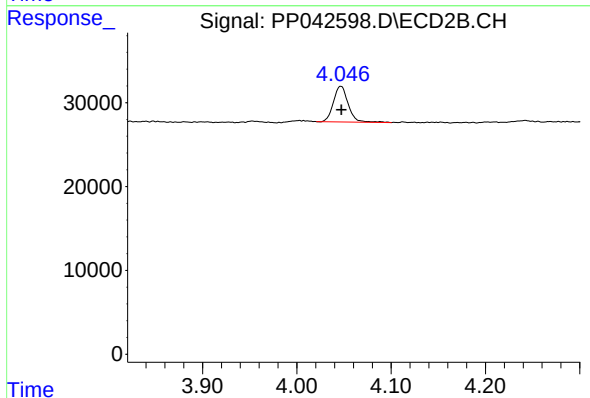


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 46101
Conc: 1.76 ng/ml

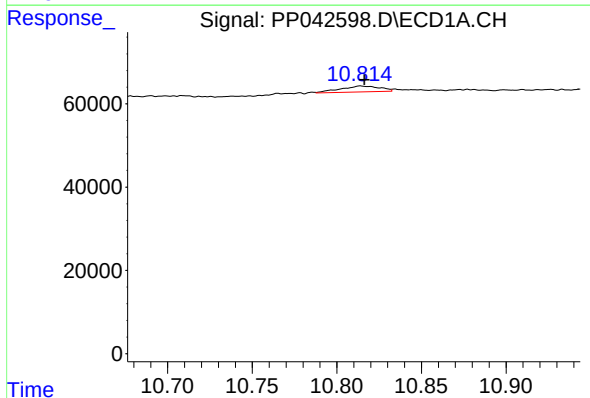


#2 Decachlorobiphenyl

R.T.: 10.814 min
Delta R.T.: -0.002 min
Response: 22772
Conc: 1.94 ng/ml

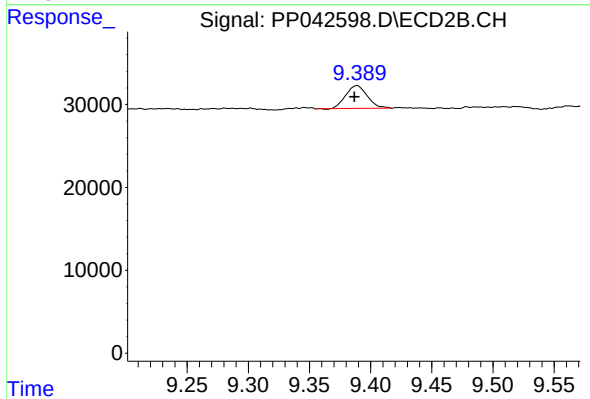

#2 Decachlorobiphenyl


R.T.: 9.389 min
Delta R.T.: 0.002 min
Response: 33908
Conc: 1.73 ng/ml

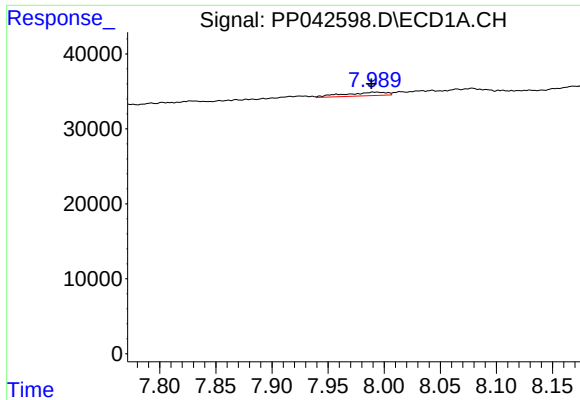

#29 AR-1254-4


R.T.: 7.990 min
Delta R.T.: 0.000 min
Response: 12466
Conc: 20.81 ng/ml

Instrument :
ECD_P
ClientSampleId :

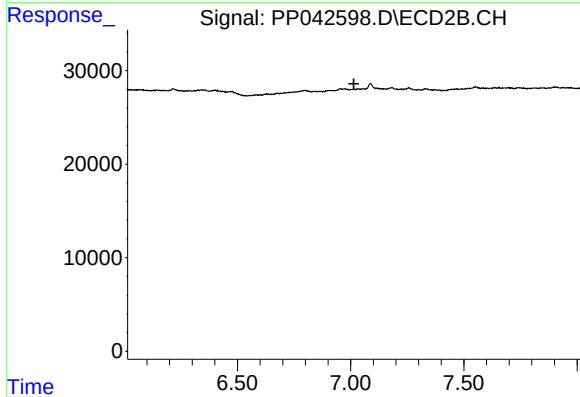


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.014 min
Response: 0
Conc: N.D.

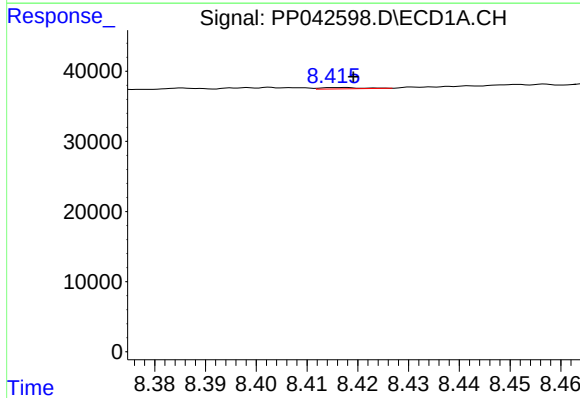


#30 AR-1254-5

R.T.: 8.418 min
Delta R.T.: -0.002 min
Response: 975
Conc: 1.54 ng/ml

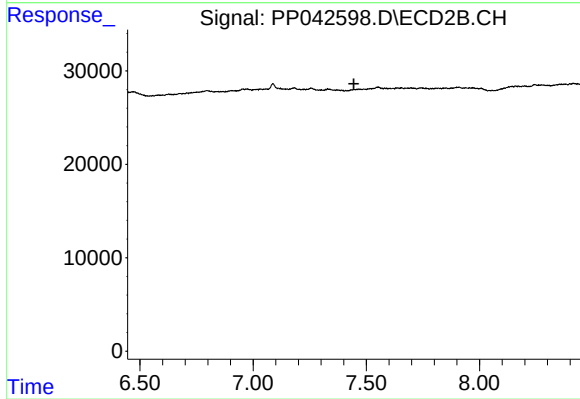

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.445 min
Response: 0
Conc: N.D.

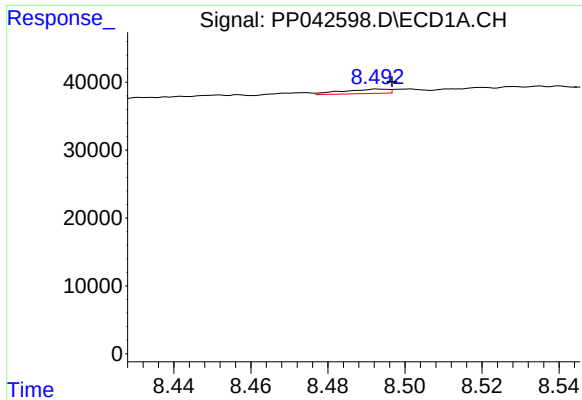

#33 AR-1260-3


R.T.: 8.493 min
Delta R.T.: -0.004 min
Response: 5211
Conc: 9.41 ng/ml

Instrument :
ECD_P
ClientSampleId :

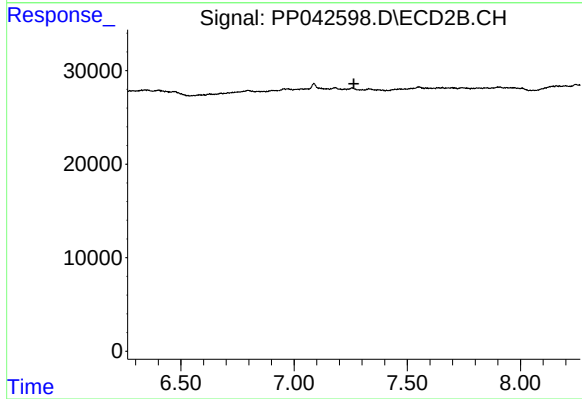


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.264 min
Response: 0
Conc: N.D.

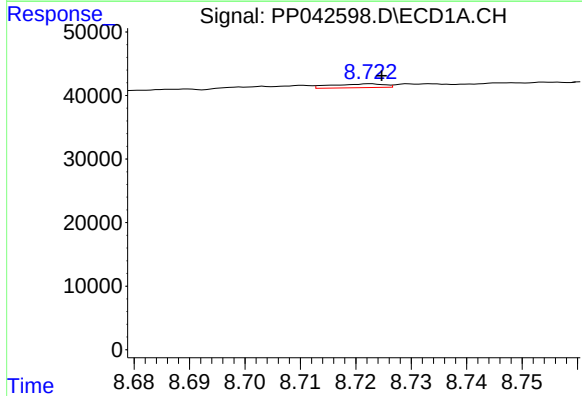


#34 AR-1260-4

R.T.: 8.723 min
Delta R.T.: -0.002 min
Response: 3948
Conc: 5.98 ng/ml

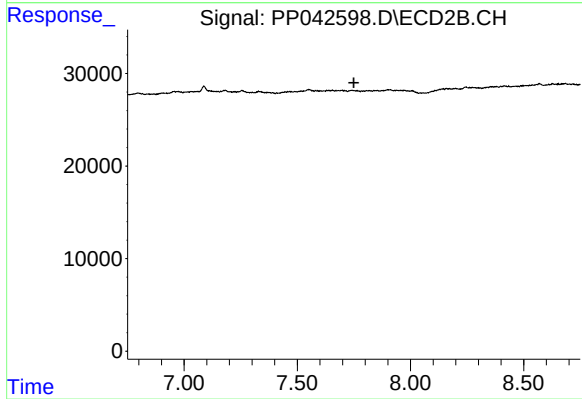

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.750 min
Response: 0
Conc: N.D.

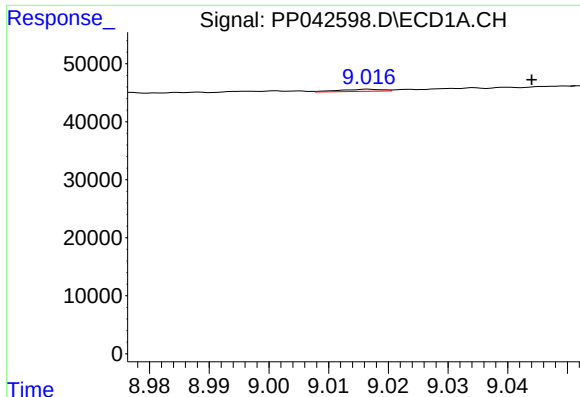

#35 AR-1260-5


R.T.: 9.017 min
Delta R.T.: -0.027 min
Response: 1803
Conc: 1.50 ng/ml

Instrument :
ECD_P
ClientSampleId :

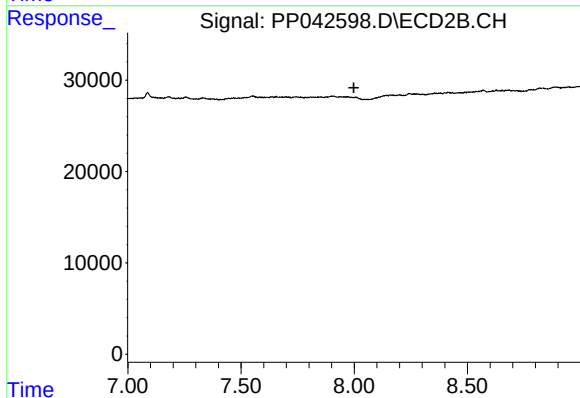


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.998 min
Response: 0
Conc: N.D.

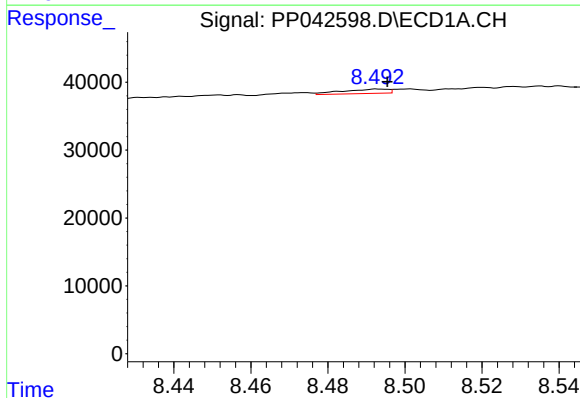


#36 AR-1262-1

R.T.: 8.493 min
Delta R.T.: -0.003 min
Response: 5211
Conc: 6.66 ng/ml

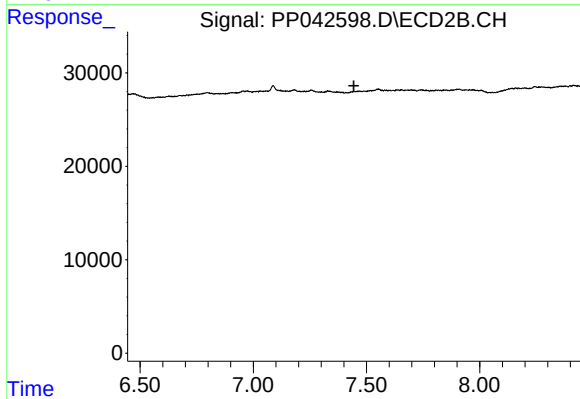

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 7.444 min
Response: 0
Conc: N.D.

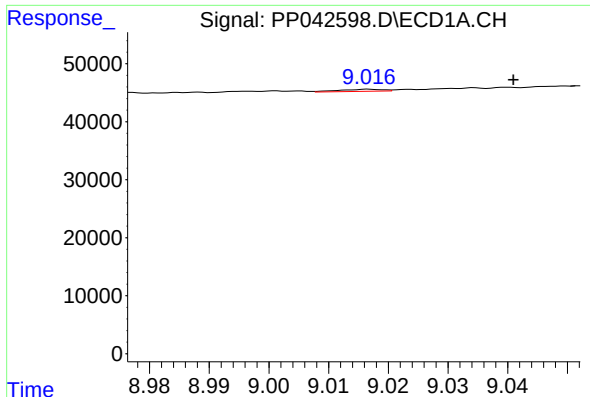

#37 AR-1262-2


R.T.: 9.017 min
Delta R.T.: -0.024 min
Response: 1803
Conc: 1.35 ng/ml

Instrument :
ECD_P
ClientSampleId :

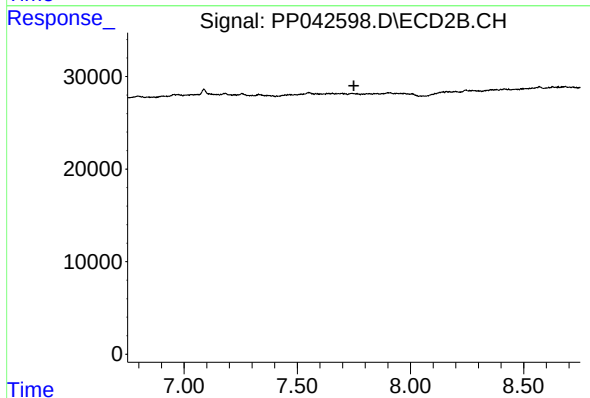


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.750 min
Response: 0
Conc: N.D.

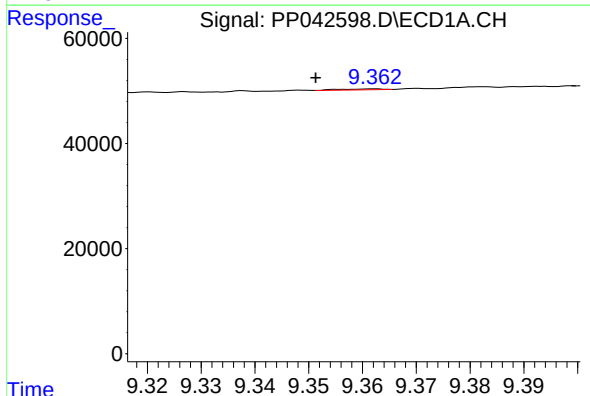


#38 AR-1262-3

R.T.: 9.362 min
Delta R.T.: 0.011 min
Response: 1026
Conc: 1.56 ng/ml

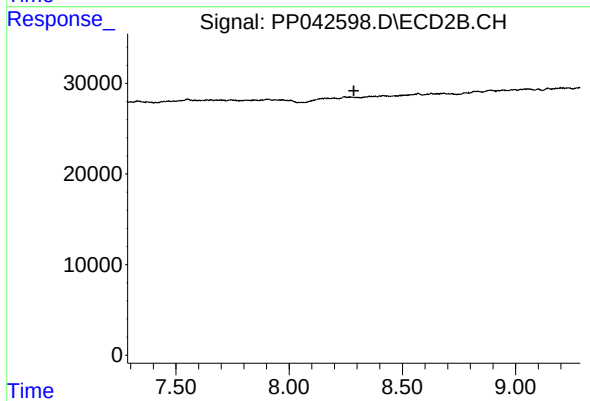

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 8.286 min
Response: 0
Conc: N.D.

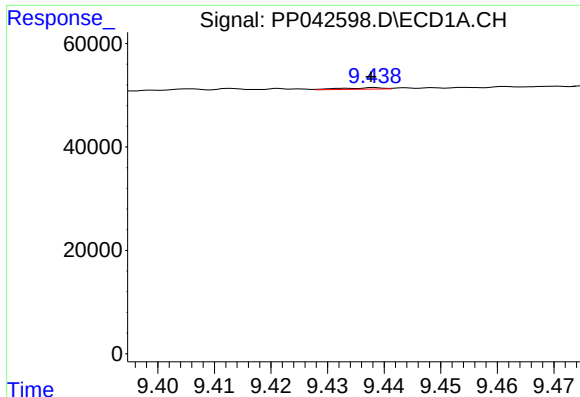

#39 AR-1262-4


R.T.: 9.438 min
Delta R.T.: 0.000 min
Response: 1416
Conc: 2.93 ng/ml

Instrument :
ECD_P
ClientSampleId :

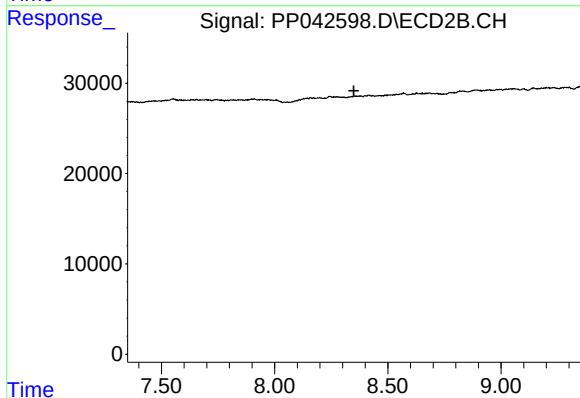


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.350 min
Response: 0
Conc: N.D.

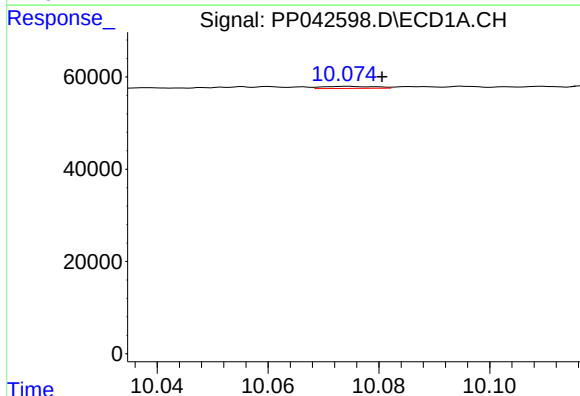


#40 AR-1262-5

R.T.: 10.074 min
Delta R.T.: -0.006 min
Response: 2953
Conc: 6.05 ng/ml

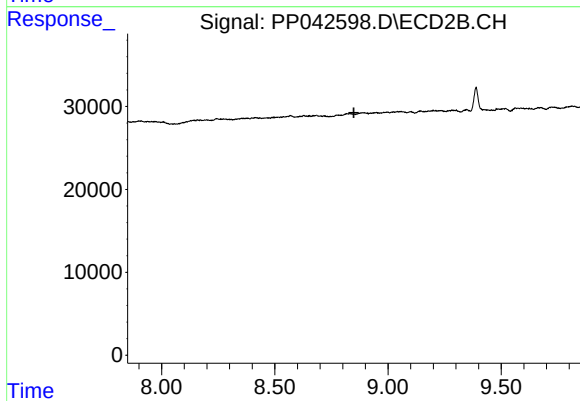

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 8.849 min
Response: 0
Conc: N.D.

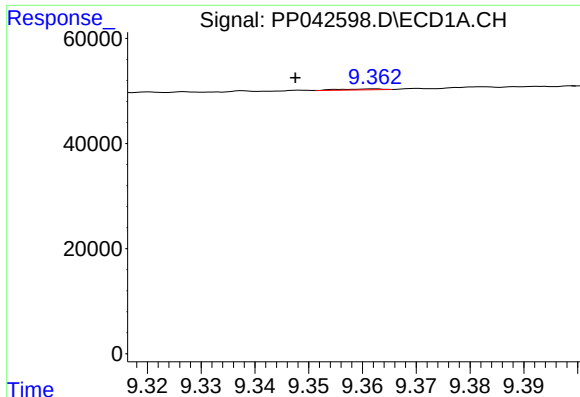

#41 AR-1268-1


R.T.: 9.362 min
Delta R.T.: 0.015 min
Response: 1026
Conc: 0.63 ng/ml

Instrument :
ECD_P
ClientSampleId :

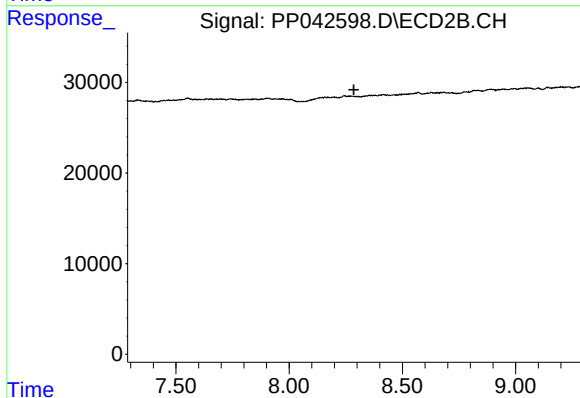


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.286 min
Response: 0
Conc: N.D.

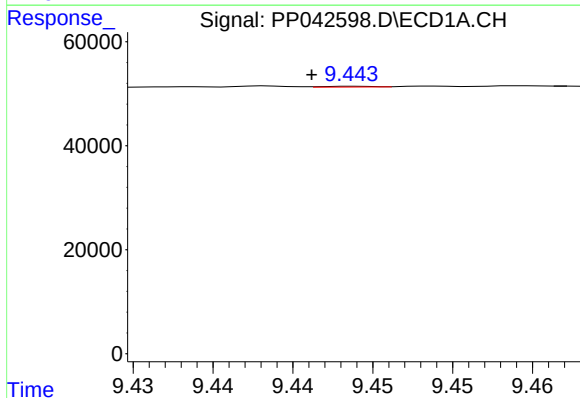


#42 AR-1268-2

R.T.: 9.444 min
Delta R.T.: 0.003 min
Response: 362
Conc: 0.24 ng/ml

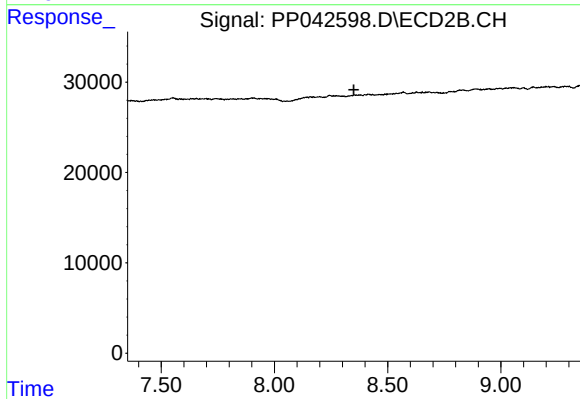

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.351 min
Response: 0
Conc: N.D.

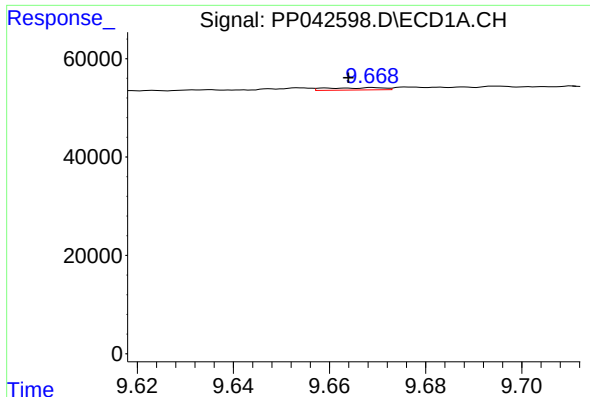

#43 AR-1268-3


R.T.: 9.669 min
Delta R.T.: 0.005 min
Response: 3708
Conc: 2.75 ng/ml

Instrument :
ECD_P
ClientSampleId :

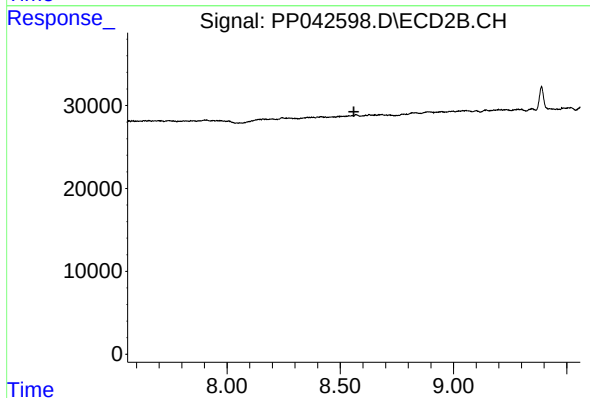


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.560 min
Response: 0
Conc: N.D.

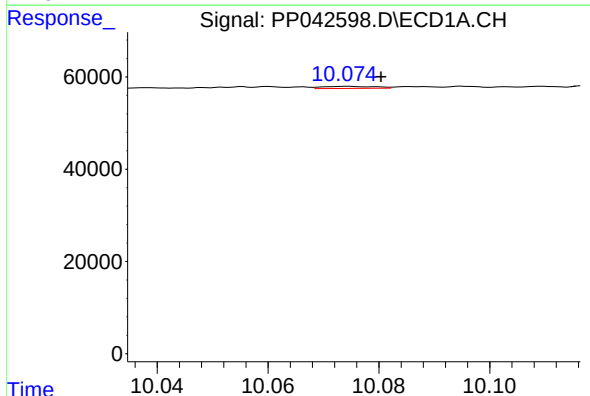


#44 AR-1268-4

R.T.: 10.074 min
Delta R.T.: -0.006 min
Response: 2953
Conc: 5.39 ng/ml

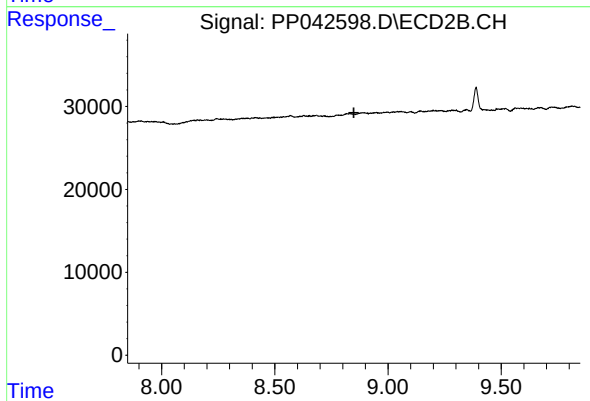

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 8.849 min
Response: 0
Conc: N.D.

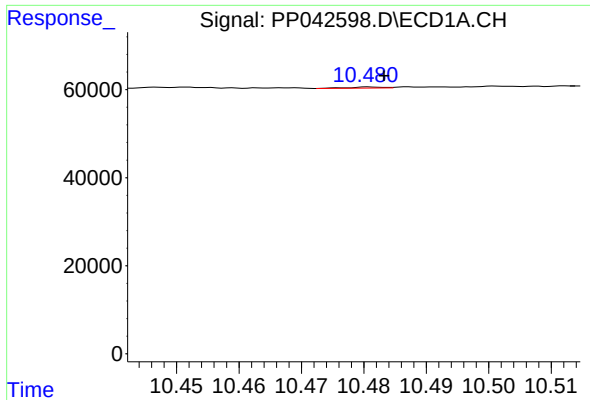

#45 AR-1268-5

R.T.: 10.481 min
Delta R.T.: -0.002 min
Response: 1019
Conc: 0.23 ng/ml

Instrument :
ECD_P
ClientSampleId :

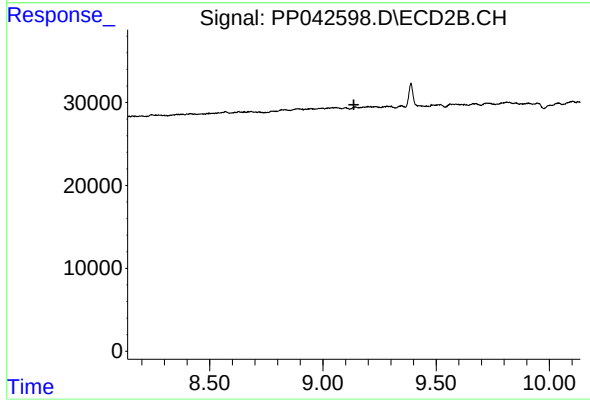

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.137 min
Response: 0
Conc: N.D.