

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010522\
 Data File : PP042544.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jan 2022 15:29
 Operator : AJ\MA
 Sample : M5334-07 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SEC-2021-79-B

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/06/2022
 Supervised By :mohammad ahmed 01/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 16:13:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 05 12:01:35 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.881	4.048	29930	48475	1.545	1.852
2) SA Decachlor...	10.817	9.389	28936	41629	2.466m	2.118m
Target Compounds						
26) L6 AR-1254-1	7.091	6.193	28267	67590	46.400	43.894
27) L6 AR-1254-2	7.320	6.352	43890	67533	47.793	50.245
28) L6 AR-1254-3	7.698	6.776	48923	94237	53.405	45.119
29) L6 AR-1254-4	7.993	7.015	27860	50121	46.513	40.954
30) L6 AR-1254-5	8.421	7.447	28541	66014	45.143	40.193

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010522\
Data File : PP042544.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jan 2022 15:29
Operator : AJ\MA
Sample : M5334-07 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SEC-2021-79-B


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/06/2022
Supervised By :mohammad ahmed 01/06/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 16:13:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 05 12:01:35 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

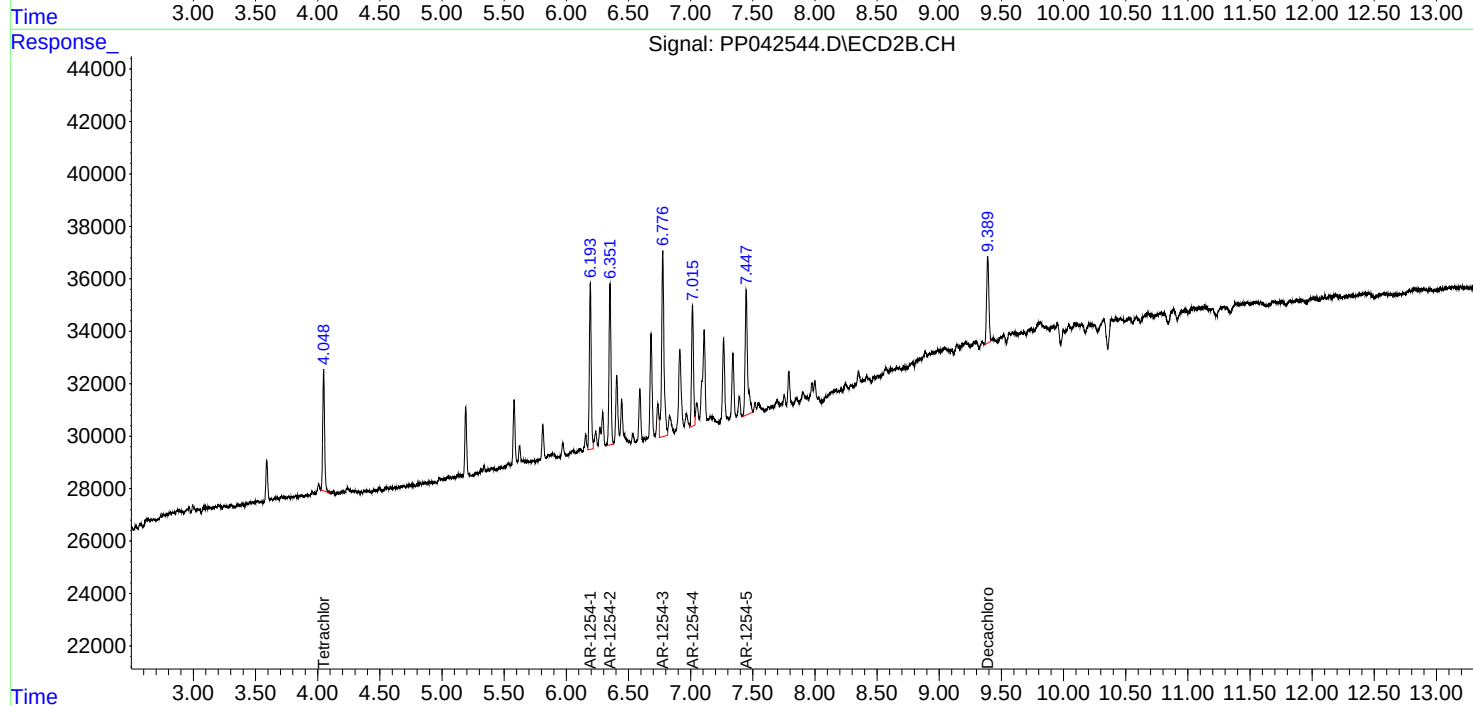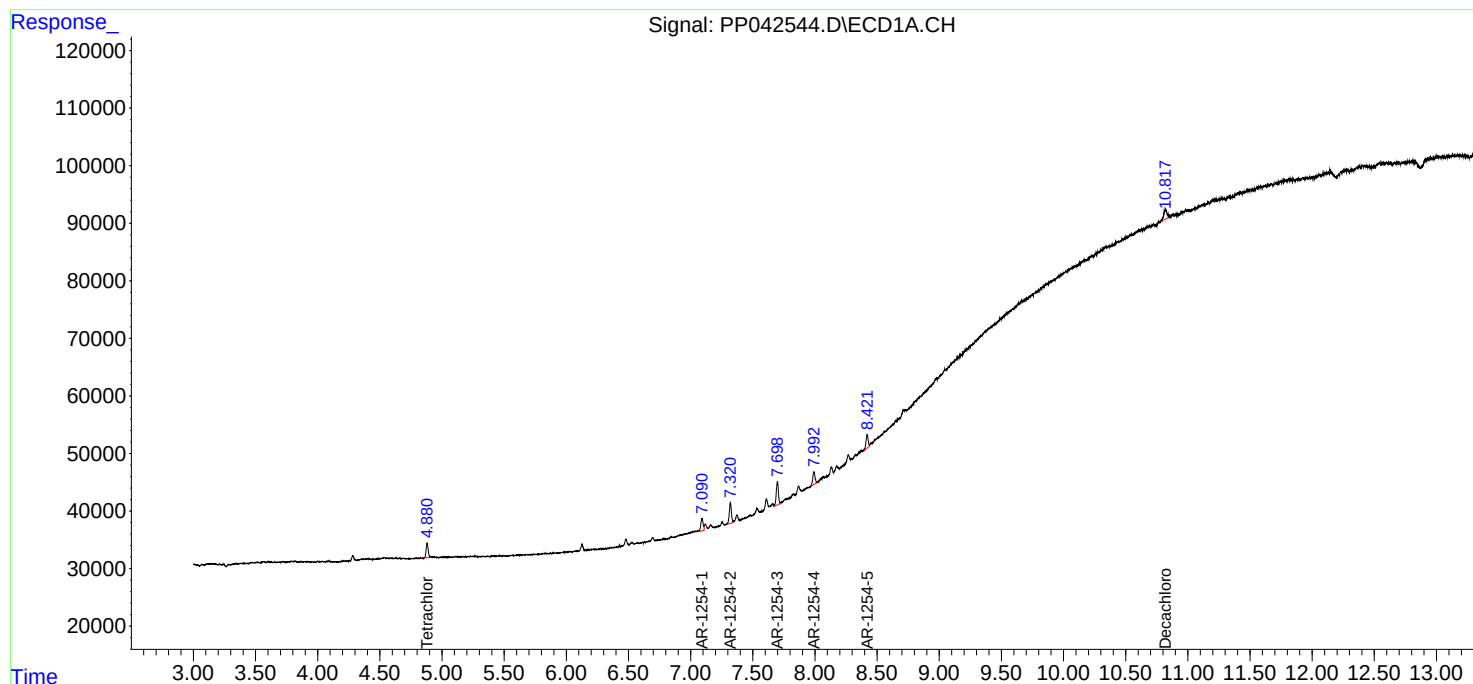

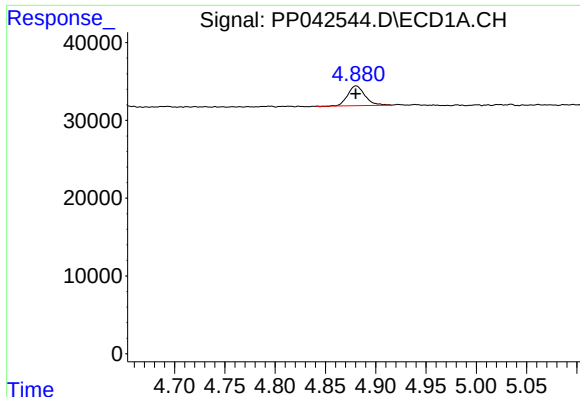


#1 Tetrachloro-m-xylene

R.T.: 4.881 min
Delta R.T.: 0.000 min
Response: 29930
Conc: 1.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
SEC-2021-79-B


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/06/2022
Supervised By :mohammad ahmed 01/06/2022

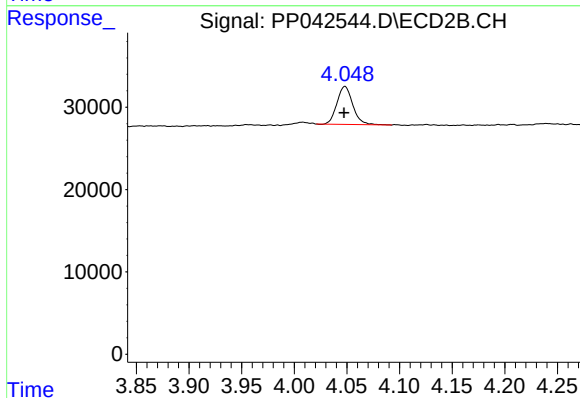


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.000 min
Response: 48475
Conc: 1.85 ng/ml

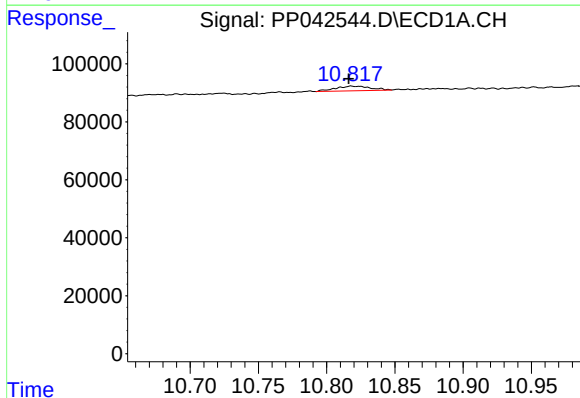


#2 Decachlorobiphenyl

R.T.: 10.817 min
Delta R.T.: 0.001 min
Response: 28936
Conc: 2.47 ng/ml m

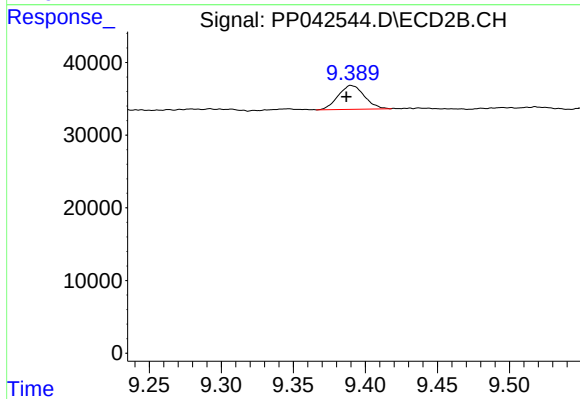

#2 Decachlorobiphenyl

R.T.: 9.389 min
Delta R.T.: 0.003 min
Response: 41629
Conc: 2.12 ng/ml m

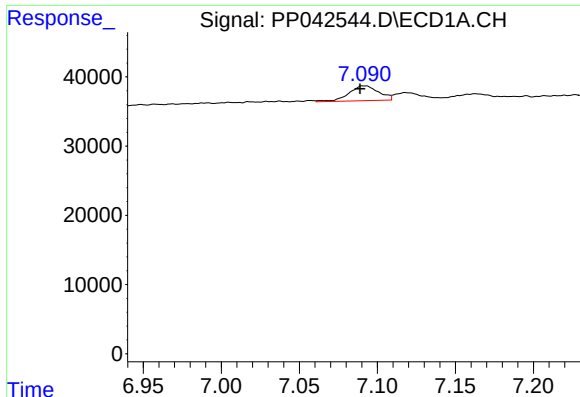


#26 AR-1254-1

R.T.: 7.091 min
Delta R.T.: 0.002 min
Response: 28267
Conc: 46.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
SEC-2021-79-B


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/06/2022
Supervised By :mohammad ahmed 01/06/2022

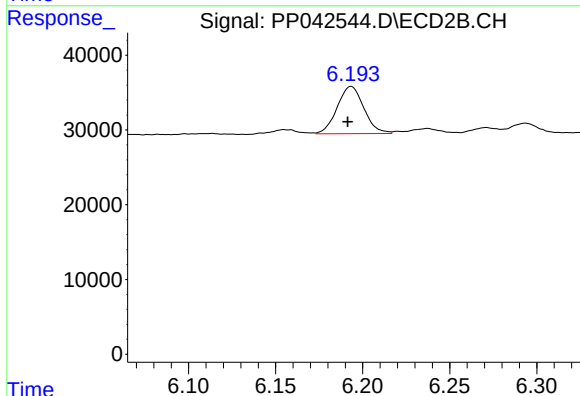


#26 AR-1254-1

R.T.: 6.193 min
Delta R.T.: 0.002 min
Response: 67590
Conc: 43.89 ng/ml

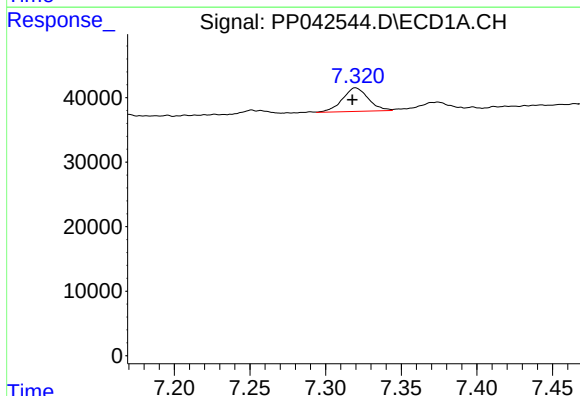


#27 AR-1254-2

R.T.: 7.320 min
Delta R.T.: 0.002 min
Response: 43890
Conc: 47.79 ng/ml

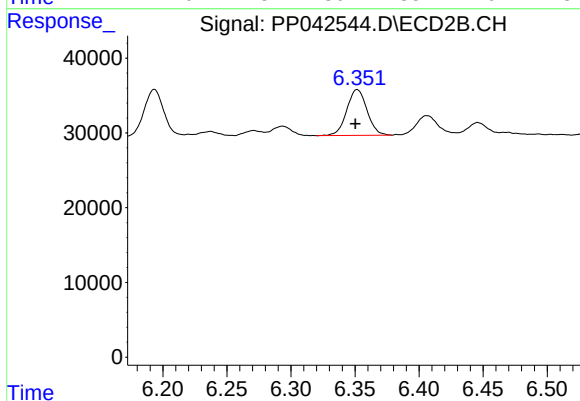

#27 AR-1254-2

R.T.: 6.352 min
Delta R.T.: 0.001 min
Response: 67533
Conc: 50.25 ng/ml

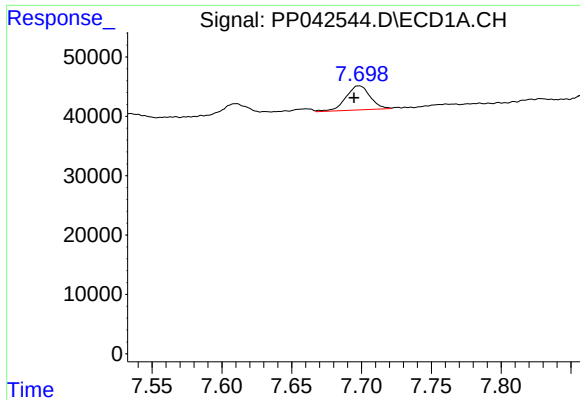


#28 AR-1254-3

R.T.: 7.698 min
Delta R.T.: 0.003 min
Response: 48923
Conc: 53.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
SEC-2021-79-B


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/06/2022
Supervised By :mohammad ahmed 01/06/2022

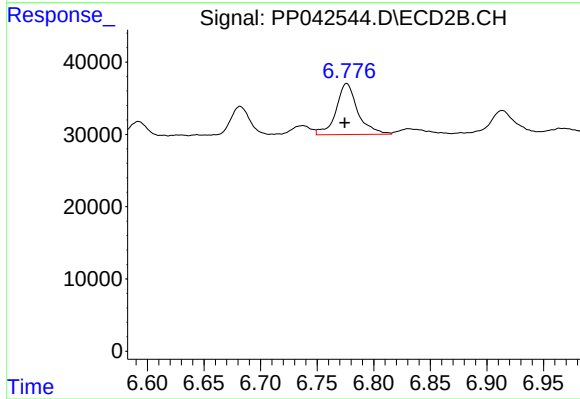


#28 AR-1254-3

R.T.: 6.776 min
Delta R.T.: 0.002 min
Response: 94237
Conc: 45.12 ng/ml

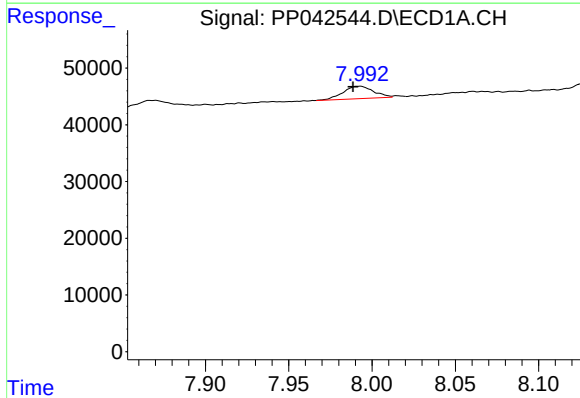


#29 AR-1254-4

R.T.: 7.993 min
Delta R.T.: 0.004 min
Response: 27860
Conc: 46.51 ng/ml

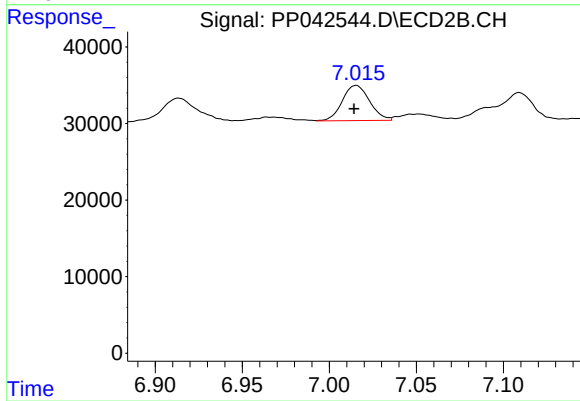

#29 AR-1254-4

R.T.: 7.015 min
Delta R.T.: 0.001 min
Response: 50121
Conc: 40.95 ng/ml

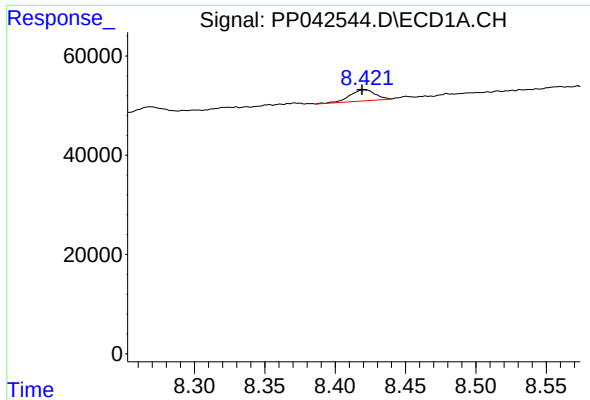


#30 AR-1254-5

R.T.: 8.421 min
Delta R.T.: 0.002 min
Response: 28541
Conc: 45.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
SEC-2021-79-B

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/06/2022
Supervised By :mohammad ahmed 01/06/2022

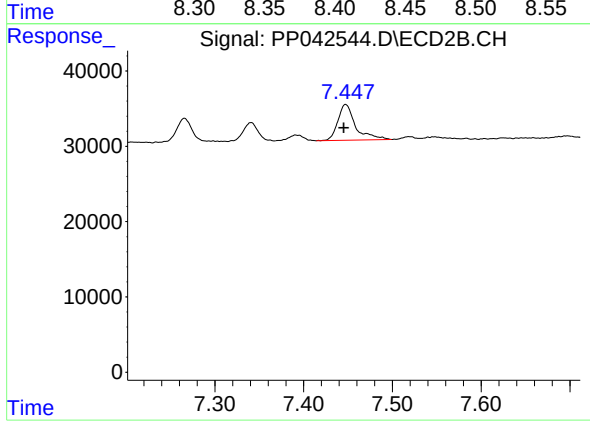

#30 AR-1254-5

R.T.: 7.447 min
Delta R.T.: 0.002 min
Response: 66014
Conc: 40.19 ng/ml