

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010523\
 Data File : PP054284.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2023 10:09
 Operator : YP\AJ
 Sample : 01012-02 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-12322-103-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 11:05:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 05 03:46:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.337	3.585	2426196	1648285	1.198	1.022
2) SA Decachlor...	10.098	8.610	2276121	1956340	1.585	1.387

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010523\
Data File : PP054284.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2023 10:09
Operator : YP\AJ
Sample : 01012-02 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PCB-12322-103-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 11:05:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010423.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 05 03:46:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

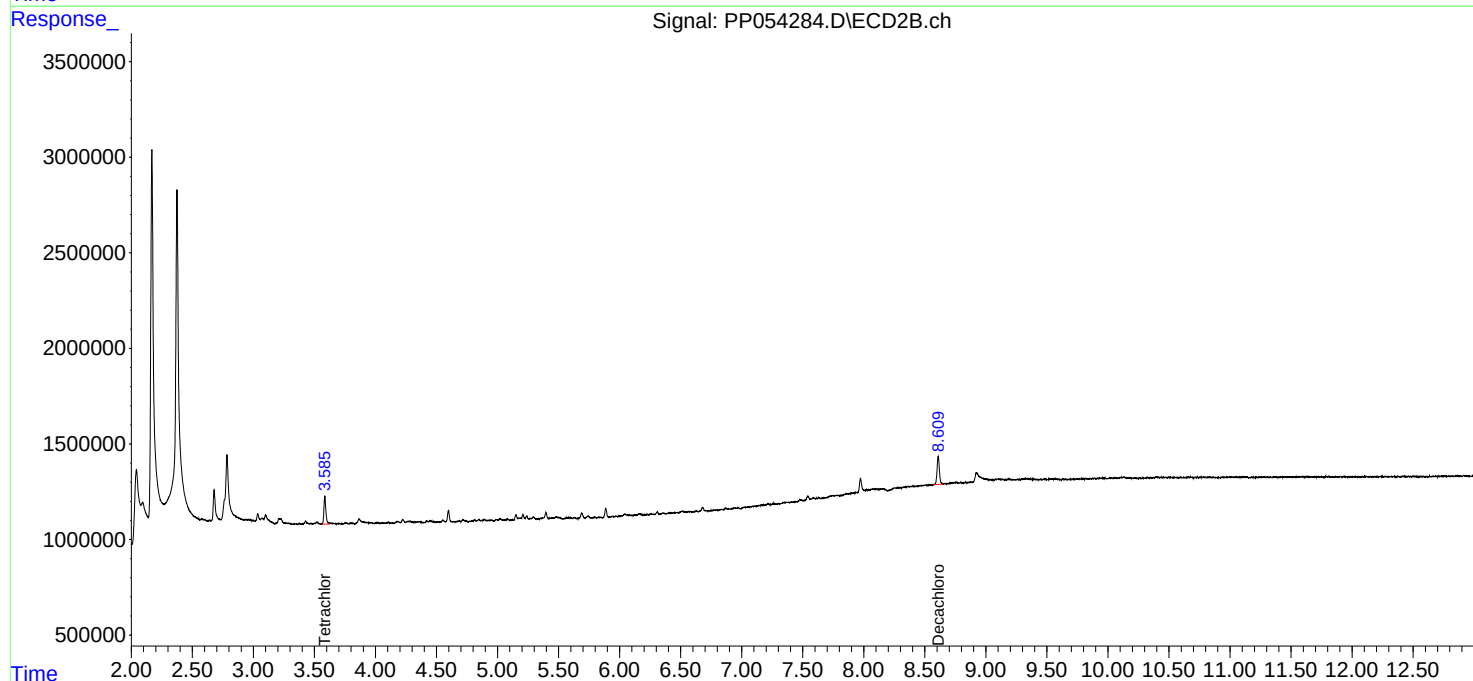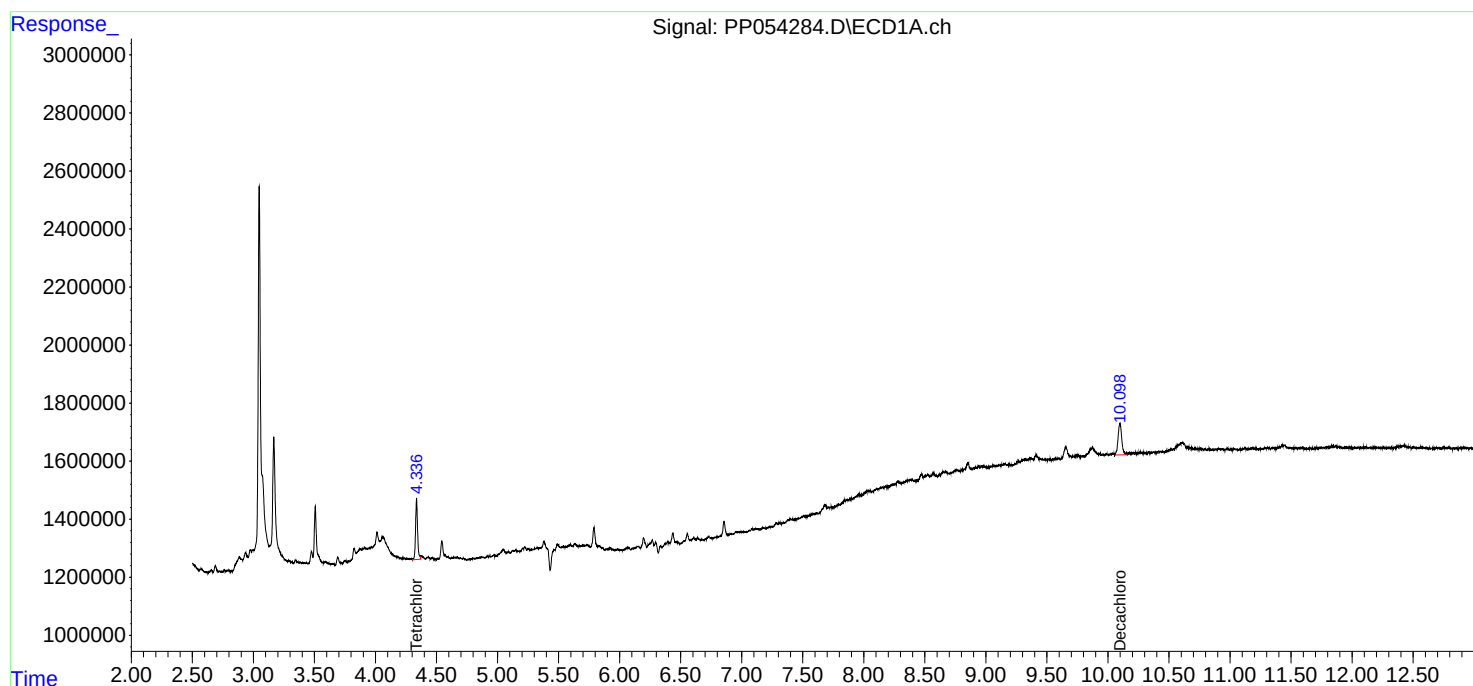


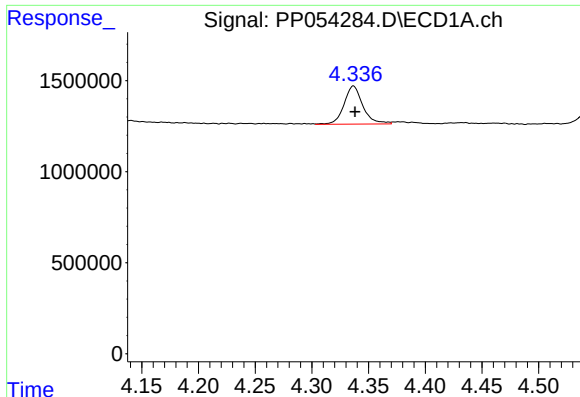

#1 Tetrachloro-m-xylene


R.T.: 4.337 min
Delta R.T.: -0.001 min
Response: 2426196
Conc: 1.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-12322-103-02

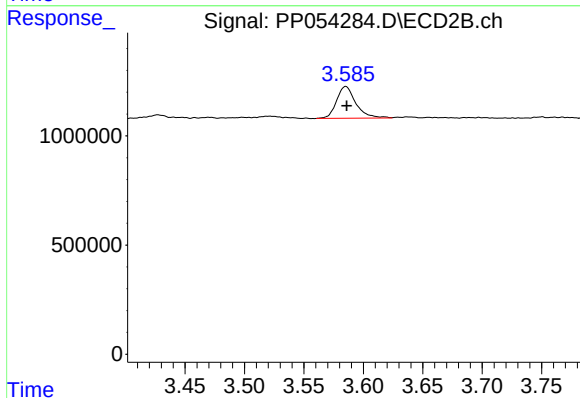


#1 Tetrachloro-m-xylene

R.T.: 3.585 min
Delta R.T.: 0.000 min
Response: 1648285
Conc: 1.02 ng/ml

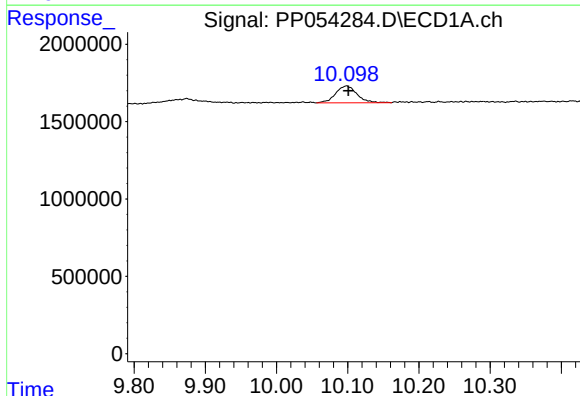

#2 Decachlorobiphenyl

R.T.: 10.098 min
Delta R.T.: -0.003 min
Response: 2276121
Conc: 1.58 ng/ml

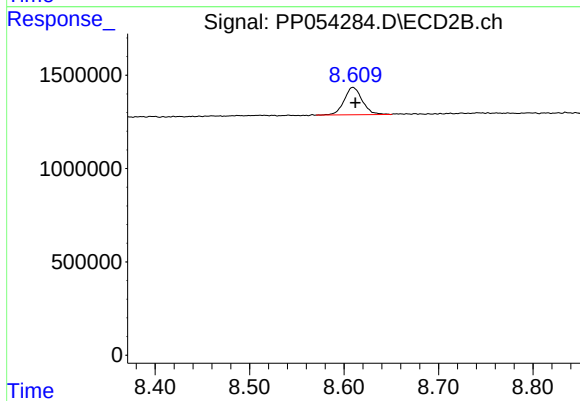

#2 Decachlorobiphenyl

R.T.: 8.610 min
Delta R.T.: -0.002 min
Response: 1956340
Conc: 1.39 ng/ml