

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010523\
 Data File : PP054303.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jan 2023 02:50
 Operator : YP\AJ
 Sample : 01011-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 NWB-1865

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/06/2023
 Supervised By :Ankita Jodhani 01/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 06 03:50:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 05 03:46:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.337	3.587	31191223	21457084	15.403	13.303m
2) SA Decachlor...	10.095	8.609	9936351	9970676	6.919m	7.068m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010523\
Data File : PP054303.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jan 2023 02:50
Operator : YP\AJ
Sample : 01011-01
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
NWB-1865


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/06/2023
Supervised By :Ankita Jodhani 01/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 06 03:50:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010423.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 05 03:46:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

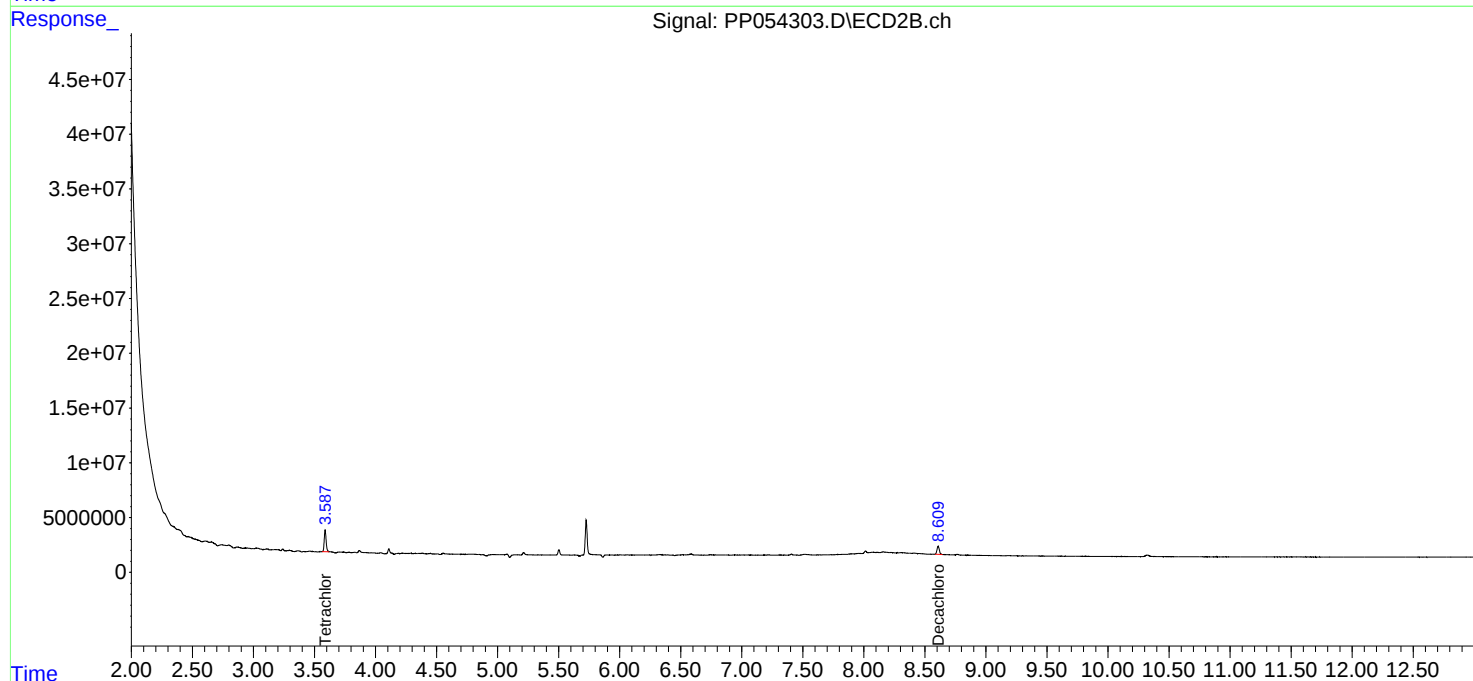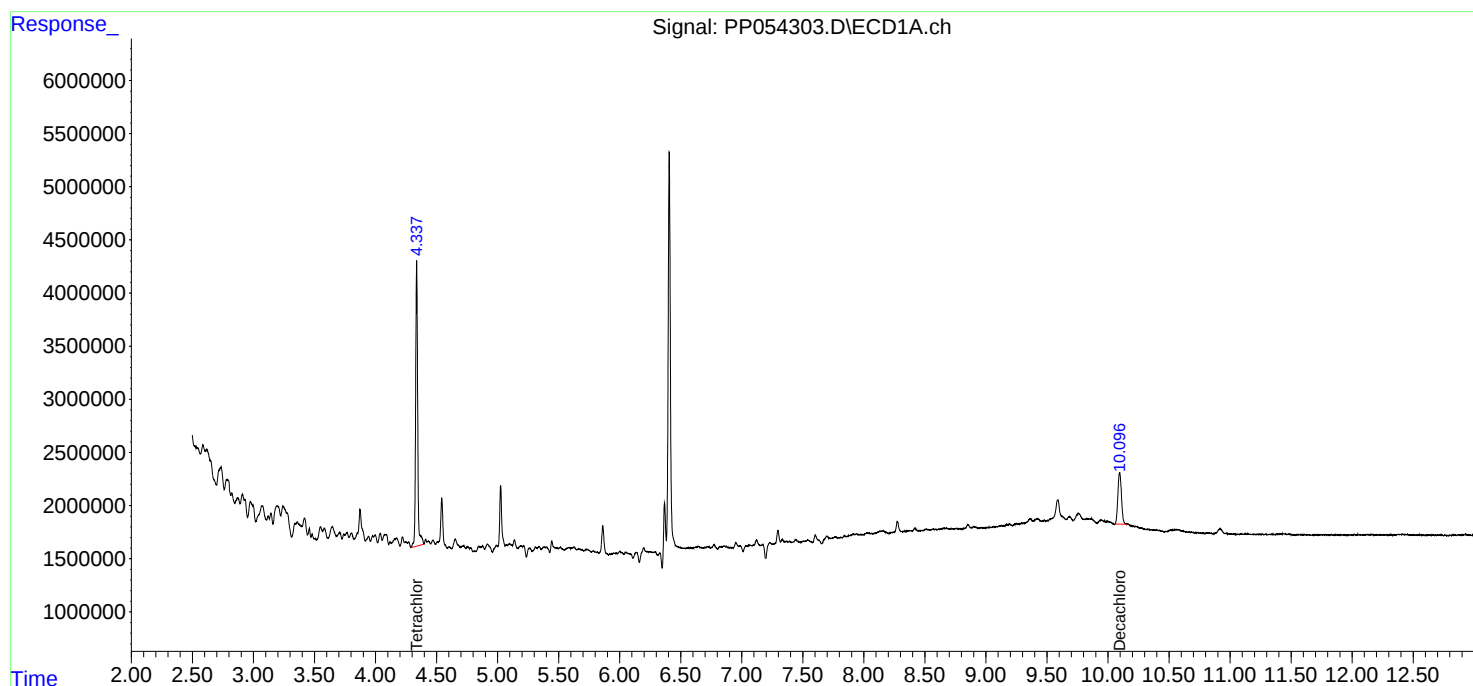

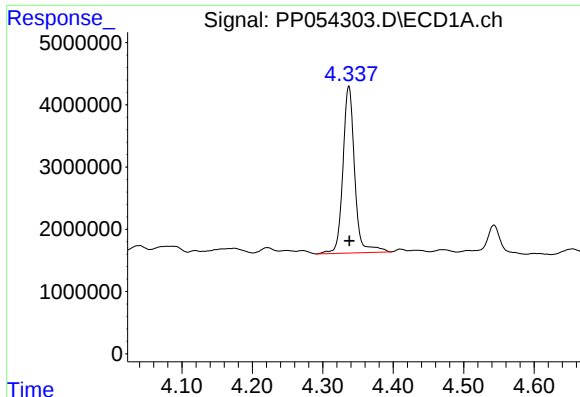


#1 Tetrachloro-m-xylene

R.T.: 4.337 min
Delta R.T.: -0.001 min
Response: 31191223
Conc: 15.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
NWB-1865


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/06/2023
Supervised By :Ankita Jodhani 01/06/2023

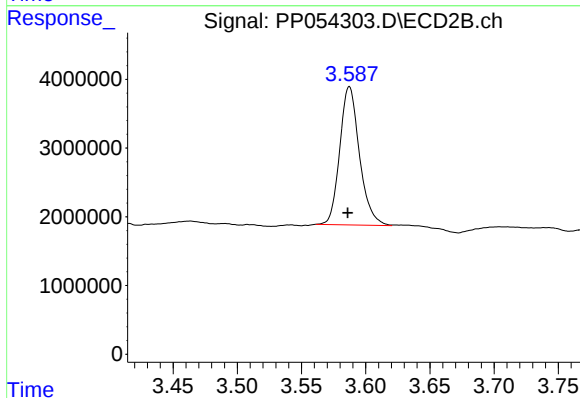


#1 Tetrachloro-m-xylene

R.T.: 3.587 min
Delta R.T.: 0.000 min
Response: 21457084
Conc: 13.30 ng/ml m

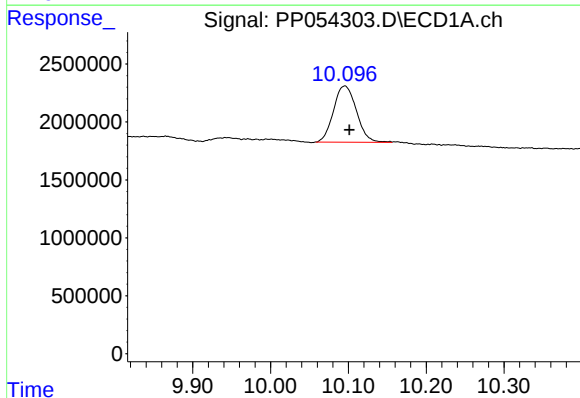

#2 Decachlorobiphenyl

R.T.: 10.095 min
Delta R.T.: -0.006 min
Response: 9936351
Conc: 6.92 ng/ml m

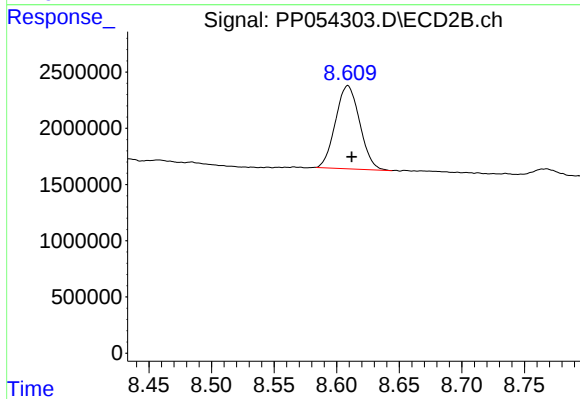

#2 Decachlorobiphenyl

R.T.: 8.609 min
Delta R.T.: -0.003 min
Response: 9970676
Conc: 7.07 ng/ml m