

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010524\
 Data File : PP062725.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2024 13:01
 Operator : YP\AJ
 Sample : PB158261BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB158261BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 23:26:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 22 03:29:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.398	3.683	51139338	68224637	23.522	22.862
2) SA Decachlor...	10.156	8.785	34199192	49241327	23.716	19.343
Target Compounds						
9) L2 AR-1221-2	4.706	3.989	915403	1015473	45.034	36.763
28) L6 AR-1254-3	7.016	0.000	2208909	0	17.108	N.D. #
30) L6 AR-1254-5	7.714	0.000	55778	0	0.569	N.D. #
32) L7 AR-1260-2	7.446	6.473	74204	902173	0.654	4.928 #
33) L7 AR-1260-3	7.795	0.000	542011	0	6.326	N.D. #
34) L7 AR-1260-4	8.042f	0.000	505898	0	5.224	N.D. #
43) L9 AR-1268-3	0.000	7.947f	0	365387	N.D.	1.166 #
45) L9 AR-1268-5	0.000	8.521	0	287938	N.D.	0.328 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010524\
Data File : PP062725.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2024 13:01
Operator : YP\AJ
Sample : PB158261BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB158261BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 23:26:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122123.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 22 03:29:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

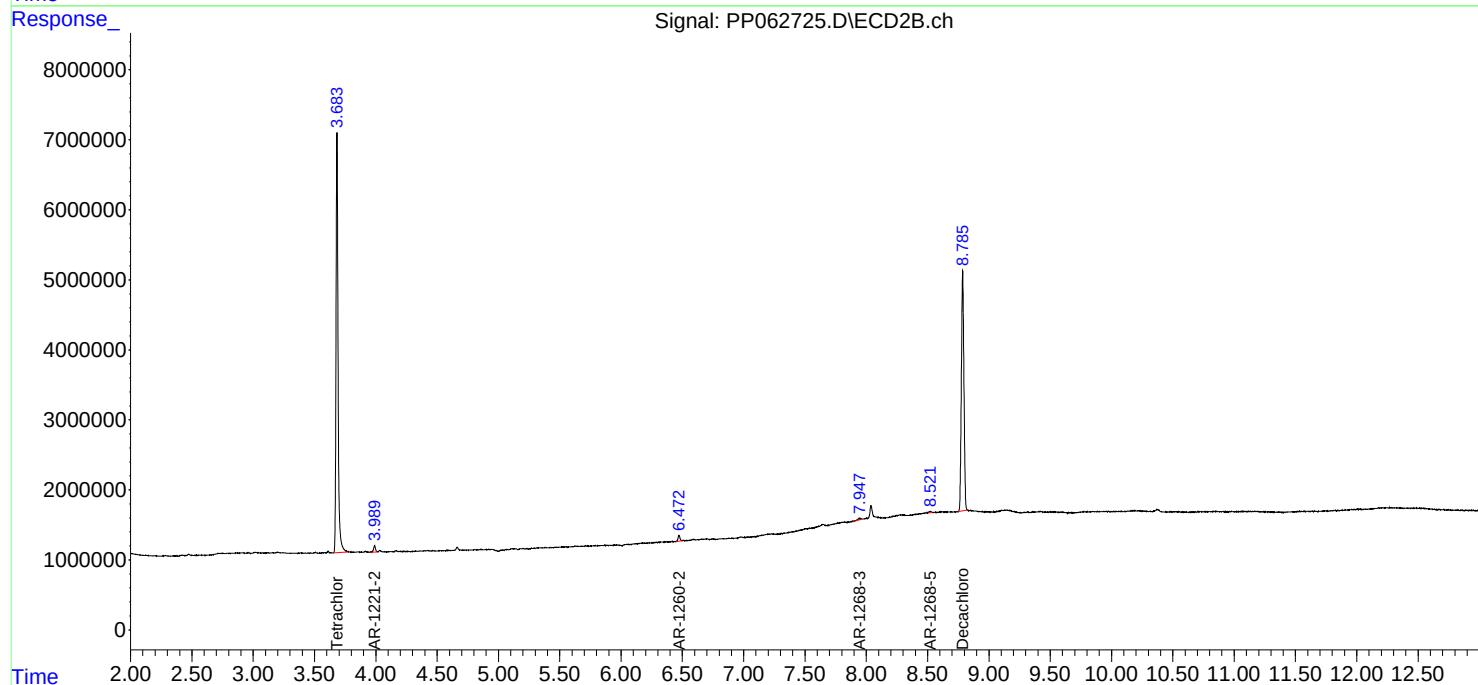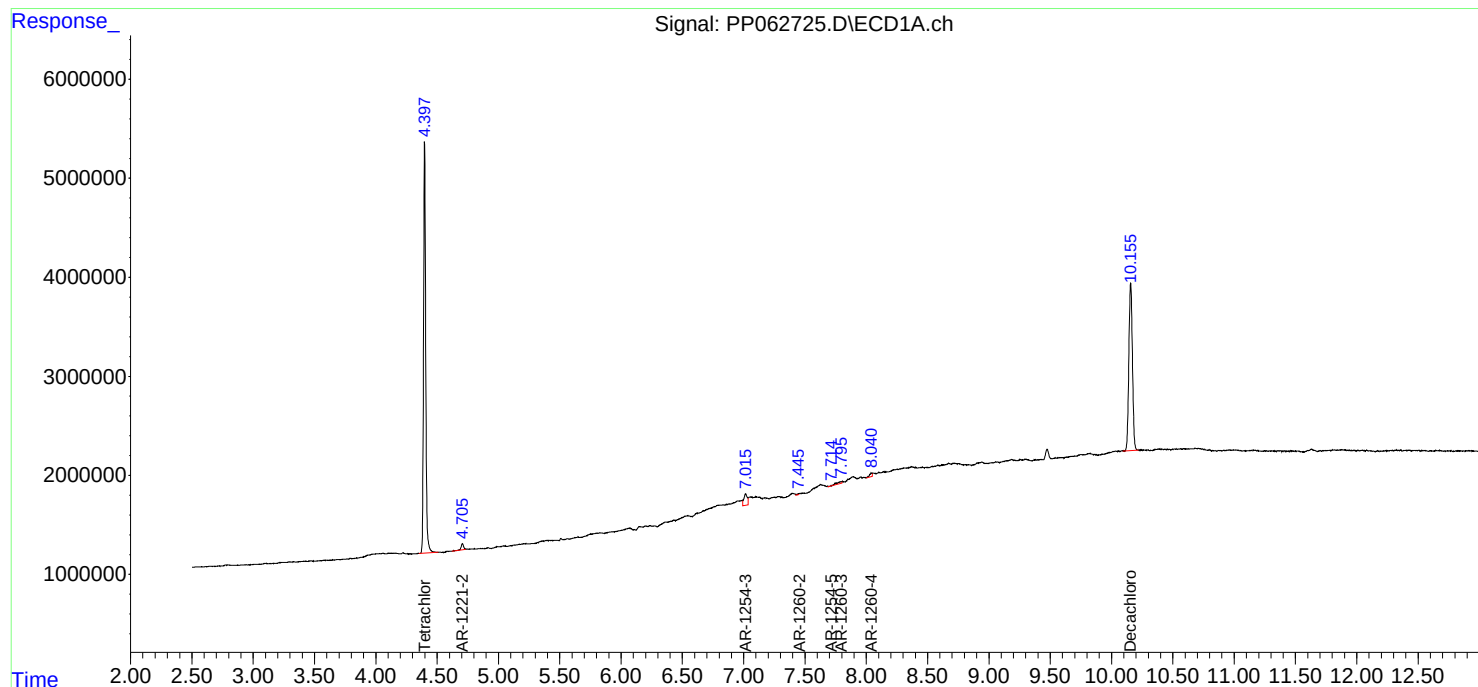


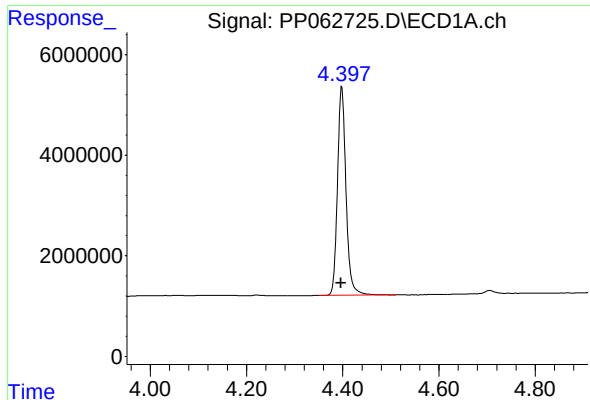

#1 Tetrachloro-m-xylene


R.T.: 4.398 min
Delta R.T.: 0.002 min
Response: 51139338
Conc: 23.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB158261BL

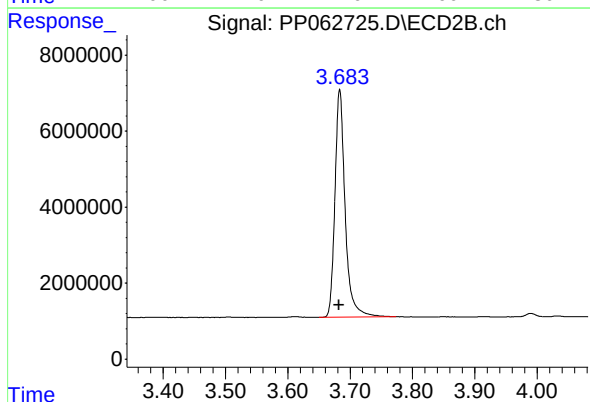


#1 Tetrachloro-m-xylene

R.T.: 3.683 min
Delta R.T.: 0.001 min
Response: 68224637
Conc: 22.86 ng/ml

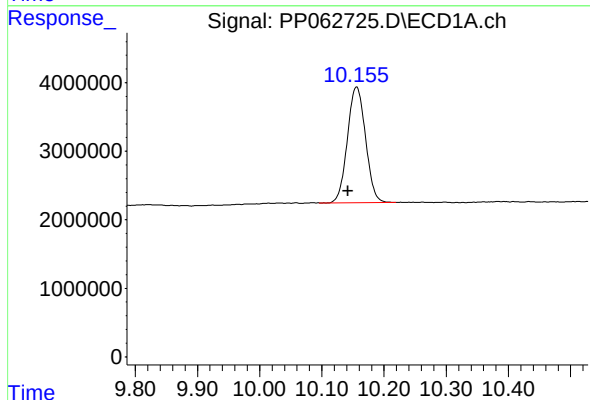


#2 Decachlorobiphenyl

R.T.: 10.156 min
Delta R.T.: 0.014 min
Response: 34199192
Conc: 23.72 ng/ml

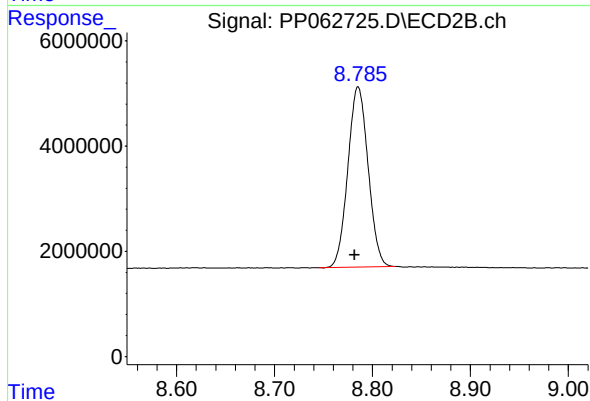

#2 Decachlorobiphenyl


R.T.: 8.785 min
Delta R.T.: 0.004 min
Response: 49241327
Conc: 19.34 ng/ml

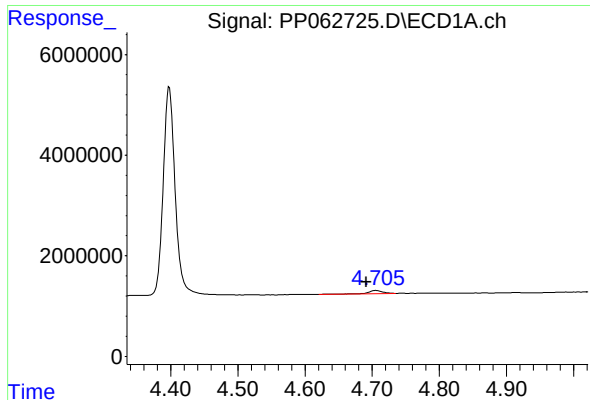

#9 AR-1221-2


R.T.: 4.706 min
Delta R.T.: 0.015 min
Response: 915403
Conc: 45.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB158261BL

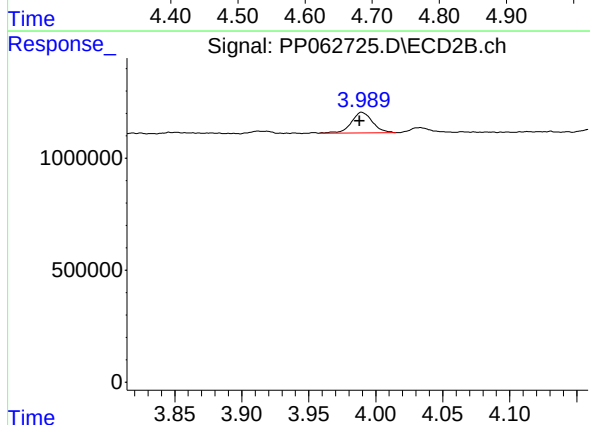


#9 AR-1221-2

R.T.: 3.989 min
Delta R.T.: 0.001 min
Response: 1015473
Conc: 36.76 ng/ml

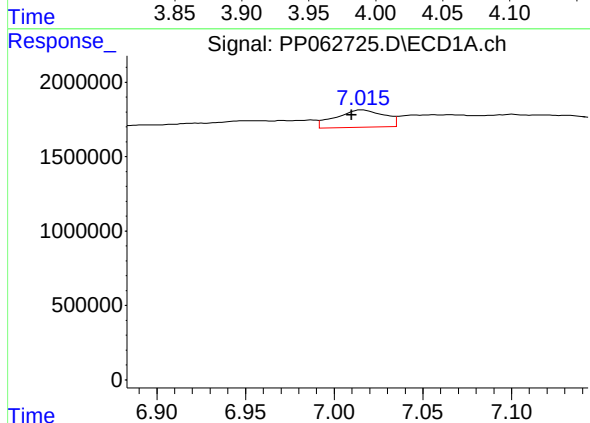


#28 AR-1254-3

R.T.: 7.016 min
Delta R.T.: 0.006 min
Response: 2208909
Conc: 17.11 ng/ml

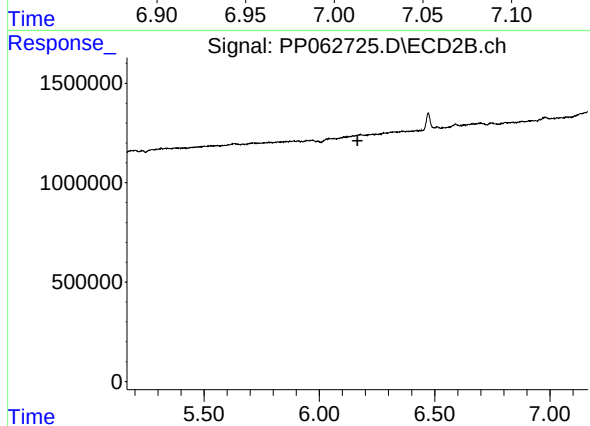

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.166 min
Response: 0
Conc: N.D.

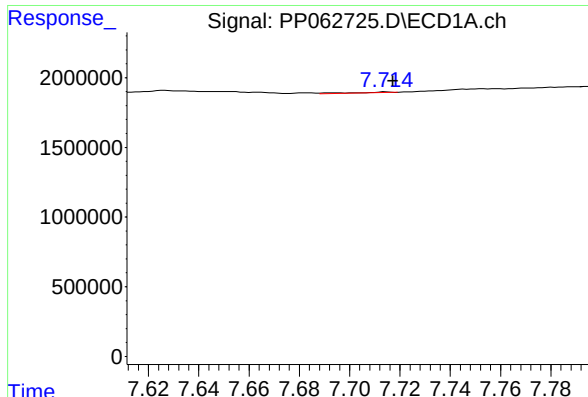

#30 AR-1254-5


R.T.: 7.714 min
Delta R.T.: -0.003 min
Response: 55778
Conc: 0.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB158261BL

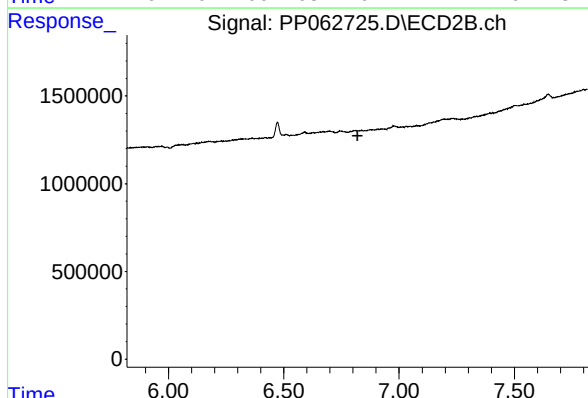


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 6.820 min
Response: 0
Conc: N.D.

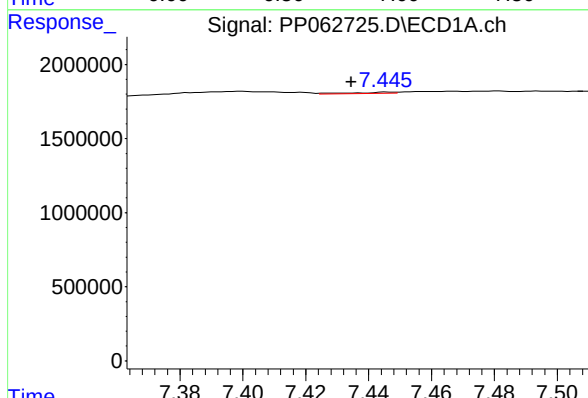


#32 AR-1260-2

R.T.: 7.446 min
Delta R.T.: 0.011 min
Response: 74204
Conc: 0.65 ng/ml

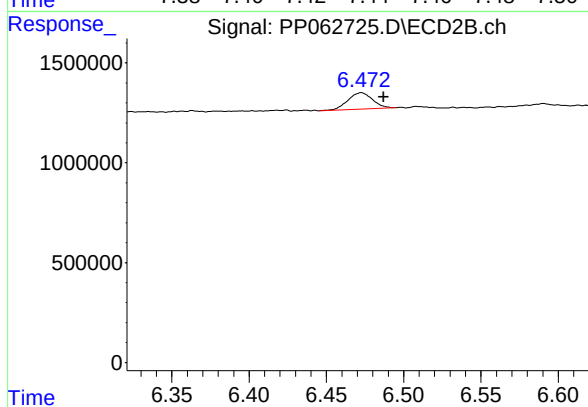

#32 AR-1260-2


R.T.: 6.473 min
Delta R.T.: -0.014 min
Response: 902173
Conc: 4.93 ng/ml

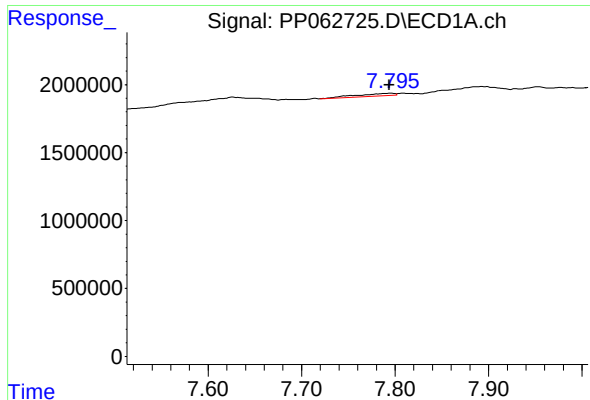

#33 AR-1260-3


R.T.: 7.795 min
Delta R.T.: 0.001 min
Response: 542011
Conc: 6.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB158261BL

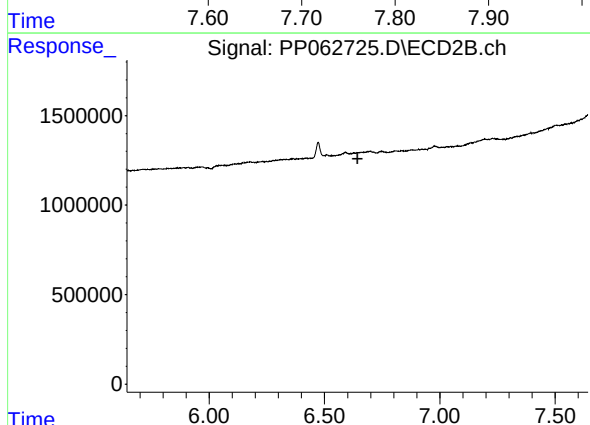


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.643 min
Response: 0
Conc: N.D.

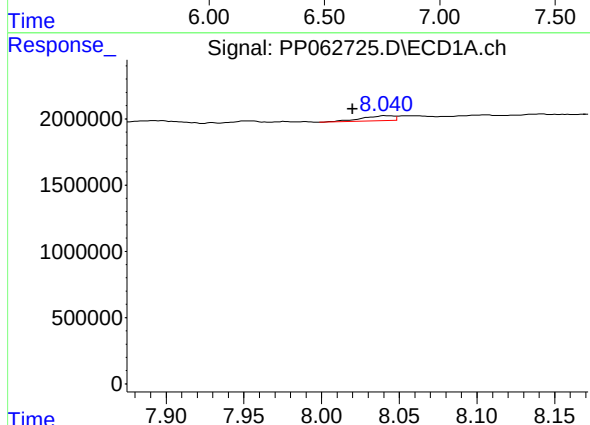


#34 AR-1260-4

R.T.: 8.042 min
Delta R.T.: 0.022 min
Response: 505898
Conc: 5.22 ng/ml

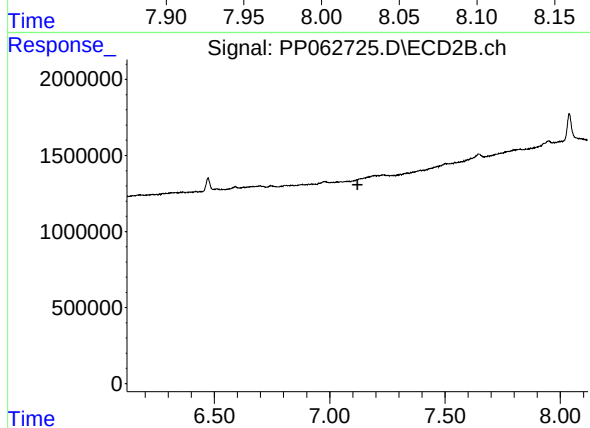

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.121 min
Response: 0
Conc: N.D.

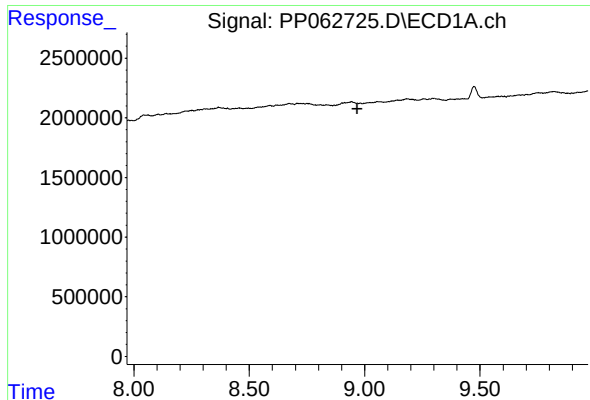

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.968 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB158261BL

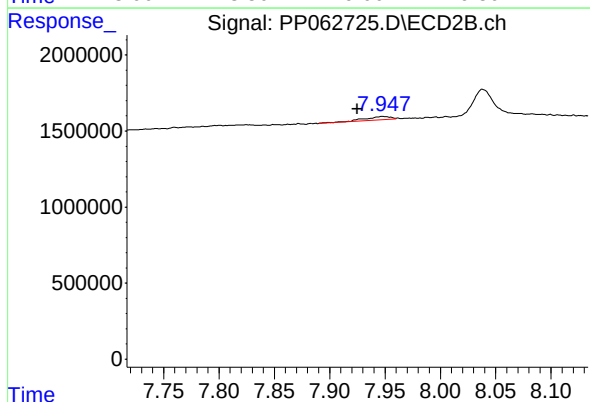


#43 AR-1268-3

R.T.: 7.947 min
Delta R.T.: 0.022 min
Response: 365387
Conc: 1.17 ng/ml

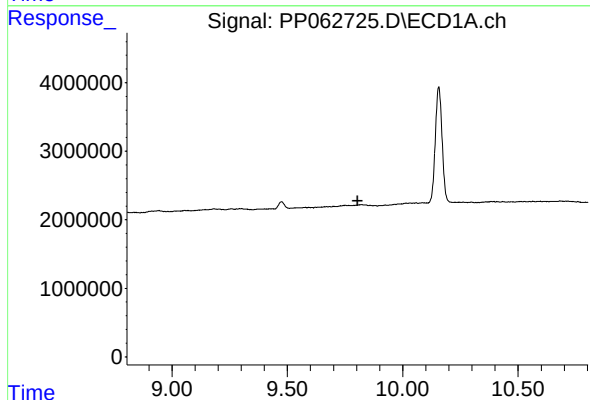

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.804 min
Response: 0
Conc: N.D.

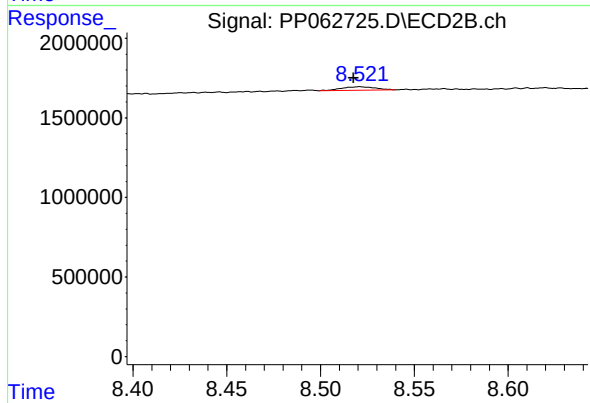

#45 AR-1268-5

R.T.: 8.521 min
Delta R.T.: 0.003 min
Response: 287938
Conc: 0.33 ng/ml