

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010524\
 Data File : PP062746.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2024 19:03
 Operator : YP\AJ
 Sample : P1039-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TREMONT-AVE-DRUM-28-PPE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 23:34:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 22 03:29:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.395	3.682	42690875	61924765	19.636	20.751
2) SA Decachlor...	10.149	8.782	34582780	48070898	23.982	18.883

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010524\
Data File : PP062746.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2024 19:03
Operator : YP\AJ
Sample : P1039-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TREMONT-AVE-DRUM-28-PPE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 23:34:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122123.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 22 03:29:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

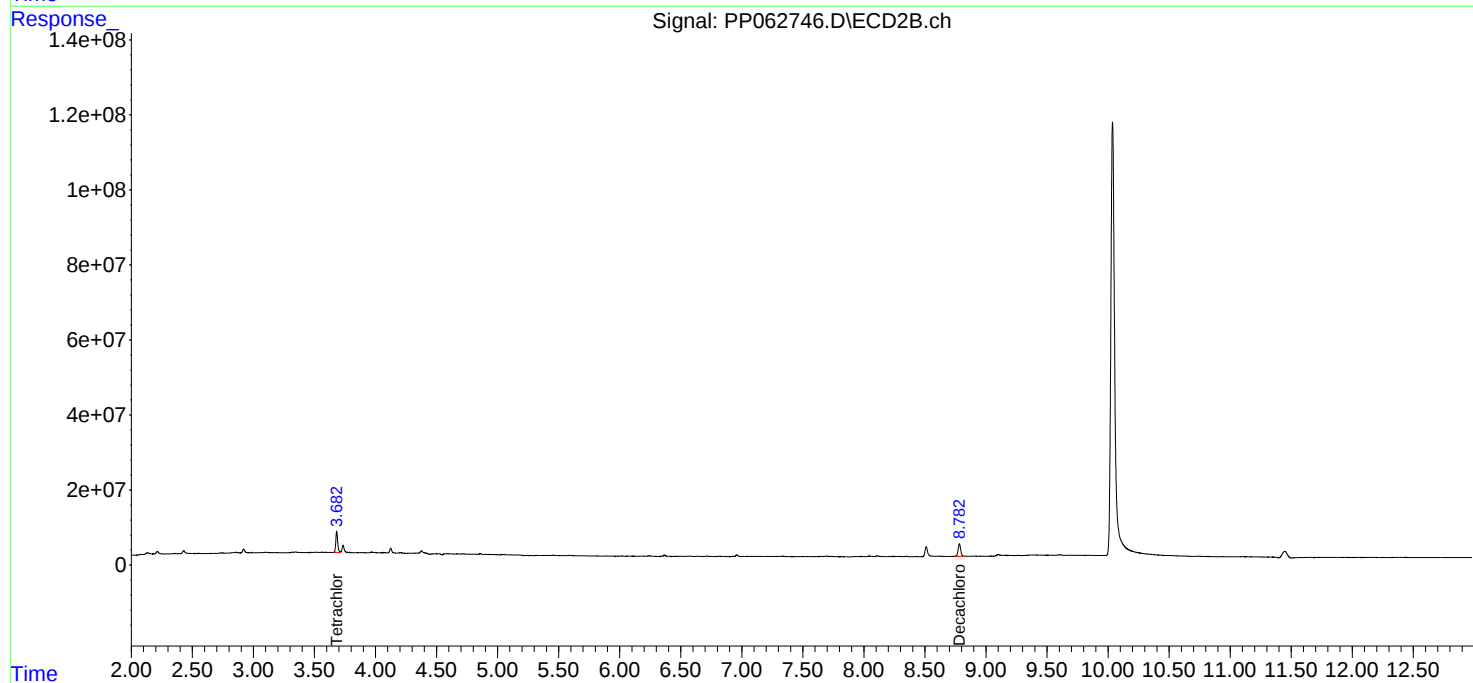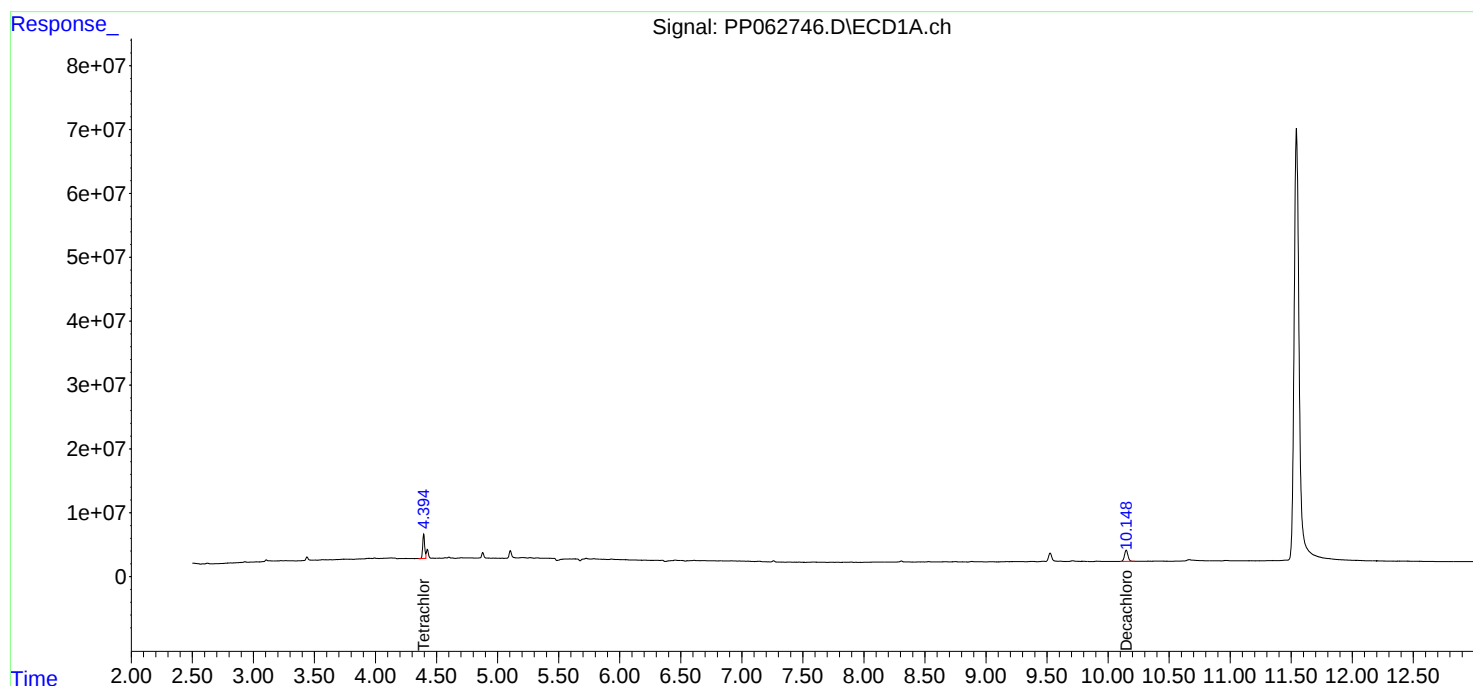


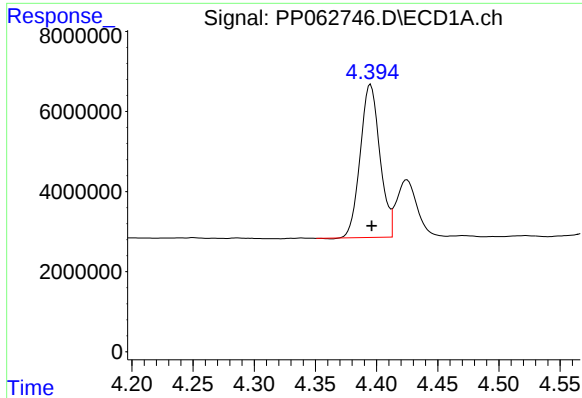

#1 Tetrachloro-m-xylene


R.T.: 4.395 min
Delta R.T.: 0.000 min
Response: 42690875
Conc: 19.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
TREMONT-AVE-DRUM-28-PPE

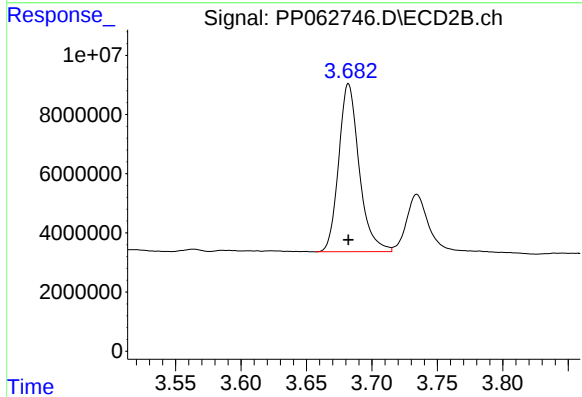


#1 Tetrachloro-m-xylene

R.T.: 3.682 min
Delta R.T.: 0.000 min
Response: 61924765
Conc: 20.75 ng/ml

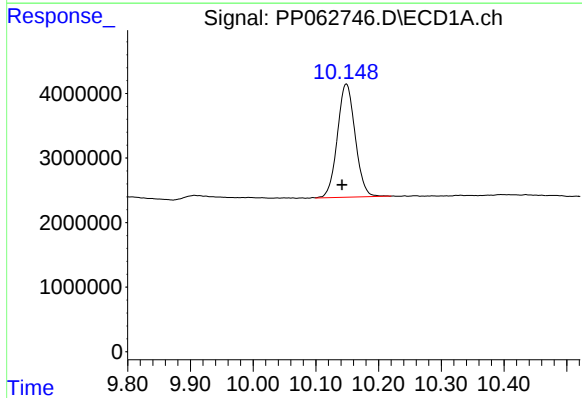

#2 Decachlorobiphenyl

R.T.: 10.149 min
Delta R.T.: 0.007 min
Response: 34582780
Conc: 23.98 ng/ml

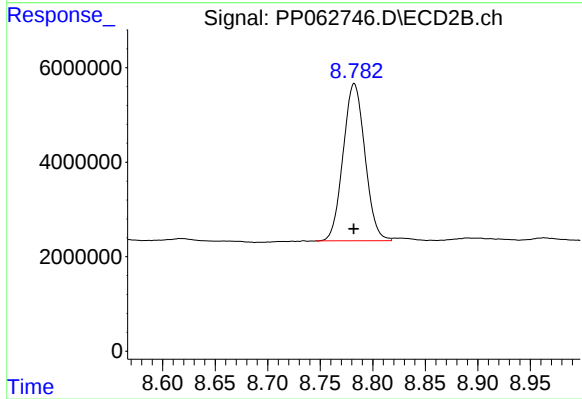

#2 Decachlorobiphenyl

R.T.: 8.782 min
Delta R.T.: 0.000 min
Response: 48070898
Conc: 18.88 ng/ml