

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010621\
 Data File : PP032568.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jan 2021 12:23
 Operator : DD\AJ
 Sample : M1012-01 10X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KKA091Y-END-1

Manual Integrations
 APPROVED

Ankita
 1/7/2021 11:20:51 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 06 17:18:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 07:49:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.748	4.033	170994	111960	3.127	2.313 #
2)	SA Decachlor...	10.586	9.320	116951	109333	2.612m	2.462
Target Compounds							
31)	L7 AR-1260-1	7.727	6.865	65930	57374	31.522	25.473
32)	L7 AR-1260-2	7.993	7.063	105421	75659	40.719	28.096 #
33)	L7 AR-1260-3	8.357	7.219	211061	71132	98.280	27.125 #
34)	L7 AR-1260-4	8.586	7.698	166741	123812	73.824	55.083 #
35)	L7 AR-1260-5	8.897	7.947	379924	293035	78.712	56.135 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010621\
Data File : PP032568.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jan 2021 12:23
Operator : DD\AJ
Sample : M1012-01 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KKA091Y-END-1


Manual Integrations
APPROVED

Ankita
1/7/2021 11:20:51 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 06 17:18:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 07:49:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

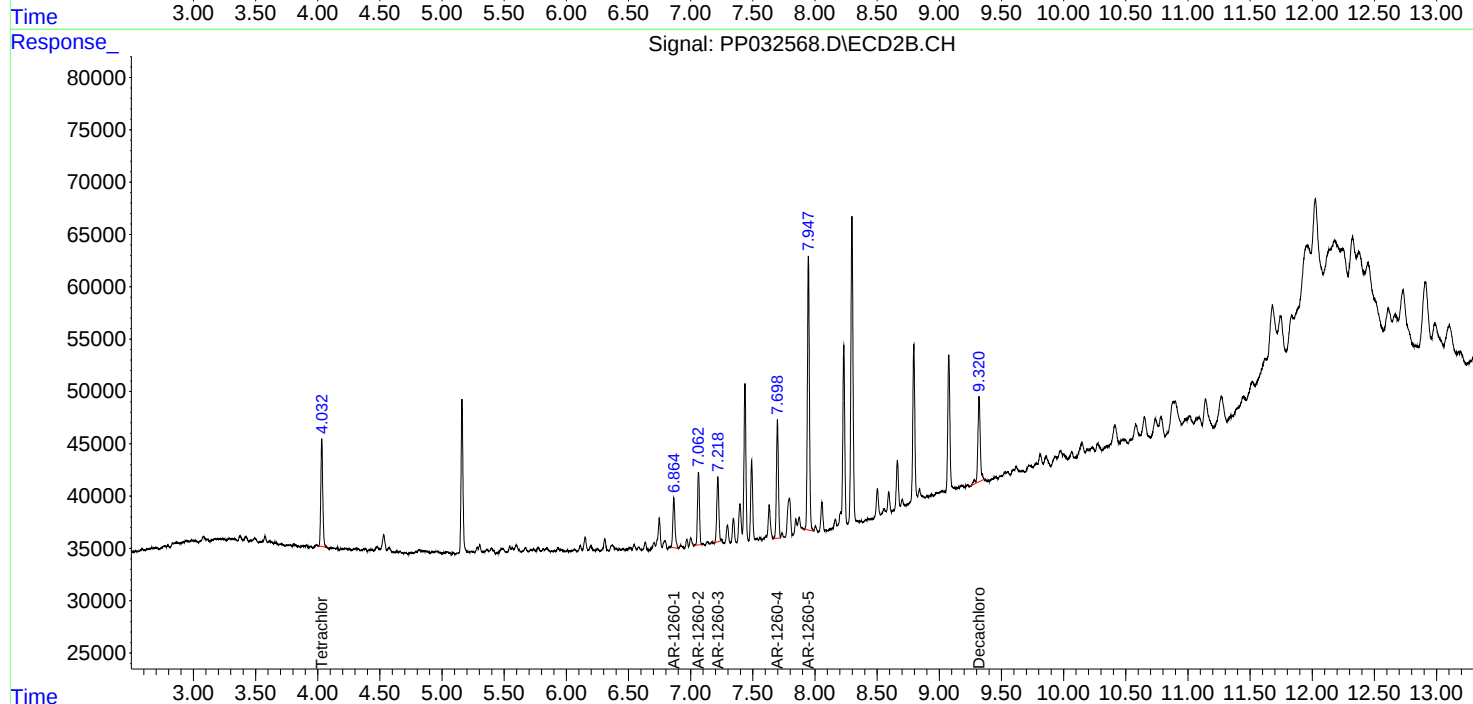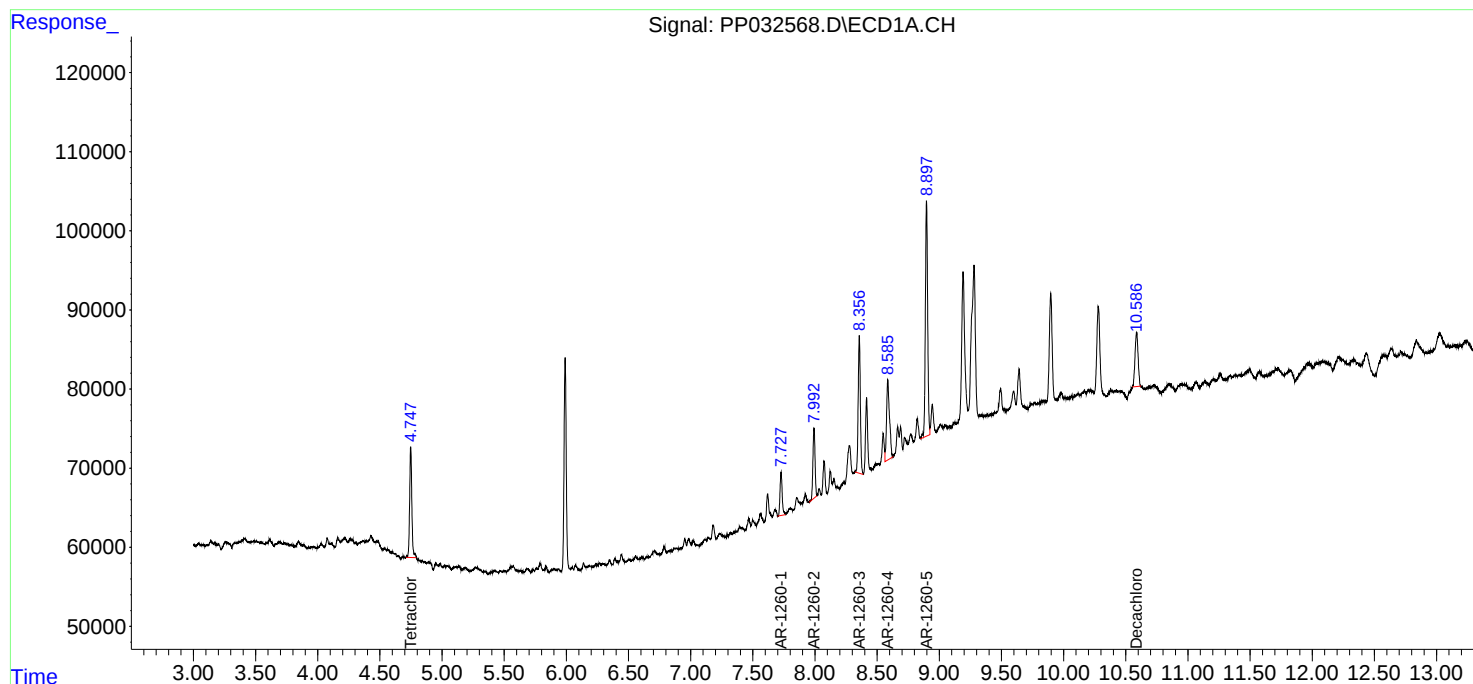

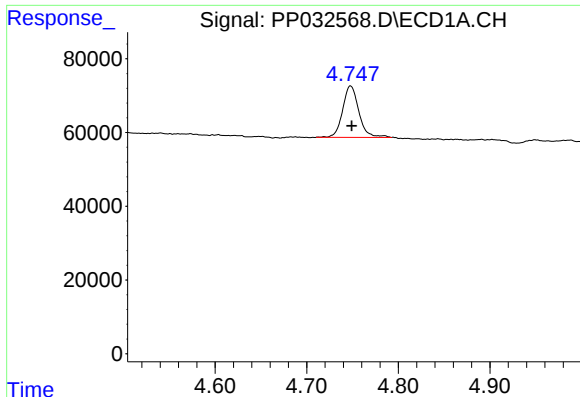


#1 Tetrachloro-m-xylene

R.T.: 4.748 min
Delta R.T.: -0.001 min
Response: 170994
Conc: 3.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
KKA091Y-END-1


Manual Integrations
APPROVED

Ankita
1/7/2021 11:20:51 AM

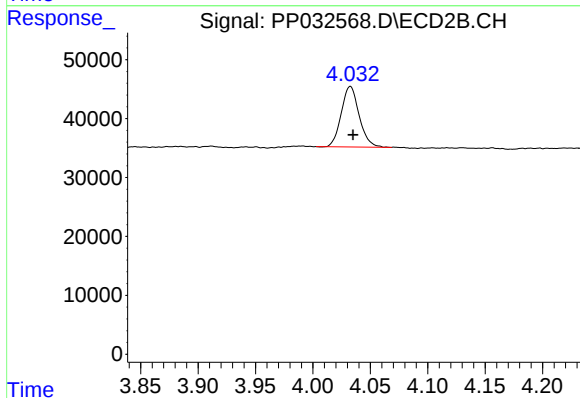


#1 Tetrachloro-m-xylene

R.T.: 4.033 min
Delta R.T.: -0.002 min
Response: 111960
Conc: 2.31 ng/ml

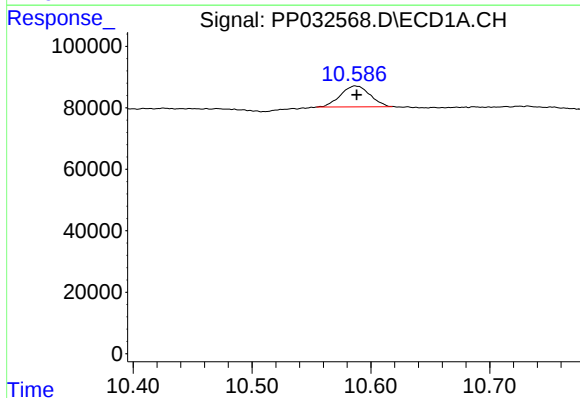


#2 Decachlorobiphenyl

R.T.: 10.586 min
Delta R.T.: -0.002 min
Response: 116951
Conc: 2.61 ng/ml m

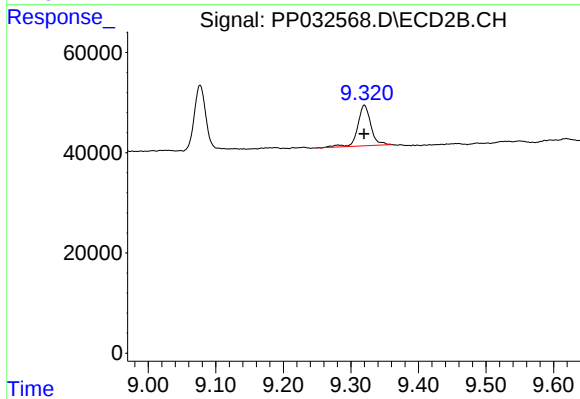

#2 Decachlorobiphenyl

R.T.: 9.320 min
Delta R.T.: 0.000 min
Response: 109333
Conc: 2.46 ng/ml

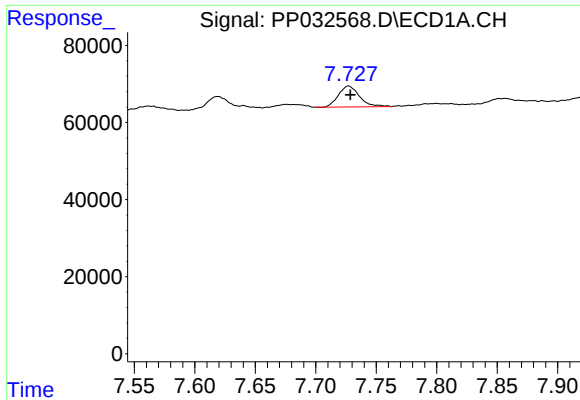


#31 AR-1260-1

R.T.: 7.727 min
Delta R.T.: -0.001 min
Response: 65930
Conc: 31.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
KKA091Y-END-1


Manual Integrations
APPROVED

Ankita
1/7/2021 11:20:51 AM

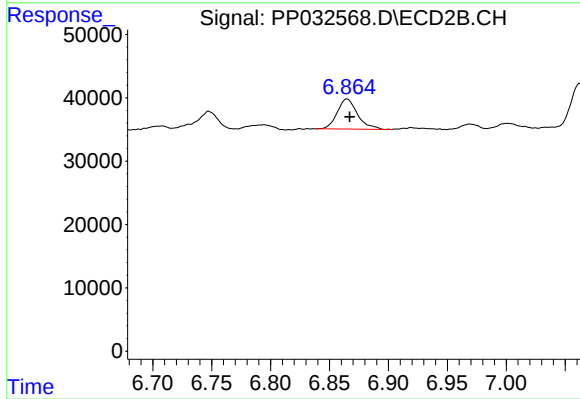


#31 AR-1260-1

R.T.: 6.865 min
Delta R.T.: -0.003 min
Response: 57374
Conc: 25.47 ng/ml

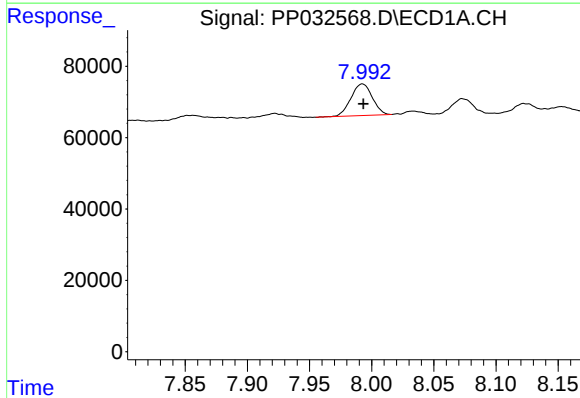


#32 AR-1260-2

R.T.: 7.993 min
Delta R.T.: 0.000 min
Response: 105421
Conc: 40.72 ng/ml

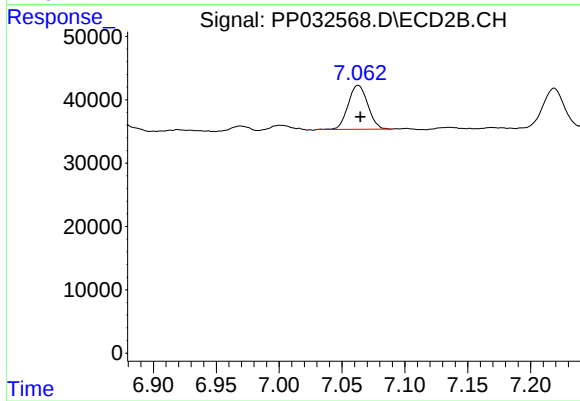

#32 AR-1260-2

R.T.: 7.063 min
Delta R.T.: -0.002 min
Response: 75659
Conc: 28.10 ng/ml

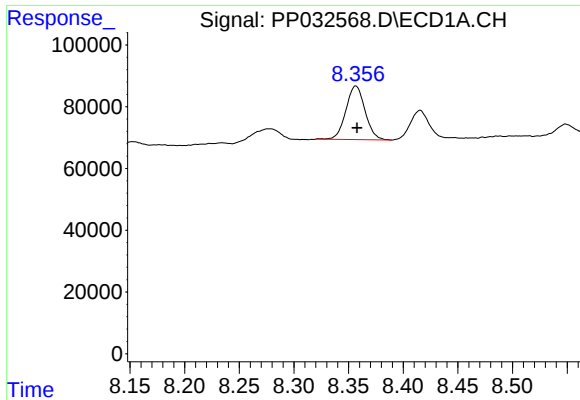


#33 AR-1260-3

R.T.: 8.357 min
Delta R.T.: -0.001 min
Response: 211061
Conc: 98.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
KKA091Y-END-1


Manual Integrations
APPROVED

Ankita
1/7/2021 11:20:51 AM

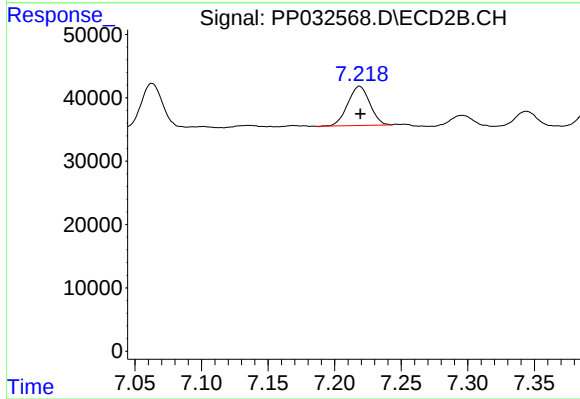


#33 AR-1260-3

R.T.: 7.219 min
Delta R.T.: 0.000 min
Response: 71132
Conc: 27.13 ng/ml

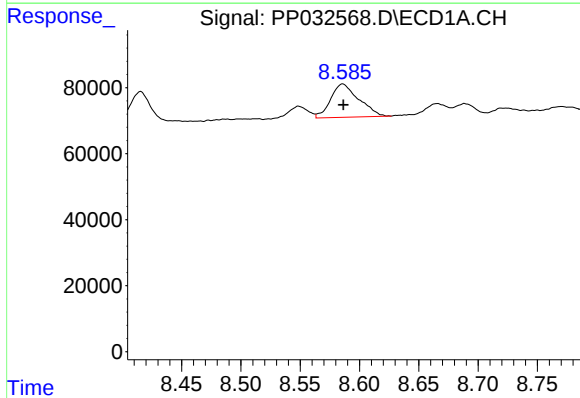


#34 AR-1260-4

R.T.: 8.586 min
Delta R.T.: 0.000 min
Response: 166741
Conc: 73.82 ng/ml

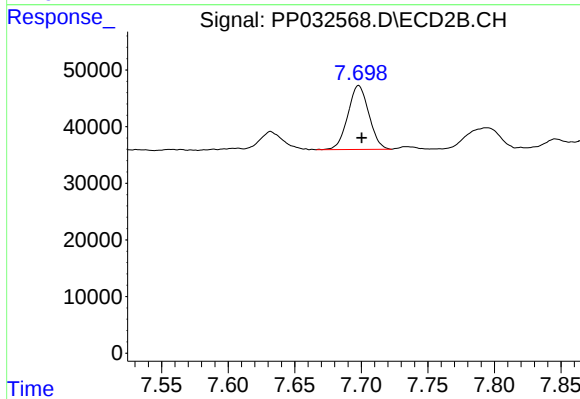

#34 AR-1260-4

R.T.: 7.698 min
Delta R.T.: -0.002 min
Response: 123812
Conc: 55.08 ng/ml

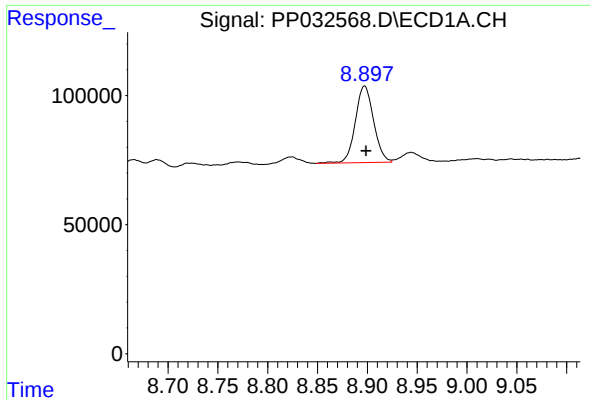


#35 AR-1260-5

R.T.: 8.897 min
Delta R.T.: -0.002 min
Response: 379924
Conc: 78.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
KKA091Y-END-1

Manual Integrations
APPROVED

Ankita
1/7/2021 11:20:51 AM

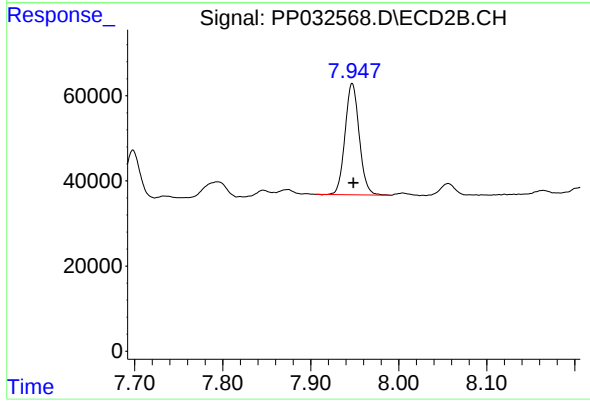

#35 AR-1260-5

R.T.: 7.947 min
Delta R.T.: -0.002 min
Response: 293035
Conc: 56.13 ng/ml