

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010621\
 Data File : PP032579.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jan 2021 15:52
 Operator : DD\AJ
 Sample : M1014-04 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC226716LOZ-LITTLE-PIECE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 06 17:22:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 07:49:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.747	4.033	172097	135053	3.147	2.790
2)	SA Decachlor...	10.584	9.318	123224	100351	2.752	2.260

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010621\
Data File : PP032579.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jan 2021 15:52
Operator : DD\AJ
Sample : M1014-04 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BC226716LOZ-LITTLE-PIECE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 06 17:22:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 07:49:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

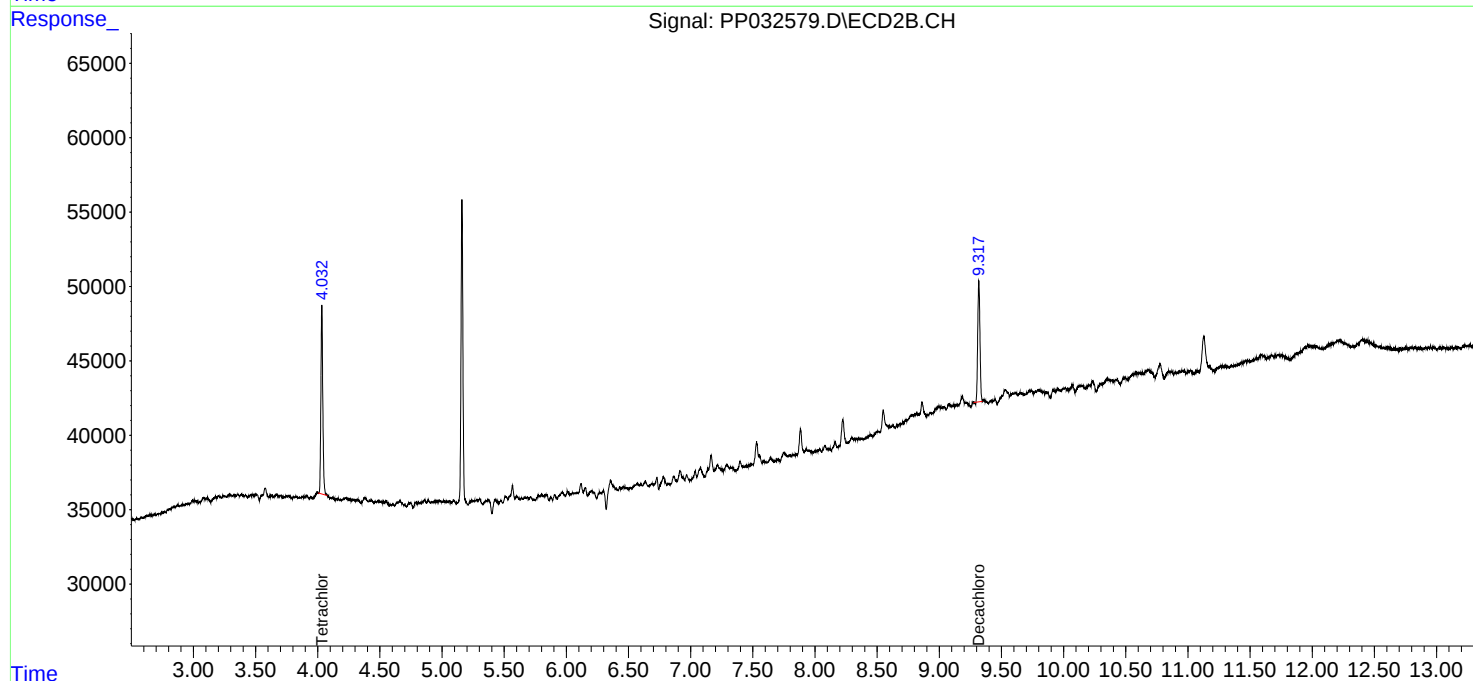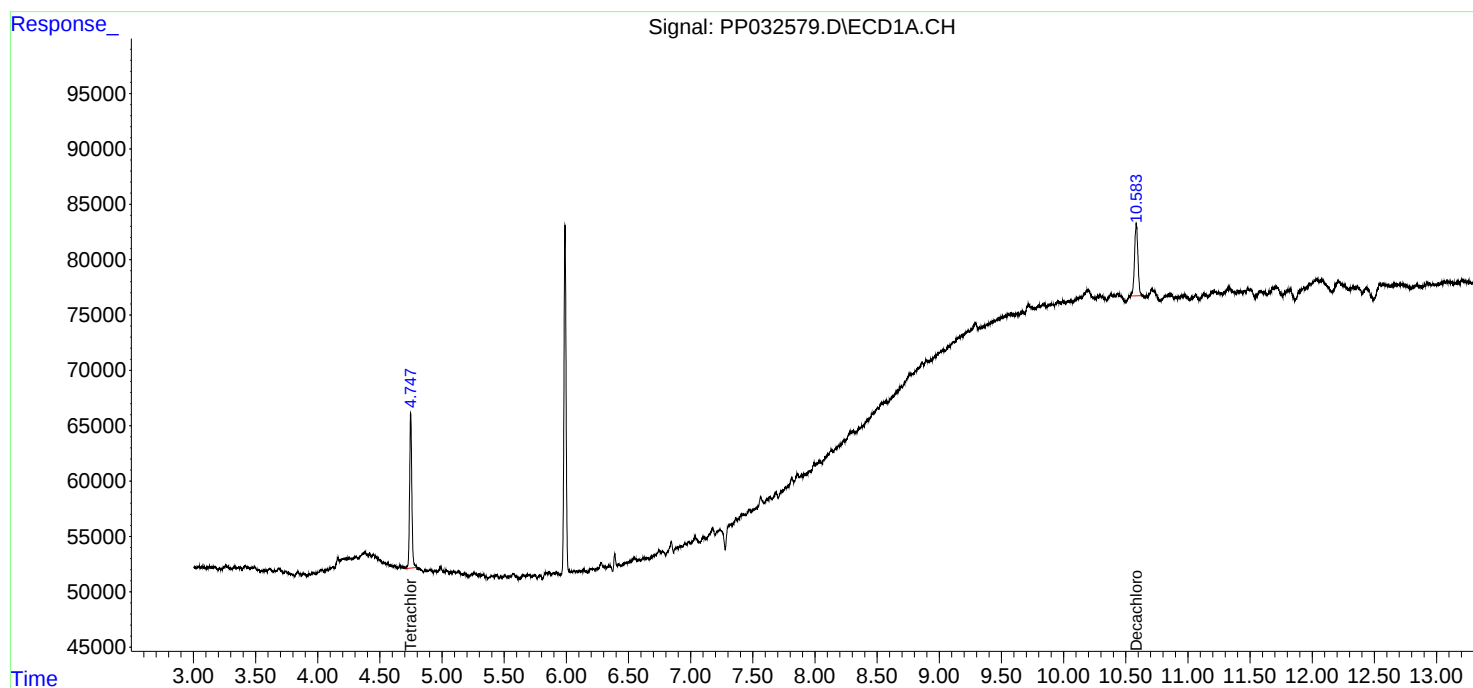


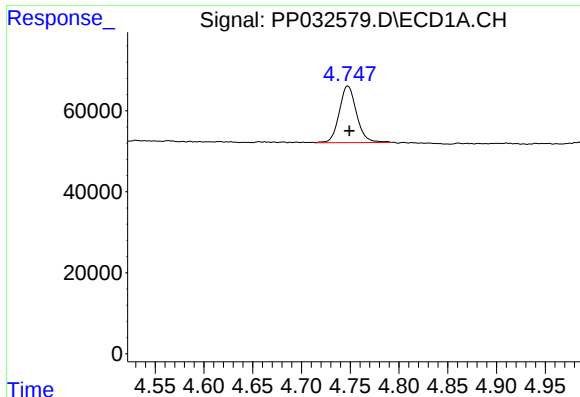

#1 Tetrachloro-m-xylene


R.T.: 4.747 min
Delta R.T.: -0.002 min
Response: 172097
Conc: 3.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC226716LOZ-LITTLE-PIECE

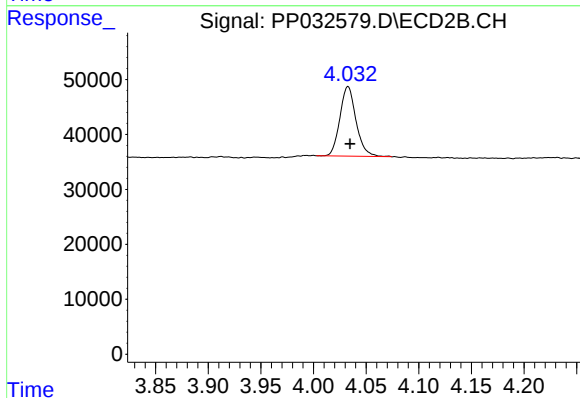


#1 Tetrachloro-m-xylene

R.T.: 4.033 min
Delta R.T.: -0.002 min
Response: 135053
Conc: 2.79 ng/ml

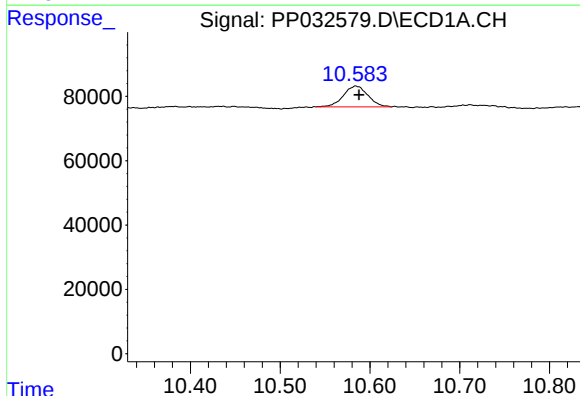

#2 Decachlorobiphenyl

R.T.: 10.584 min
Delta R.T.: -0.004 min
Response: 123224
Conc: 2.75 ng/ml

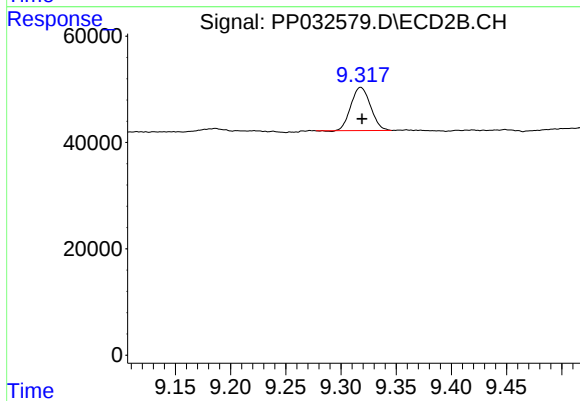

#2 Decachlorobiphenyl

R.T.: 9.318 min
Delta R.T.: -0.001 min
Response: 100351
Conc: 2.26 ng/ml