

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010622\
 Data File : PP042641.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jan 2022 21:19
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 03:39:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 05 12:01:35 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.885	4.050	383223	526293	19.781	20.105
2) SA Decachlor...	10.825	9.390	261406	418821	22.282	21.311
Target Compounds						
28) L6 AR-1254-3	7.702	0.000	2693	0	2.940	N.D. #
30) L6 AR-1254-5	8.418	0.000	1947	0	3.079	N.D. #
32) L7 AR-1260-2	8.149f	0.000	3176	0	4.515	N.D. #
39) L8 AR-1262-4	9.418f	0.000	11734	0	24.279	N.D. #
40) L8 AR-1262-5	10.070	0.000	7873	0	16.136	N.D. #
42) L9 AR-1268-2	9.418f	0.000	11734	0	7.758	N.D. #
43) L9 AR-1268-3	9.674	0.000	3451	0	2.564	N.D. #
44) L9 AR-1268-4	10.070	0.000	7873	0	14.382	N.D. #
45) L9 AR-1268-5	10.471	0.000	1497	0	0.335	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010622\
Data File : PP042641.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jan 2022 21:19
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 03:39:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 05 12:01:35 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

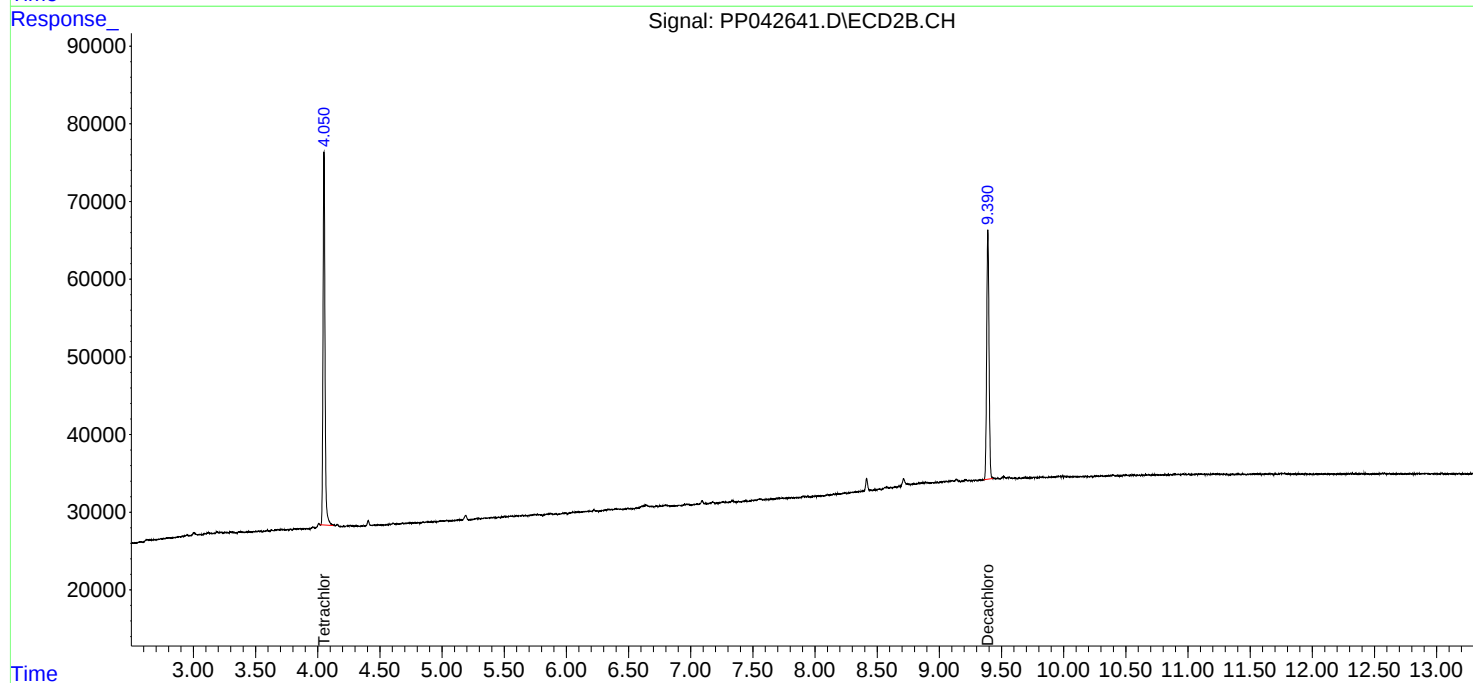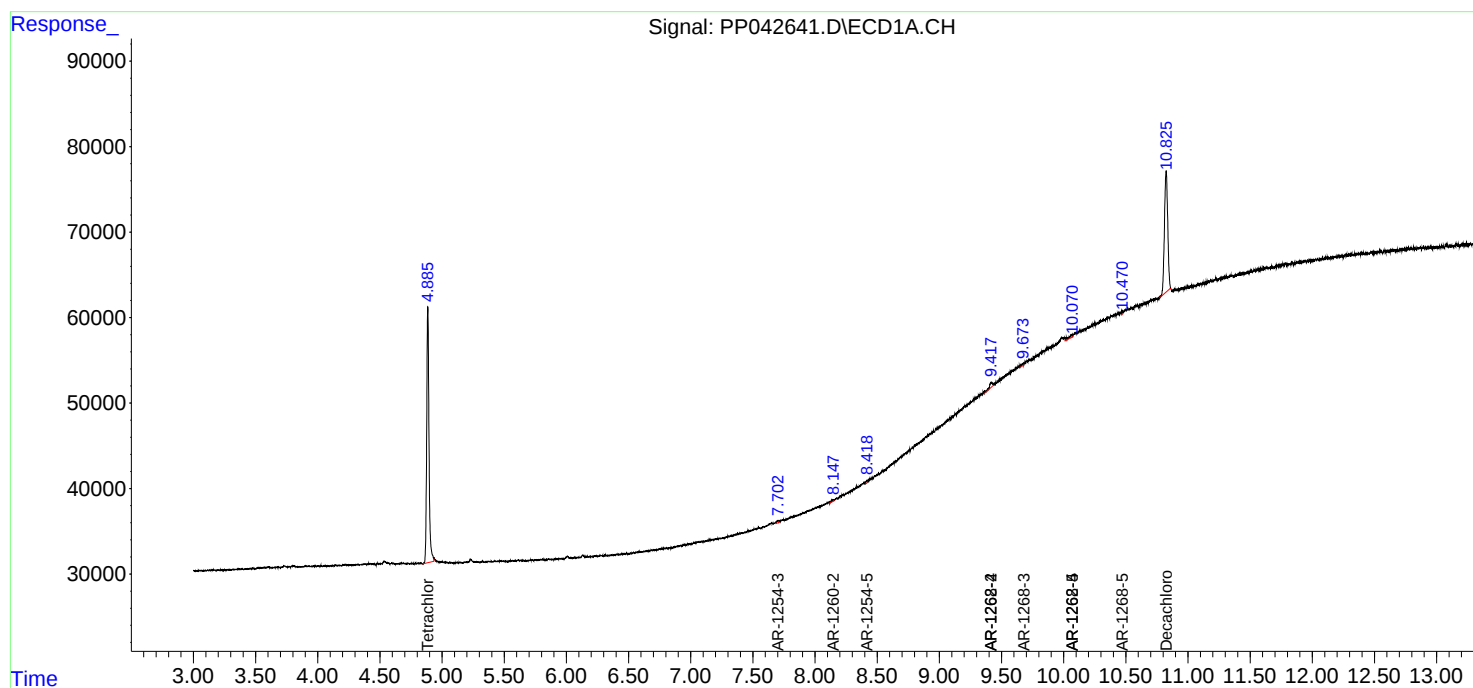


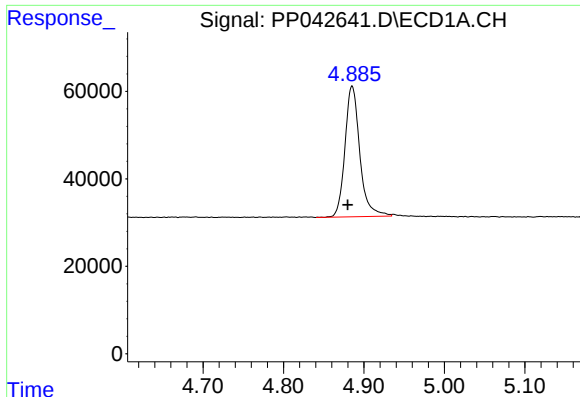

#1 Tetrachloro-m-xylene


R.T.: 4.885 min
Delta R.T.: 0.005 min
Response: 383223
Conc: 19.78 ng/ml

Instrument :
ECD_P
ClientSampleId :

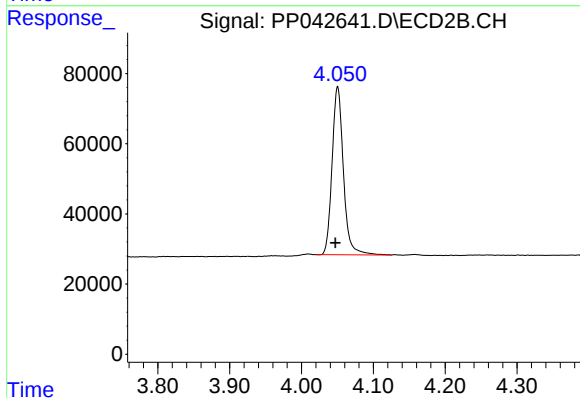


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: 0.003 min
Response: 526293
Conc: 20.10 ng/ml

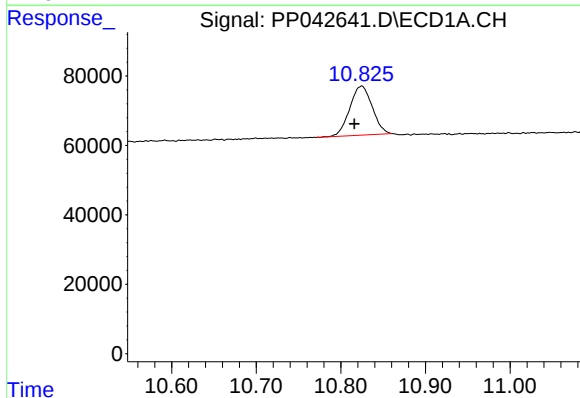


#2 Decachlorobiphenyl

R.T.: 10.825 min
Delta R.T.: 0.008 min
Response: 261406
Conc: 22.28 ng/ml

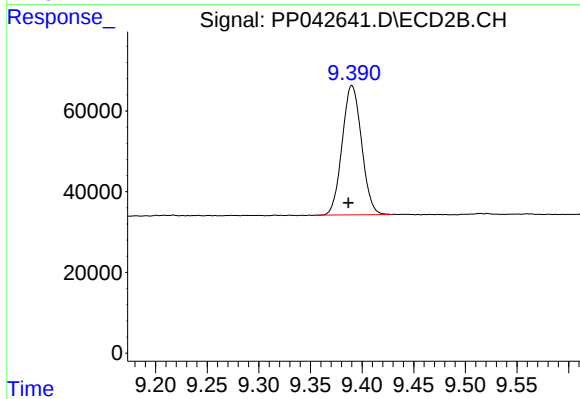

#2 Decachlorobiphenyl


R.T.: 9.390 min
Delta R.T.: 0.003 min
Response: 418821
Conc: 21.31 ng/ml

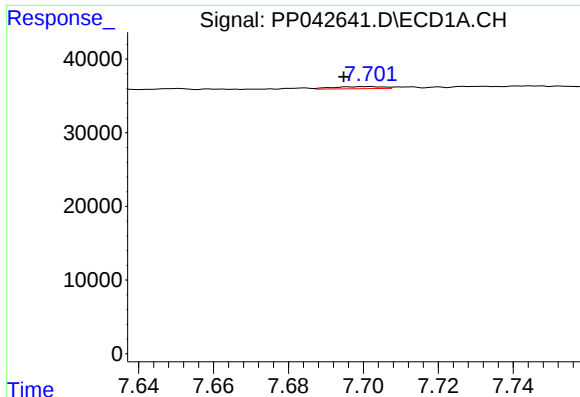

#28 AR-1254-3


R.T.: 7.702 min
Delta R.T.: 0.007 min
Response: 2693
Conc: 2.94 ng/ml

Instrument :
ECD_P
ClientSampleId :

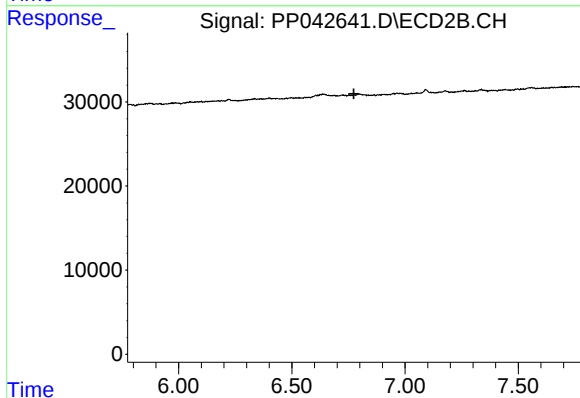


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.774 min
Response: 0
Conc: N.D.

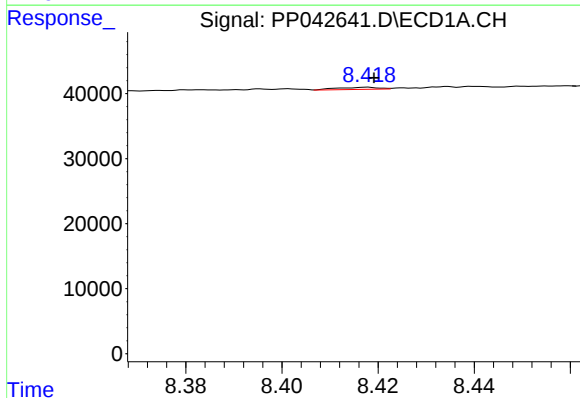


#30 AR-1254-5

R.T.: 8.418 min
Delta R.T.: -0.002 min
Response: 1947
Conc: 3.08 ng/ml

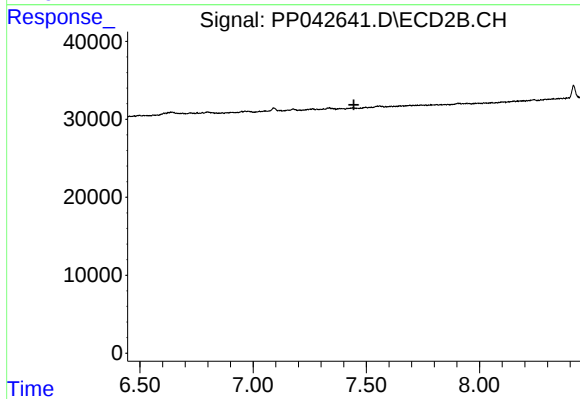

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.445 min
Response: 0
Conc: N.D.

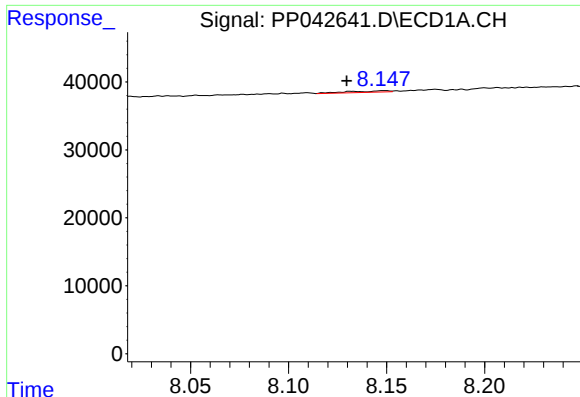

#32 AR-1260-2


R.T.: 8.149 min
Delta R.T.: 0.019 min
Response: 3176
Conc: 4.51 ng/ml

Instrument :
ECD_P
ClientSampleId :

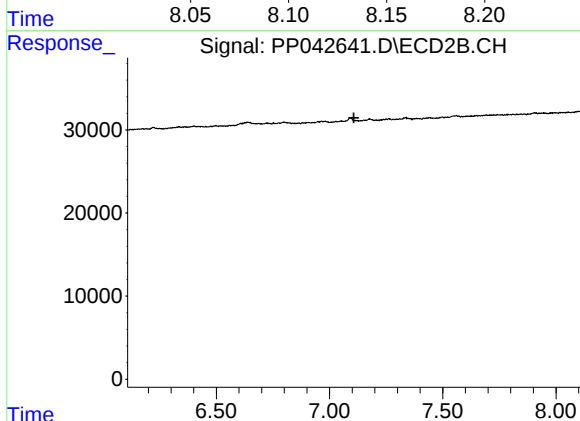


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.108 min
Response: 0
Conc: N.D.

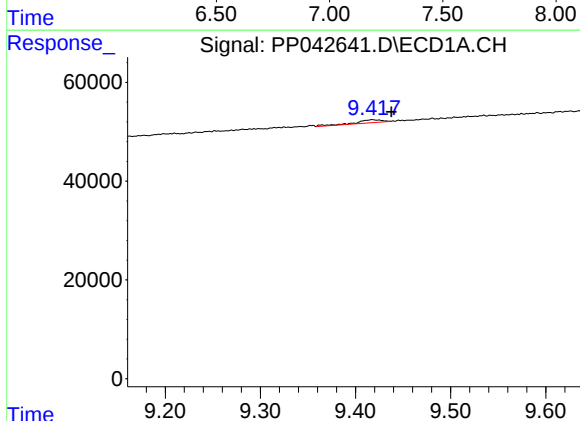


#39 AR-1262-4

R.T.: 9.418 min
Delta R.T.: -0.020 min
Response: 11734
Conc: 24.28 ng/ml

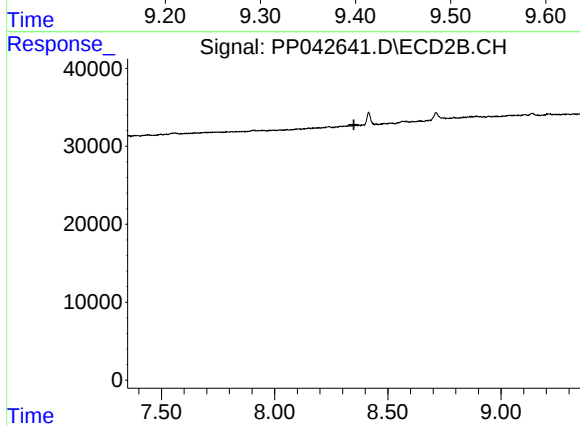

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.350 min
Response: 0
Conc: N.D.

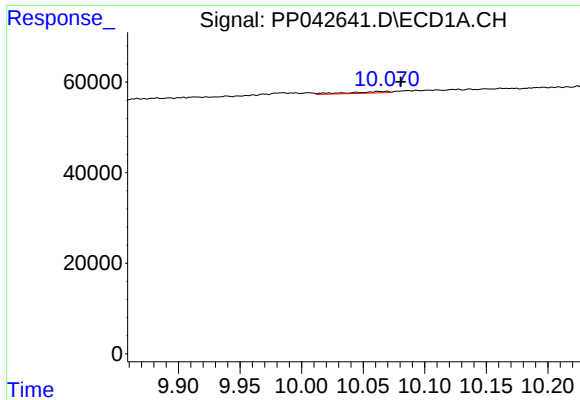

#40 AR-1262-5


R.T.: 10.070 min
Delta R.T.: -0.011 min
Response: 7873
Conc: 16.14 ng/ml

Instrument :
ECD_P
ClientSampleId :

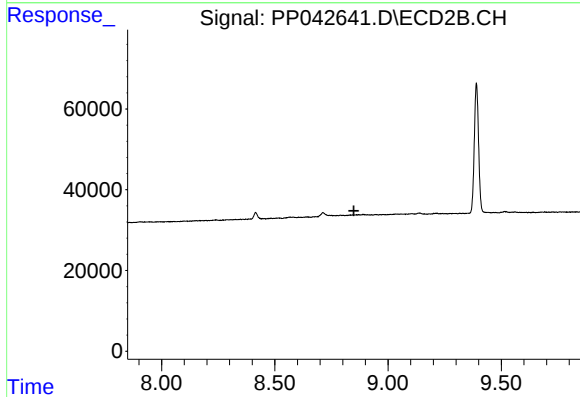


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 8.849 min
Response: 0
Conc: N.D.

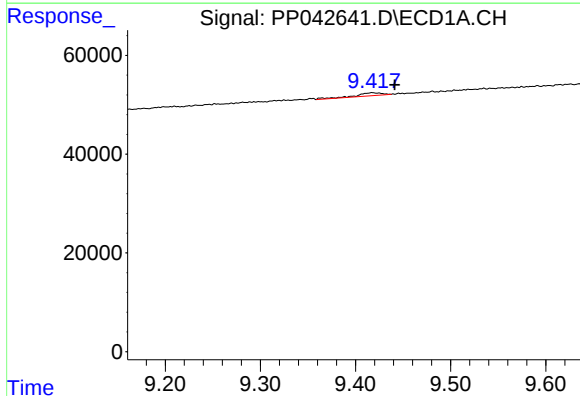


#42 AR-1268-2

R.T.: 9.418 min
Delta R.T.: -0.023 min
Response: 11734
Conc: 7.76 ng/ml

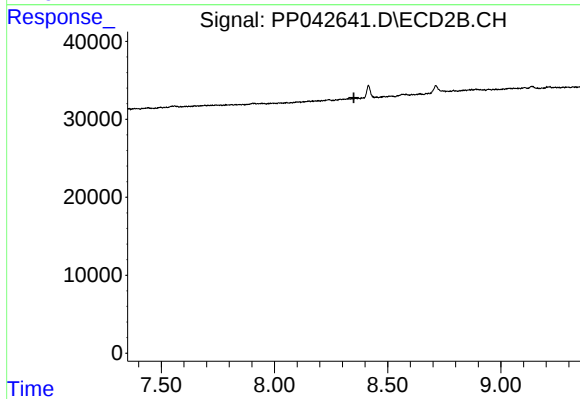

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.351 min
Response: 0
Conc: N.D.

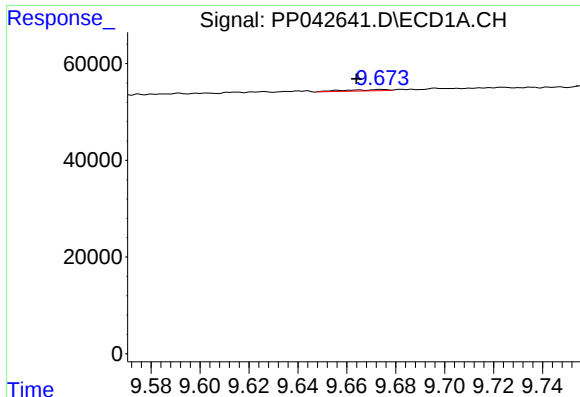

#43 AR-1268-3


R.T.: 9.674 min
Delta R.T.: 0.010 min
Response: 3451
Conc: 2.56 ng/ml

Instrument :
ECD_P
ClientSampleId :

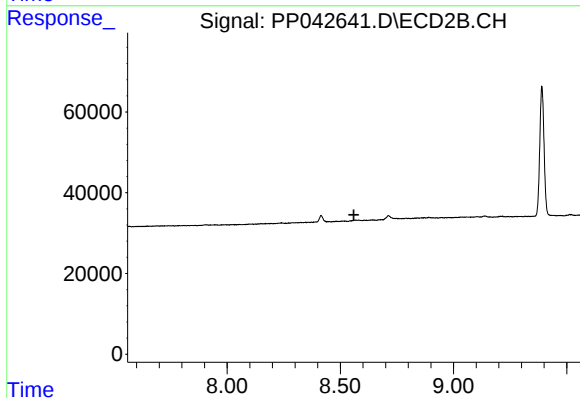


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.560 min
Response: 0
Conc: N.D.

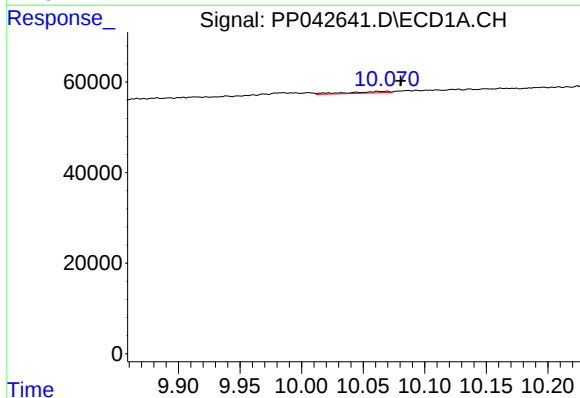


#44 AR-1268-4

R.T.: 10.070 min
Delta R.T.: -0.011 min
Response: 7873
Conc: 14.38 ng/ml

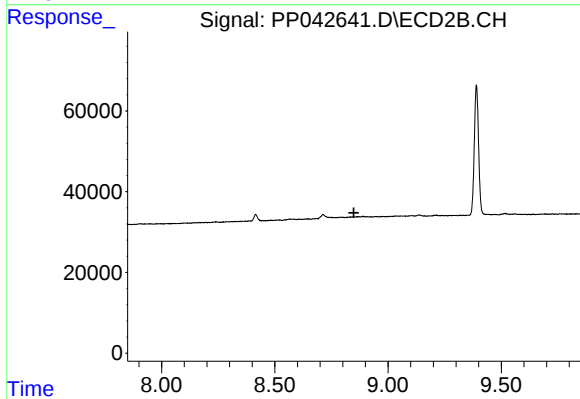

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 8.849 min
Response: 0
Conc: N.D.

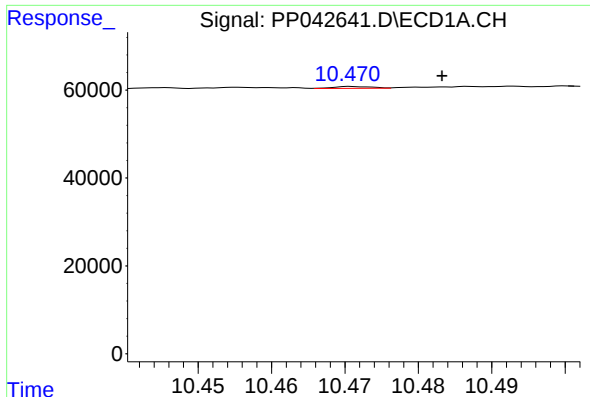

#45 AR-1268-5

R.T.: 10.471 min
Delta R.T.: -0.012 min
Response: 1497
Conc: 0.34 ng/ml

Instrument :
ECD_P
ClientSampleId :

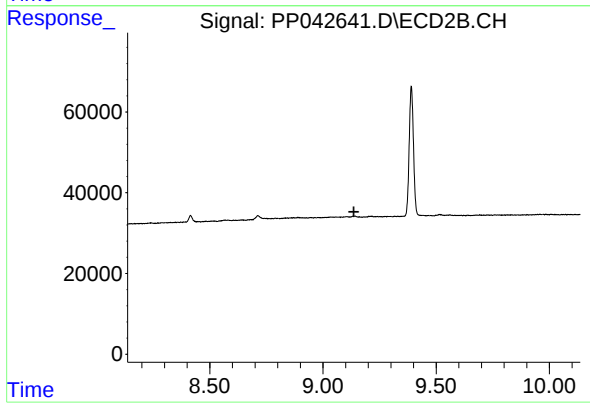

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.137 min
Response: 0
Conc: N.D.