

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010622\
 Data File : PP042671.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jan 2022 5:49
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 06:24:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 05 12:01:35 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.884	4.050	404813	535326	20.895	20.450
2)	SA Decachlor...	10.824	9.390	265187	430506	22.605	21.906
Target Compounds							
9)	L2 AR-1221-2	5.228	0.000	536	0	3.387	N.D. #
20)	L4 AR-1242-5	0.000	6.220f	0	10556	N.D.	14.392 #
25)	L5 AR-1248-5	0.000	6.220	0	10556	N.D.	10.639 #
26)	L6 AR-1254-1	0.000	6.220f	0	10556	N.D.	6.855 #
28)	L6 AR-1254-3	7.702	0.000	10239	0	11.177	N.D. #
29)	L6 AR-1254-4	7.974	0.000	1264	0	2.111	N.D. #
30)	L6 AR-1254-5	8.425	0.000	828	0	1.310	N.D. #
32)	L7 AR-1260-2	0.000	7.091f	0	16264	N.D.	10.698 #
33)	L7 AR-1260-3	8.494	0.000	1307	0	2.359	N.D. #
34)	L7 AR-1260-4	8.722	0.000	821	0	1.244	N.D. #
35)	L7 AR-1260-5	9.033	0.000	1001	0	0.830	N.D. #
36)	L8 AR-1262-1	8.494	0.000	1307	0	1.669	N.D. #
37)	L8 AR-1262-2	9.033	0.000	1001	0	0.749	N.D. #
38)	L8 AR-1262-3	9.366f	0.000	651	0	0.987	N.D. #
39)	L8 AR-1262-4	9.442	0.000	423	0	0.875	N.D. #
40)	L8 AR-1262-5	10.075	0.000	607	0	1.244	N.D. #
41)	L9 AR-1268-1	9.366f	0.000	651	0	0.398	N.D. #
42)	L9 AR-1268-2	9.442	0.000	423	0	0.280	N.D. #
43)	L9 AR-1268-3	9.659	0.000	825	0	0.613	N.D. #
44)	L9 AR-1268-4	10.075	0.000	607	0	1.109	N.D. #
45)	L9 AR-1268-5	10.486	0.000	1797	0	0.403	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010622\
Data File : PP042671.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jan 2022 5:49
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 06:24:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 05 12:01:35 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

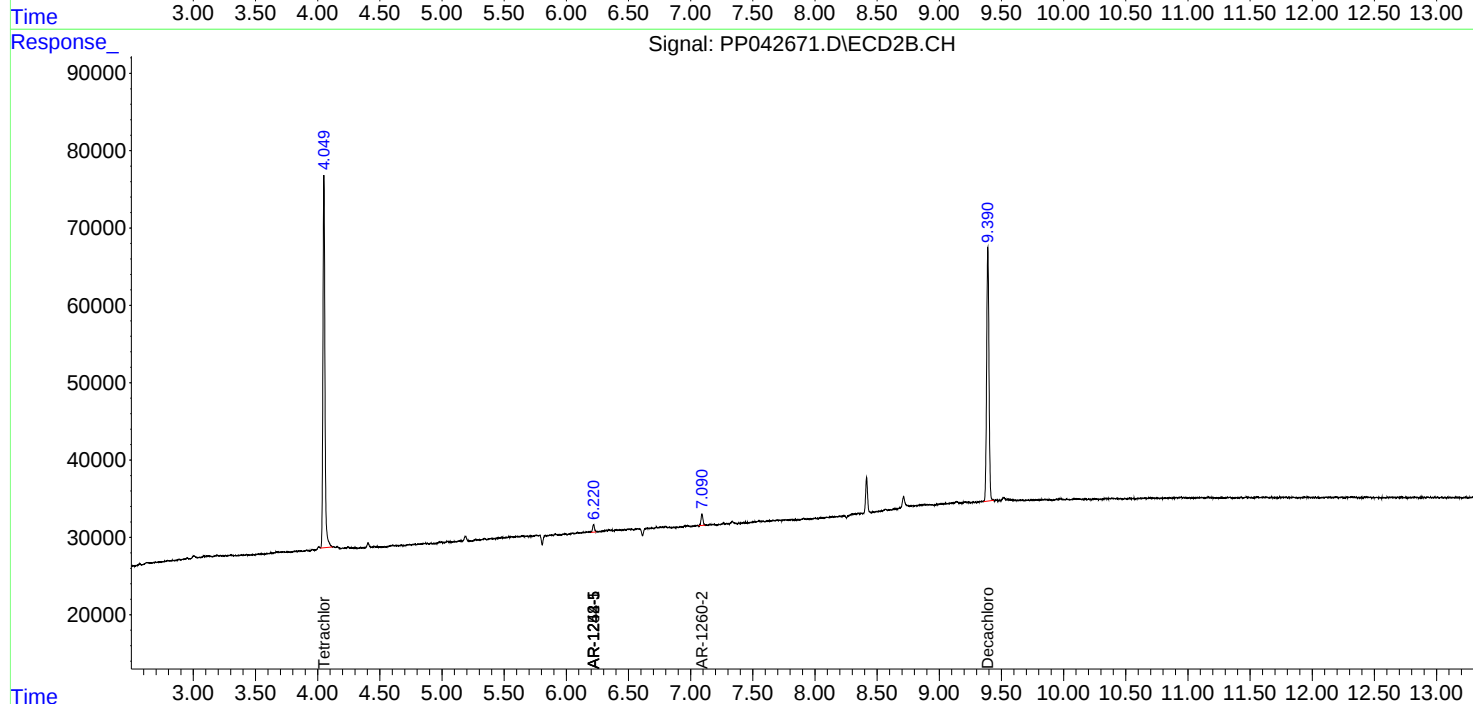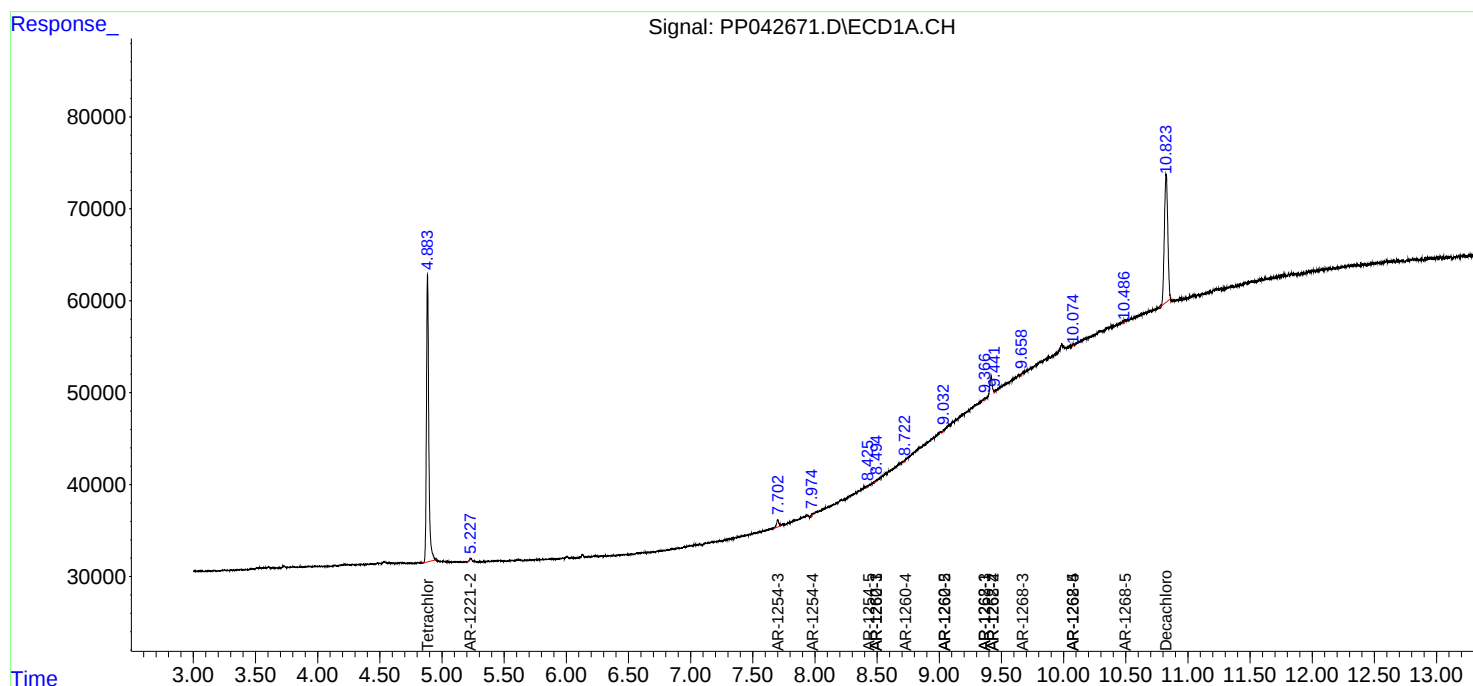


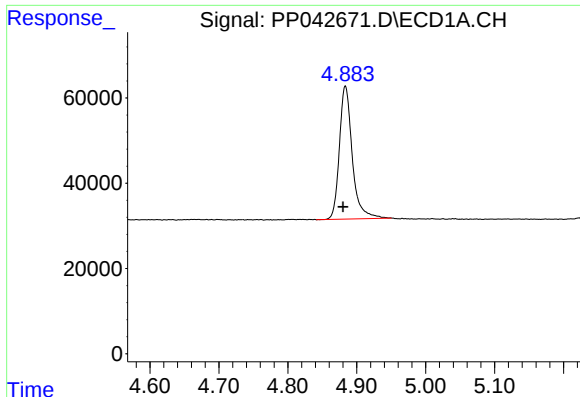

#1 Tetrachloro-m-xylene


R.T.: 4.884 min
Delta R.T.: 0.004 min
Response: 404813
Conc: 20.90 ng/ml

Instrument :
ECD_P
ClientSampleId :

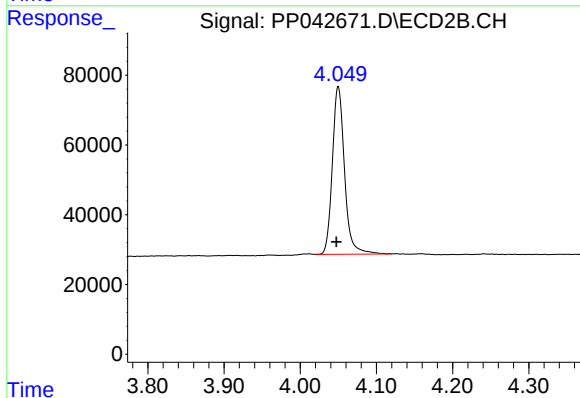


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: 0.003 min
Response: 535326
Conc: 20.45 ng/ml

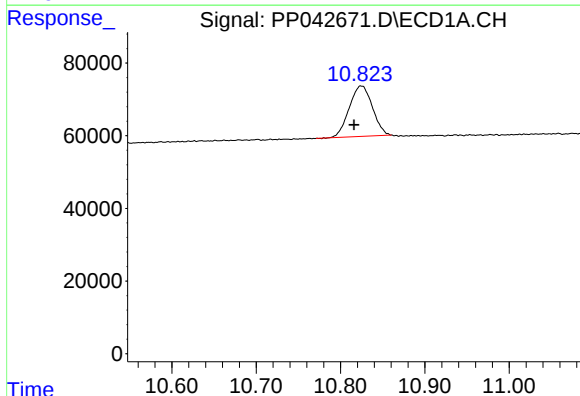


#2 Decachlorobiphenyl

R.T.: 10.824 min
Delta R.T.: 0.008 min
Response: 265187
Conc: 22.60 ng/ml

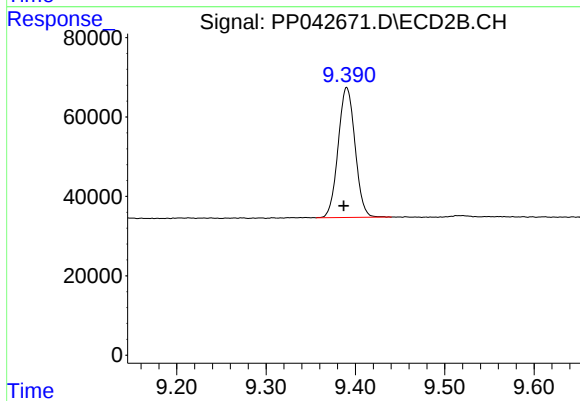

#2 Decachlorobiphenyl


R.T.: 9.390 min
Delta R.T.: 0.003 min
Response: 430506
Conc: 21.91 ng/ml

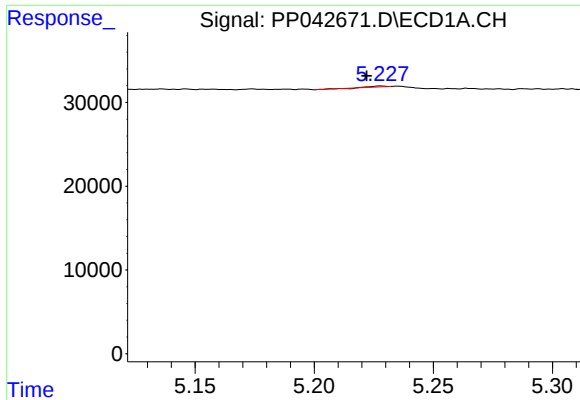

#9 AR-1221-2


R.T.: 5.228 min
Delta R.T.: 0.006 min
Response: 536
Conc: 3.39 ng/ml

Instrument :
ECD_P
ClientSampleId :

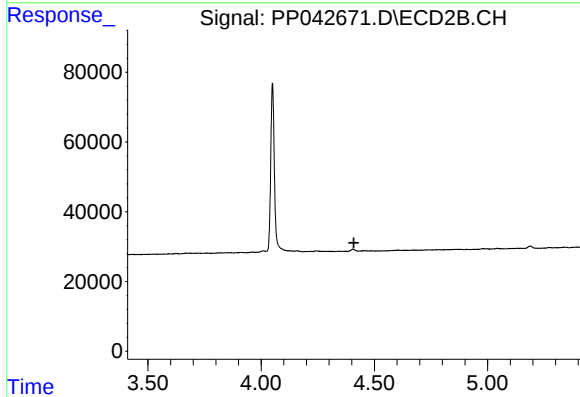


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.410 min
Response: 0
Conc: N.D.

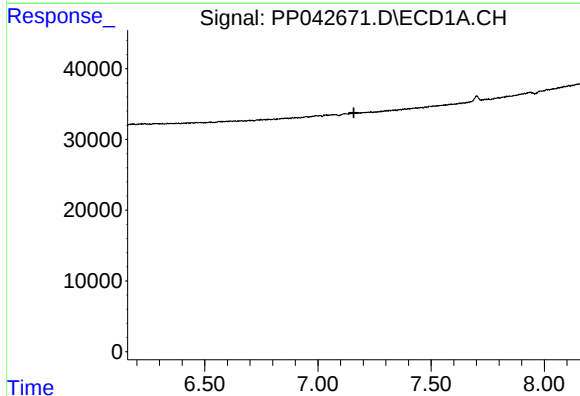


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 7.158 min
Response: 0
Conc: N.D.

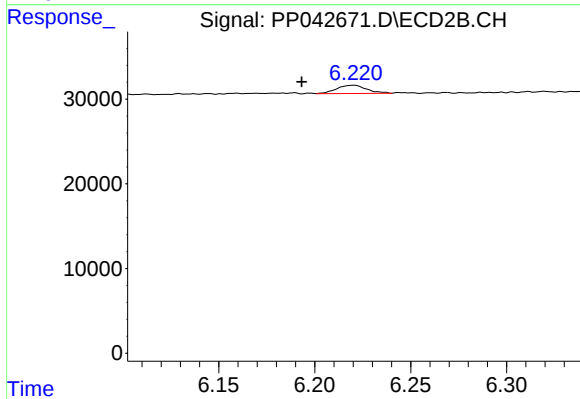

#20 AR-1242-5


R.T.: 6.220 min
Delta R.T.: 0.027 min
Response: 10556
Conc: 14.39 ng/ml

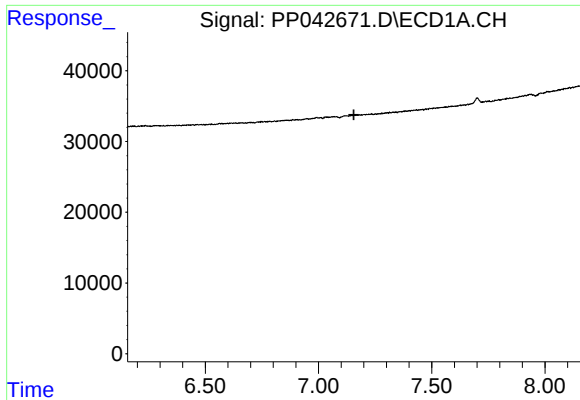

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.156 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

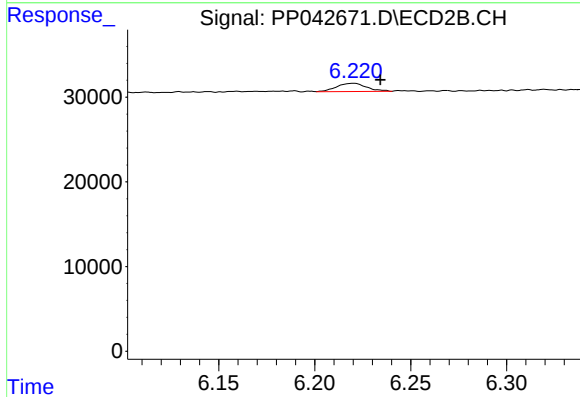


#25 AR-1248-5

R.T.: 6.220 min
Delta R.T.: -0.014 min
Response: 10556
Conc: 10.64 ng/ml

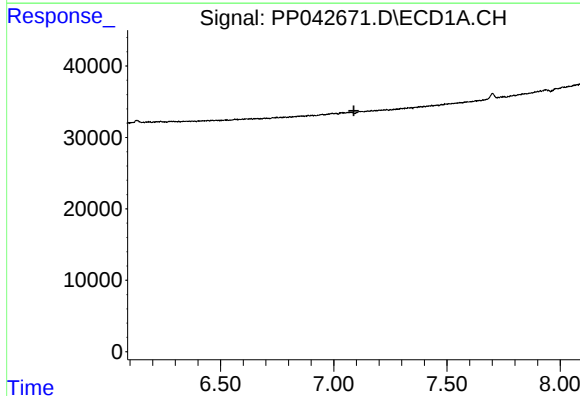


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 7.089 min
Response: 0
Conc: N.D.

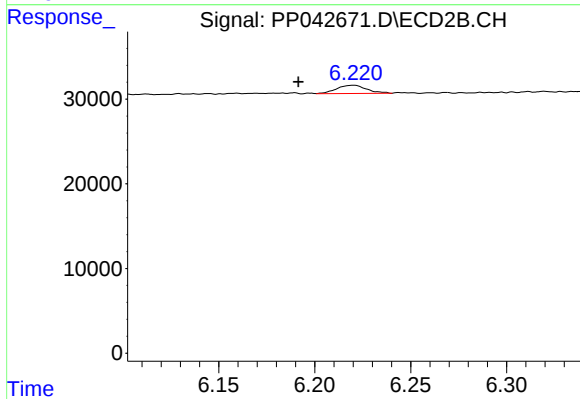

#26 AR-1254-1


R.T.: 6.220 min
Delta R.T.: 0.029 min
Response: 10556
Conc: 6.86 ng/ml

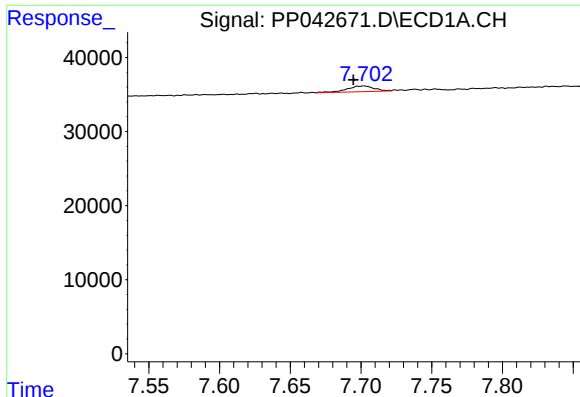

#28 AR-1254-3


R.T.: 7.702 min
Delta R.T.: 0.007 min
Response: 10239
Conc: 11.18 ng/ml

Instrument :
ECD_P
ClientSampleId :

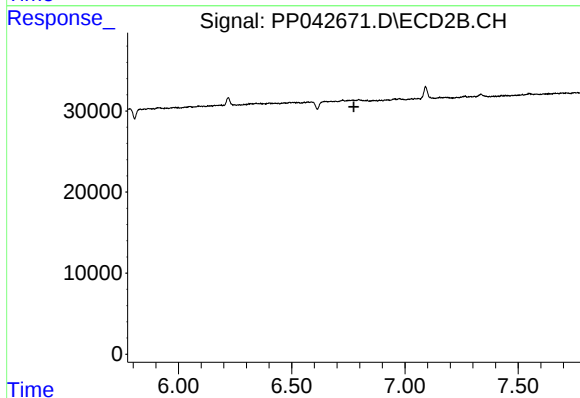


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.774 min
Response: 0
Conc: N.D.

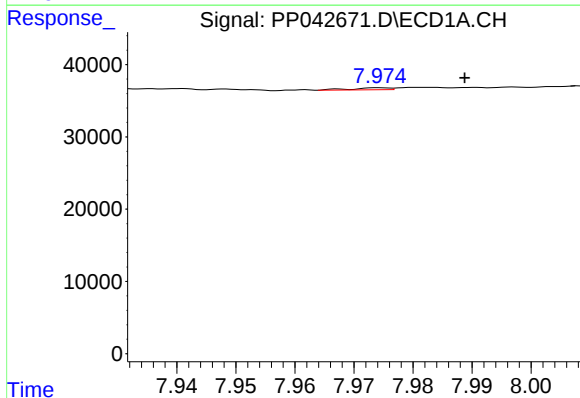


#29 AR-1254-4

R.T.: 7.974 min
Delta R.T.: -0.015 min
Response: 1264
Conc: 2.11 ng/ml

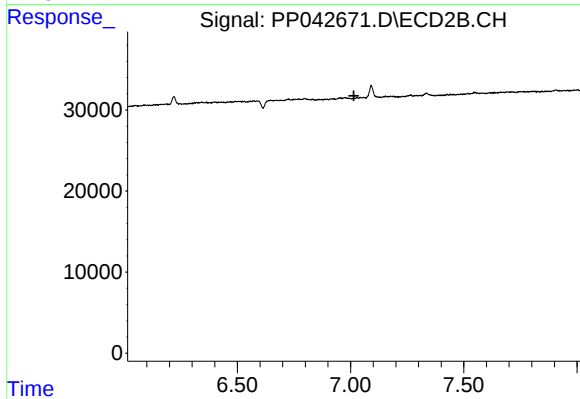

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 7.014 min
Response: 0
Conc: N.D.

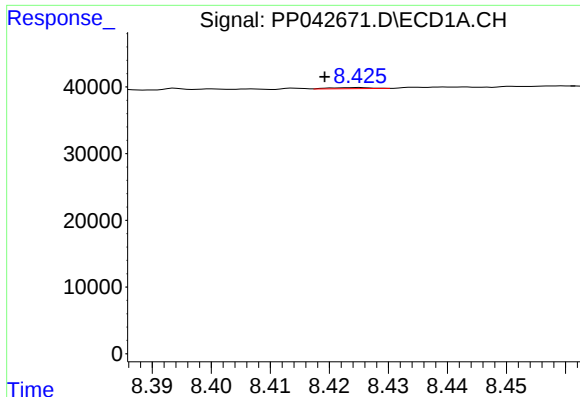

#30 AR-1254-5


R.T.: 8.425 min
Delta R.T.: 0.006 min
Response: 828
Conc: 1.31 ng/ml

Instrument :
ECD_P
ClientSampleId :

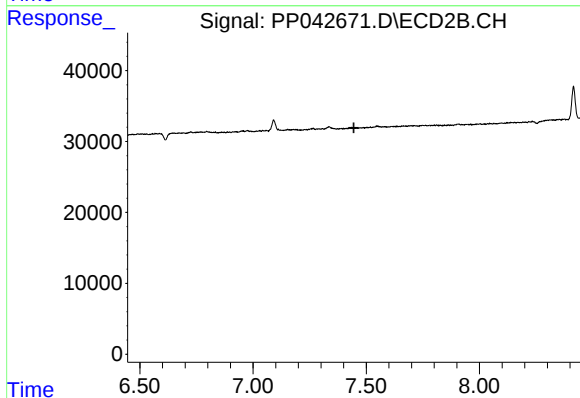


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.445 min
Response: 0
Conc: N.D.

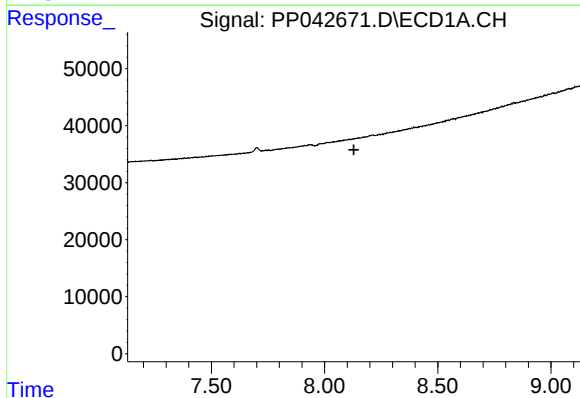


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 8.130 min
Response: 0
Conc: N.D.

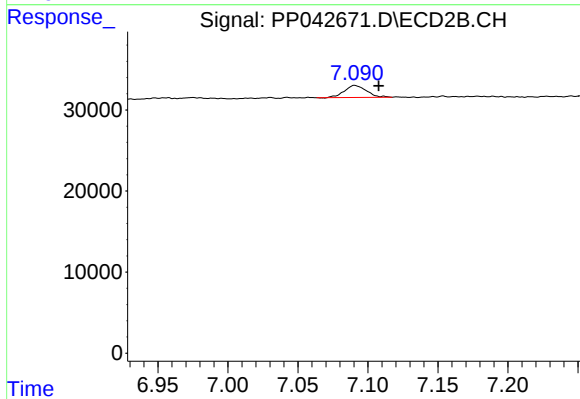

#32 AR-1260-2


R.T.: 7.091 min
Delta R.T.: -0.017 min
Response: 16264
Conc: 10.70 ng/ml

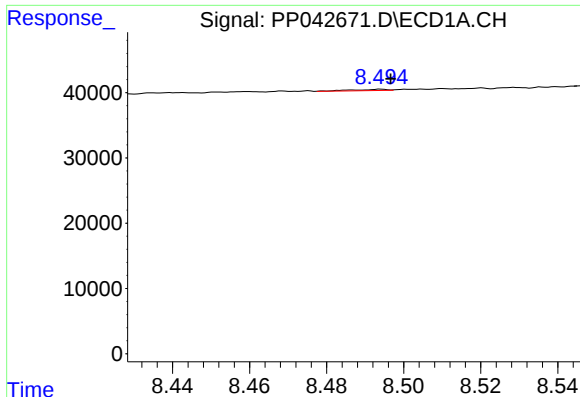

#33 AR-1260-3


R.T.: 8.494 min
Delta R.T.: -0.002 min
Response: 1307
Conc: 2.36 ng/ml

Instrument :
ECD_P
ClientSampleId :

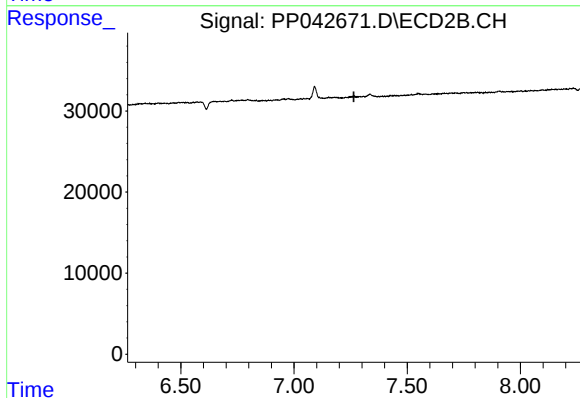


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.264 min
Response: 0
Conc: N.D.

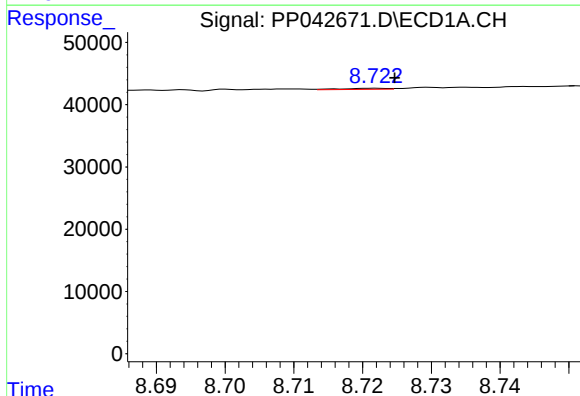


#34 AR-1260-4

R.T.: 8.722 min
Delta R.T.: -0.003 min
Response: 821
Conc: 1.24 ng/ml

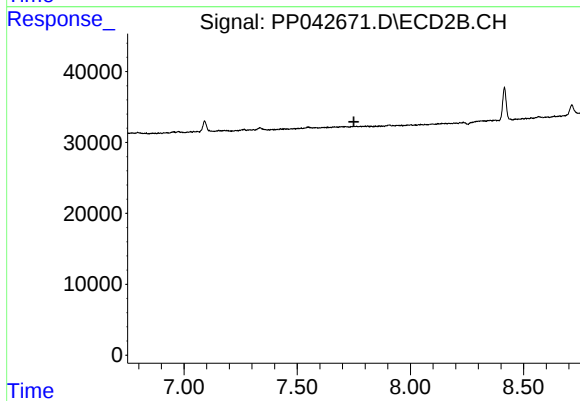

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.750 min
Response: 0
Conc: N.D.

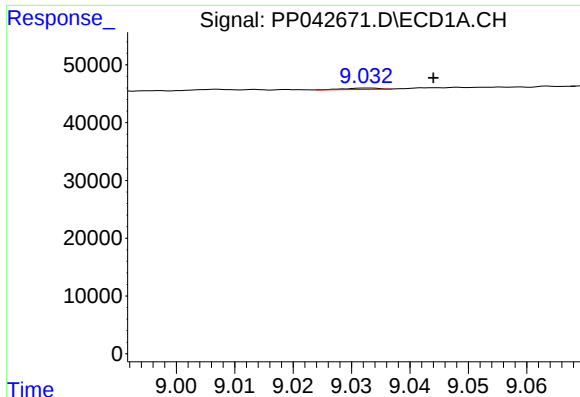

#35 AR-1260-5


R.T.: 9.033 min
Delta R.T.: -0.011 min
Response: 1001
Conc: 0.83 ng/ml

Instrument :
ECD_P
ClientSampleId :

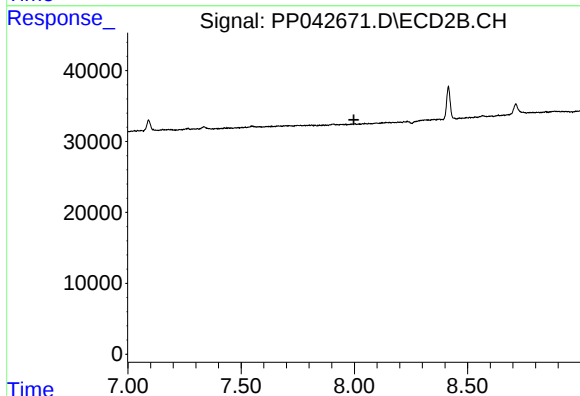


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.998 min
Response: 0
Conc: N.D.

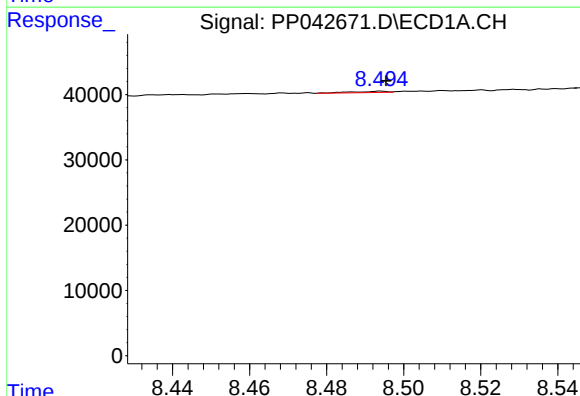


#36 AR-1262-1

R.T.: 8.494 min
Delta R.T.: -0.001 min
Response: 1307
Conc: 1.67 ng/ml

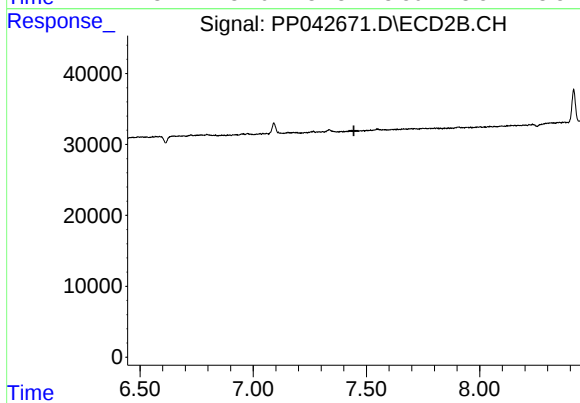

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 7.444 min
Response: 0
Conc: N.D.

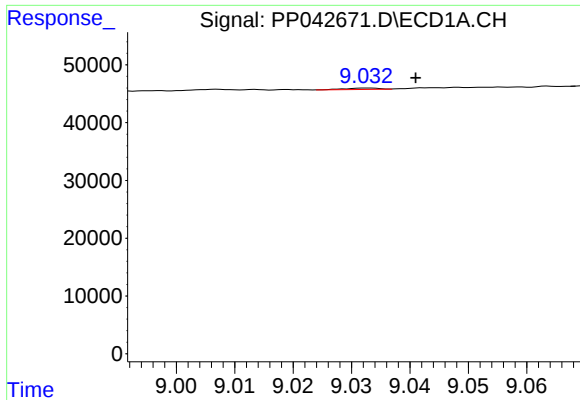

#37 AR-1262-2


R.T.: 9.033 min
Delta R.T.: -0.008 min
Response: 1001
Conc: 0.75 ng/ml

Instrument :
ECD_P
ClientSampleId :

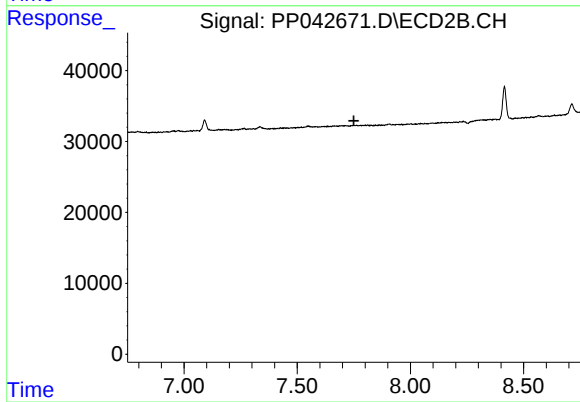


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.750 min
Response: 0
Conc: N.D.

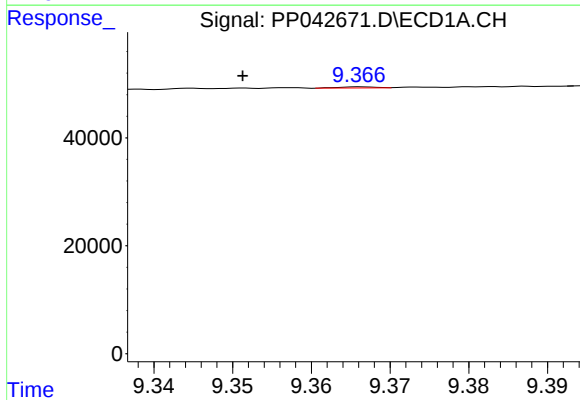


#38 AR-1262-3

R.T.: 9.366 min
Delta R.T.: 0.015 min
Response: 651
Conc: 0.99 ng/ml

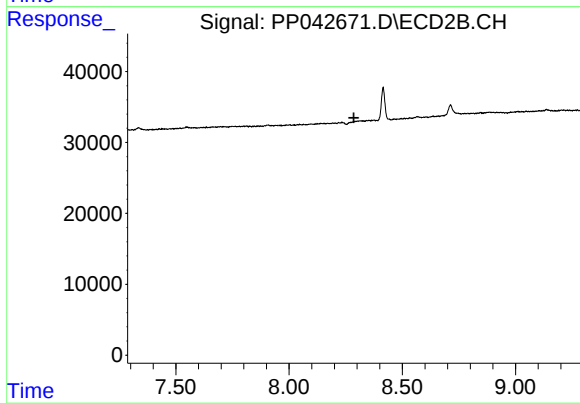

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 8.286 min
Response: 0
Conc: N.D.

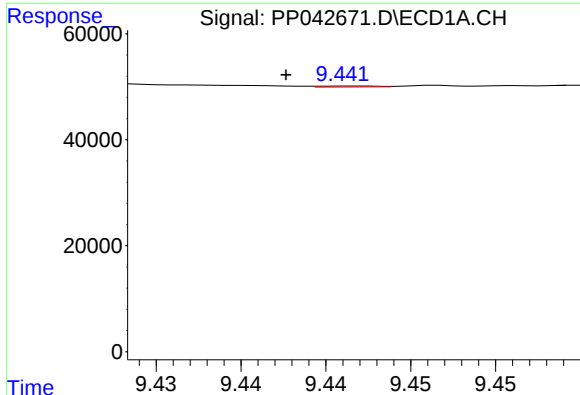

#39 AR-1262-4


R.T.: 9.442 min
Delta R.T.: 0.004 min
Response: 423
Conc: 0.88 ng/ml

Instrument :
ECD_P
ClientSampleId :

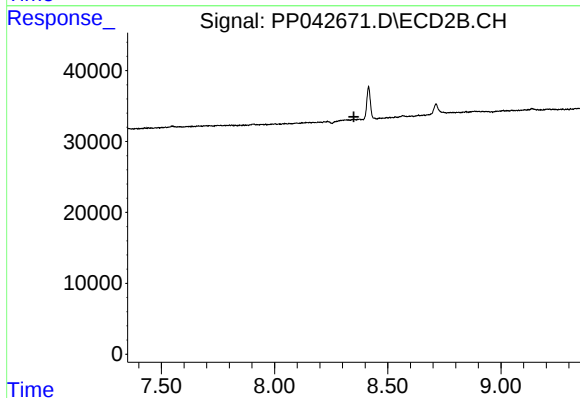


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.350 min
Response: 0
Conc: N.D.

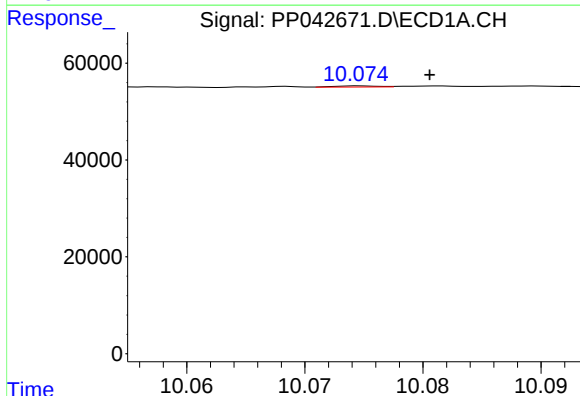


#40 AR-1262-5

R.T.: 10.075 min
Delta R.T.: -0.006 min
Response: 607
Conc: 1.24 ng/ml

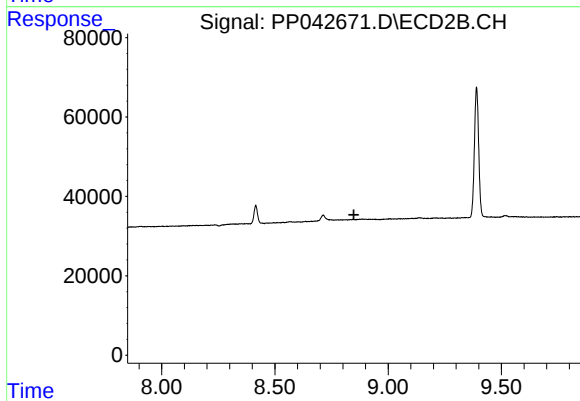

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 8.849 min
Response: 0
Conc: N.D.

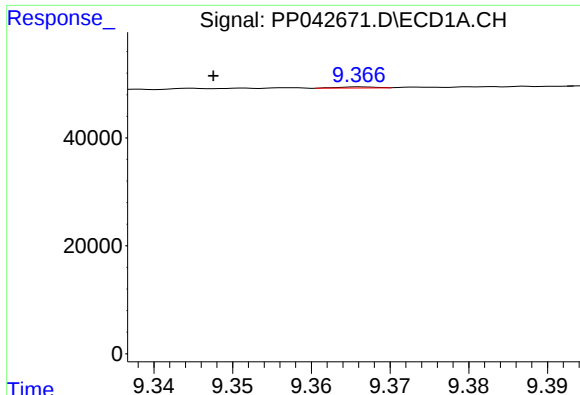

#41 AR-1268-1


R.T.: 9.366 min
Delta R.T.: 0.019 min
Response: 651
Conc: 0.40 ng/ml

Instrument :
ECD_P
ClientSampleId :

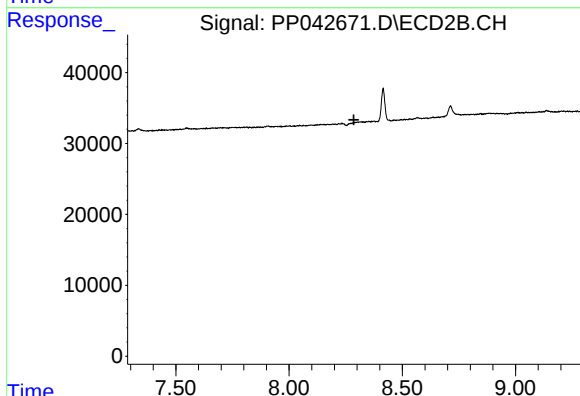


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.286 min
Response: 0
Conc: N.D.

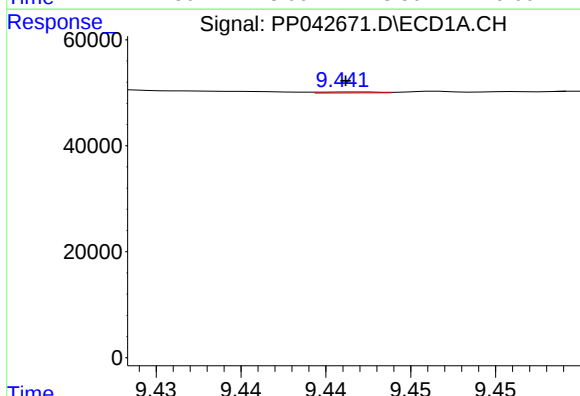


#42 AR-1268-2

R.T.: 9.442 min
Delta R.T.: 0.000 min
Response: 423
Conc: 0.28 ng/ml

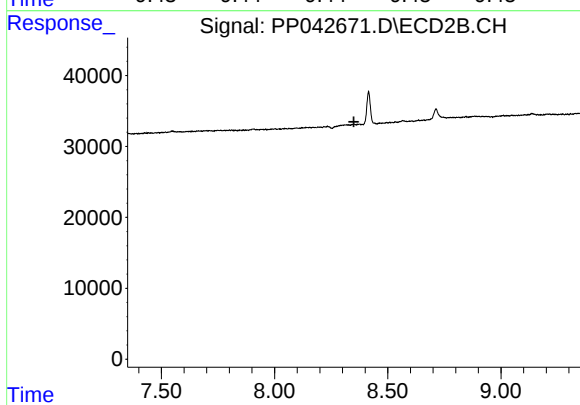

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.351 min
Response: 0
Conc: N.D.

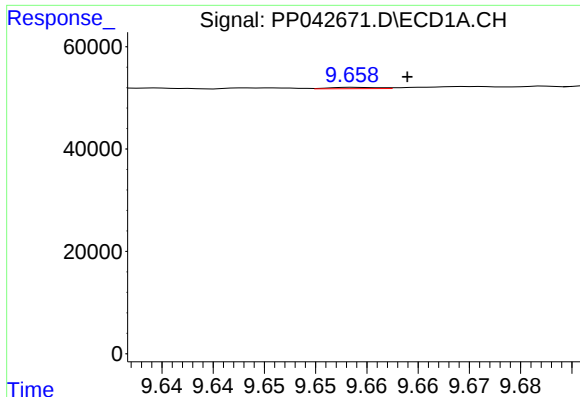

#43 AR-1268-3


R.T.: 9.659 min
Delta R.T.: -0.005 min
Response: 825
Conc: 0.61 ng/ml

Instrument :
ECD_P
ClientSampleId :

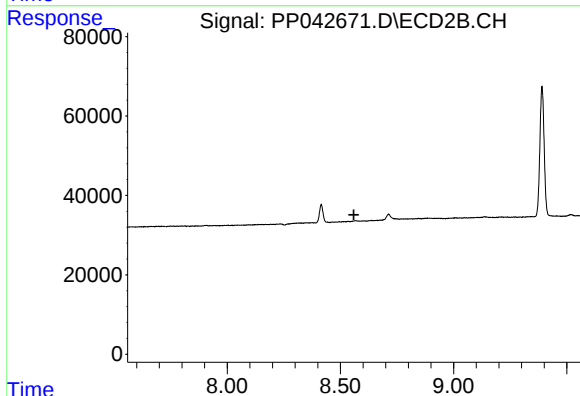


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.560 min
Response: 0
Conc: N.D.

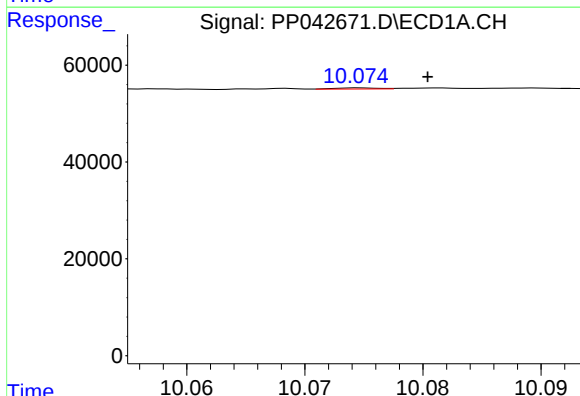


#44 AR-1268-4

R.T.: 10.075 min
Delta R.T.: -0.006 min
Response: 607
Conc: 1.11 ng/ml

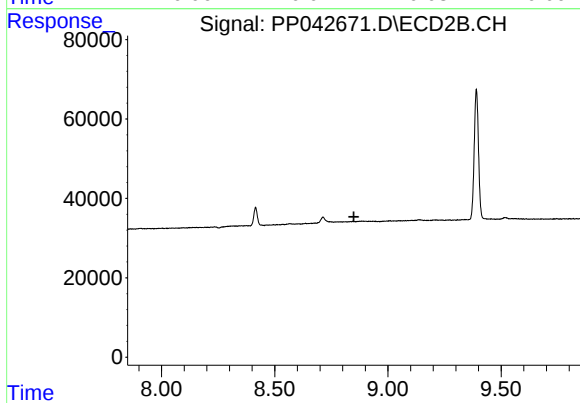

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 8.849 min
Response: 0
Conc: N.D.

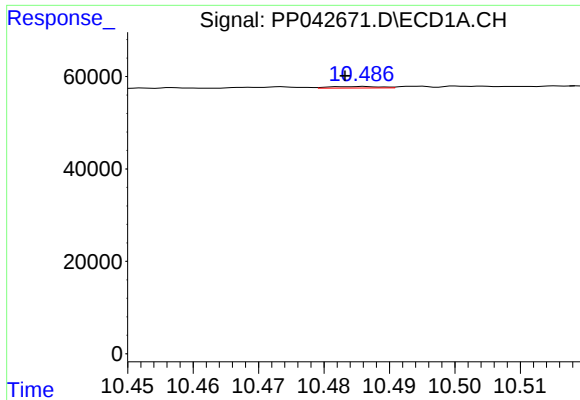

#45 AR-1268-5

R.T.: 10.486 min
Delta R.T.: 0.003 min
Response: 1797
Conc: 0.40 ng/ml

Instrument :
ECD_P
ClientSampleId :

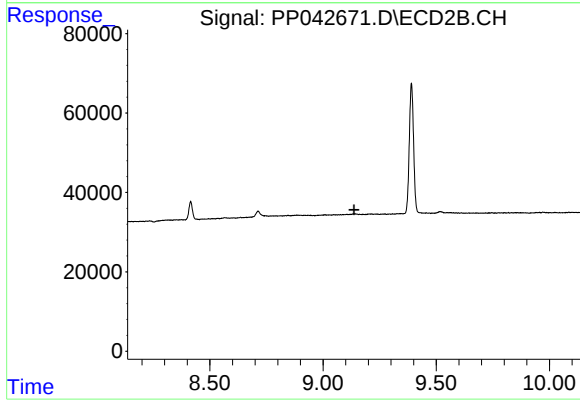

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.137 min
Response: 0
Conc: N.D.