

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010622\
 Data File : PP042672.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jan 2022 6:06
 Operator : AJ\MA
 Sample : N1032-05 10X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 06:25:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 05 12:01:35 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.885	4.050	30396	45221	1.569	1.727
2)	SA Decachlor...	10.823	9.392	28344	33671	2.416	1.713 #
Target Compounds							
28)	L6 AR-1254-3	7.700	0.000	8142	0	8.888	N.D. #
29)	L6 AR-1254-4	7.977	0.000	812	0	1.355	N.D. #
30)	L6 AR-1254-5	8.423	0.000	1786	0	2.824	N.D. #
32)	L7 AR-1260-2	8.136	7.092f	1542	11664	2.192	7.672 #
33)	L7 AR-1260-3	8.500	0.000	773	0	1.395	N.D. #
34)	L7 AR-1260-4	8.721	0.000	2505	0	3.797	N.D. #
35)	L7 AR-1260-5	9.036	0.000	1968	0	1.631	N.D. #
36)	L8 AR-1262-1	8.491	0.000	832	0	1.063	N.D. #
37)	L8 AR-1262-2	9.036	0.000	1968	0	1.471	N.D. #
38)	L8 AR-1262-3	9.357	0.000	707	0	1.072	N.D. #
39)	L8 AR-1262-4	9.435	0.000	1916	0	3.964	N.D. #
41)	L9 AR-1268-1	9.357	0.000	707	0	0.432	N.D. #
42)	L9 AR-1268-2	9.447	0.000	1319	0	0.872	N.D. #
43)	L9 AR-1268-3	9.666	0.000	335	0	0.249	N.D. #
45)	L9 AR-1268-5	10.504f	0.000	1563	0	0.350	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010622\
Data File : PP042672.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jan 2022 6:06
Operator : AJ\MA
Sample : N1032-05 10X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 06:25:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 05 12:01:35 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

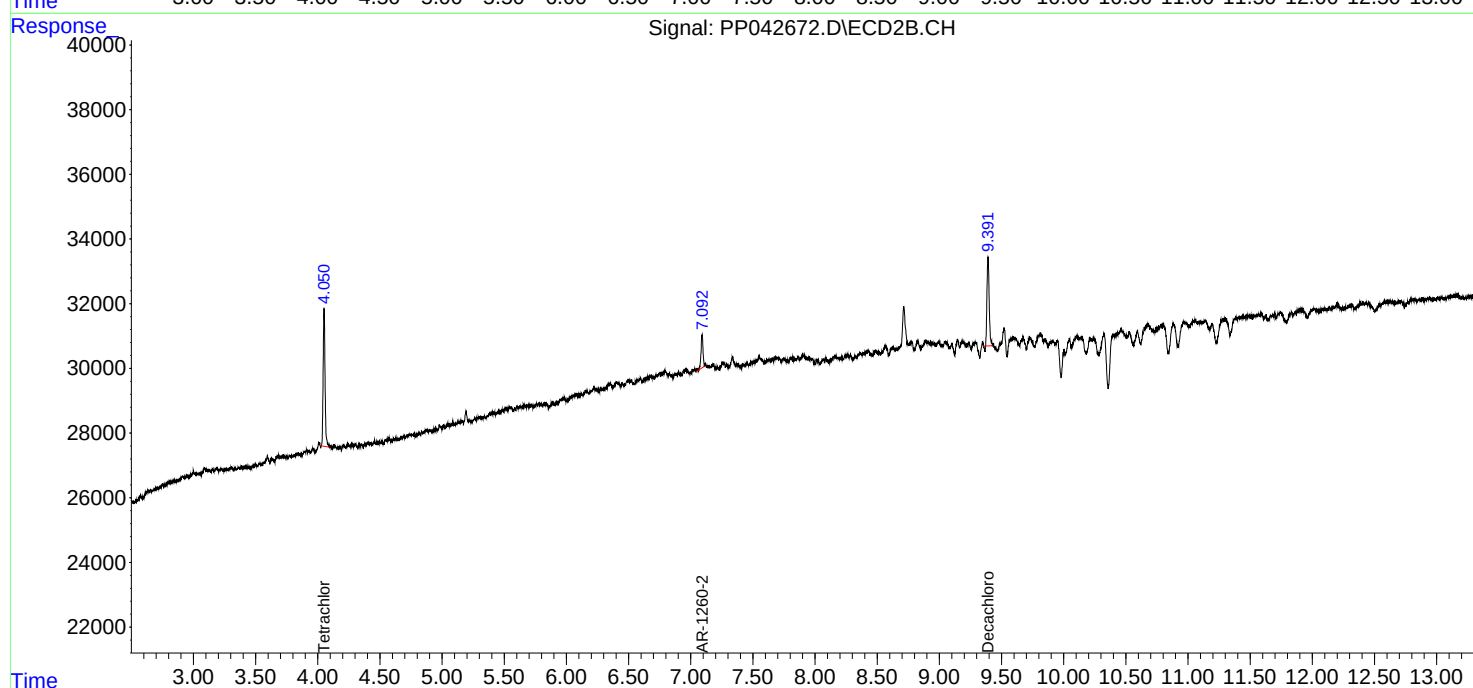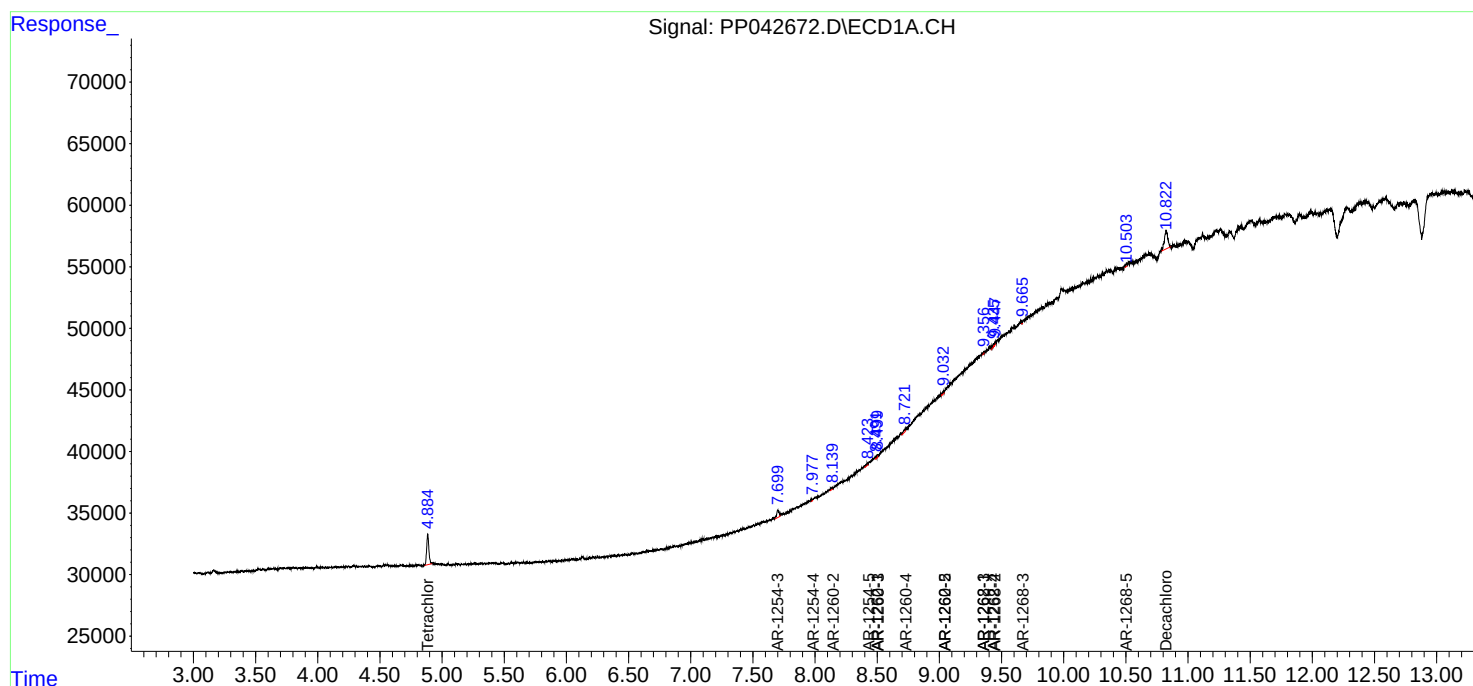


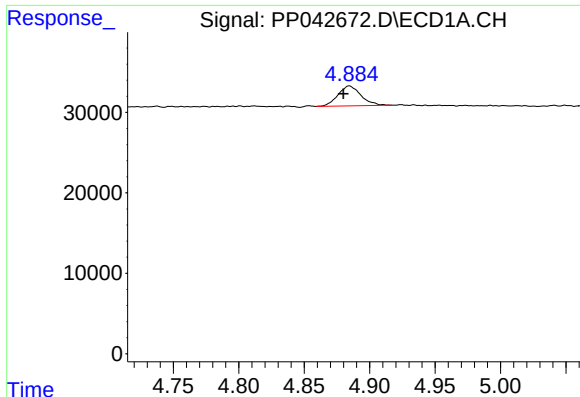

#1 Tetrachloro-m-xylene


R.T.: 4.885 min
Delta R.T.: 0.005 min
Response: 30396
Conc: 1.57 ng/ml

Instrument :
ECD_P
ClientSampleId :

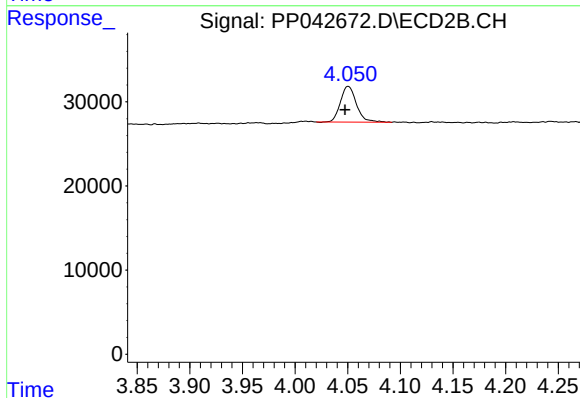


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: 0.003 min
Response: 45221
Conc: 1.73 ng/ml

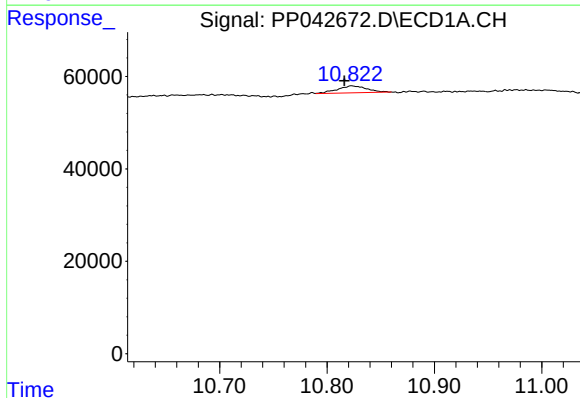


#2 Decachlorobiphenyl

R.T.: 10.823 min
Delta R.T.: 0.007 min
Response: 28344
Conc: 2.42 ng/ml

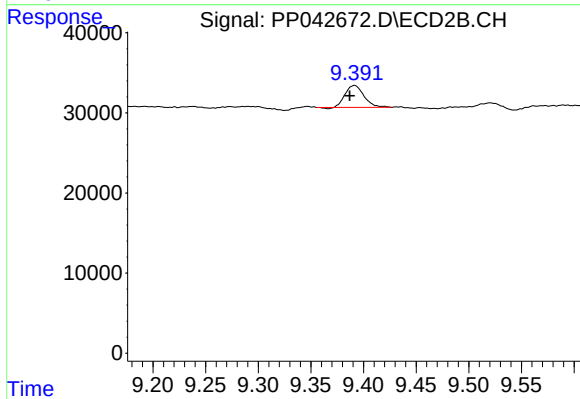

#2 Decachlorobiphenyl


R.T.: 9.392 min
Delta R.T.: 0.005 min
Response: 33671
Conc: 1.71 ng/ml

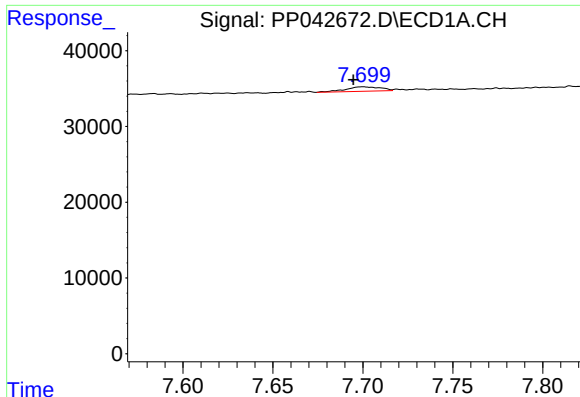

#28 AR-1254-3


R.T.: 7.700 min
Delta R.T.: 0.005 min
Response: 8142
Conc: 8.89 ng/ml

Instrument :
ECD_P
ClientSampleId :

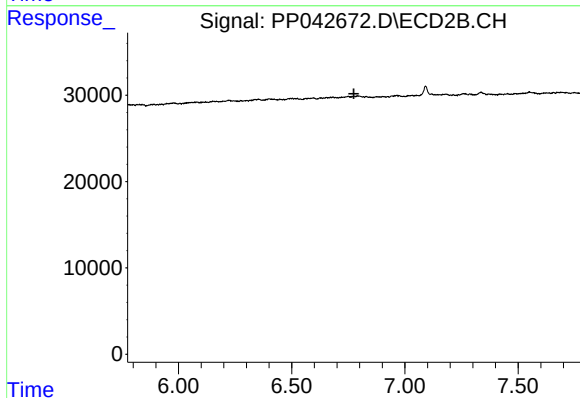


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.774 min
Response: 0
Conc: N.D.

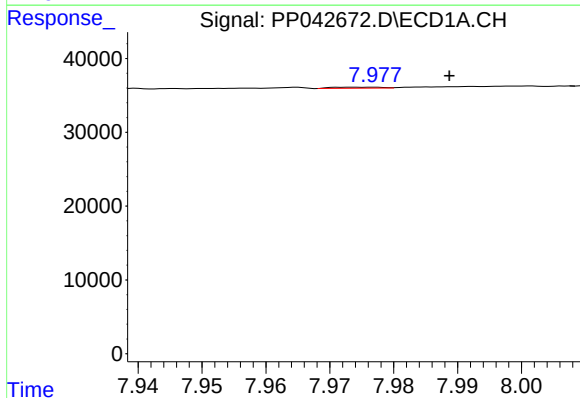


#29 AR-1254-4

R.T.: 7.977 min
Delta R.T.: -0.012 min
Response: 812
Conc: 1.36 ng/ml

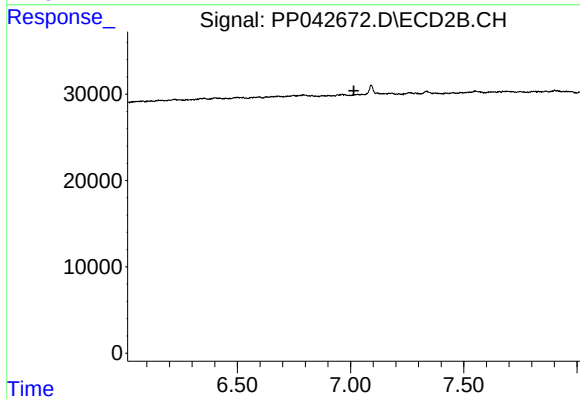

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 7.014 min
Response: 0
Conc: N.D.

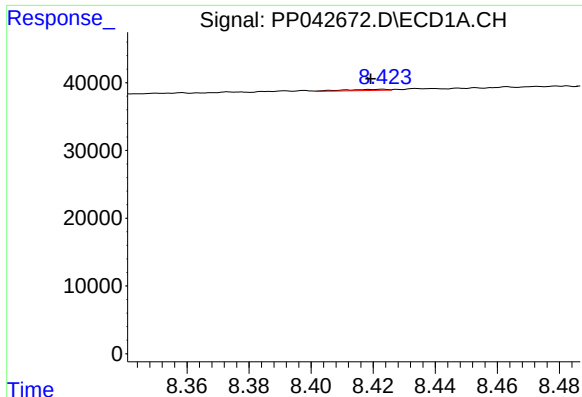

#30 AR-1254-5


R.T.: 8.423 min
Delta R.T.: 0.004 min
Response: 1786
Conc: 2.82 ng/ml

Instrument :
ECD_P
ClientSampleId :

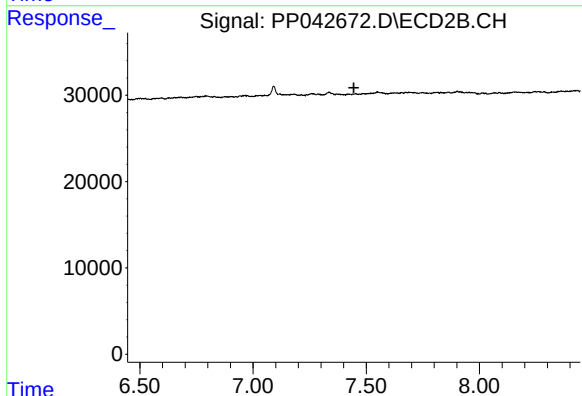


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.445 min
Response: 0
Conc: N.D.

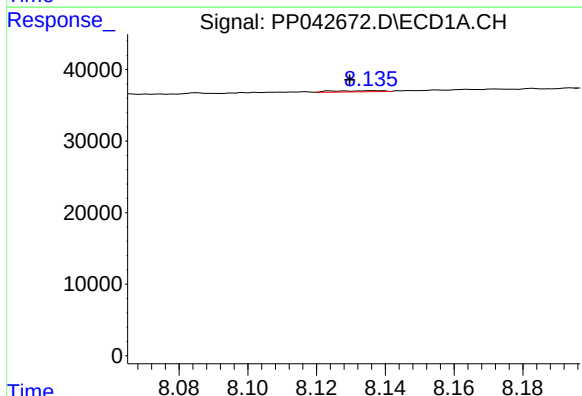


#32 AR-1260-2

R.T.: 8.136 min
Delta R.T.: 0.006 min
Response: 1542
Conc: 2.19 ng/ml

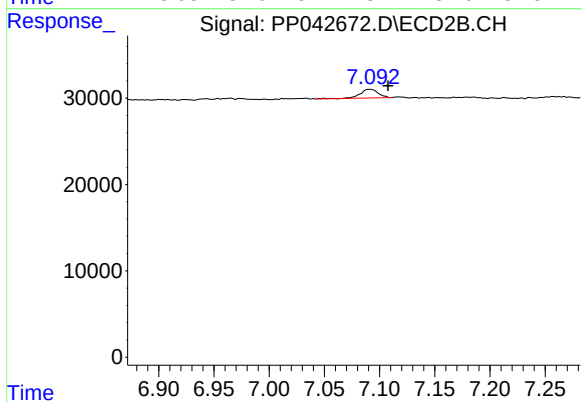

#32 AR-1260-2


R.T.: 7.092 min
Delta R.T.: -0.016 min
Response: 11664
Conc: 7.67 ng/ml

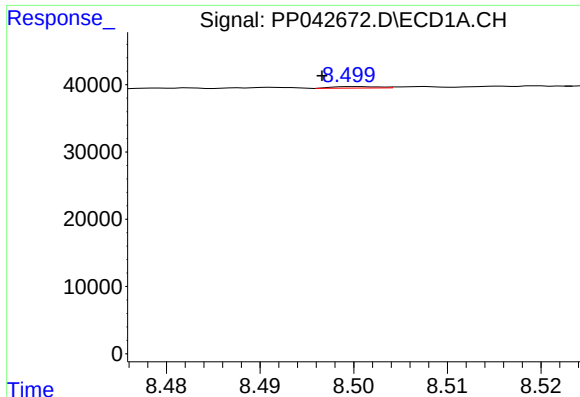

#33 AR-1260-3


R.T.: 8.500 min
Delta R.T.: 0.004 min
Response: 773
Conc: 1.39 ng/ml

Instrument :
ECD_P
ClientSampleId :

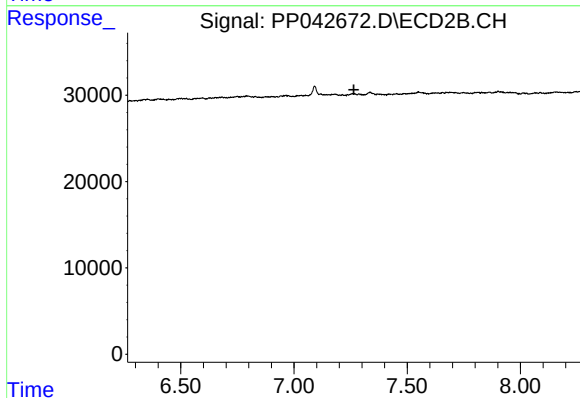


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.264 min
Response: 0
Conc: N.D.

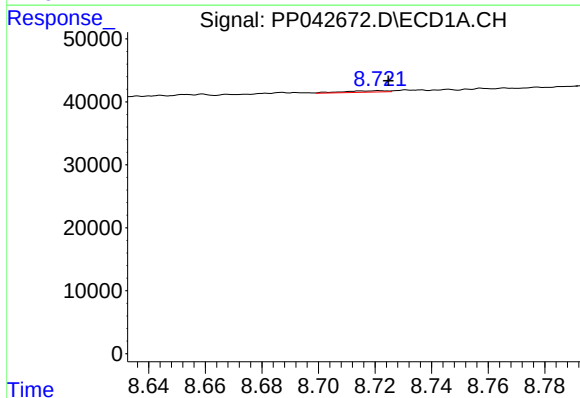


#34 AR-1260-4

R.T.: 8.721 min
Delta R.T.: -0.003 min
Response: 2505
Conc: 3.80 ng/ml

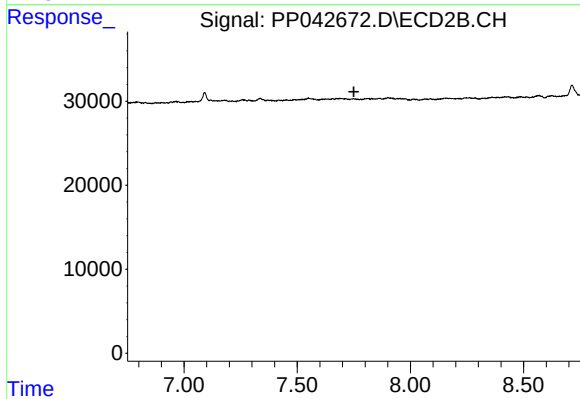

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.750 min
Response: 0
Conc: N.D.

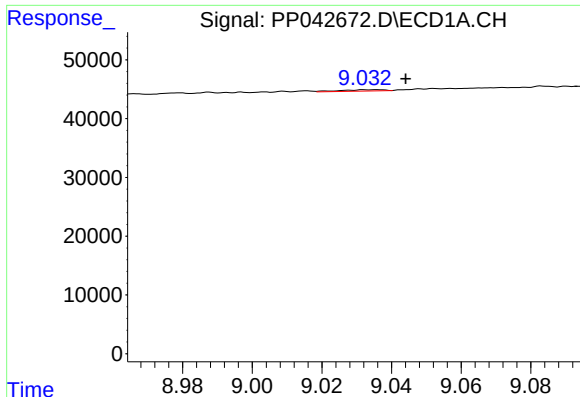

#35 AR-1260-5


R.T.: 9.036 min
Delta R.T.: -0.008 min
Response: 1968
Conc: 1.63 ng/ml

Instrument :
ECD_P
ClientSampleId :

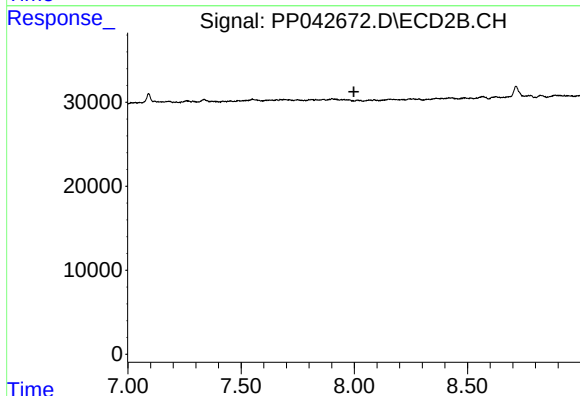


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.998 min
Response: 0
Conc: N.D.

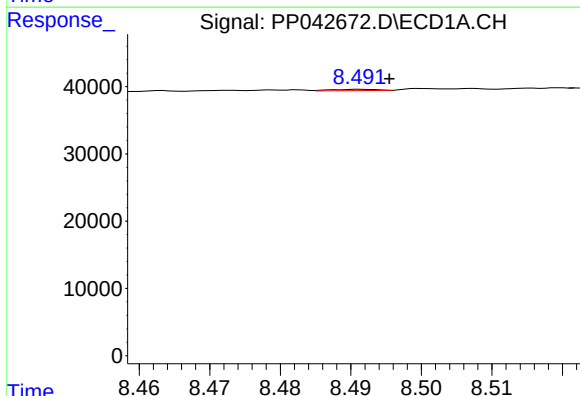


#36 AR-1262-1

R.T.: 8.491 min
Delta R.T.: -0.004 min
Response: 832
Conc: 1.06 ng/ml

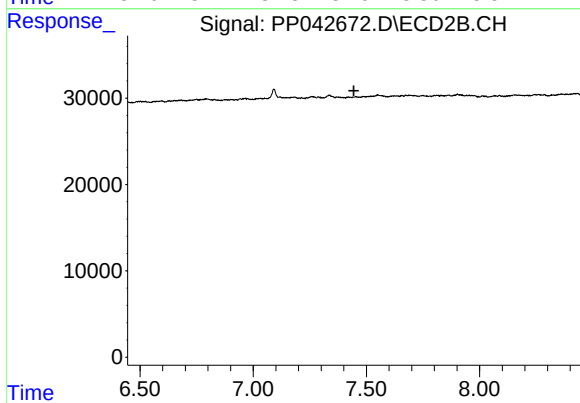

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 7.444 min
Response: 0
Conc: N.D.

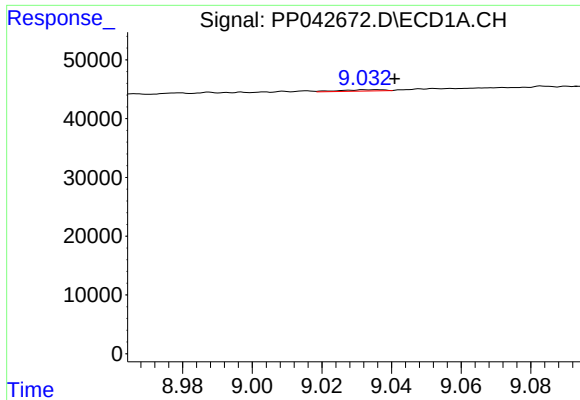

#37 AR-1262-2


R.T.: 9.036 min
Delta R.T.: -0.005 min
Response: 1968
Conc: 1.47 ng/ml

Instrument :
ECD_P
ClientSampleId :

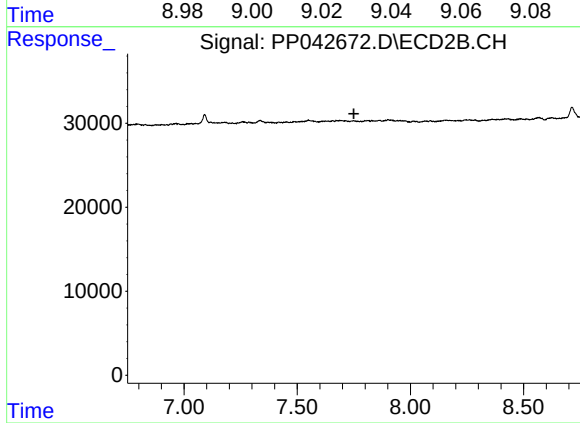


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.750 min
Response: 0
Conc: N.D.

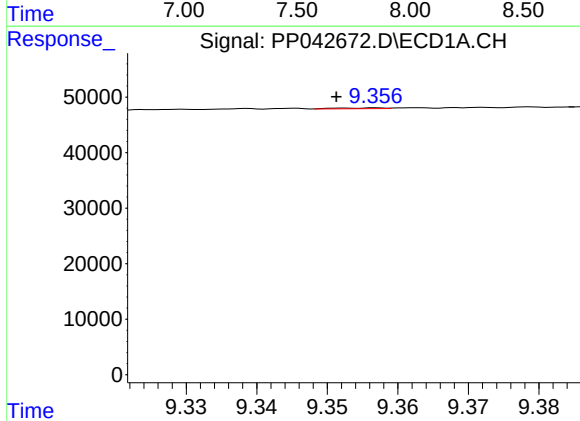


#38 AR-1262-3

R.T.: 9.357 min
Delta R.T.: 0.006 min
Response: 707
Conc: 1.07 ng/ml

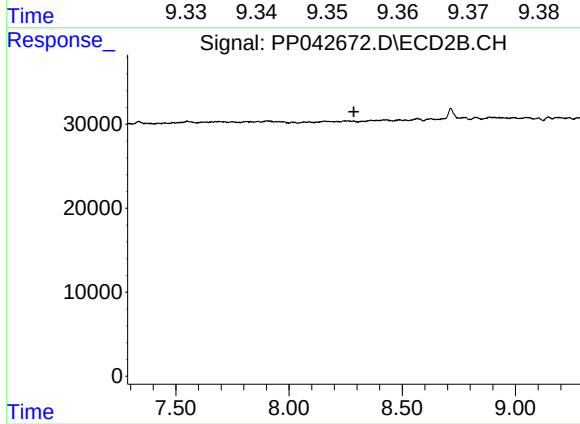

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 8.286 min
Response: 0
Conc: N.D.

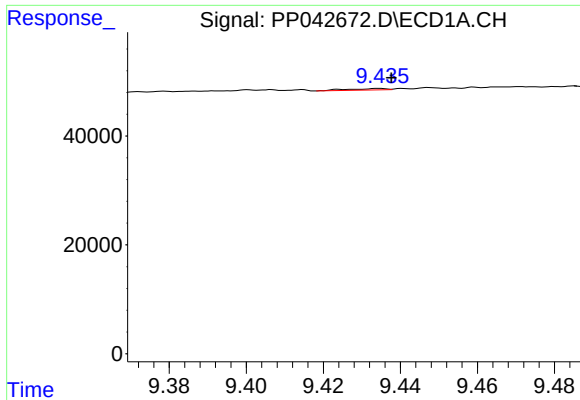

#39 AR-1262-4


R.T.: 9.435 min
Delta R.T.: -0.003 min
Response: 1916
Conc: 3.96 ng/ml

Instrument :
ECD_P
ClientSampleId :

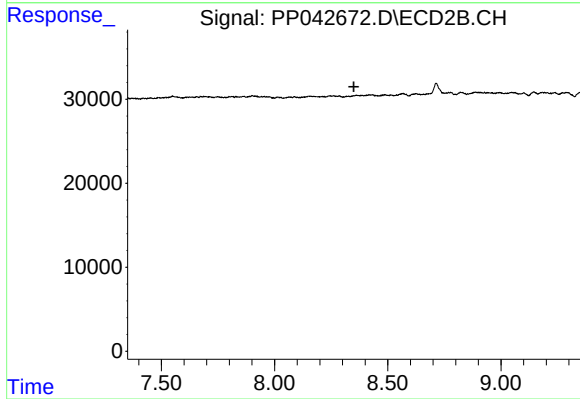


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.350 min
Response: 0
Conc: N.D.

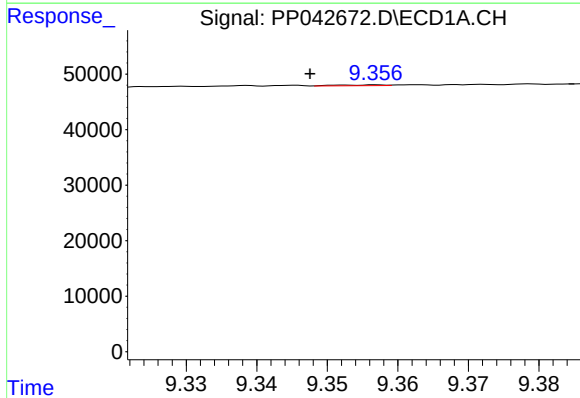


#41 AR-1268-1

R.T.: 9.357 min
Delta R.T.: 0.009 min
Response: 707
Conc: 0.43 ng/ml

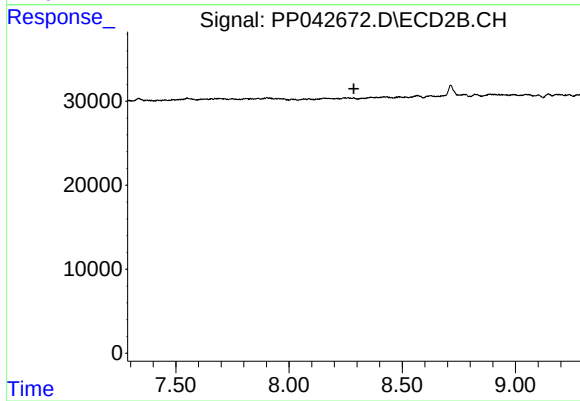

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 8.286 min
Response: 0
Conc: N.D.

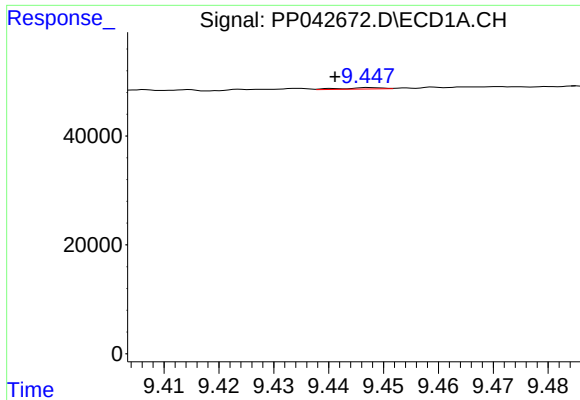

#42 AR-1268-2


R.T.: 9.447 min
Delta R.T.: 0.006 min
Response: 1319
Conc: 0.87 ng/ml

Instrument :
ECD_P
ClientSampleId :

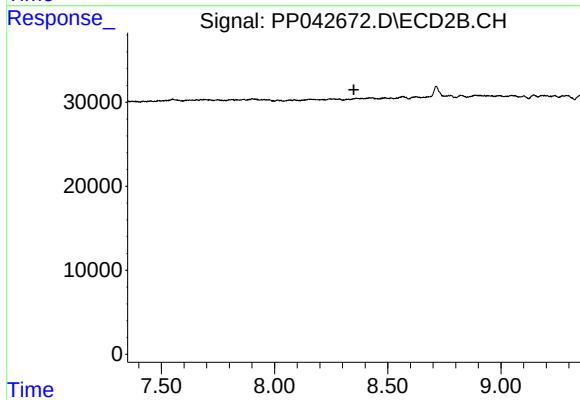


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.351 min
Response: 0
Conc: N.D.

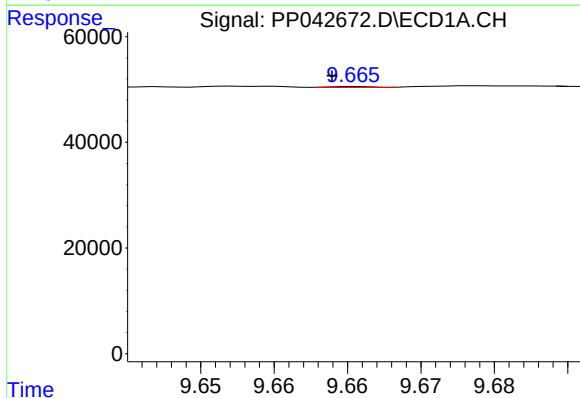


#43 AR-1268-3

R.T.: 9.666 min
Delta R.T.: 0.002 min
Response: 335
Conc: 0.25 ng/ml

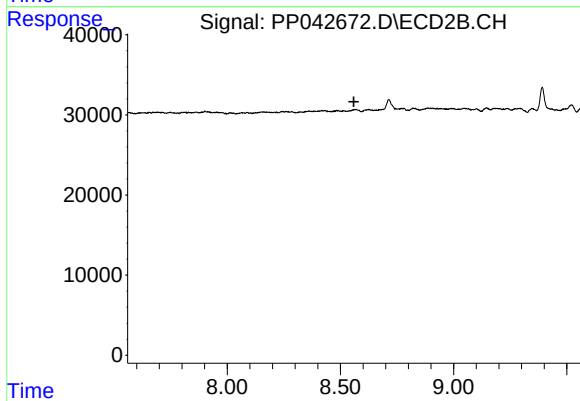

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 8.560 min
Response: 0
Conc: N.D.

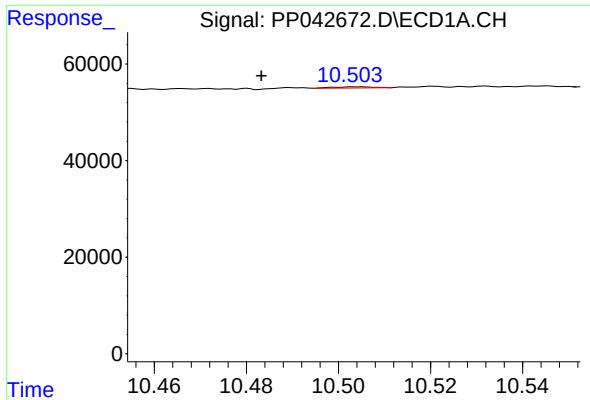

#45 AR-1268-5

R.T.: 10.504 min
Delta R.T.: 0.020 min
Response: 1563
Conc: 0.35 ng/ml

Instrument :
ECD_P
ClientSampleId :

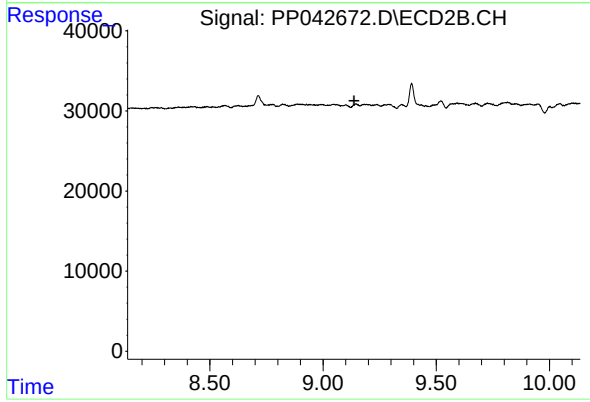

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.137 min
Response: 0
Conc: N.D.