

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010622\
 Data File : PP042684.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jan 2022 9:38
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 22:28:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 05 12:01:35 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.884	4.051	403176	533764	20.811	20.390
2)	SA Decachlor...	10.824	9.390	271759	421368	23.165	21.441
Target Compounds							
20)	L4 AR-1242-5	0.000	6.220f	0	12697	N.D.	17.311 #
25)	L5 AR-1248-5	0.000	6.220	0	12697	N.D.	12.797 #
26)	L6 AR-1254-1	0.000	6.220f	0	12697	N.D.	8.246 #
28)	L6 AR-1254-3	7.701	0.000	9514	0	10.386	N.D. #
32)	L7 AR-1260-2	0.000	7.091f	0	12254	N.D.	8.060 #
33)	L7 AR-1260-3	8.509	0.000	10165	0	18.348	N.D. #
36)	L8 AR-1262-1	8.509	0.000	10165	0	12.985	N.D. #
38)	L8 AR-1262-3	9.375f	0.000	3429	0	5.203	N.D. #
39)	L8 AR-1262-4	9.415f	0.000	27346	0	56.579	N.D. #
40)	L8 AR-1262-5	10.079	0.000	1888	0	3.870	N.D. #
41)	L9 AR-1268-1	9.375f	0.000	3429	0	2.096	N.D. #
42)	L9 AR-1268-2	9.415f	0.000	27346	0	18.079	N.D. #
43)	L9 AR-1268-3	9.663	0.000	11088	0	8.238	N.D. #
44)	L9 AR-1268-4	10.079	0.000	1888	0	3.449	N.D. #
45)	L9 AR-1268-5	10.481	0.000	3528	0	0.791	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010622\
Data File : PP042684.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jan 2022 9:38
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 22:28:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 05 12:01:35 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

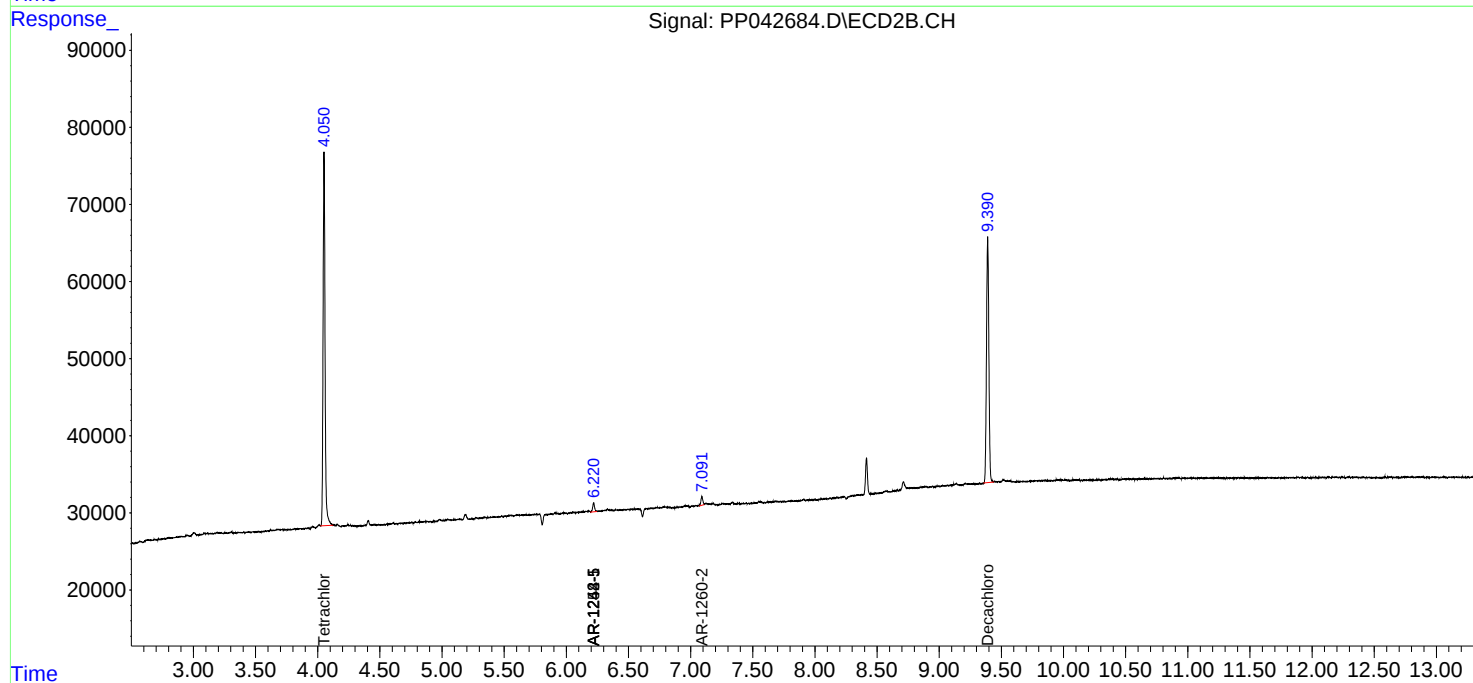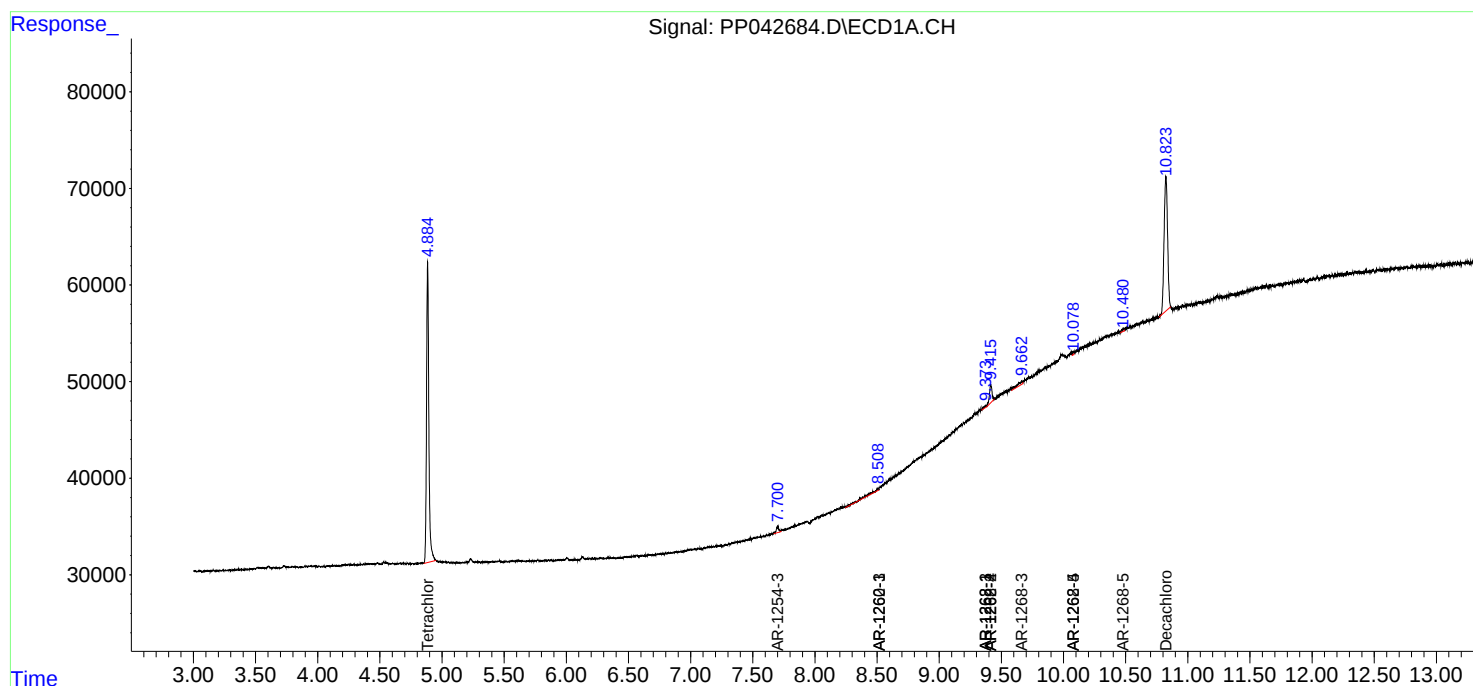


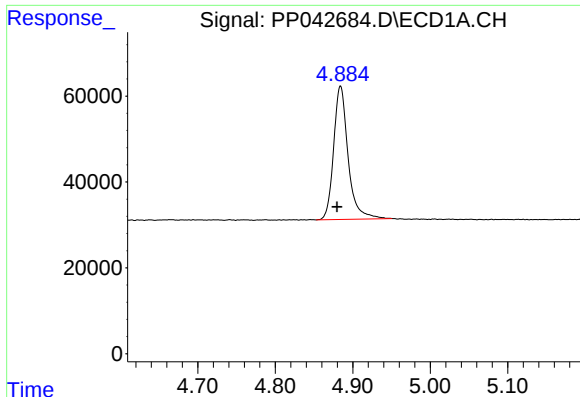

#1 Tetrachloro-m-xylene


R.T.: 4.884 min
Delta R.T.: 0.004 min
Response: 403176
Conc: 20.81 ng/ml

Instrument :
ECD_P
ClientSampleId :

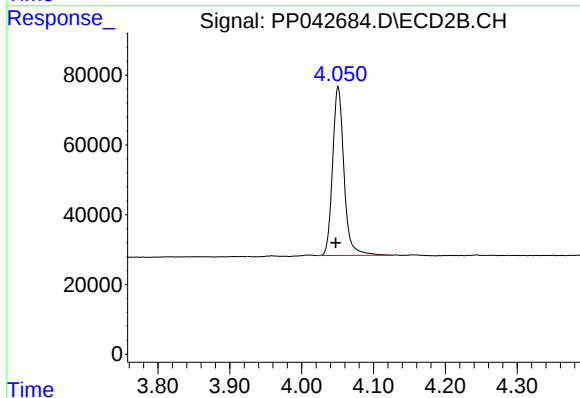


#1 Tetrachloro-m-xylene

R.T.: 4.051 min
Delta R.T.: 0.003 min
Response: 533764
Conc: 20.39 ng/ml

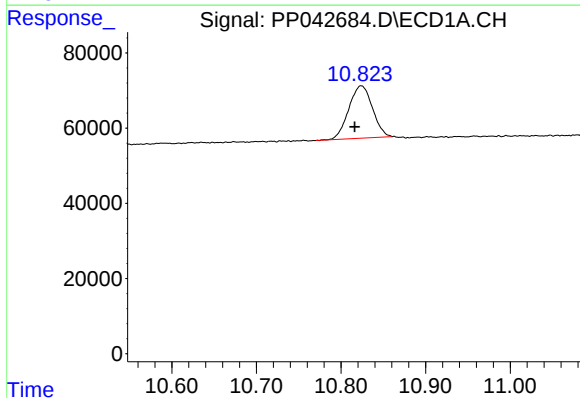


#2 Decachlorobiphenyl

R.T.: 10.824 min
Delta R.T.: 0.008 min
Response: 271759
Conc: 23.16 ng/ml

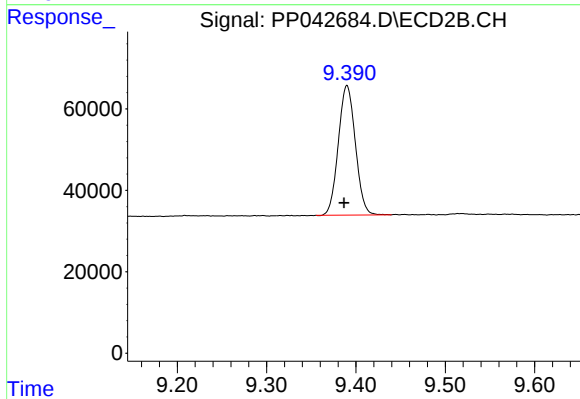

#2 Decachlorobiphenyl


R.T.: 9.390 min
Delta R.T.: 0.003 min
Response: 421368
Conc: 21.44 ng/ml

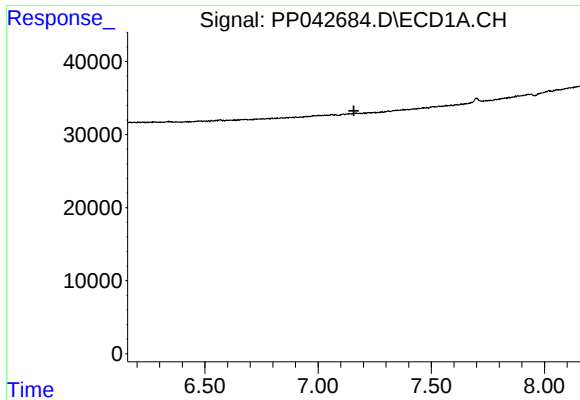

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.158 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

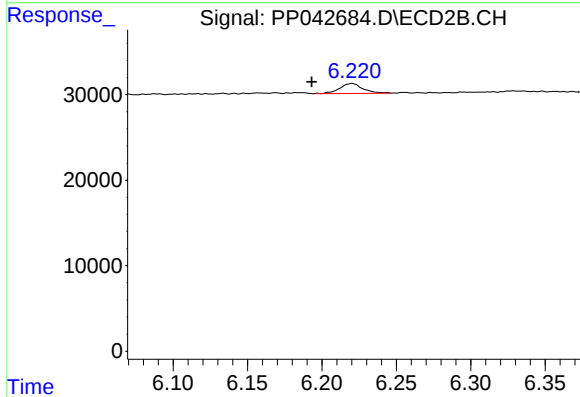


#20 AR-1242-5

R.T.: 6.220 min
Delta R.T.: 0.027 min
Response: 12697
Conc: 17.31 ng/ml

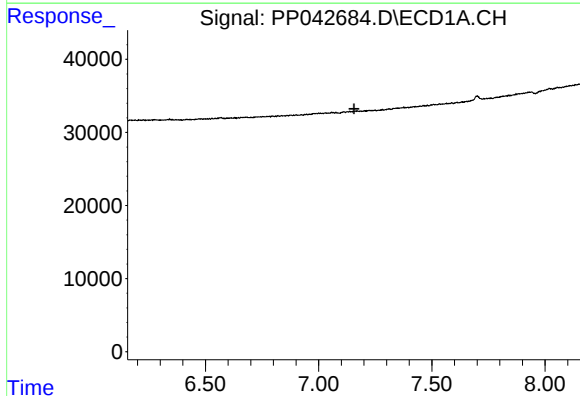


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 7.156 min
Response: 0
Conc: N.D.

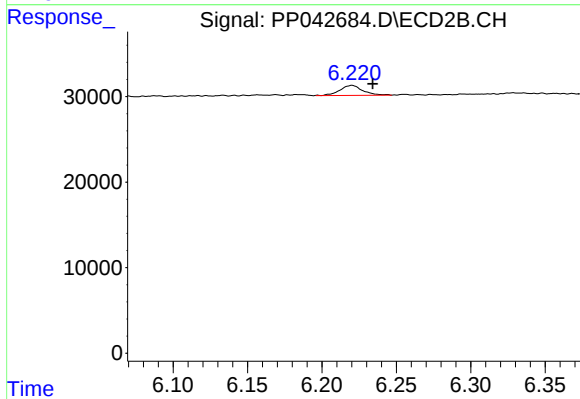

#25 AR-1248-5


R.T.: 6.220 min
Delta R.T.: -0.014 min
Response: 12697
Conc: 12.80 ng/ml

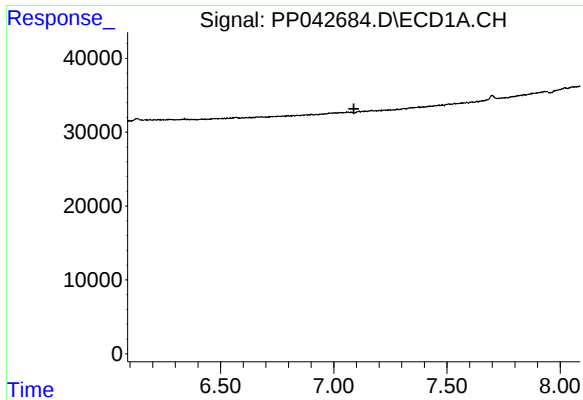

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 7.089 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

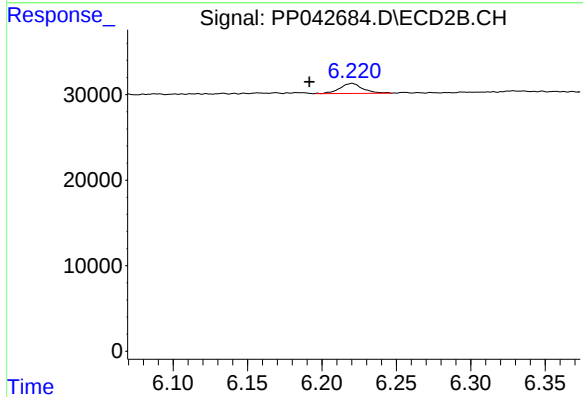


#26 AR-1254-1

R.T.: 6.220 min
Delta R.T.: 0.029 min
Response: 12697
Conc: 8.25 ng/ml

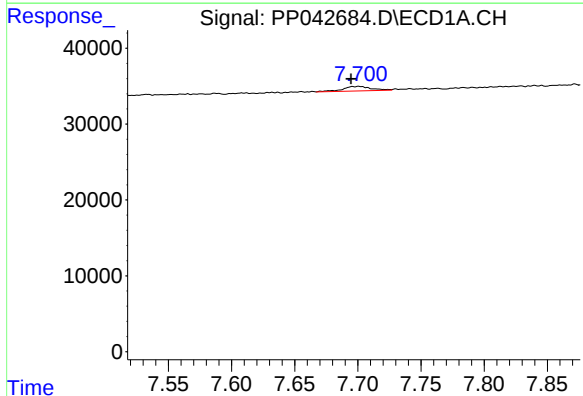


#28 AR-1254-3

R.T.: 7.701 min
Delta R.T.: 0.006 min
Response: 9514
Conc: 10.39 ng/ml

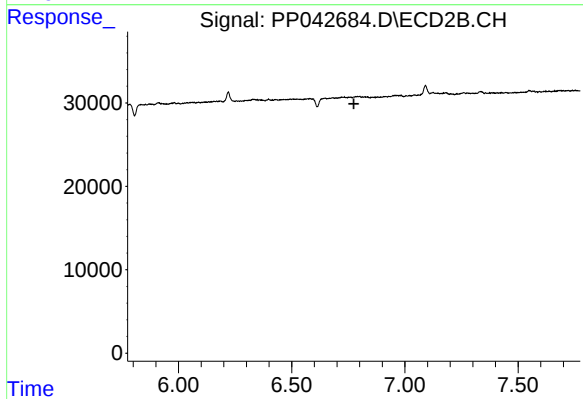

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.774 min
Response: 0
Conc: N.D.

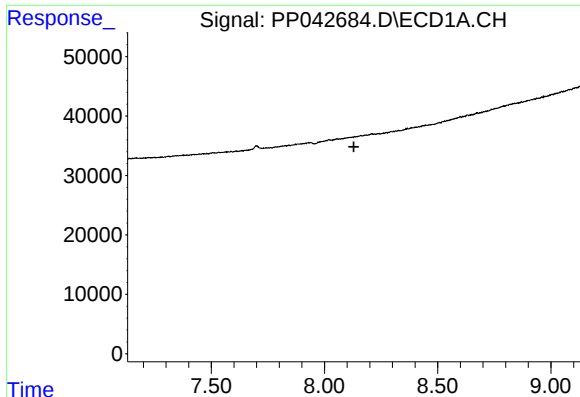

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 8.130 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

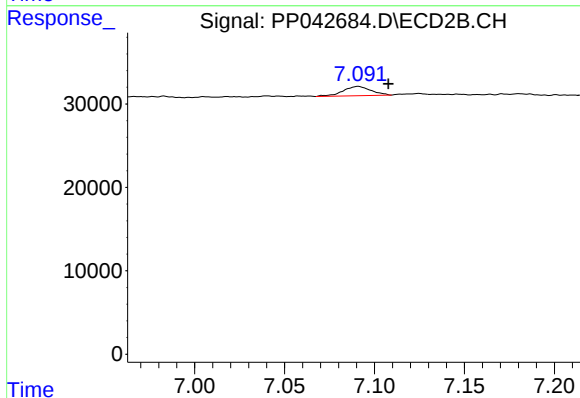


#32 AR-1260-2

R.T.: 7.091 min
Delta R.T.: -0.017 min
Response: 12254
Conc: 8.06 ng/ml

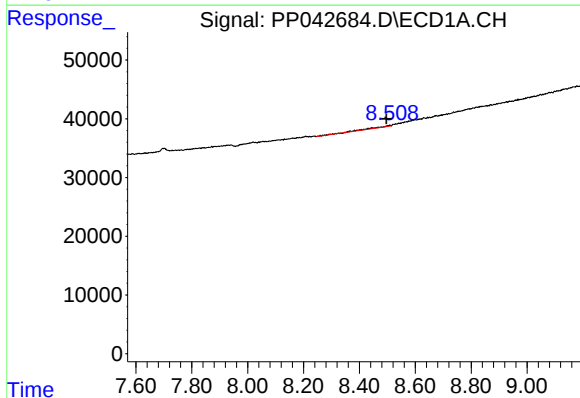


#33 AR-1260-3

R.T.: 8.509 min
Delta R.T.: 0.013 min
Response: 10165
Conc: 18.35 ng/ml

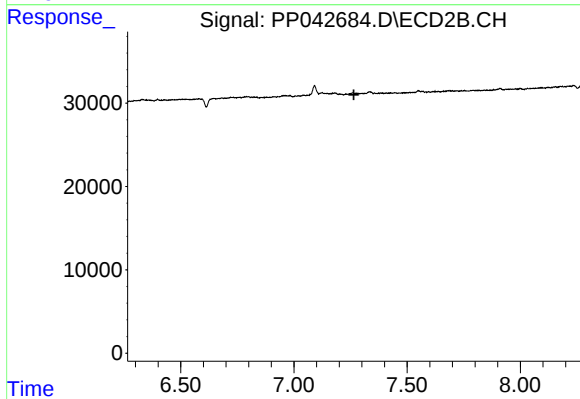

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.264 min
Response: 0
Conc: N.D.

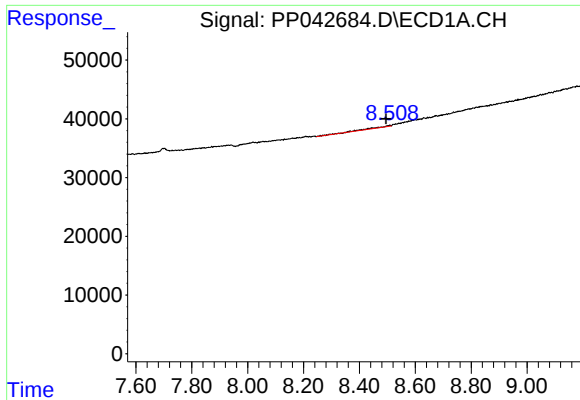

#36 AR-1262-1


R.T.: 8.509 min
Delta R.T.: 0.014 min
Response: 10165
Conc: 12.98 ng/ml

Instrument :
ECD_P
ClientSampleId :

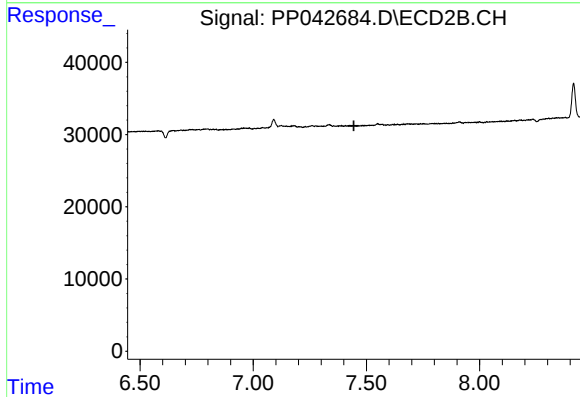


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.444 min
Response: 0
Conc: N.D.

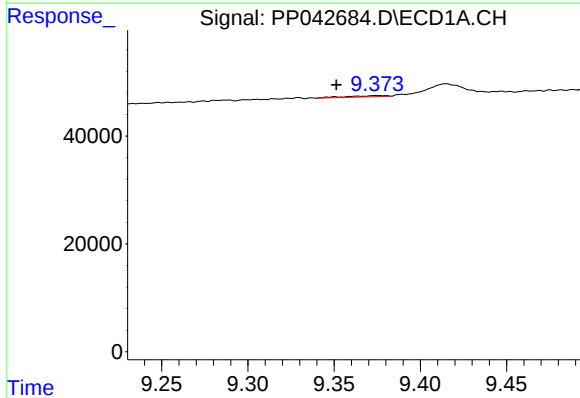


#38 AR-1262-3

R.T.: 9.375 min
Delta R.T.: 0.024 min
Response: 3429
Conc: 5.20 ng/ml

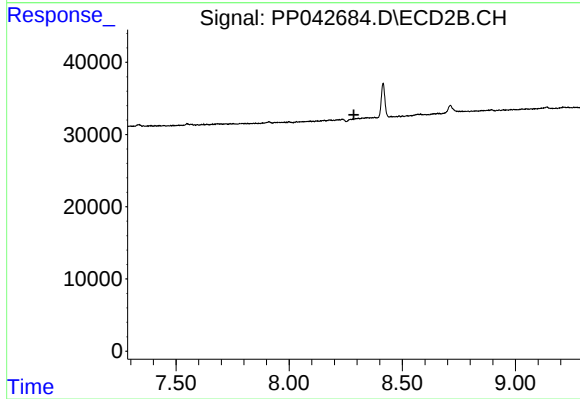

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 8.286 min
Response: 0
Conc: N.D.

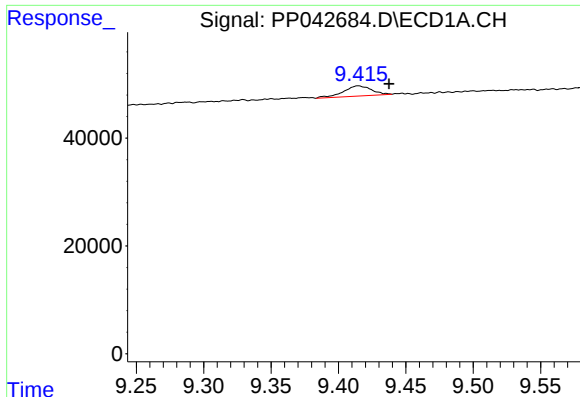

#39 AR-1262-4


R.T.: 9.415 min
Delta R.T.: -0.023 min
Response: 27346
Conc: 56.58 ng/ml

Instrument :
ECD_P
ClientSampleId :

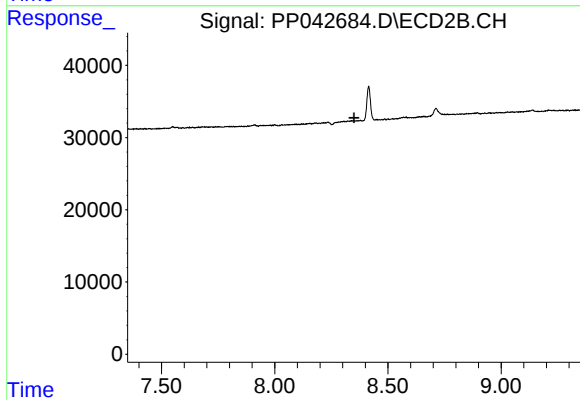


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.350 min
Response: 0
Conc: N.D.

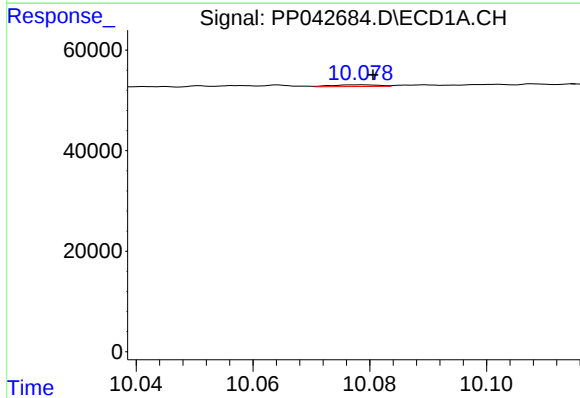


#40 AR-1262-5

R.T.: 10.079 min
Delta R.T.: -0.002 min
Response: 1888
Conc: 3.87 ng/ml

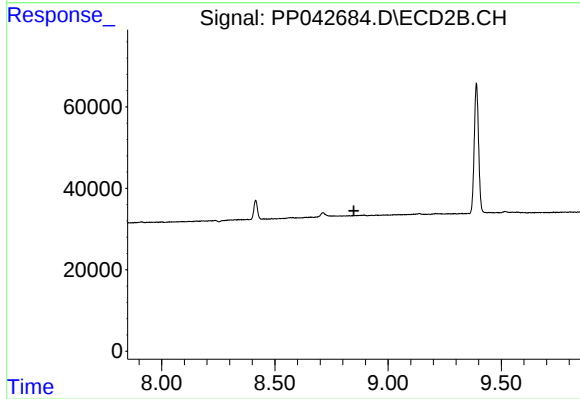

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 8.849 min
Response: 0
Conc: N.D.

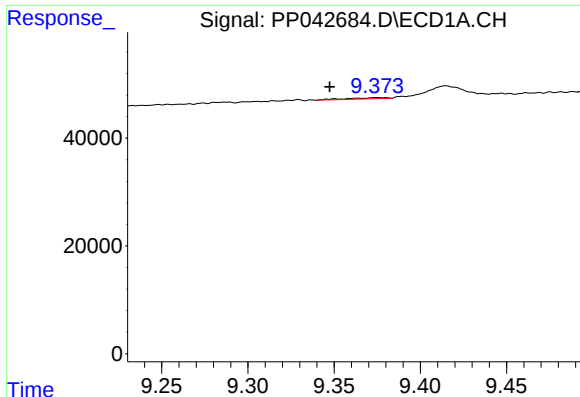

#41 AR-1268-1


R.T.: 9.375 min
Delta R.T.: 0.027 min
Response: 3429
Conc: 2.10 ng/ml

Instrument :
ECD_P
ClientSampleId :

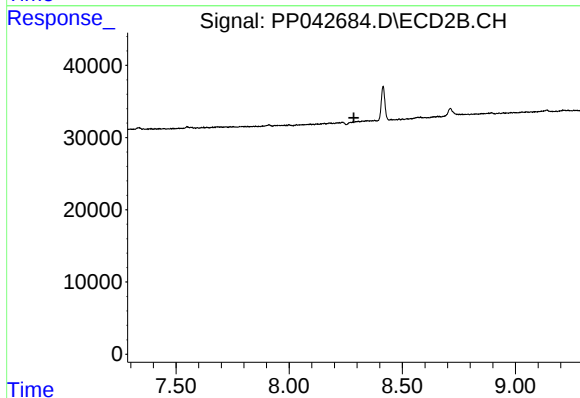


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.286 min
Response: 0
Conc: N.D.

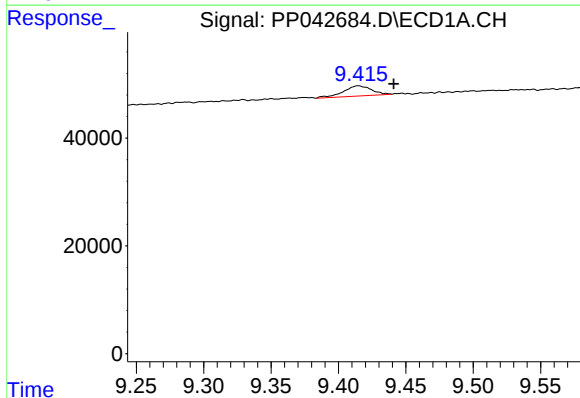


#42 AR-1268-2

R.T.: 9.415 min
Delta R.T.: -0.027 min
Response: 27346
Conc: 18.08 ng/ml

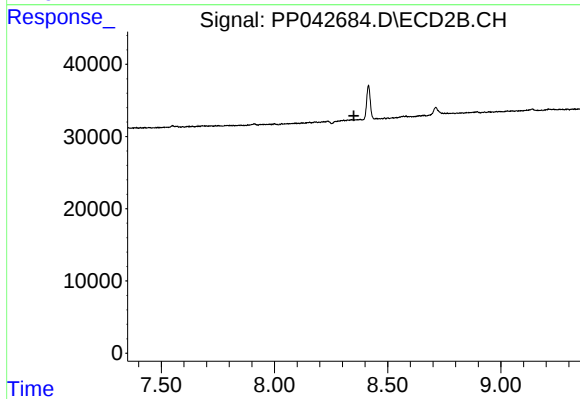

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.351 min
Response: 0
Conc: N.D.

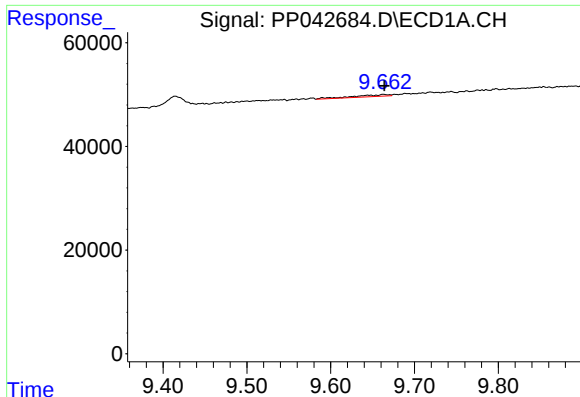

#43 AR-1268-3


R.T.: 9.663 min
Delta R.T.: -0.001 min
Response: 11088
Conc: 8.24 ng/ml

Instrument :
ECD_P
ClientSampleId :

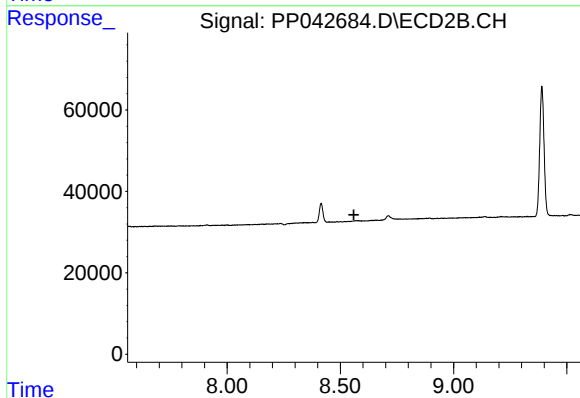


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.560 min
Response: 0
Conc: N.D.

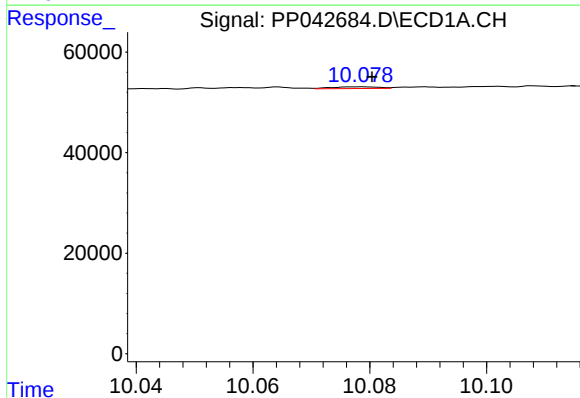


#44 AR-1268-4

R.T.: 10.079 min
Delta R.T.: -0.002 min
Response: 1888
Conc: 3.45 ng/ml

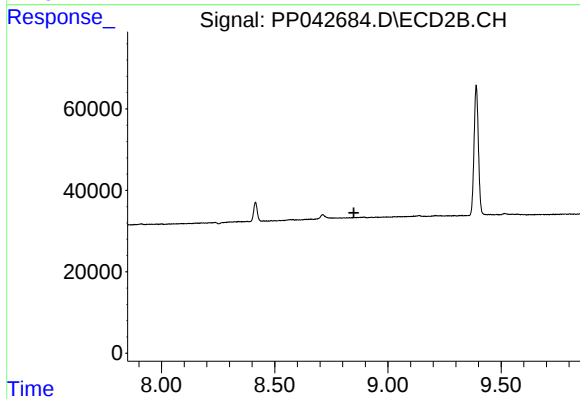

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 8.849 min
Response: 0
Conc: N.D.

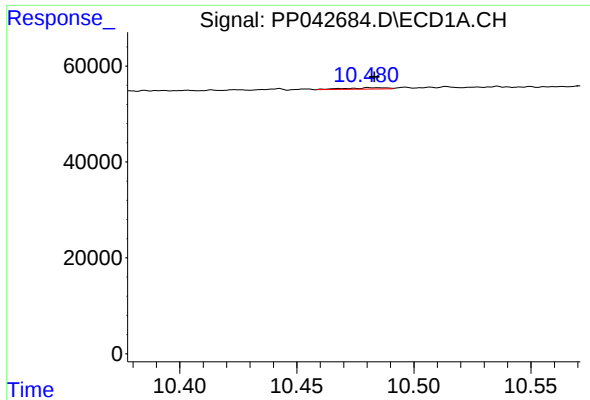

#45 AR-1268-5

R.T.: 10.481 min
Delta R.T.: -0.002 min
Response: 3528
Conc: 0.79 ng/ml

Instrument :
ECD_P
ClientSampleId :

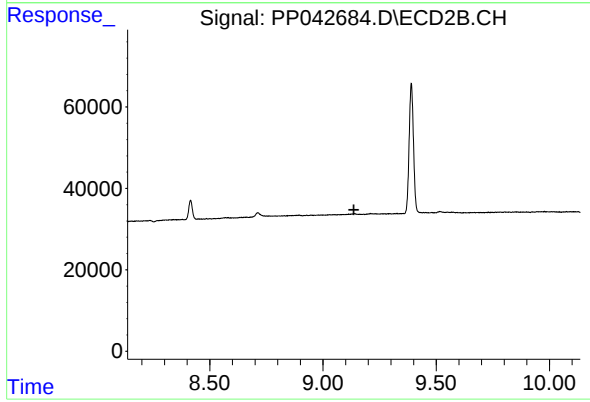

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.137 min
Response: 0
Conc: N.D.