

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010622\
 Data File : PP042645.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jan 2022 22:25
 Operator : AJ\MA
 Sample : N1042-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TRE-1522

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/07/2022
 Supervised By :mohammad ahmed 01/10/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 03:41:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 05 12:01:35 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.885	4.051	518625	536379	26.770	20.490
2)	SA Decachlor...	10.824	9.390	326580	460664	27.838	23.440
Target Compounds							
26)	L6 AR-1254-1	7.096	6.193	32140	105161	52.757	68.294 #
27)	L6 AR-1254-2	7.324	6.353	67869	72531	73.905	53.964 #
28)	L6 AR-1254-3	7.702	6.777	72037	140963	78.638	67.491
29)	L6 AR-1254-4	7.993	7.016	55918	67843	93.356m	55.435 #
30)	L6 AR-1254-5	8.423	7.446	48219	101407	76.265m	61.742m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010622\
Data File : PP042645.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jan 2022 22:25
Operator : AJ\MA
Sample : N1042-03
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TRE-1522


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/07/2022
Supervised By :mohammad ahmed 01/10/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 03:41:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 05 12:01:35 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

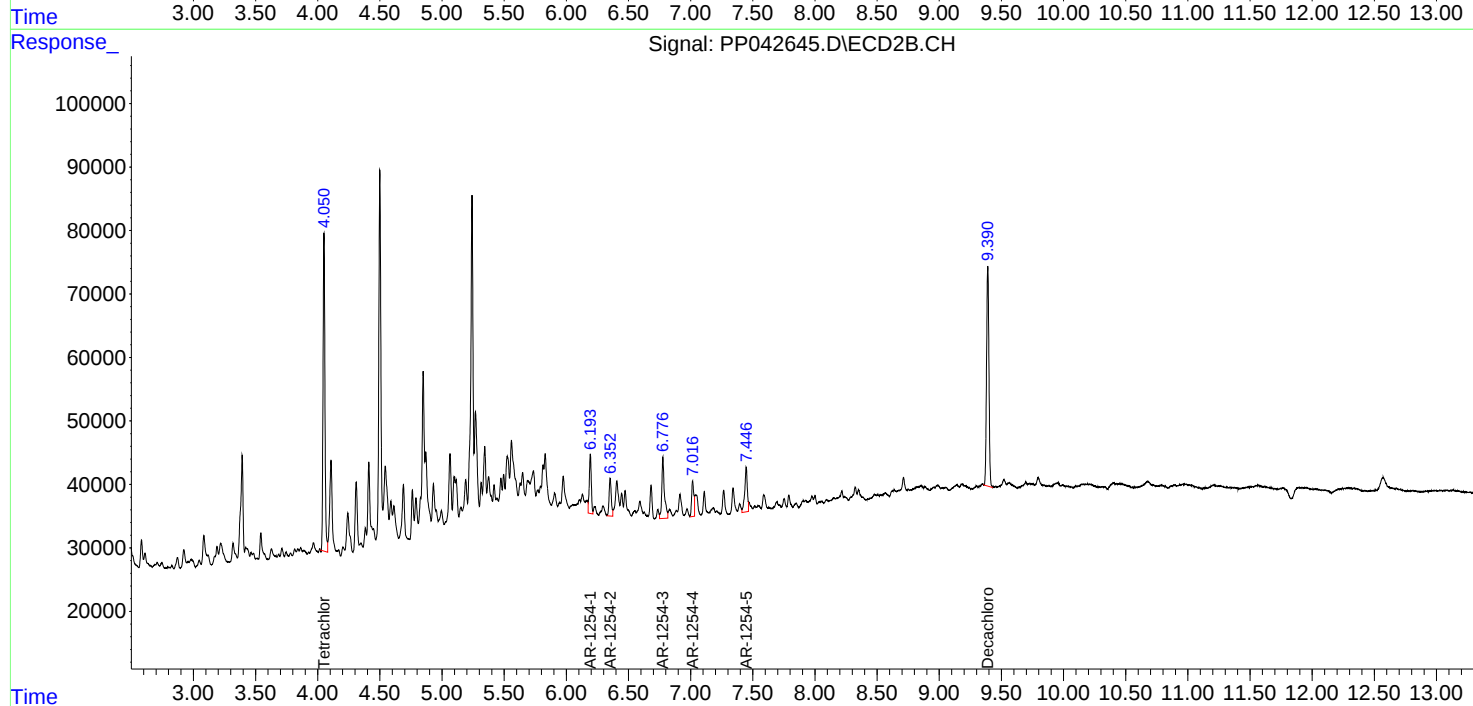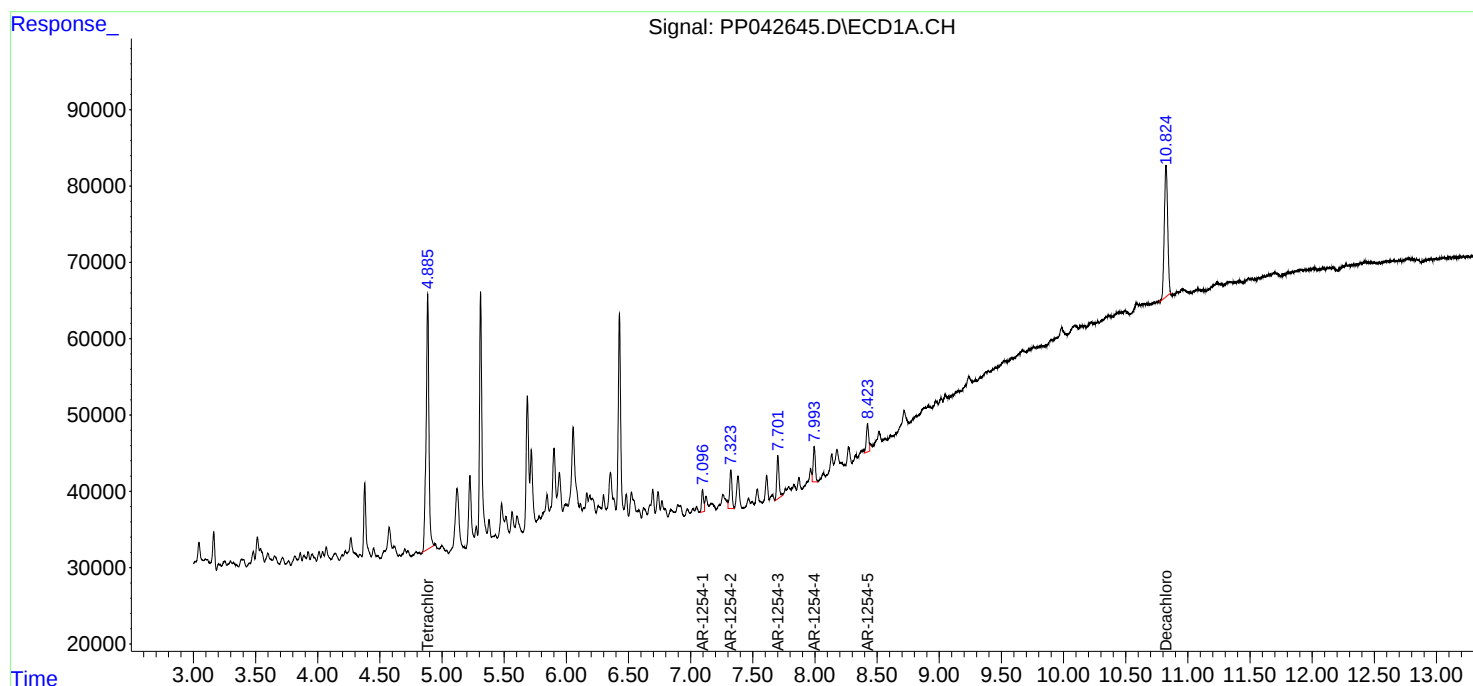

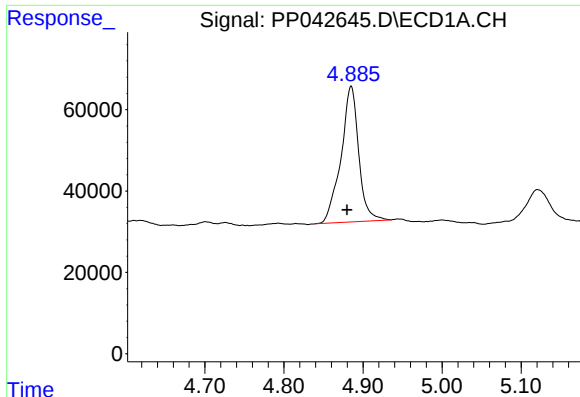


#1 Tetrachloro-m-xylene

R.T.: 4.885 min
Delta R.T.: 0.005 min
Response: 518625
Conc: 26.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRE-1522


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/07/2022
Supervised By :mohammad ahmed 01/10/2022

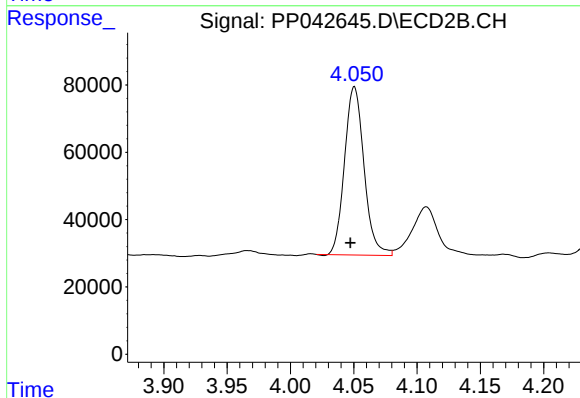


#1 Tetrachloro-m-xylene

R.T.: 4.051 min
Delta R.T.: 0.003 min
Response: 536379
Conc: 20.49 ng/ml

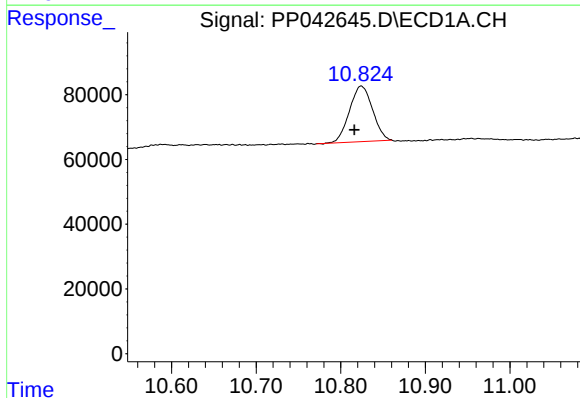


#2 Decachlorobiphenyl

R.T.: 10.824 min
Delta R.T.: 0.008 min
Response: 326580
Conc: 27.84 ng/ml

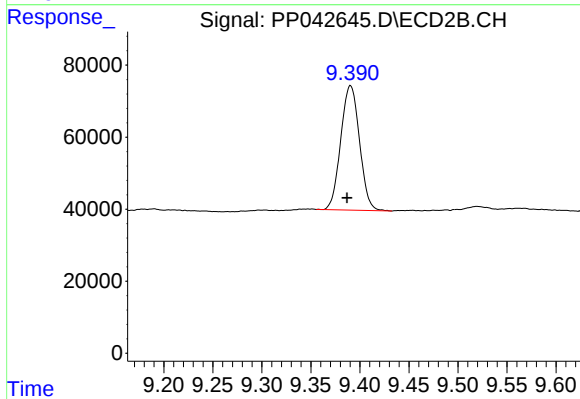

#2 Decachlorobiphenyl

R.T.: 9.390 min
Delta R.T.: 0.004 min
Response: 460664
Conc: 23.44 ng/ml

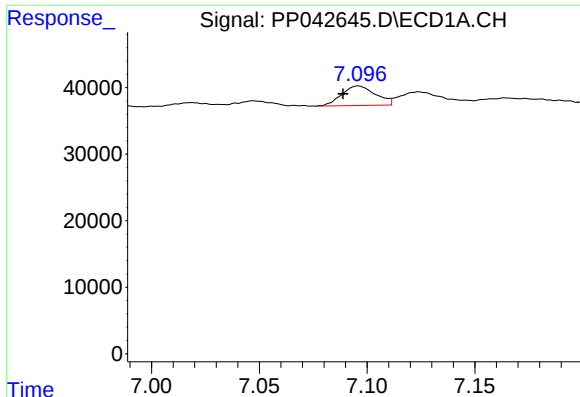


#26 AR-1254-1

R.T.: 7.096 min
Delta R.T.: 0.007 min
Response: 32140
Conc: 52.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRE-1522


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/07/2022
Supervised By :mohammad ahmed 01/10/2022

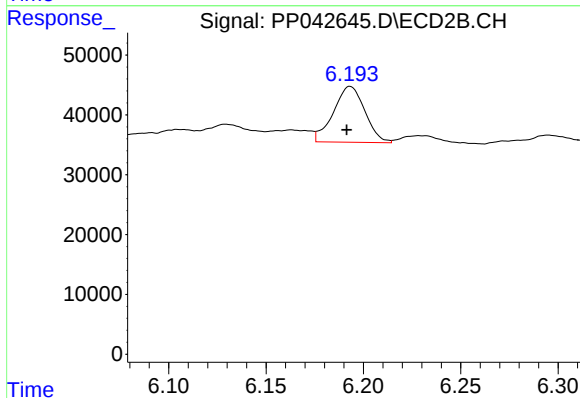


#26 AR-1254-1

R.T.: 6.193 min
Delta R.T.: 0.002 min
Response: 105161
Conc: 68.29 ng/ml

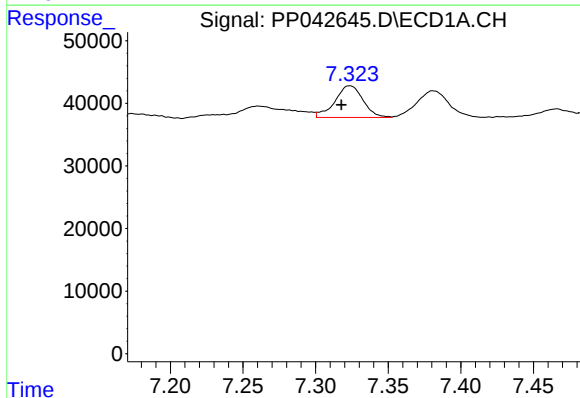


#27 AR-1254-2

R.T.: 7.324 min
Delta R.T.: 0.006 min
Response: 67869
Conc: 73.90 ng/ml

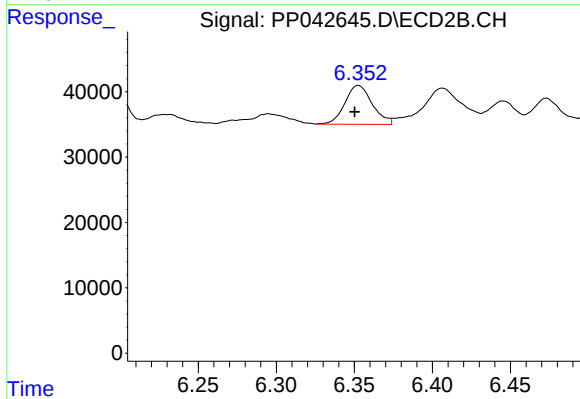

#27 AR-1254-2

R.T.: 6.353 min
Delta R.T.: 0.002 min
Response: 72531
Conc: 53.96 ng/ml

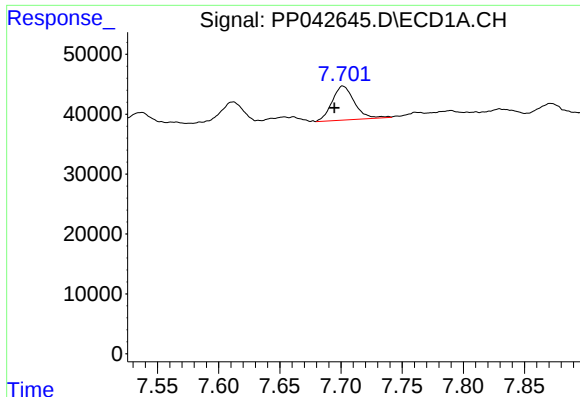


#28 AR-1254-3

R.T.: 7.702 min
Delta R.T.: 0.007 min
Response: 72037
Conc: 78.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRE-1522


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/07/2022
Supervised By :mohammad ahmed 01/10/2022

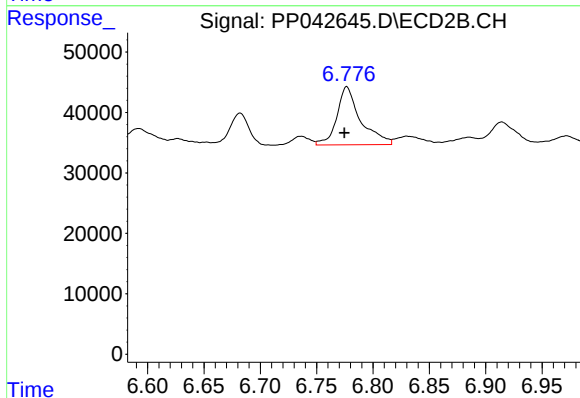


#28 AR-1254-3

R.T.: 6.777 min
Delta R.T.: 0.002 min
Response: 140963
Conc: 67.49 ng/ml

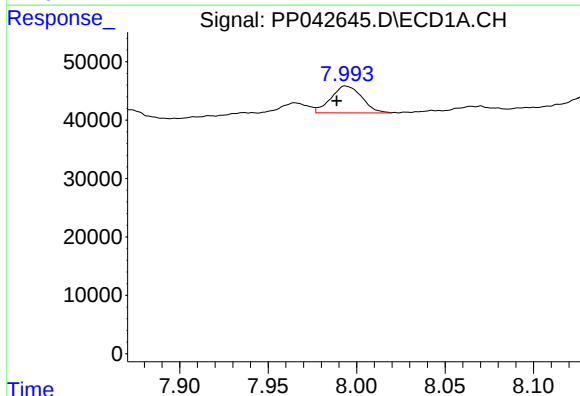


#29 AR-1254-4

R.T.: 7.993 min
Delta R.T.: 0.004 min
Response: 55918
Conc: 93.36 ng/ml m

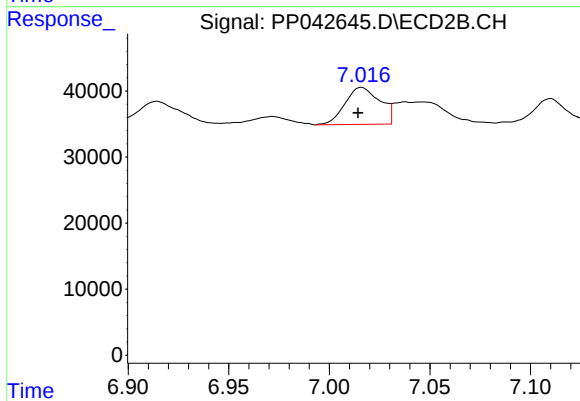

#29 AR-1254-4

R.T.: 7.016 min
Delta R.T.: 0.002 min
Response: 67843
Conc: 55.43 ng/ml

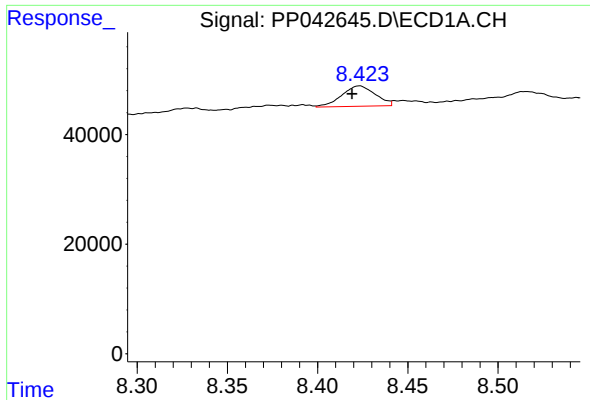


#30 AR-1254-5

R.T.: 8.423 min
Delta R.T.: 0.004 min
Response: 48219
Conc: 76.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRE-1522

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/07/2022
Supervised By :mohammad ahmed 01/10/2022

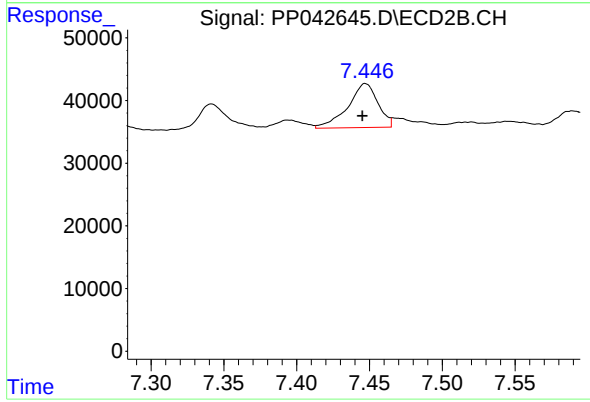

#30 AR-1254-5

R.T.: 7.446 min
Delta R.T.: 0.001 min
Response: 101407
Conc: 61.74 ng/ml m