

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010721\
 Data File : PP032591.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jan 2021 10:32
 Operator : DD\AJ
 Sample : M1014-05 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC226716LOZ-END-1

Manual Integrations
 APPROVED

Ankita
 1/8/2021 10:10:13 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 17:09:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 07:49:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.745	4.031	55421	46510	1.013	0.961m
2) SA Decachlor...	10.550f	9.314	465328	100859	10.394m	2.272 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010721\
Data File : PP032591.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jan 2021 10:32
Operator : DD\AJ
Sample : M1014-05 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC226716LOZ-END-1


Manual Integrations
APPROVED

Ankita
1/8/2021 10:10:13 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 17:09:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 07:49:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

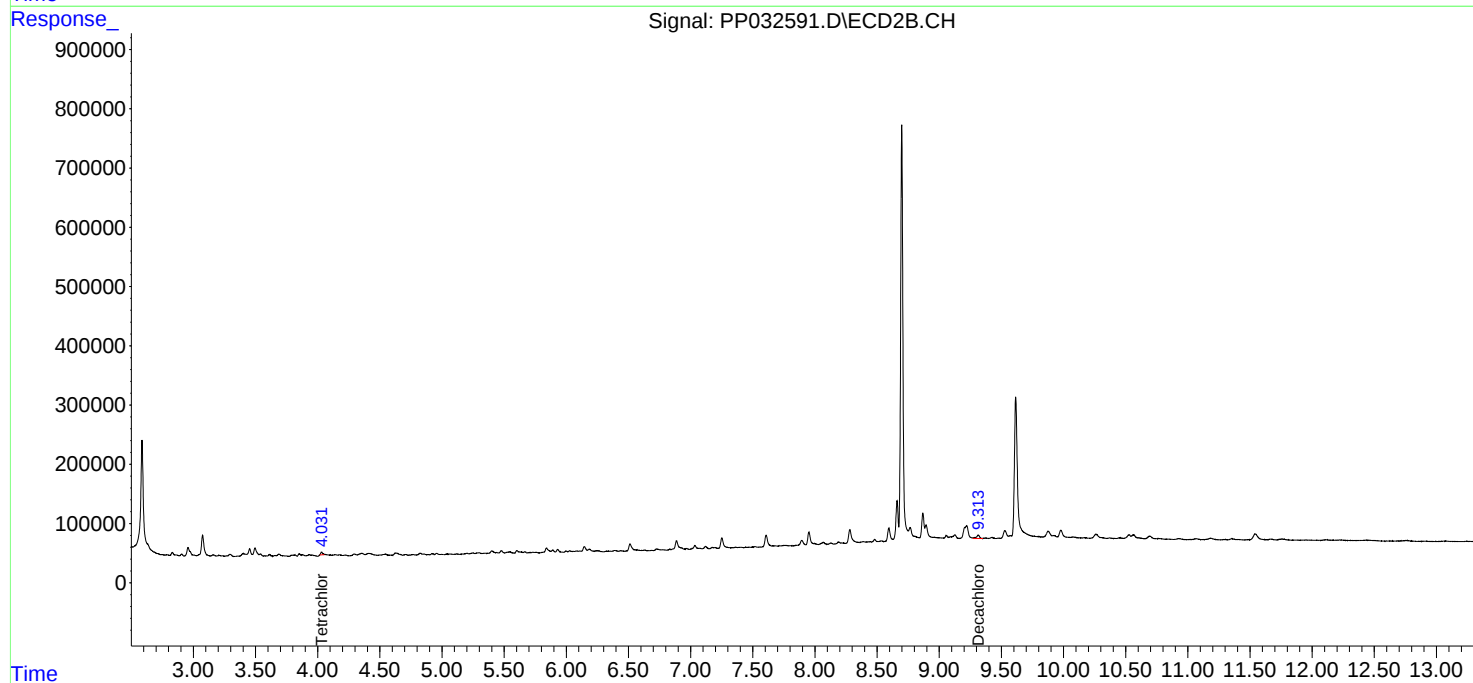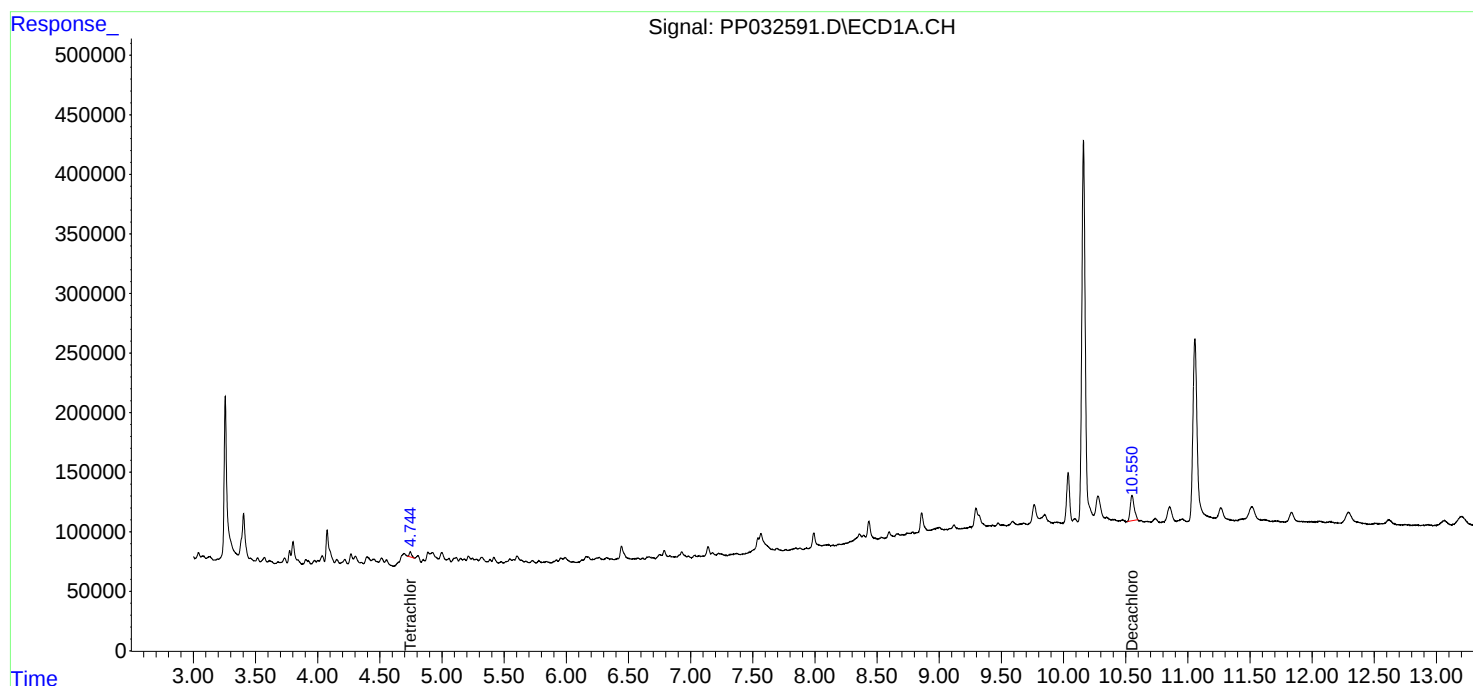

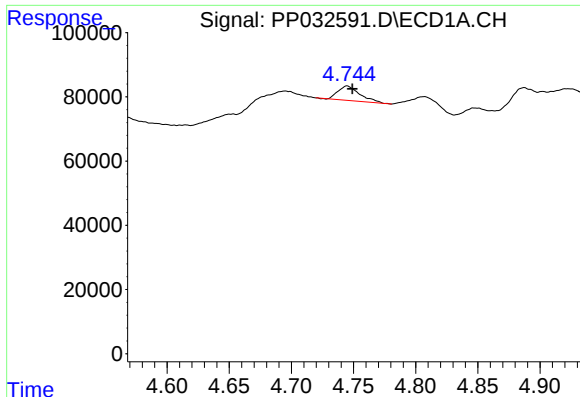


#1 Tetrachloro-m-xylene

R.T.: 4.745 min
Delta R.T.: -0.004 min
Response: 55421
Conc: 1.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC226716LOZ-END-1


Manual Integrations
APPROVED

Ankita
1/8/2021 10:10:13 AM

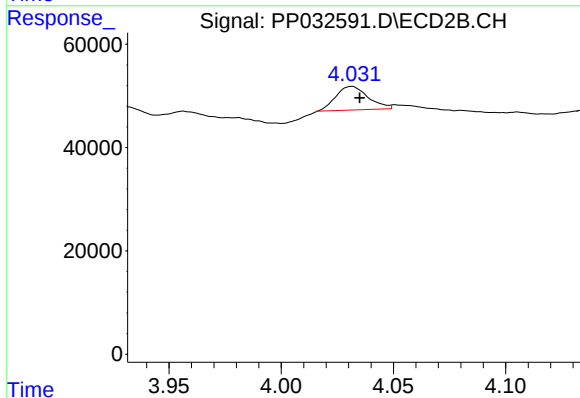


#1 Tetrachloro-m-xylene

R.T.: 4.031 min
Delta R.T.: -0.004 min
Response: 46510
Conc: 0.96 ng/ml m

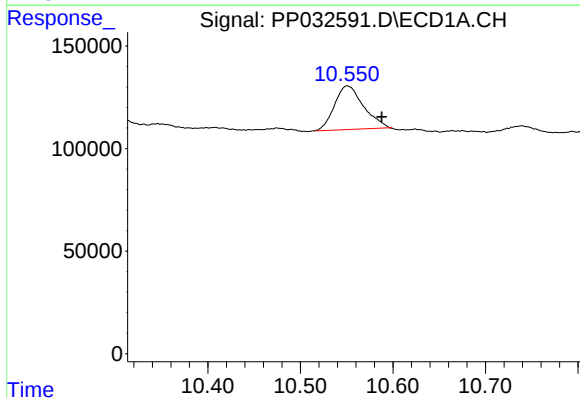

#2 Decachlorobiphenyl

R.T.: 10.550 min
Delta R.T.: -0.038 min
Response: 465328
Conc: 10.39 ng/ml m

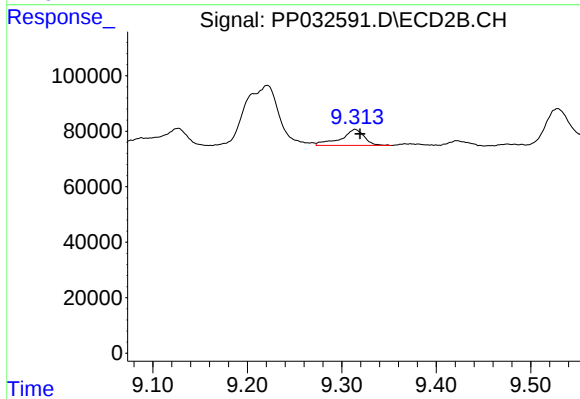

#2 Decachlorobiphenyl

R.T.: 9.314 min
Delta R.T.: -0.005 min
Response: 100859
Conc: 2.27 ng/ml