

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010721\
 Data File : PP032597.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jan 2021 12:43
 Operator : DD\AJ
 Sample : M1035-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 R-LA-37-3-WC

Manual Integrations
 APPROVED

Ankita
 1/8/2021 10:10:19 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 17:11:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 07:49:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.747	4.032	1565578	1417599	28.628	29.288
2) SA Decachlor...	10.582	9.314	1068443	1012242	23.866	22.797m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010721\
Data File : PP032597.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jan 2021 12:43
Operator : DD\AJ
Sample : M1035-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
R-LA-37-3-WC


Manual Integrations
APPROVED

Ankita
1/8/2021 10:10:19 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 17:11:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 07:49:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

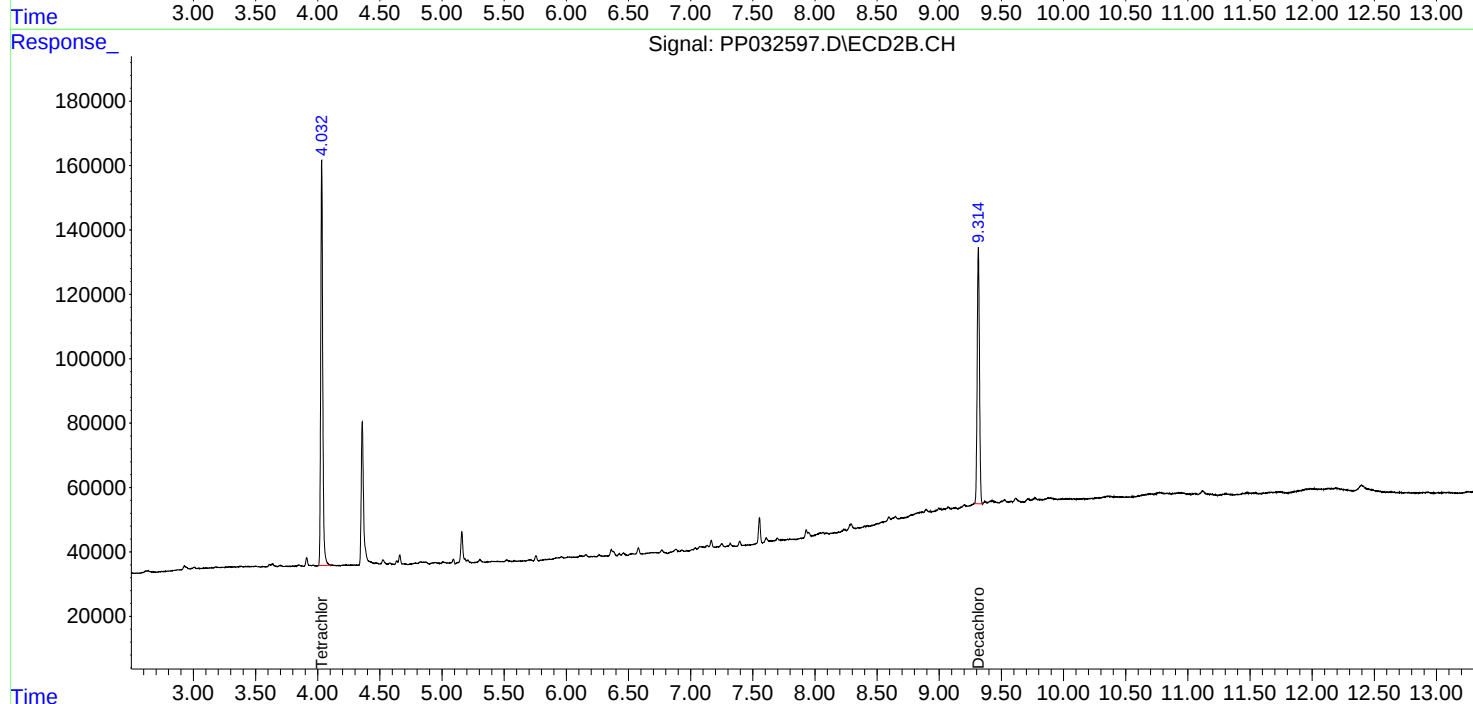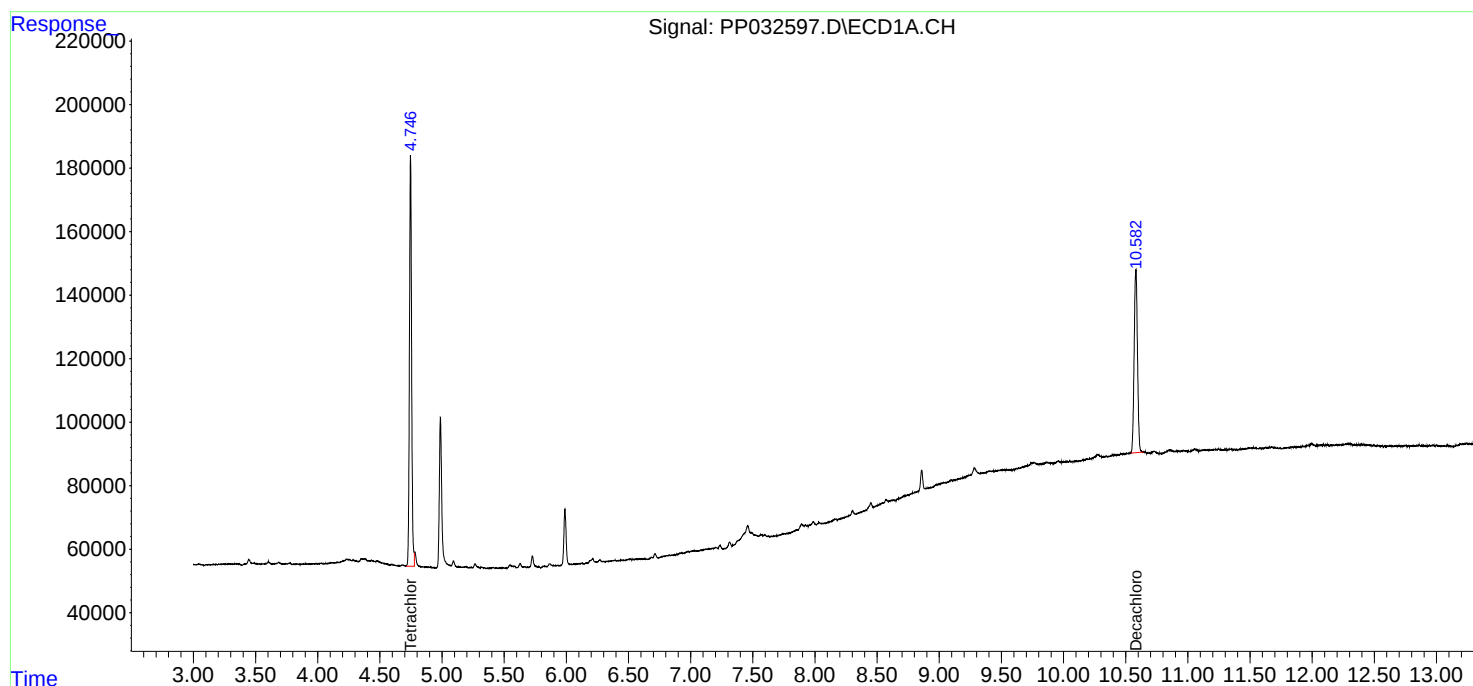

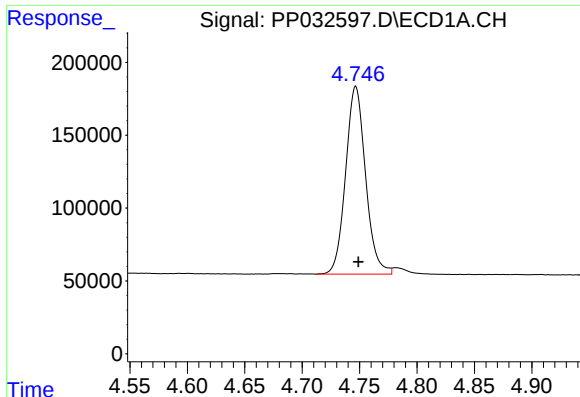


#1 Tetrachloro-m-xylene

R.T.: 4.747 min
Delta R.T.: -0.002 min
Response: 1565578
Conc: 28.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
R-LA-37-3-WC


Manual Integrations
APPROVED

Ankita
1/8/2021 10:10:19 AM

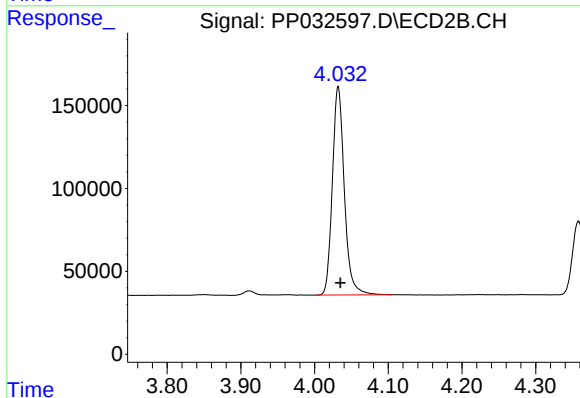


#1 Tetrachloro-m-xylene

R.T.: 4.032 min
Delta R.T.: -0.003 min
Response: 1417599
Conc: 29.29 ng/ml

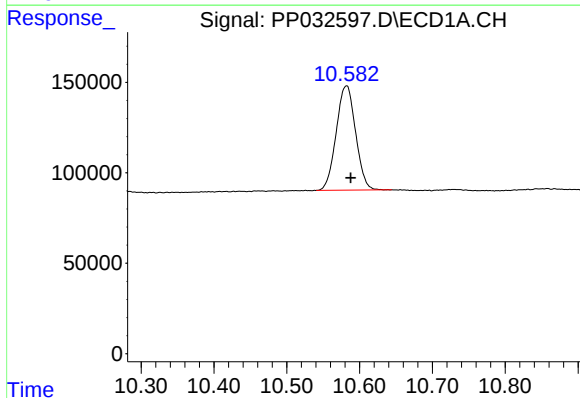

#2 Decachlorobiphenyl

R.T.: 10.582 min
Delta R.T.: -0.006 min
Response: 1068443
Conc: 23.87 ng/ml

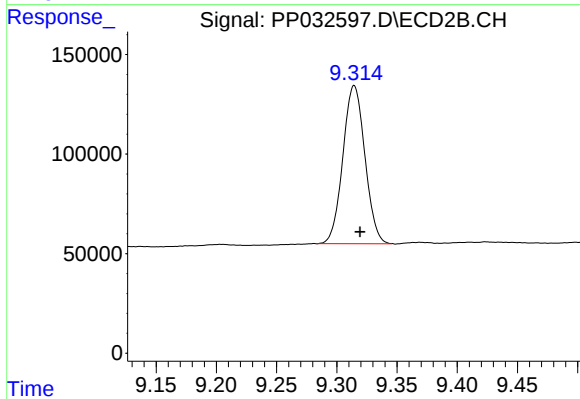

#2 Decachlorobiphenyl

R.T.: 9.314 min
Delta R.T.: -0.005 min
Response: 1012242
Conc: 22.80 ng/ml m