

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010722\
 Data File : PP042721.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jan 2022 20:40
 Operator : AJ\MA
 Sample : N1071-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FM-E6-01-4.5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 02:06:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 05 12:01:35 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.881	4.049	404109	528944	20.859	20.206
2)	SA Decachlor...	10.816	9.386	266638	337400	22.728	17.168
Target Compounds							
8)	L2 AR-1221-1	5.115	0.000	31704	0	153.601	N.D. #
9)	L2 AR-1221-2	0.000	4.382f	0	52546	N.D.	195.673 #
28)	L6 AR-1254-3	7.696	0.000	49056	0	53.551	N.D. #
30)	L6 AR-1254-5	8.412	0.000	6803	0	10.760	N.D. #
32)	L7 AR-1260-2	0.000	7.088f	0	83013	N.D.	54.604 #
33)	L7 AR-1260-3	8.498	0.000	985	0	1.777	N.D. #
34)	L7 AR-1260-4	8.725	0.000	1156	0	1.753	N.D. #
35)	L7 AR-1260-5	9.054	0.000	4110	0	3.407	N.D. #
36)	L8 AR-1262-1	8.498	0.000	985	0	1.258	N.D. #
37)	L8 AR-1262-2	9.034	0.000	1973	0	1.475	N.D. #
38)	L8 AR-1262-3	9.365	0.000	6805	0	10.325	N.D. #
39)	L8 AR-1262-4	9.439	0.000	1770	0	3.663	N.D. #
40)	L8 AR-1262-5	10.082	0.000	1951	0	3.999	N.D. #
41)	L9 AR-1268-1	9.365f	0.000	6805	0	4.159	N.D. #
42)	L9 AR-1268-2	9.439	0.000	1770	0	1.170	N.D. #
43)	L9 AR-1268-3	9.641f	0.000	4249	0	3.157	N.D. #
44)	L9 AR-1268-4	10.082	0.000	1951	0	3.565	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010722\
Data File : PP042721.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jan 2022 20:40
Operator : AJ\MA
Sample : N1071-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FM-E6-01-4.5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 02:06:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 05 12:01:35 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

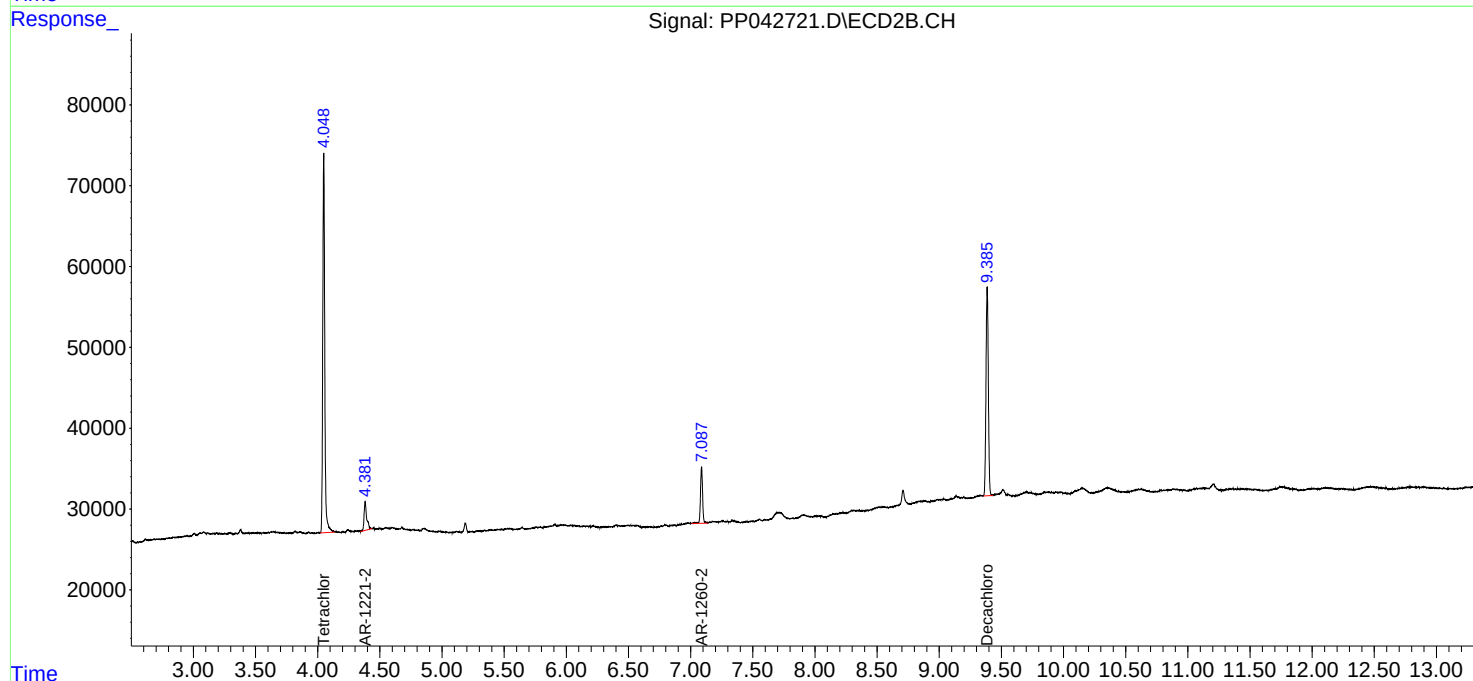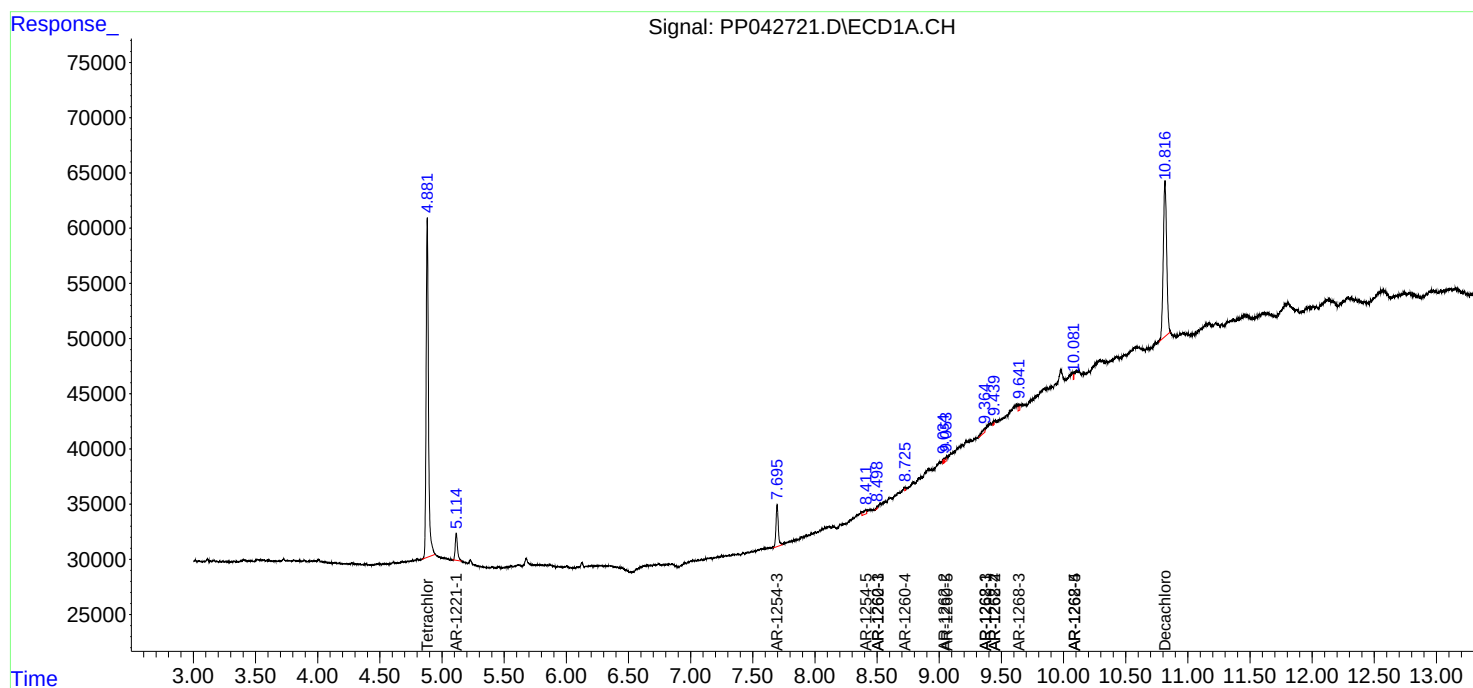


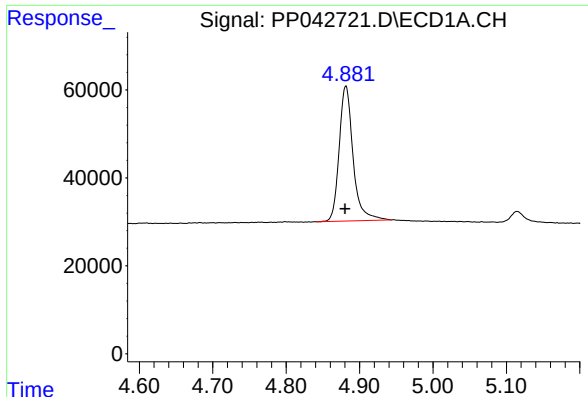

#1 Tetrachloro-m-xylene


R.T.: 4.881 min
Delta R.T.: 0.001 min
Response: 404109
Conc: 20.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
FM-E6-01-4.5

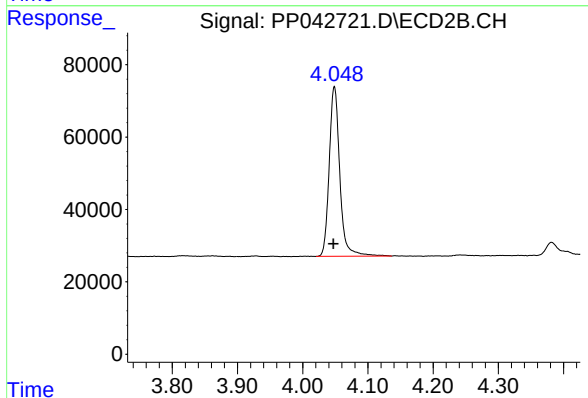


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: 0.001 min
Response: 528944
Conc: 20.21 ng/ml

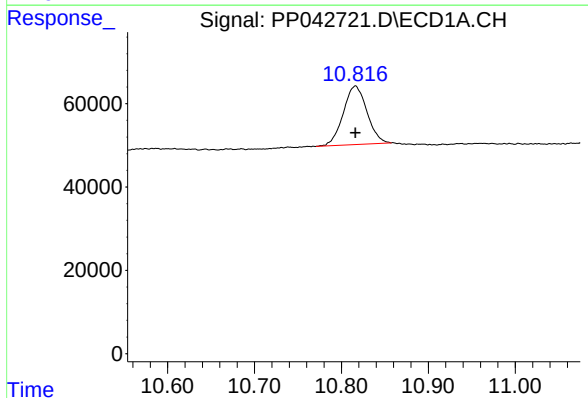


#2 Decachlorobiphenyl

R.T.: 10.816 min
Delta R.T.: 0.000 min
Response: 266638
Conc: 22.73 ng/ml

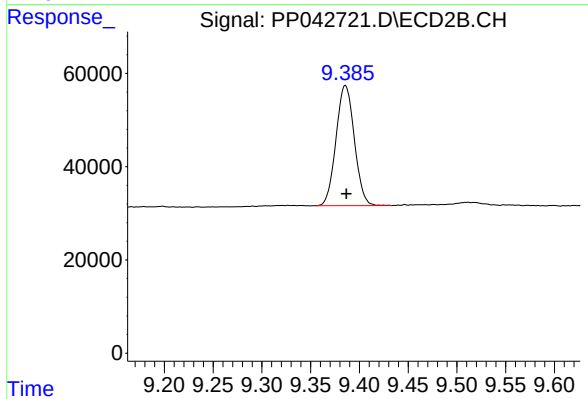

#2 Decachlorobiphenyl


R.T.: 9.386 min
Delta R.T.: -0.001 min
Response: 337400
Conc: 17.17 ng/ml

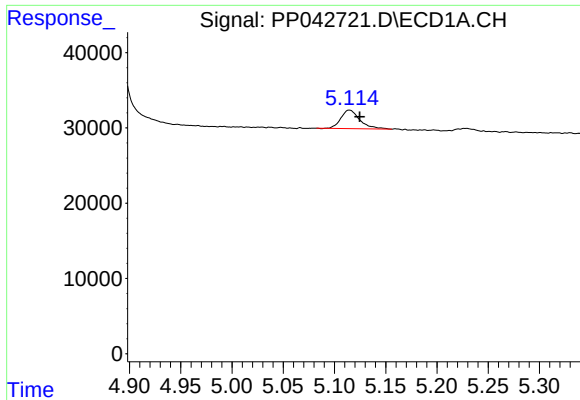

#8 AR-1221-1


R.T.: 5.115 min
Delta R.T.: -0.010 min
Response: 31704
Conc: 153.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
FM-E6-01-4.5

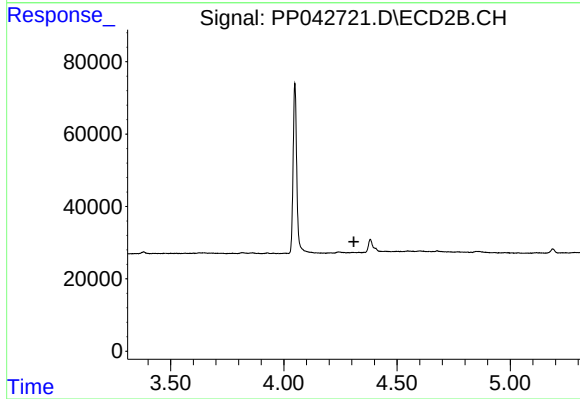


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.310 min
Response: 0
Conc: N.D.

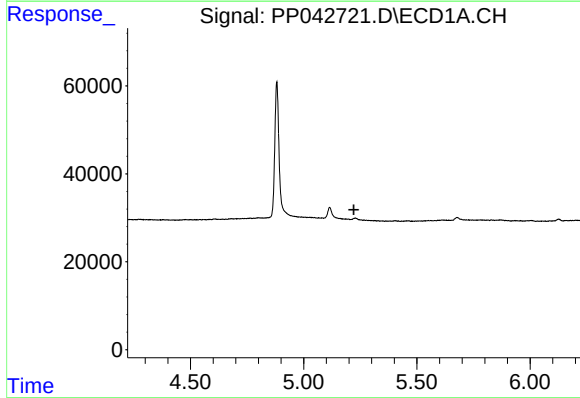


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.222 min
Response: 0
Conc: N.D.

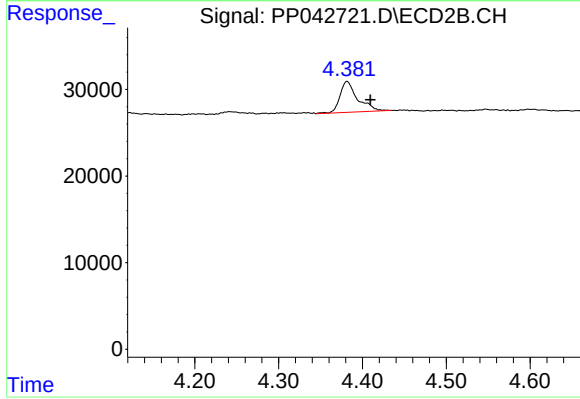

#9 AR-1221-2


R.T.: 4.382 min
Delta R.T.: -0.028 min
Response: 52546
Conc: 195.67 ng/ml

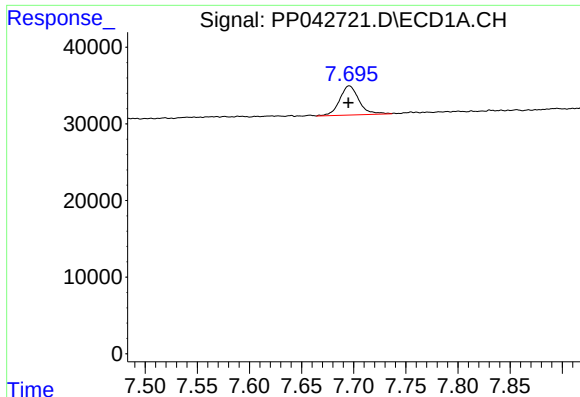

#28 AR-1254-3


R.T.: 7.696 min
Delta R.T.: 0.001 min
Response: 49056
Conc: 53.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
FM-E6-01-4.5

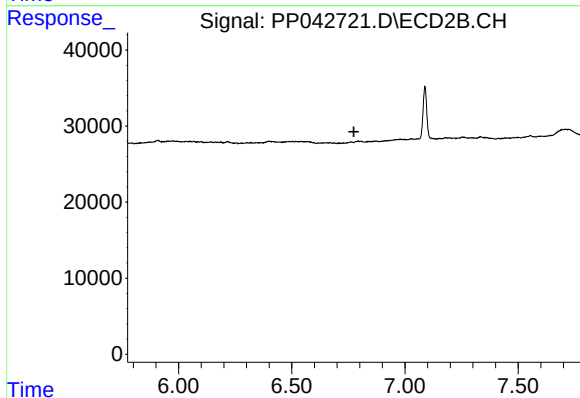


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.774 min
Response: 0
Conc: N.D.

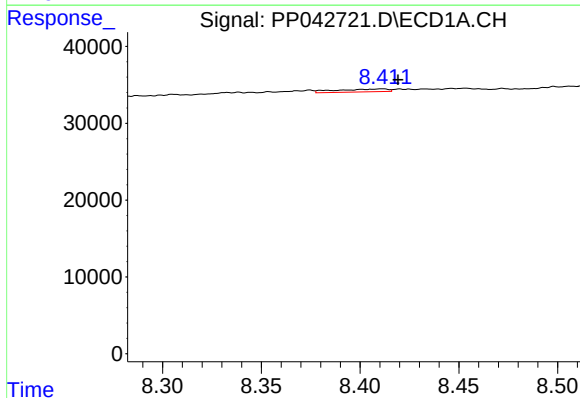


#30 AR-1254-5

R.T.: 8.412 min
Delta R.T.: -0.007 min
Response: 6803
Conc: 10.76 ng/ml

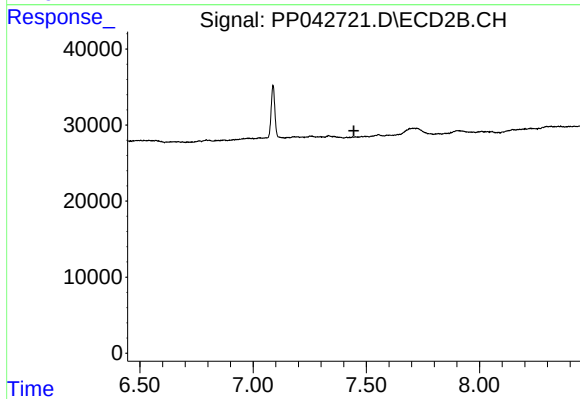

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.445 min
Response: 0
Conc: N.D.

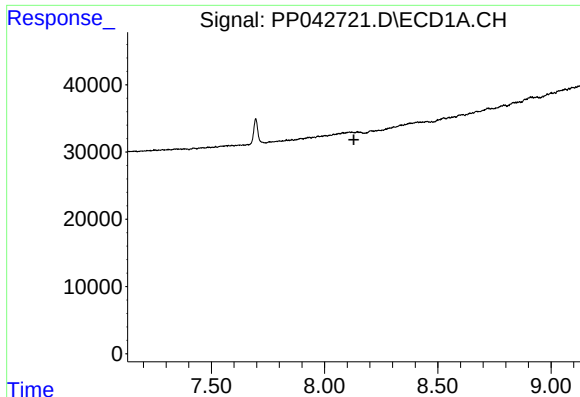

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 8.130 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
FM-E6-01-4.5

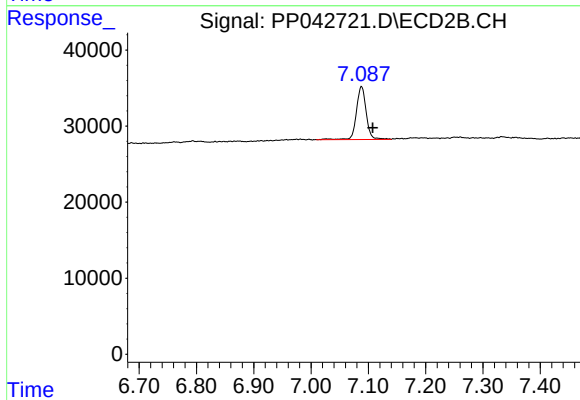


#32 AR-1260-2

R.T.: 7.088 min
Delta R.T.: -0.020 min
Response: 83013
Conc: 54.60 ng/ml

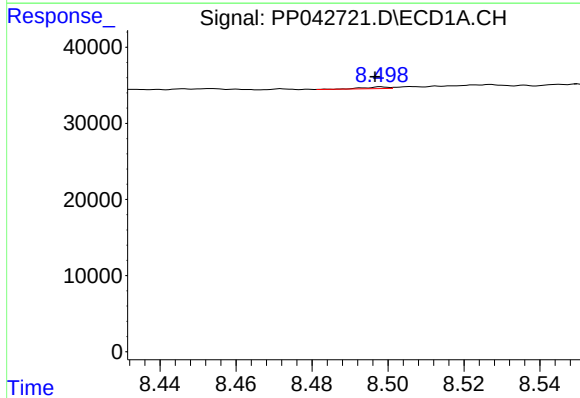


#33 AR-1260-3

R.T.: 8.498 min
Delta R.T.: 0.002 min
Response: 985
Conc: 1.78 ng/ml

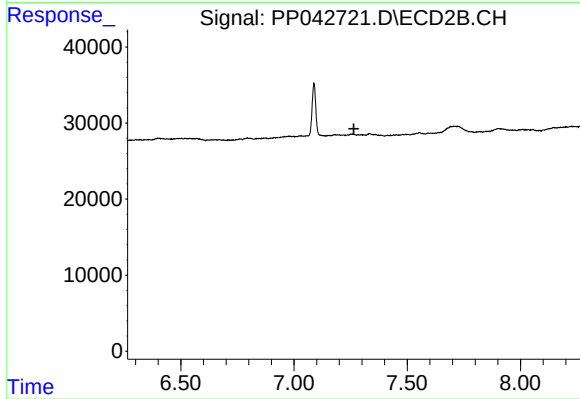

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.264 min
Response: 0
Conc: N.D.

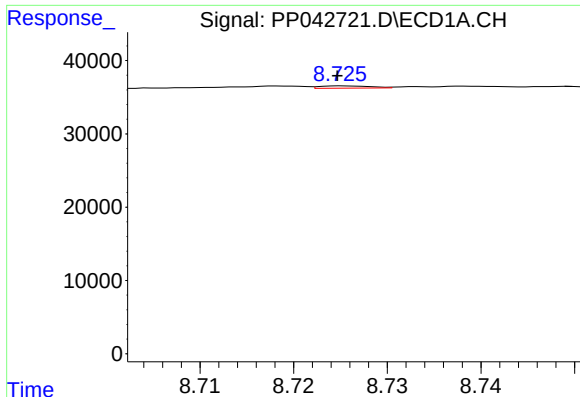

#34 AR-1260-4


R.T.: 8.725 min
Delta R.T.: 0.000 min
Response: 1156
Conc: 1.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
FM-E6-01-4.5

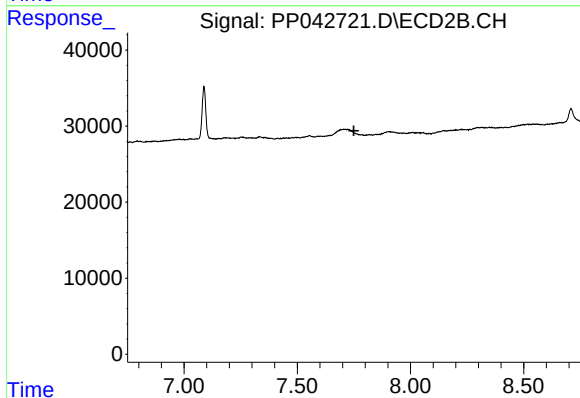


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.750 min
Response: 0
Conc: N.D.

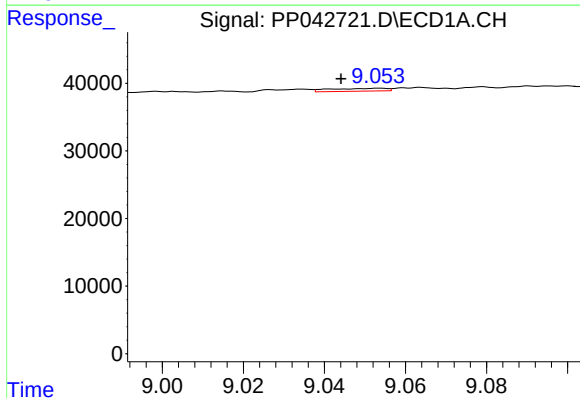


#35 AR-1260-5

R.T.: 9.054 min
Delta R.T.: 0.010 min
Response: 4110
Conc: 3.41 ng/ml

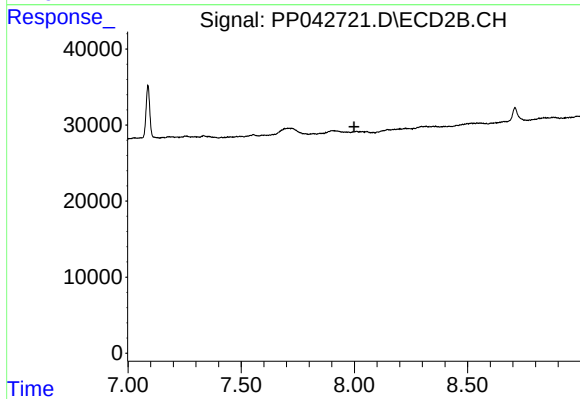

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.998 min
Response: 0
Conc: N.D.

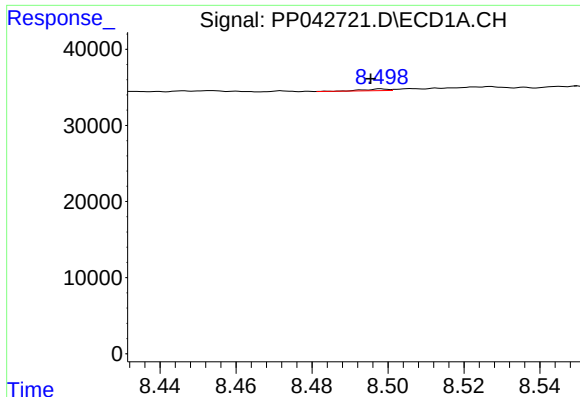

#36 AR-1262-1


R.T.: 8.498 min
Delta R.T.: 0.003 min
Response: 985
Conc: 1.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
FM-E6-01-4.5

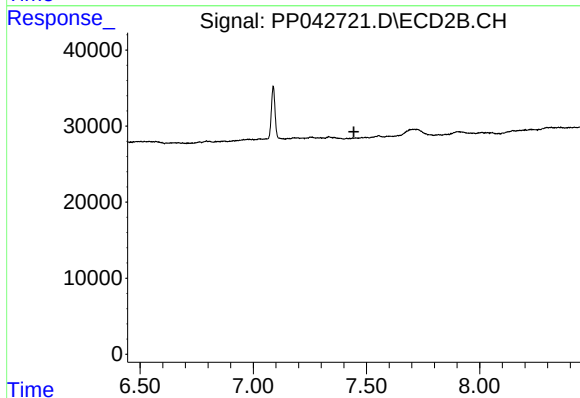


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.444 min
Response: 0
Conc: N.D.

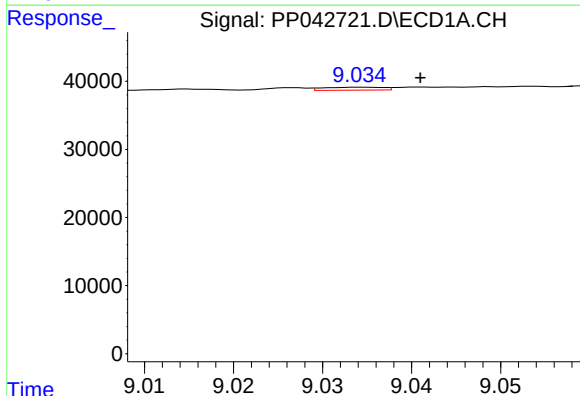


#37 AR-1262-2

R.T.: 9.034 min
Delta R.T.: -0.007 min
Response: 1973
Conc: 1.48 ng/ml

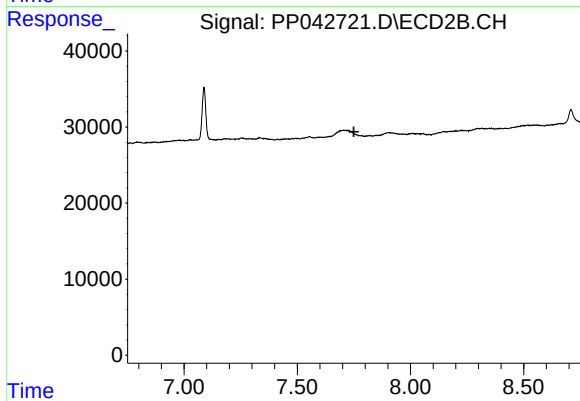

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.750 min
Response: 0
Conc: N.D.

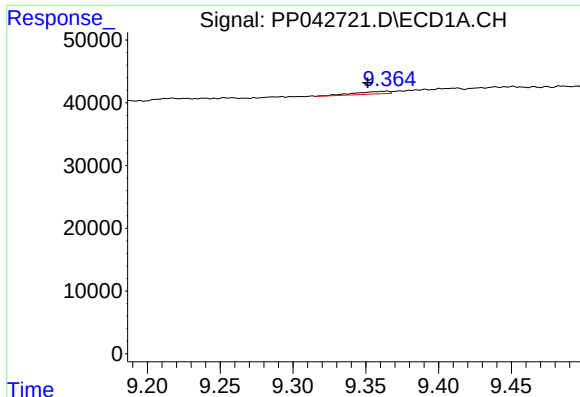

#38 AR-1262-3


R.T.: 9.365 min
Delta R.T.: 0.013 min
Response: 6805
Conc: 10.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
FM-E6-01-4.5

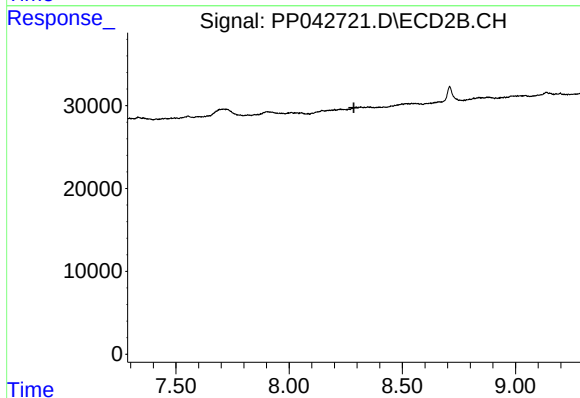


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.286 min
Response: 0
Conc: N.D.

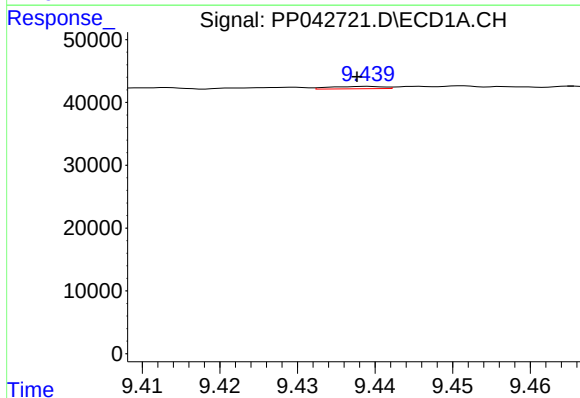


#39 AR-1262-4

R.T.: 9.439 min
Delta R.T.: 0.001 min
Response: 1770
Conc: 3.66 ng/ml

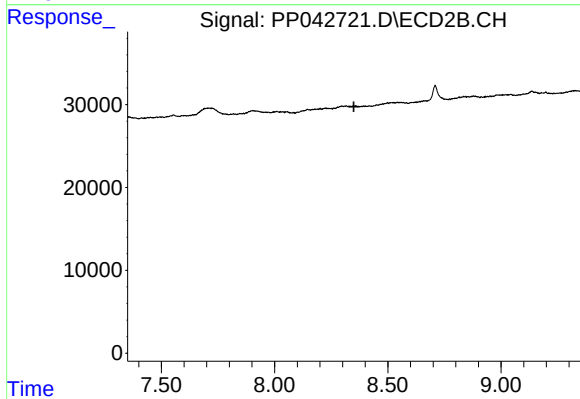

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.350 min
Response: 0
Conc: N.D.

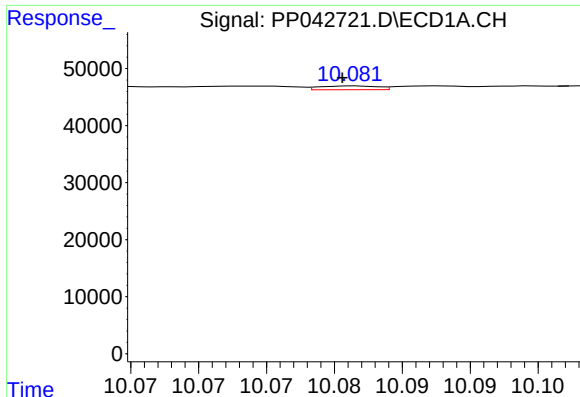

#40 AR-1262-5


R.T.: 10.082 min
Delta R.T.: 0.000 min
Response: 1951
Conc: 4.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
FM-E6-01-4.5

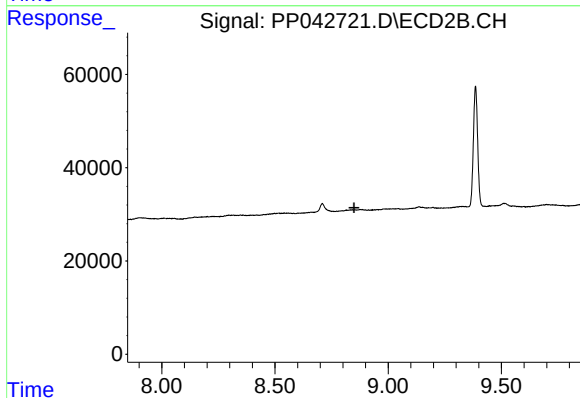


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 8.849 min
Response: 0
Conc: N.D.

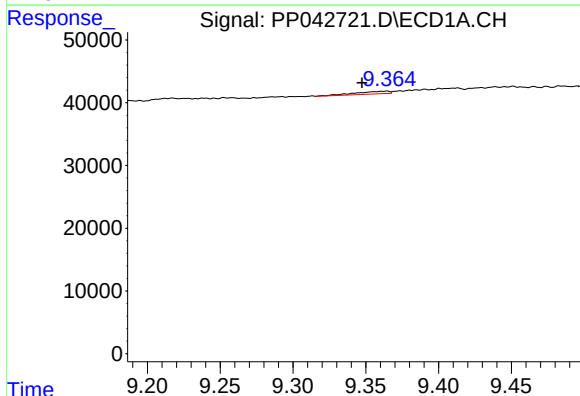


#41 AR-1268-1

R.T.: 9.365 min
Delta R.T.: 0.017 min
Response: 6805
Conc: 4.16 ng/ml

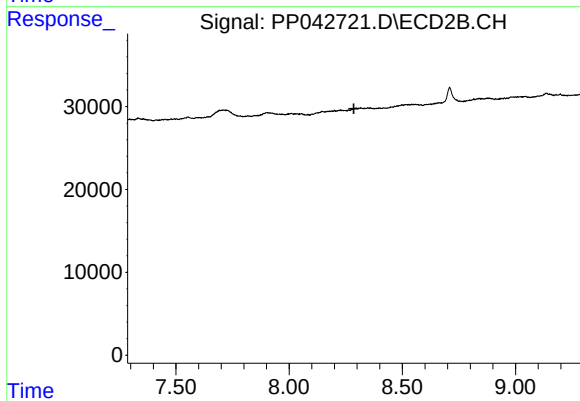

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 8.286 min
Response: 0
Conc: N.D.

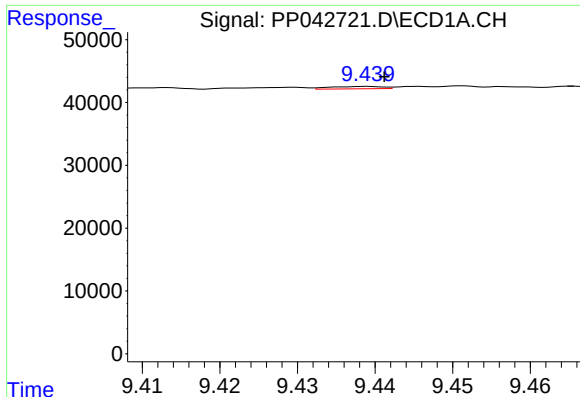

#42 AR-1268-2


R.T.: 9.439 min
Delta R.T.: -0.002 min
Response: 1770
Conc: 1.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
FM-E6-01-4.5

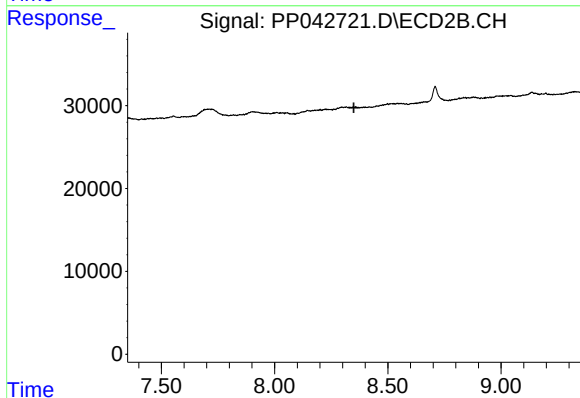


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.351 min
Response: 0
Conc: N.D.

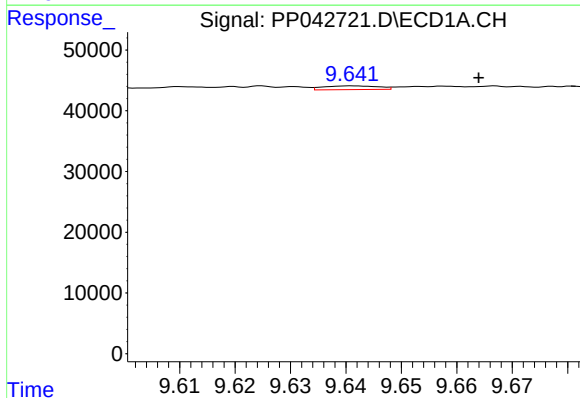


#43 AR-1268-3

R.T.: 9.641 min
Delta R.T.: -0.023 min
Response: 4249
Conc: 3.16 ng/ml

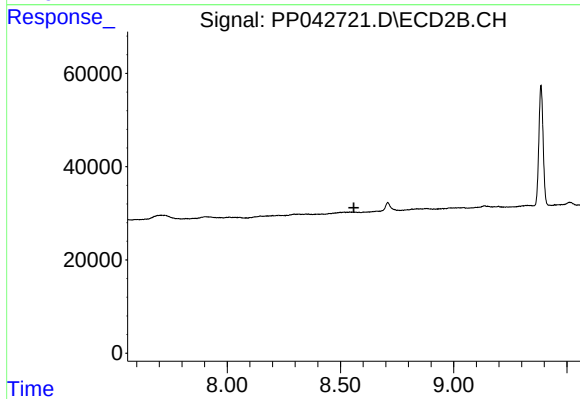

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 8.560 min
Response: 0
Conc: N.D.

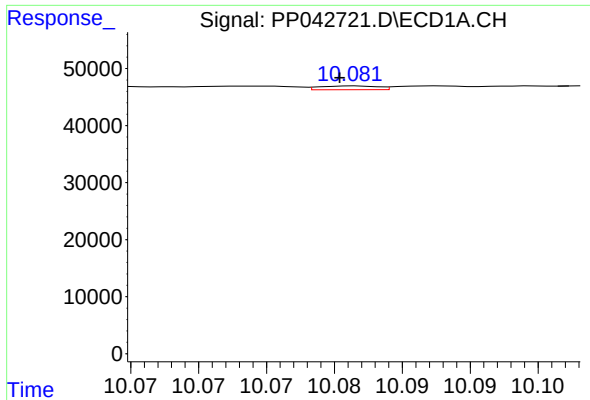

#44 AR-1268-4

R.T.: 10.082 min
Delta R.T.: 0.001 min
Response: 1951
Conc: 3.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
FM-E6-01-4.5

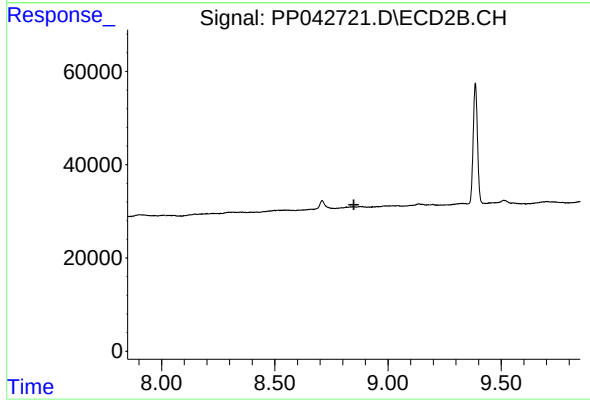

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.849 min
Response: 0
Conc: N.D.