

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010722\
 Data File : PP042723.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jan 2022 21:13
 Operator : AJ\MA
 Sample : N1071-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FM-0226-01-4.5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 02:07:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 05 12:01:35 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.881	4.049	439157	592521	22.668	22.635
2)	SA Decachlor...	10.815	9.386	293501	389334	25.018	19.811
Target Compounds							
7)	L1 AR-1016-5	6.710f	0.000	613	0	1.419	N.D. #
8)	L2 AR-1221-1	5.115	0.000	21538	0	104.349	N.D. #
9)	L2 AR-1221-2	0.000	4.403	0	8304	N.D.	30.923 #
23)	L5 AR-1248-3	6.710f	0.000	613	0	1.077	N.D. #
28)	L6 AR-1254-3	7.696	0.000	27315	0	29.818	N.D. #
30)	L6 AR-1254-5	8.406	7.444	1720	13612	2.721	8.288 #
32)	L7 AR-1260-2	8.120	7.088f	22882	45416	32.530	29.874
33)	L7 AR-1260-3	8.490	0.000	14235	0	25.694	N.D. #
36)	L8 AR-1262-1	8.490	7.444	14235	13612	18.184	15.681
39)	L8 AR-1262-4	9.451	0.000	8543	0	17.676	N.D. #
40)	L8 AR-1262-5	10.093	0.000	4640	0	9.509	N.D. #
42)	L9 AR-1268-2	9.451	0.000	8543	0	5.648	N.D. #
43)	L9 AR-1268-3	9.670	0.000	14057	0	10.444	N.D. #
44)	L9 AR-1268-4	10.093	0.000	4640	0	8.476	N.D. #
45)	L9 AR-1268-5	10.508f	0.000	47747	0	10.698	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010722\
Data File : PP042723.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jan 2022 21:13
Operator : AJ\MA
Sample : N1071-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FM-0226-01-4.5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 02:07:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 05 12:01:35 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

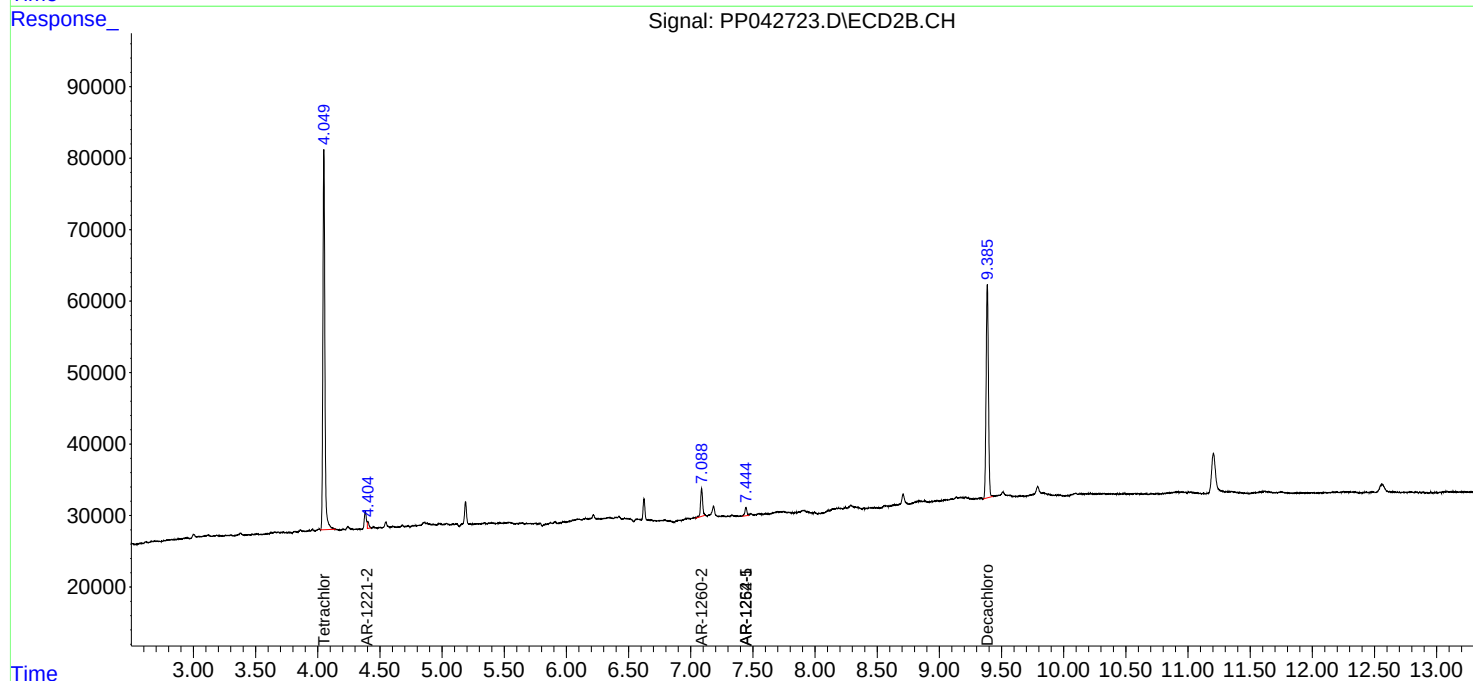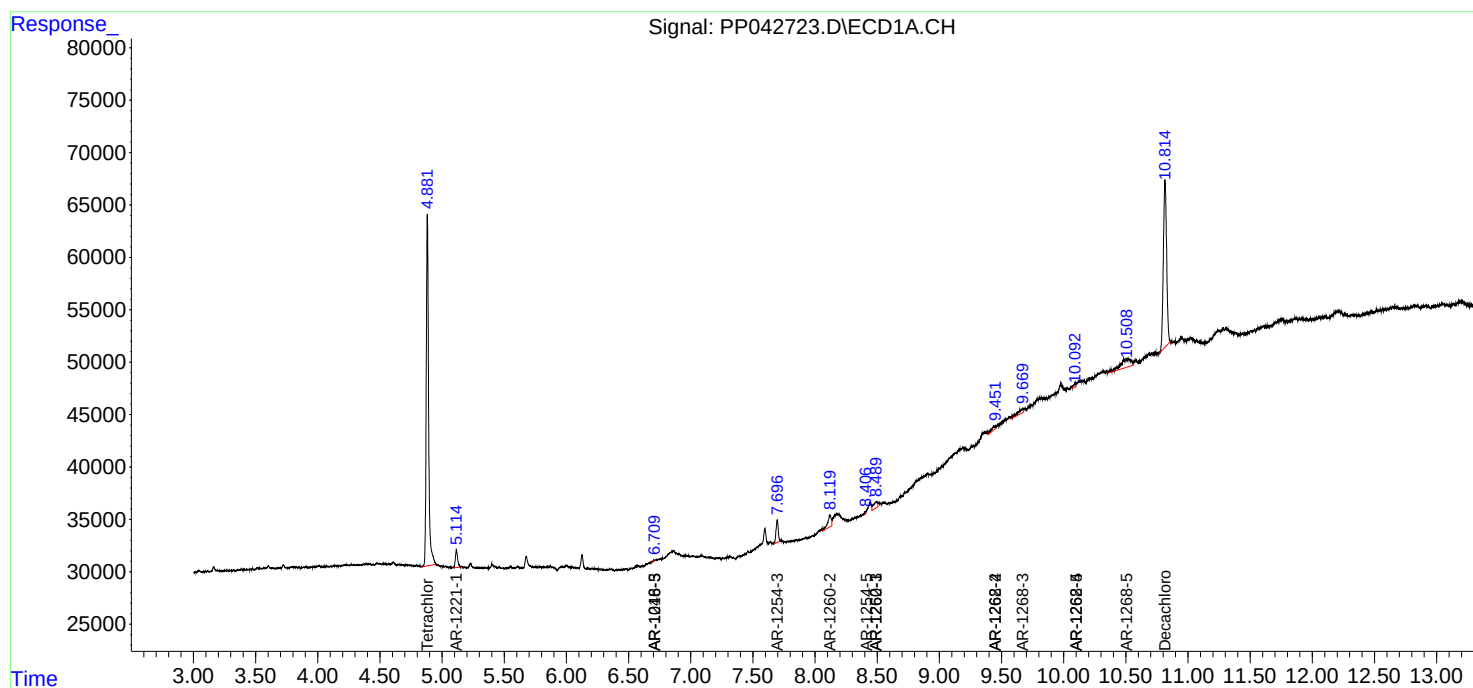


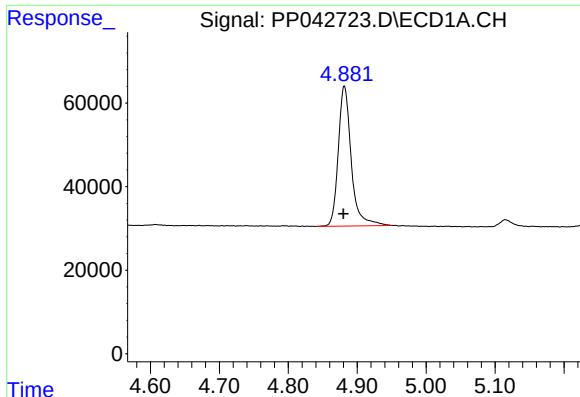

#1 Tetrachloro-m-xylene


R.T.: 4.881 min
Delta R.T.: 0.001 min
Response: 439157
Conc: 22.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
FM-0226-01-4.5

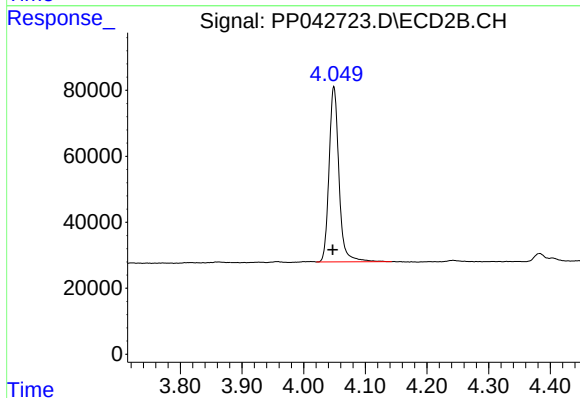


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: 0.002 min
Response: 592521
Conc: 22.63 ng/ml

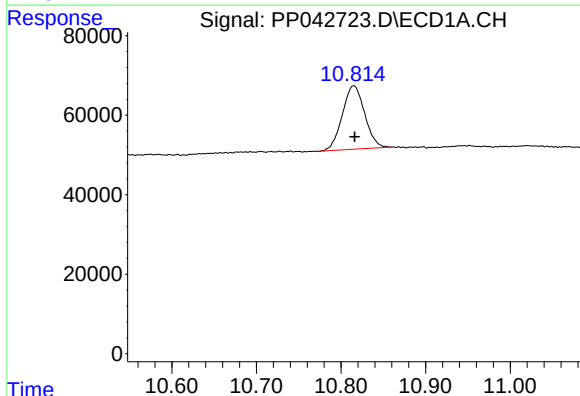


#2 Decachlorobiphenyl

R.T.: 10.815 min
Delta R.T.: -0.001 min
Response: 293501
Conc: 25.02 ng/ml

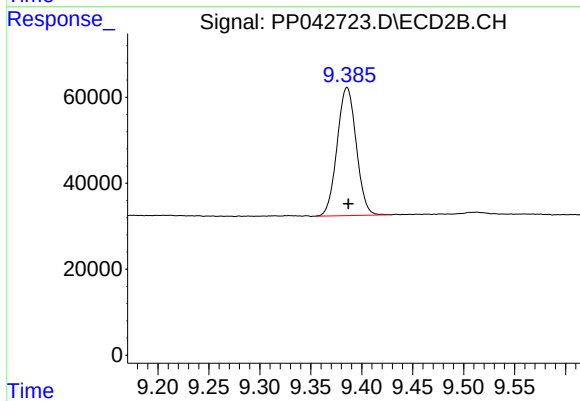

#2 Decachlorobiphenyl


R.T.: 9.386 min
Delta R.T.: -0.001 min
Response: 389334
Conc: 19.81 ng/ml

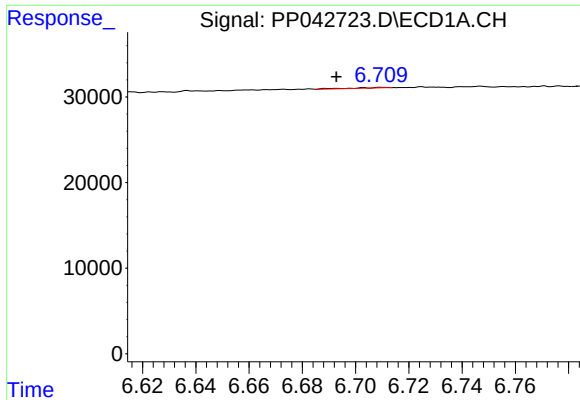

#7 AR-1016-5


R.T.: 6.710 min
Delta R.T.: 0.017 min
Response: 613
Conc: 1.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
FM-0226-01-4.5

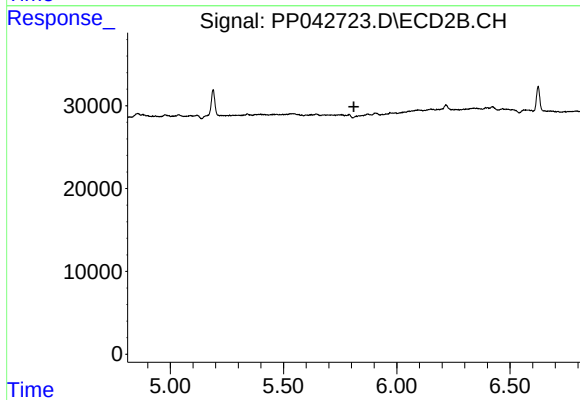


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 5.811 min
Response: 0
Conc: N.D.

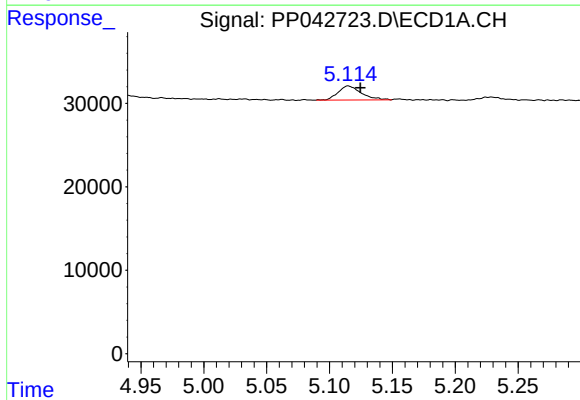


#8 AR-1221-1

R.T.: 5.115 min
Delta R.T.: -0.010 min
Response: 21538
Conc: 104.35 ng/ml

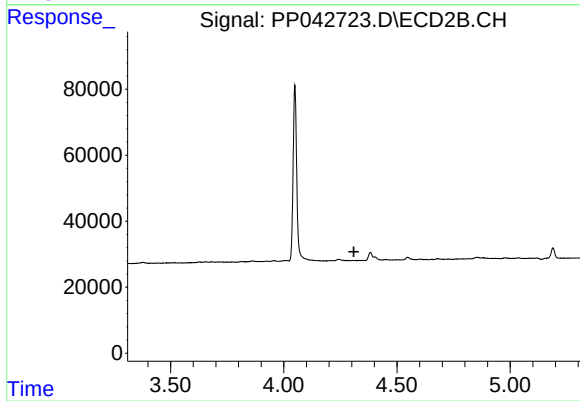

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 4.310 min
Response: 0
Conc: N.D.

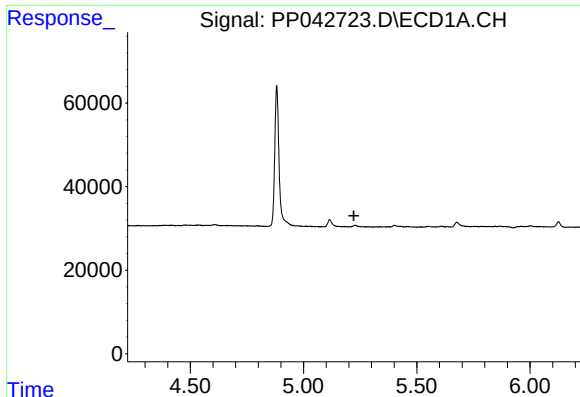

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 5.222 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
FM-0226-01-4.5

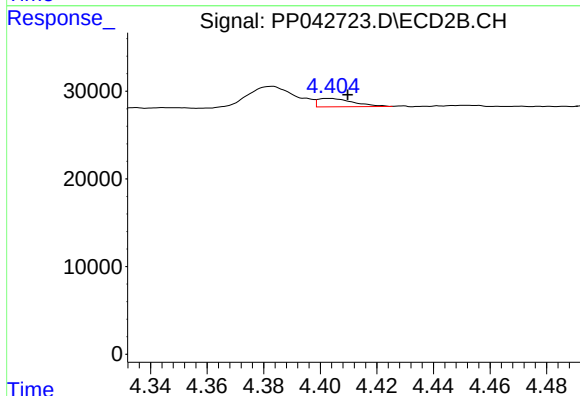


#9 AR-1221-2

R.T.: 4.403 min
Delta R.T.: -0.006 min
Response: 8304
Conc: 30.92 ng/ml

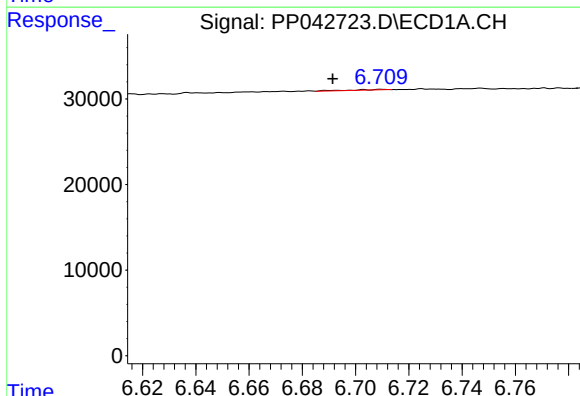


#23 AR-1248-3

R.T.: 6.710 min
Delta R.T.: 0.018 min
Response: 613
Conc: 1.08 ng/ml

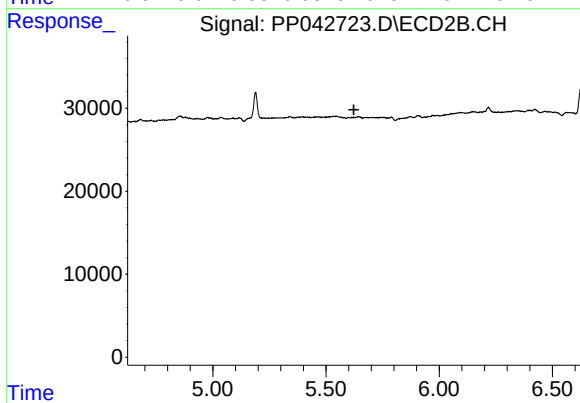

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 5.623 min
Response: 0
Conc: N.D.

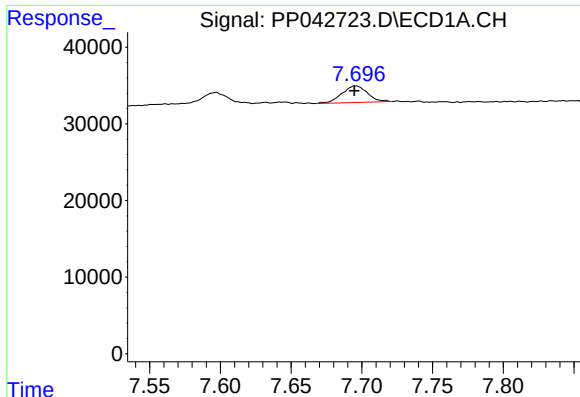

#28 AR-1254-3


R.T.: 7.696 min
Delta R.T.: 0.001 min
Response: 27315
Conc: 29.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
FM-0226-01-4.5

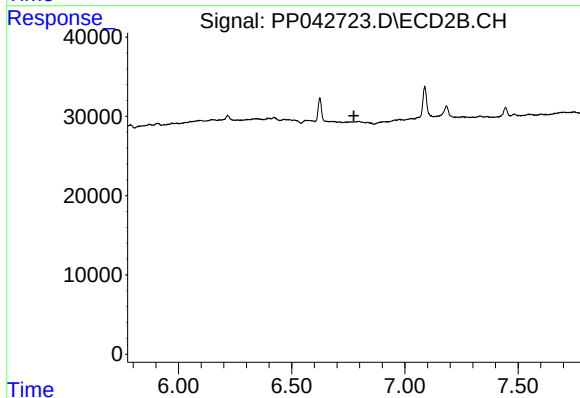


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.774 min
Response: 0
Conc: N.D.

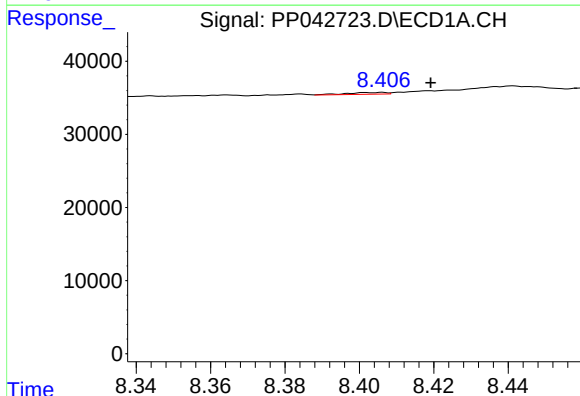


#30 AR-1254-5

R.T.: 8.406 min
Delta R.T.: -0.013 min
Response: 1720
Conc: 2.72 ng/ml

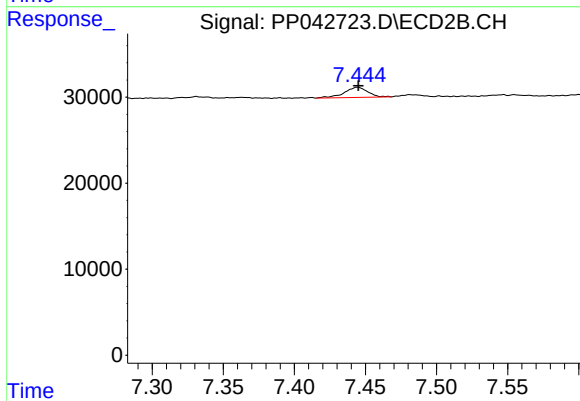

#30 AR-1254-5


R.T.: 7.444 min
Delta R.T.: 0.000 min
Response: 13612
Conc: 8.29 ng/ml

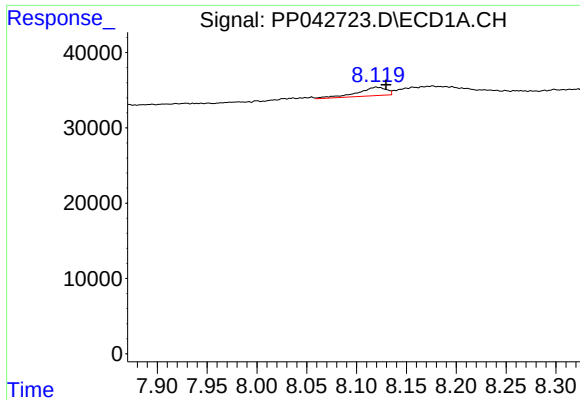

#32 AR-1260-2


R.T.: 8.120 min
Delta R.T.: -0.010 min
Response: 22882
Conc: 32.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
FM-0226-01-4.5

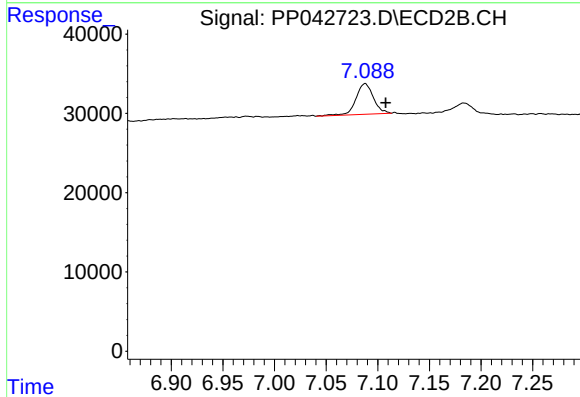


#32 AR-1260-2

R.T.: 7.088 min
Delta R.T.: -0.020 min
Response: 45416
Conc: 29.87 ng/ml

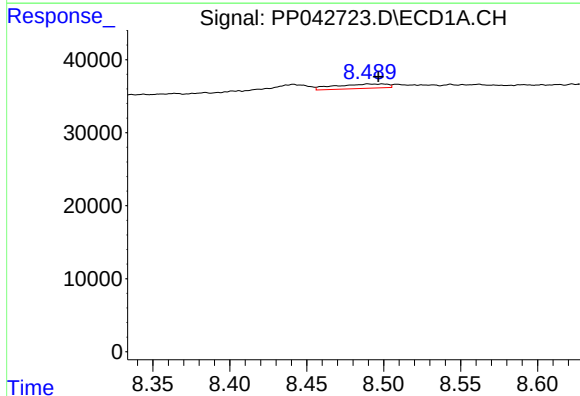


#33 AR-1260-3

R.T.: 8.490 min
Delta R.T.: -0.007 min
Response: 14235
Conc: 25.69 ng/ml

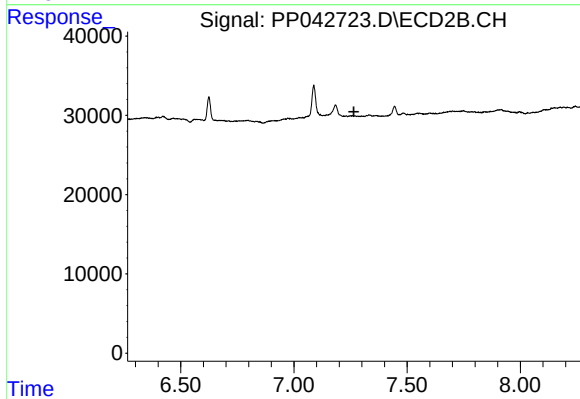

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.264 min
Response: 0
Conc: N.D.

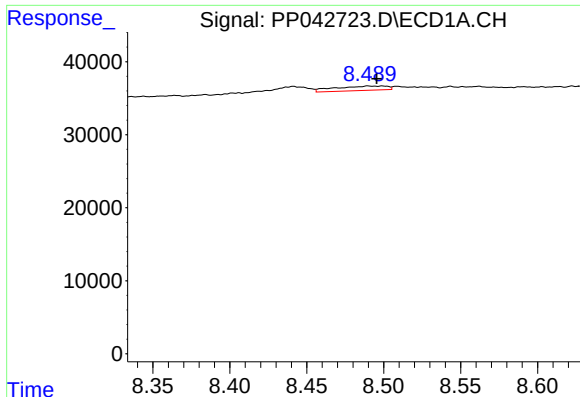

#36 AR-1262-1


R.T.: 8.490 min
Delta R.T.: -0.006 min
Response: 14235
Conc: 18.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
FM-0226-01-4.5

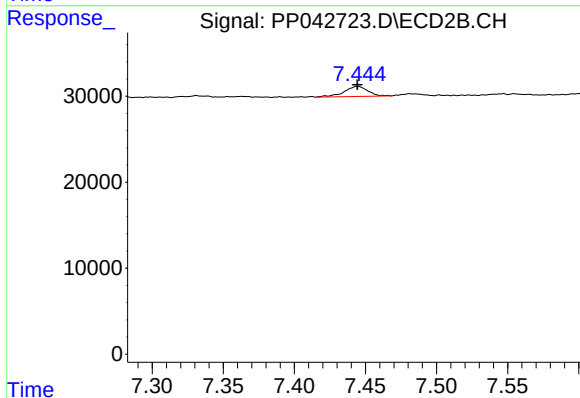


#36 AR-1262-1

R.T.: 7.444 min
Delta R.T.: 0.000 min
Response: 13612
Conc: 15.68 ng/ml

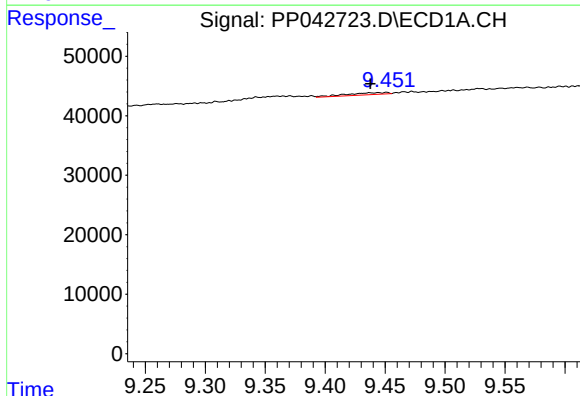


#39 AR-1262-4

R.T.: 9.451 min
Delta R.T.: 0.014 min
Response: 8543
Conc: 17.68 ng/ml

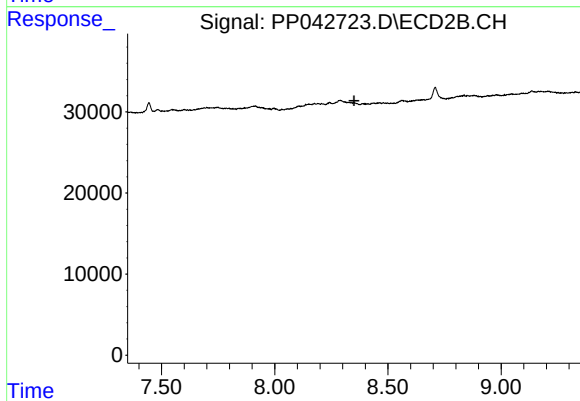

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.350 min
Response: 0
Conc: N.D.

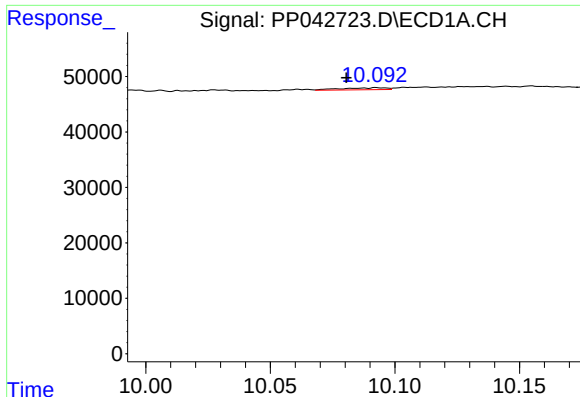

#40 AR-1262-5


R.T.: 10.093 min
Delta R.T.: 0.012 min
Response: 4640
Conc: 9.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
FM-0226-01-4.5

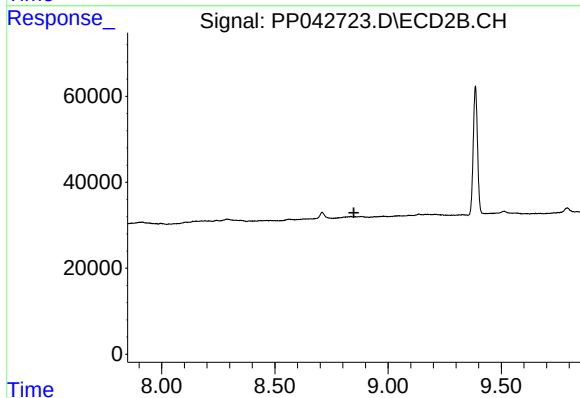


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 8.849 min
Response: 0
Conc: N.D.

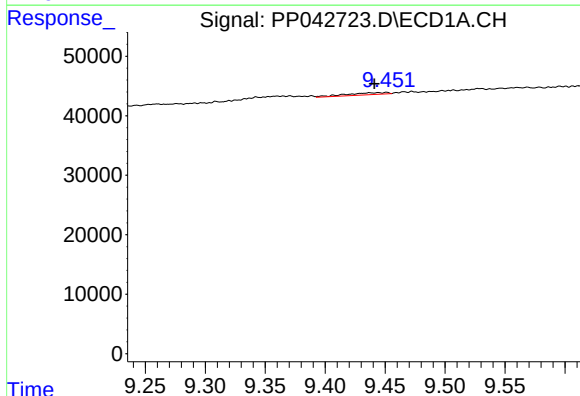


#42 AR-1268-2

R.T.: 9.451 min
Delta R.T.: 0.010 min
Response: 8543
Conc: 5.65 ng/ml

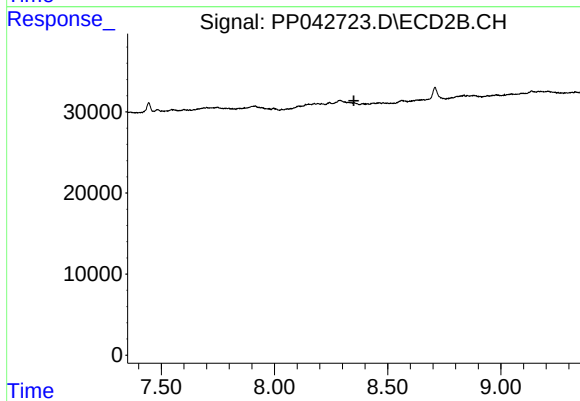

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.351 min
Response: 0
Conc: N.D.

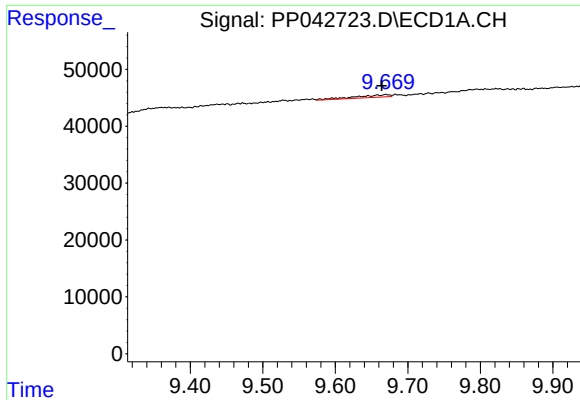

#43 AR-1268-3


R.T.: 9.670 min
Delta R.T.: 0.006 min
Response: 14057
Conc: 10.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
FM-0226-01-4.5

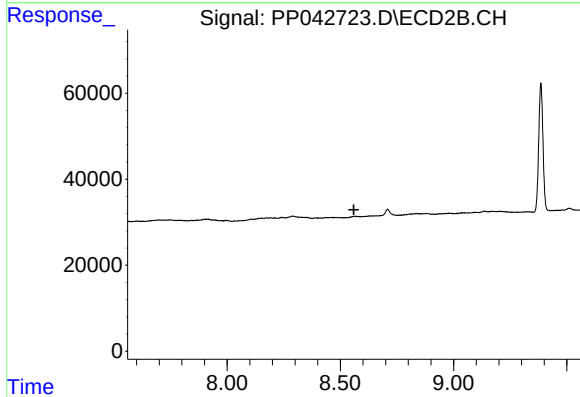


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.560 min
Response: 0
Conc: N.D.

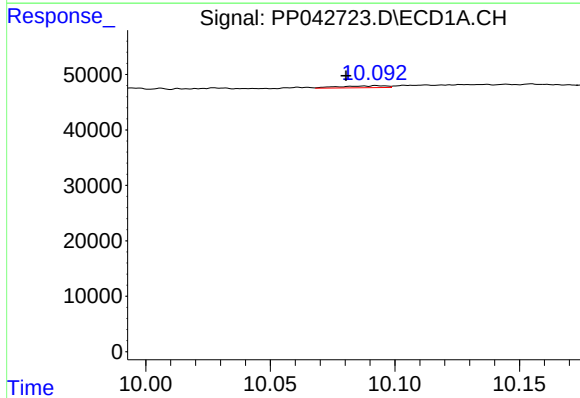


#44 AR-1268-4

R.T.: 10.093 min
Delta R.T.: 0.013 min
Response: 4640
Conc: 8.48 ng/ml

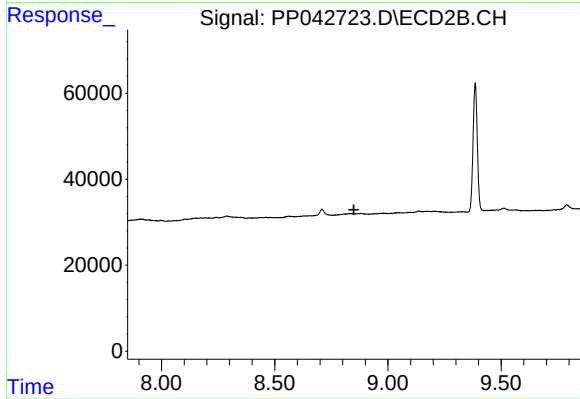

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 8.849 min
Response: 0
Conc: N.D.

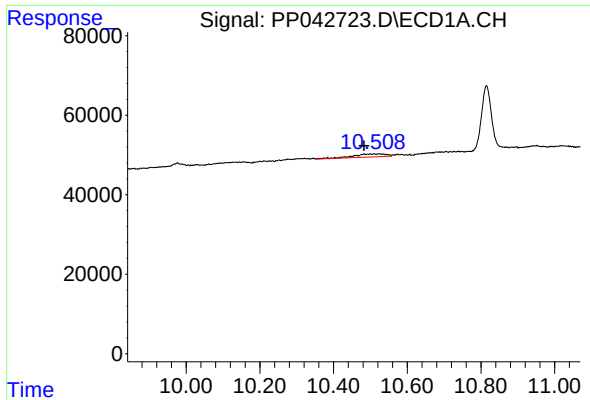

#45 AR-1268-5

R.T.: 10.508 min
Delta R.T.: 0.025 min
Response: 47747
Conc: 10.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
FM-0226-01-4.5

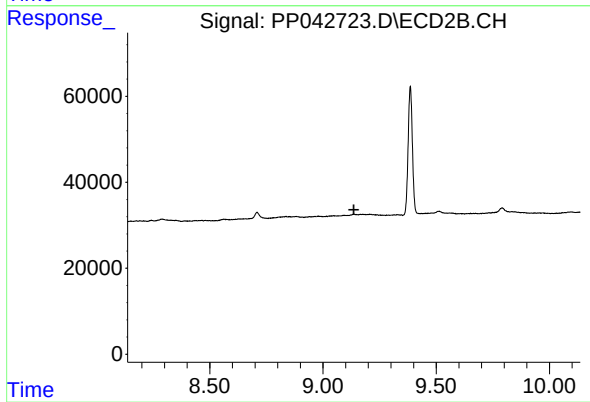

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.137 min
Response: 0
Conc: N.D.