

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010722\
 Data File : PP042727.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jan 2022 22:19
 Operator : AJ\MA
 Sample : N1065-05
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AMI-1-CONCRETE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 02:08:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 05 12:01:35 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.882	4.049	507895	637397	26.216	24.349
2)	SA Decachlor...	10.819	9.387	348177	471671	29.679	24.000
Target Compounds							
8)	L2 AR-1221-1	5.115	0.000	39525	0	191.497	N.D. #
9)	L2 AR-1221-2	5.228	4.383f	7007	62452	44.285	232.562 #
28)	L6 AR-1254-3	7.697	0.000	6485	0	7.080	N.D. #
30)	L6 AR-1254-5	8.415	0.000	1785	0	2.824	N.D. #
32)	L7 AR-1260-2	8.130	0.000	399	0	0.567	N.D. #
33)	L7 AR-1260-3	8.498	0.000	934	0	1.687	N.D. #
34)	L7 AR-1260-4	8.723	0.000	2345	0	3.555	N.D. #
35)	L7 AR-1260-5	9.046	0.000	1464	0	1.213	N.D. #
36)	L8 AR-1262-1	8.498	0.000	934	0	1.194	N.D. #
37)	L8 AR-1262-2	9.046	0.000	1464	0	1.094	N.D. #
38)	L8 AR-1262-3	9.345	0.000	1079	0	1.637	N.D. #
39)	L8 AR-1262-4	9.414f	0.000	180	0	0.372	N.D. #
40)	L8 AR-1262-5	10.057f	0.000	2017	0	4.134	N.D. #
41)	L9 AR-1268-1	9.345	0.000	1079	0	0.659	N.D. #
42)	L9 AR-1268-2	9.414f	0.000	180	0	0.119	N.D. #
43)	L9 AR-1268-3	9.669	0.000	2021	0	1.502	N.D. #
44)	L9 AR-1268-4	10.057f	0.000	2017	0	3.685	N.D. #
45)	L9 AR-1268-5	10.479	0.000	1751	0	0.392	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010722\
Data File : PP042727.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jan 2022 22:19
Operator : AJ\MA
Sample : N1065-05
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AMI-1-CONCRETE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 02:08:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 05 12:01:35 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

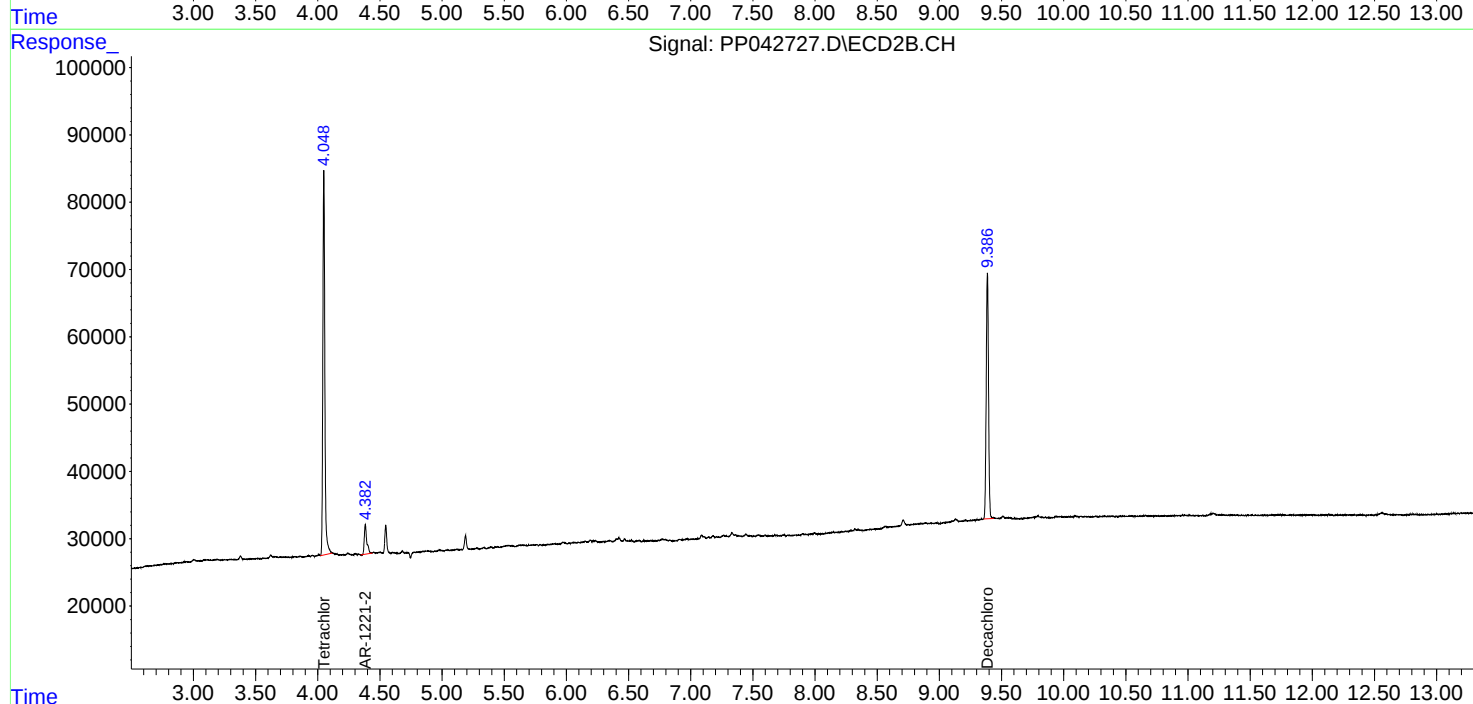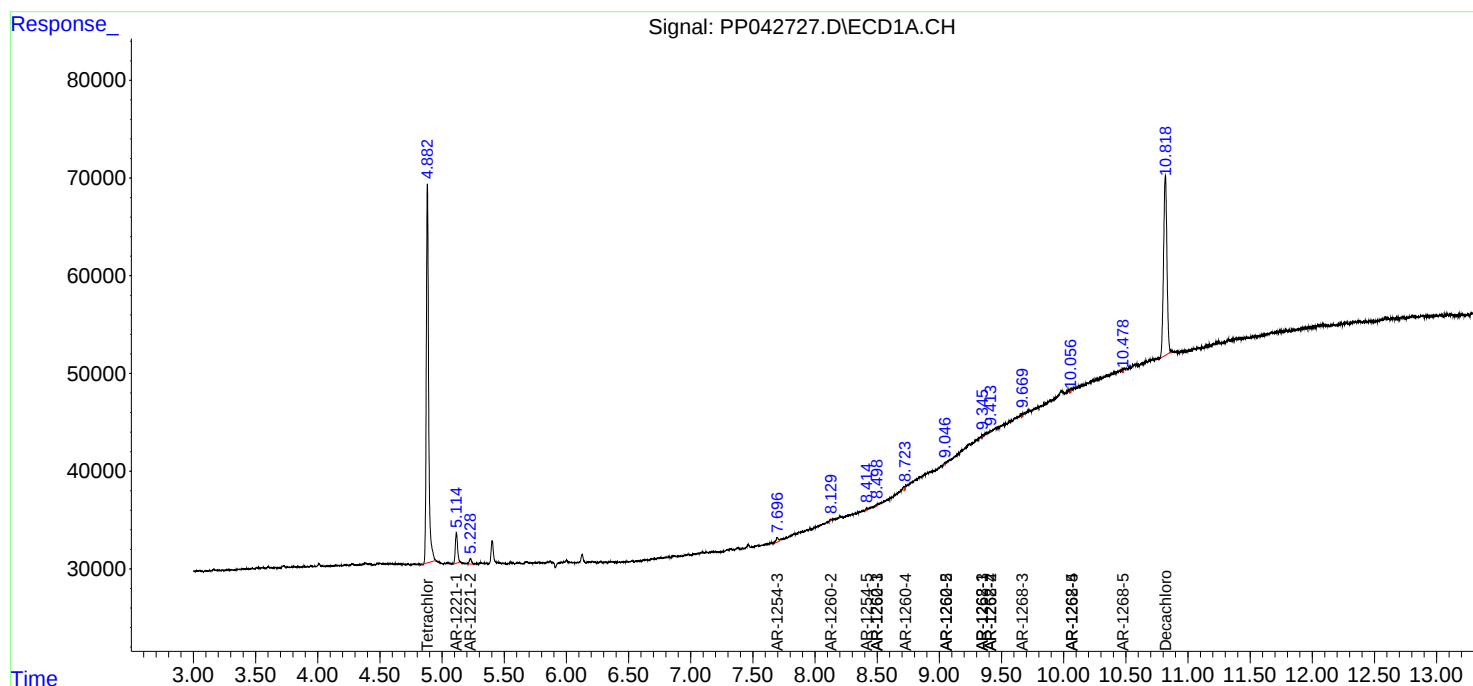


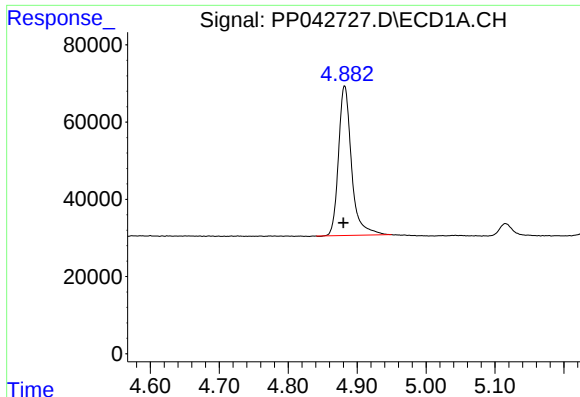

#1 Tetrachloro-m-xylene


R.T.: 4.882 min
Delta R.T.: 0.002 min
Response: 507895
Conc: 26.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
AMI-1-CONCRETE

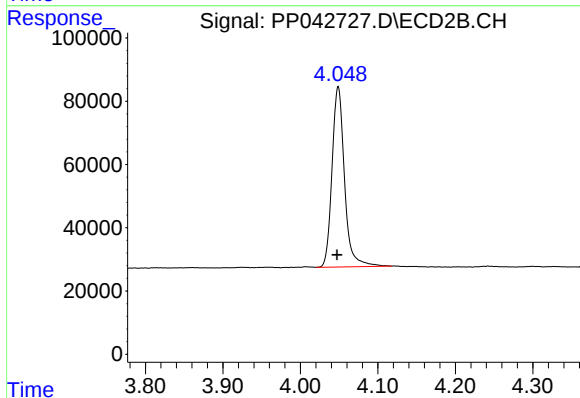


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: 0.002 min
Response: 637397
Conc: 24.35 ng/ml

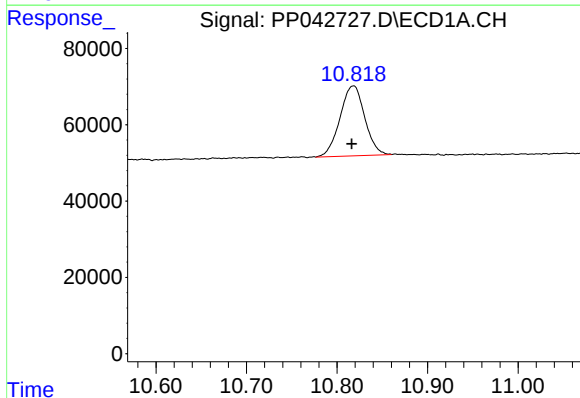


#2 Decachlorobiphenyl

R.T.: 10.819 min
Delta R.T.: 0.002 min
Response: 348177
Conc: 29.68 ng/ml

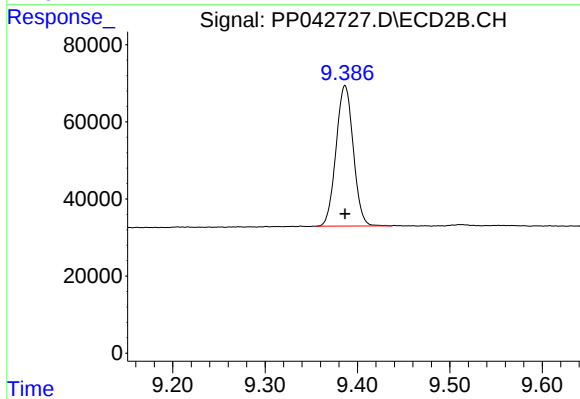

#2 Decachlorobiphenyl


R.T.: 9.387 min
Delta R.T.: 0.000 min
Response: 471671
Conc: 24.00 ng/ml

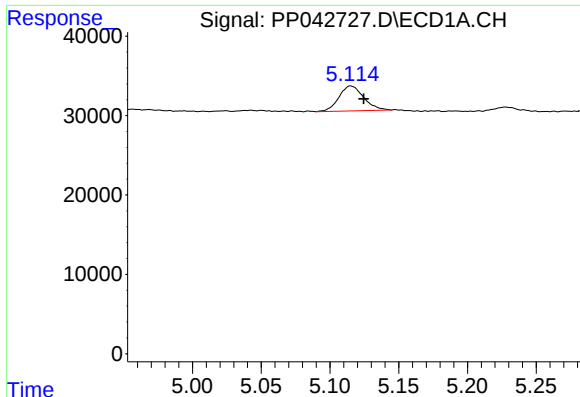

#8 AR-1221-1


R.T.: 5.115 min
Delta R.T.: -0.010 min
Response: 39525
Conc: 191.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
AMI-1-CONCRETE

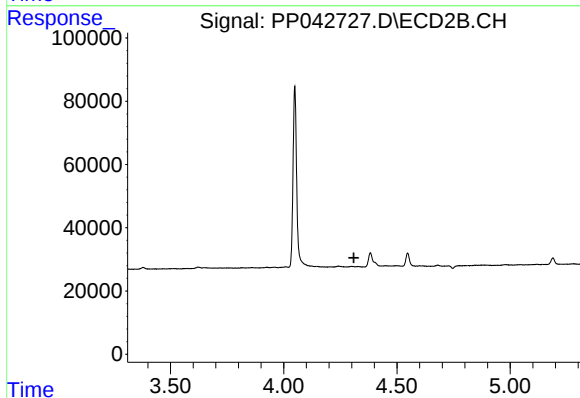


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.310 min
Response: 0
Conc: N.D.

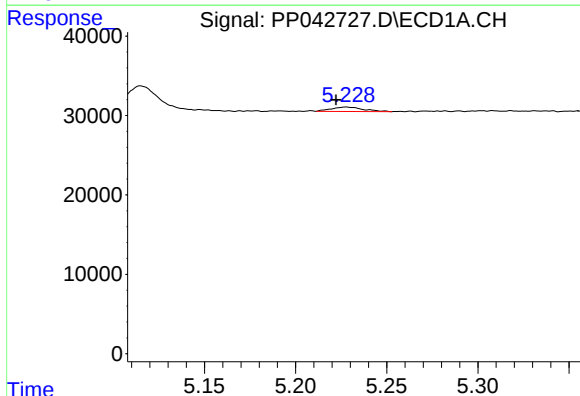


#9 AR-1221-2

R.T.: 5.228 min
Delta R.T.: 0.006 min
Response: 7007
Conc: 44.28 ng/ml

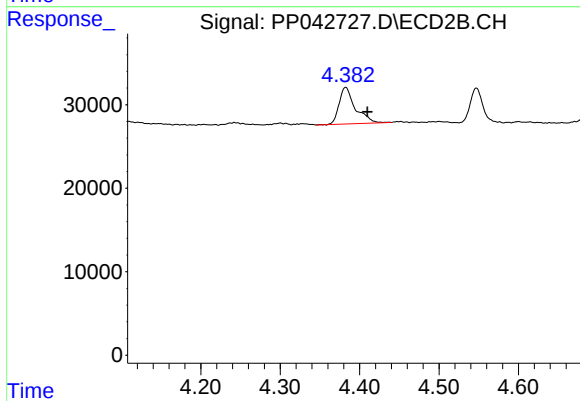

#9 AR-1221-2


R.T.: 4.383 min
Delta R.T.: -0.027 min
Response: 62452
Conc: 232.56 ng/ml

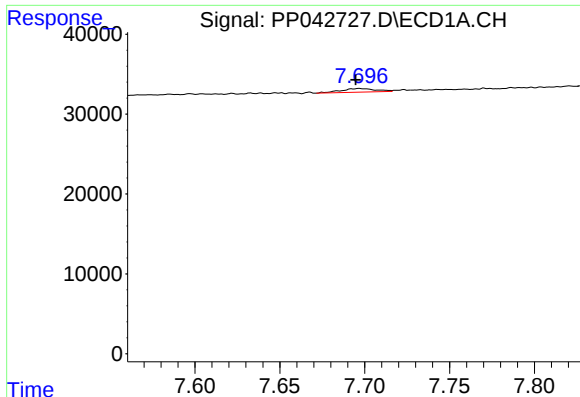

#28 AR-1254-3


R.T.: 7.697 min
Delta R.T.: 0.002 min
Response: 6485
Conc: 7.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
AMI-1-CONCRETE

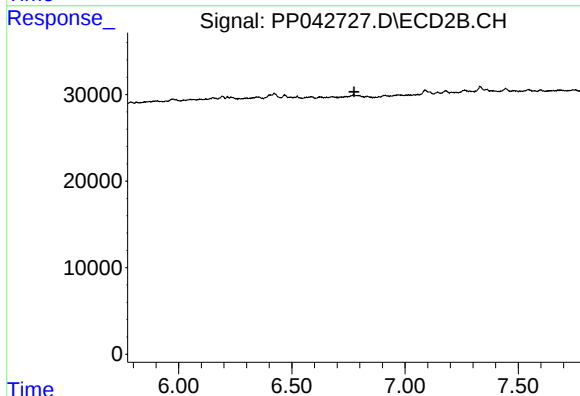


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.774 min
Response: 0
Conc: N.D.

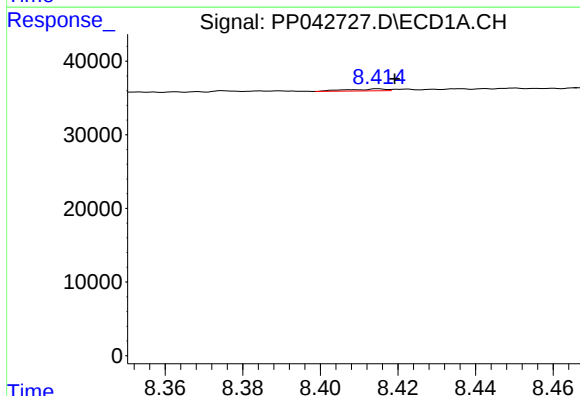


#30 AR-1254-5

R.T.: 8.415 min
Delta R.T.: -0.004 min
Response: 1785
Conc: 2.82 ng/ml

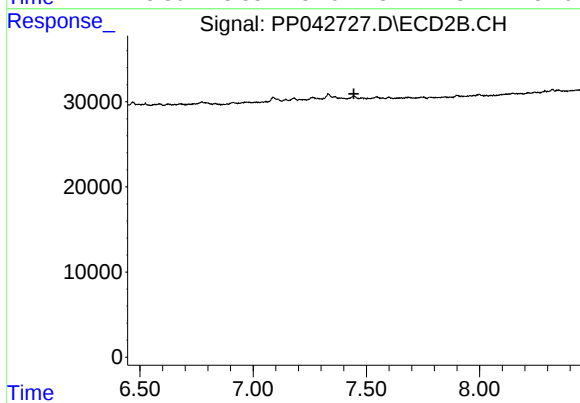

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.445 min
Response: 0
Conc: N.D.

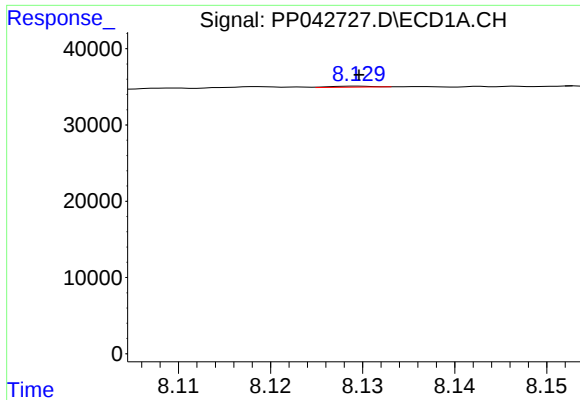

#32 AR-1260-2


R.T.: 8.130 min
Delta R.T.: 0.000 min
Response: 399
Conc: 0.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
AMI-1-CONCRETE

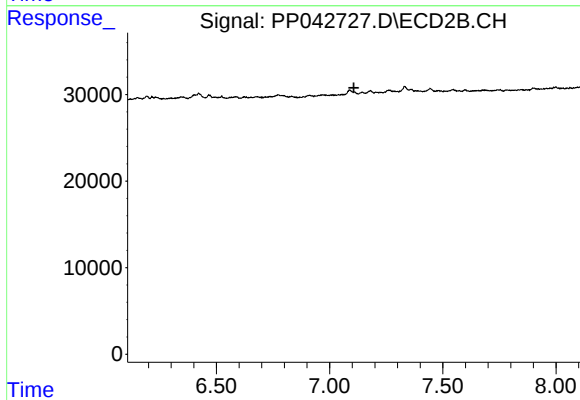


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.108 min
Response: 0
Conc: N.D.

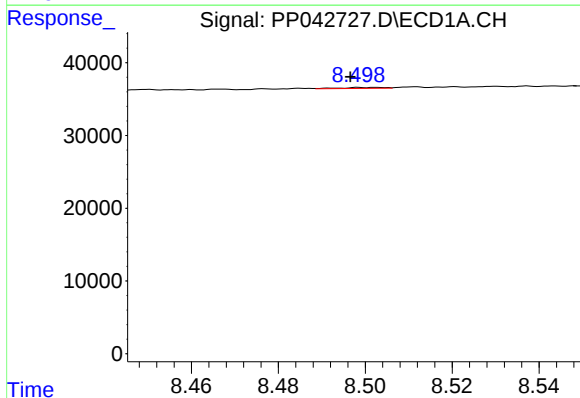


#33 AR-1260-3

R.T.: 8.498 min
Delta R.T.: 0.002 min
Response: 934
Conc: 1.69 ng/ml

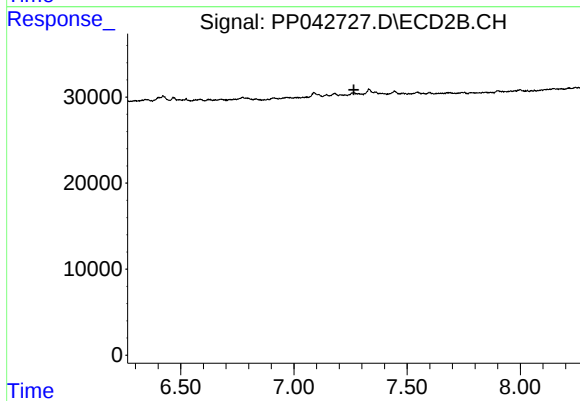

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.264 min
Response: 0
Conc: N.D.

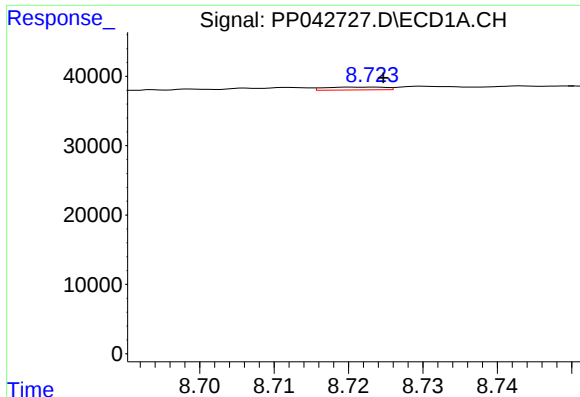

#34 AR-1260-4


R.T.: 8.723 min
Delta R.T.: -0.001 min
Response: 2345
Conc: 3.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
AMI-1-CONCRETE

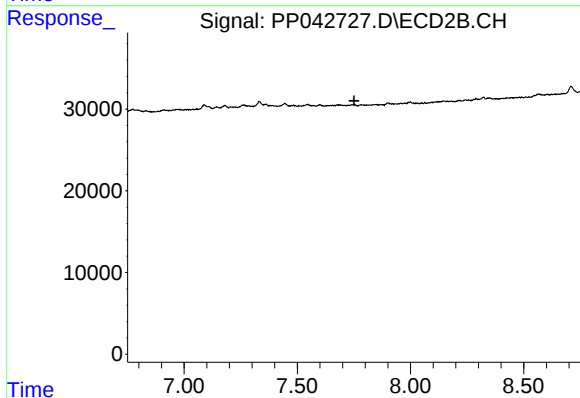


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.750 min
Response: 0
Conc: N.D.

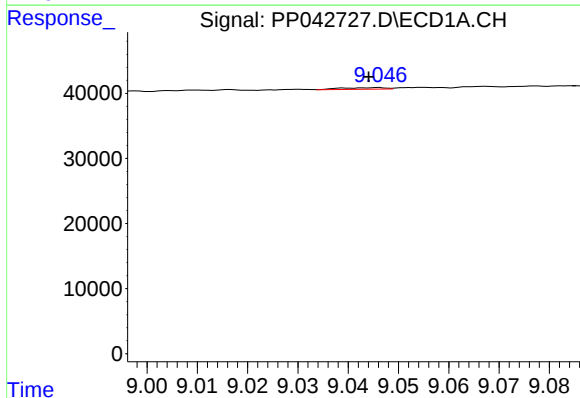


#35 AR-1260-5

R.T.: 9.046 min
Delta R.T.: 0.002 min
Response: 1464
Conc: 1.21 ng/ml

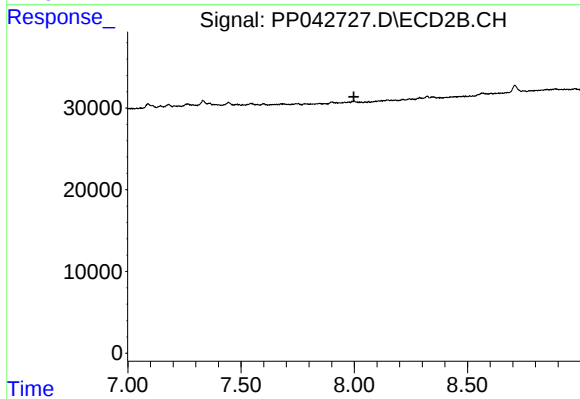

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.998 min
Response: 0
Conc: N.D.

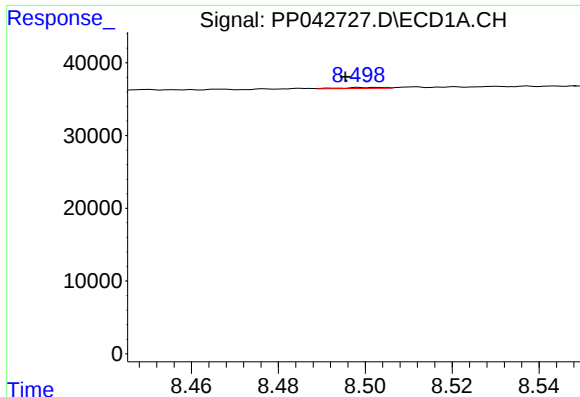

#36 AR-1262-1


R.T.: 8.498 min
Delta R.T.: 0.003 min
Response: 934
Conc: 1.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
AMI-1-CONCRETE

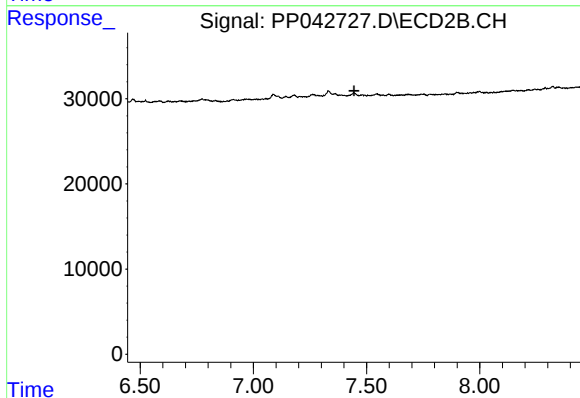


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.444 min
Response: 0
Conc: N.D.

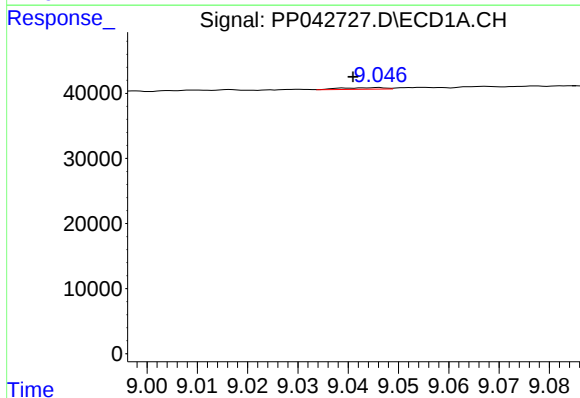


#37 AR-1262-2

R.T.: 9.046 min
Delta R.T.: 0.005 min
Response: 1464
Conc: 1.09 ng/ml

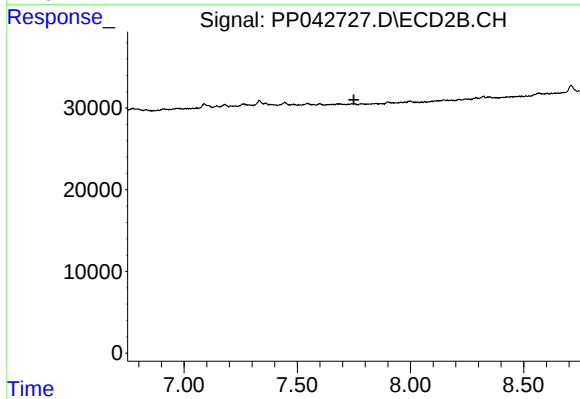

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.750 min
Response: 0
Conc: N.D.

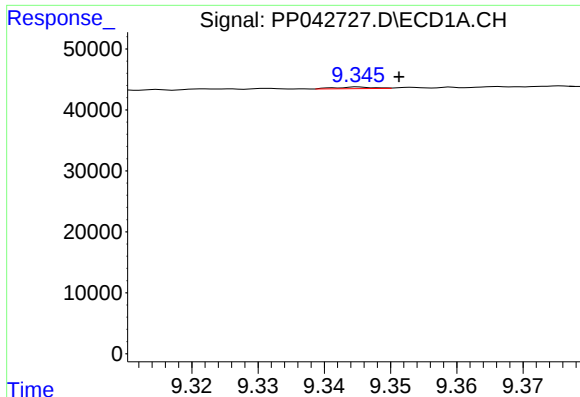

#38 AR-1262-3


R.T.: 9.345 min
Delta R.T.: -0.006 min
Response: 1079
Conc: 1.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
AMI-1-CONCRETE

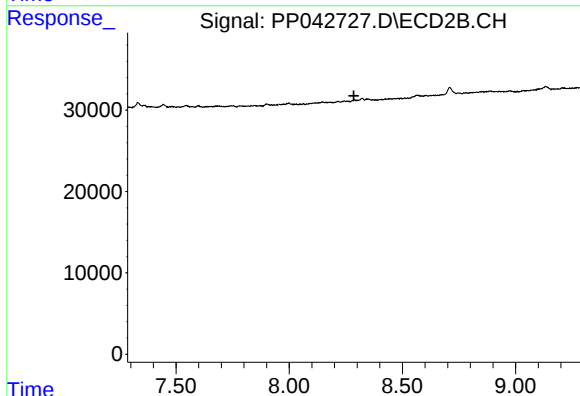


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.286 min
Response: 0
Conc: N.D.

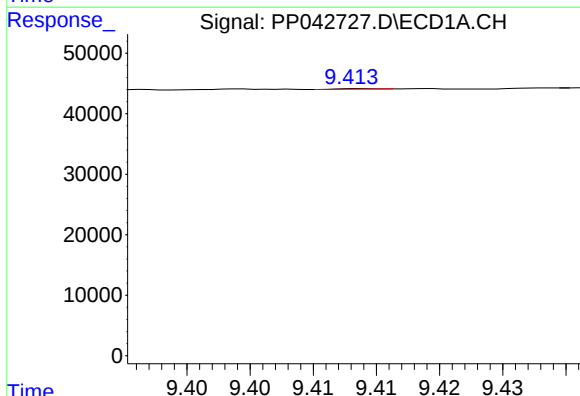


#39 AR-1262-4

R.T.: 9.414 min
Delta R.T.: -0.024 min
Response: 180
Conc: 0.37 ng/ml

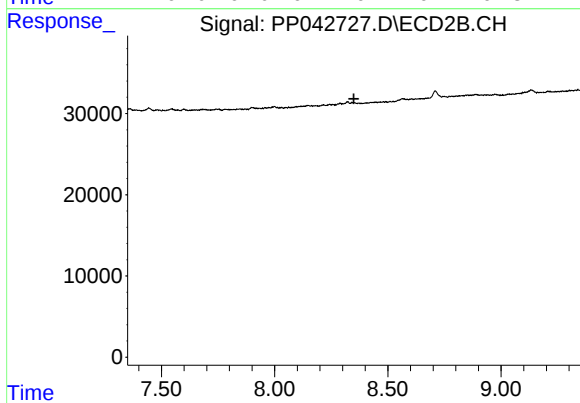

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.350 min
Response: 0
Conc: N.D.

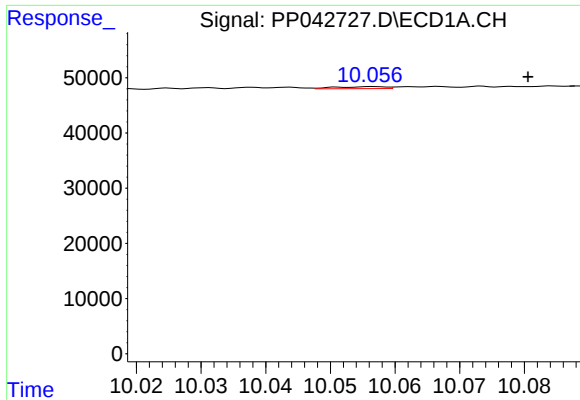

#40 AR-1262-5


R.T.: 10.057 min
Delta R.T.: -0.024 min
Response: 2017
Conc: 4.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
AMI-1-CONCRETE

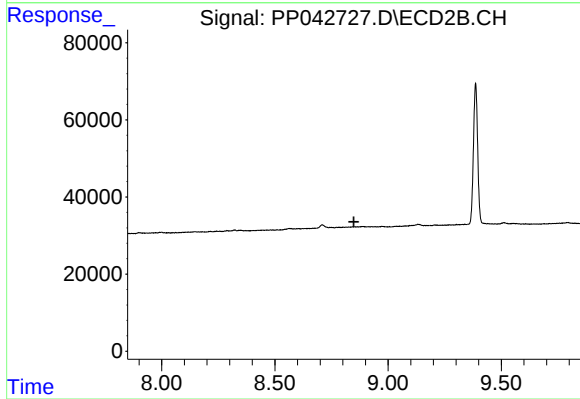


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 8.849 min
Response: 0
Conc: N.D.

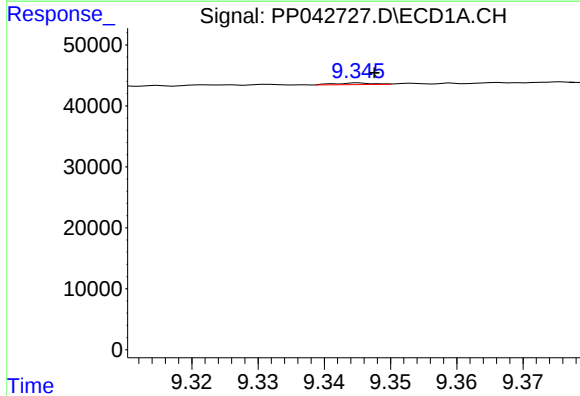


#41 AR-1268-1

R.T.: 9.345 min
Delta R.T.: -0.002 min
Response: 1079
Conc: 0.66 ng/ml

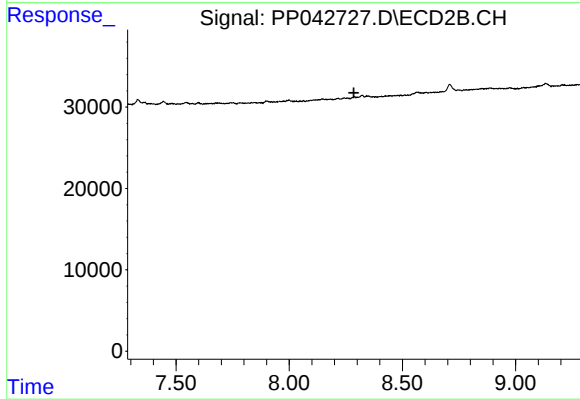

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 8.286 min
Response: 0
Conc: N.D.

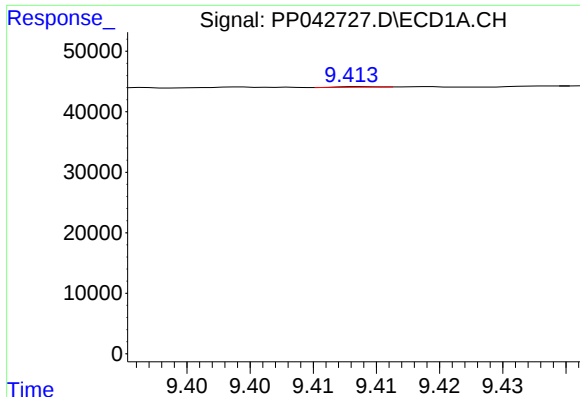

#42 AR-1268-2


R.T.: 9.414 min
Delta R.T.: -0.027 min
Response: 180
Conc: 0.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
AMI-1-CONCRETE

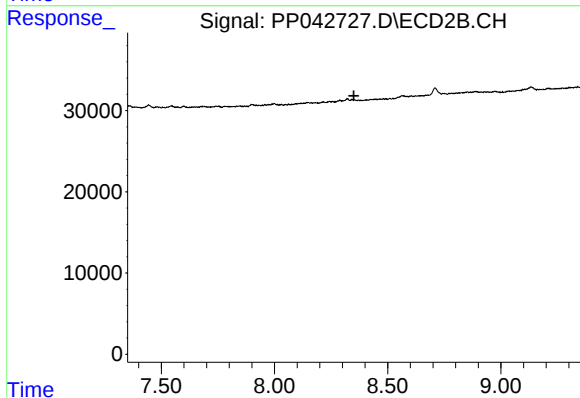


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.351 min
Response: 0
Conc: N.D.

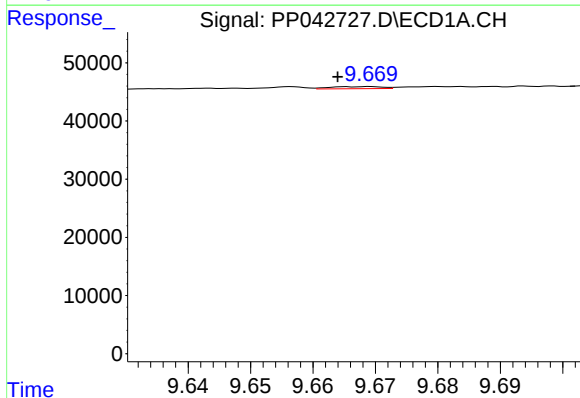


#43 AR-1268-3

R.T.: 9.669 min
Delta R.T.: 0.005 min
Response: 2021
Conc: 1.50 ng/ml

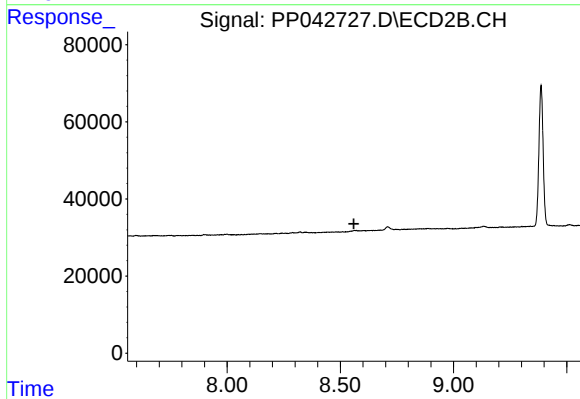

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 8.560 min
Response: 0
Conc: N.D.

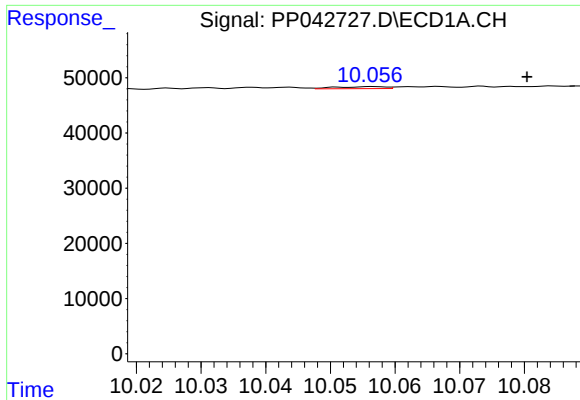

#44 AR-1268-4


R.T.: 10.057 min
Delta R.T.: -0.024 min
Response: 2017
Conc: 3.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
AMI-1-CONCRETE

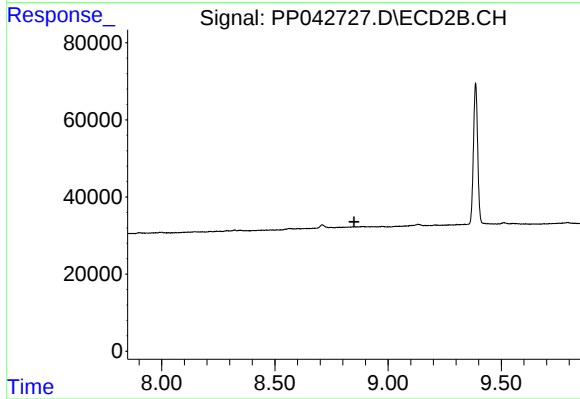


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.849 min
Response: 0
Conc: N.D.

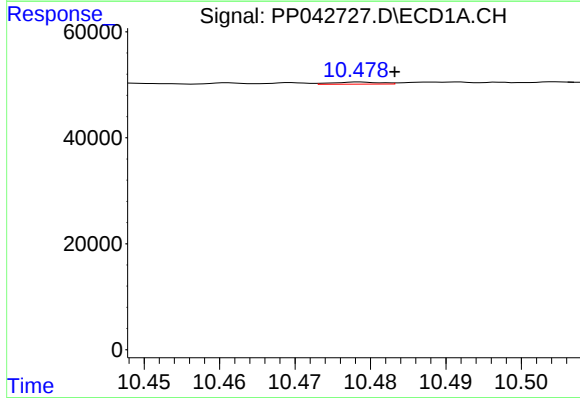

#45 AR-1268-5

R.T.: 10.479 min
Delta R.T.: -0.005 min
Response: 1751
Conc: 0.39 ng/ml

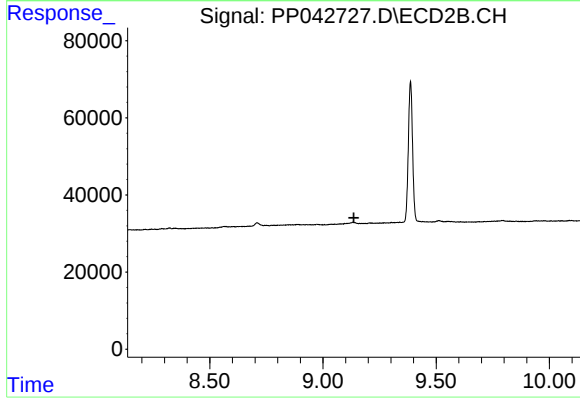

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.137 min
Response: 0
Conc: N.D.