

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010722\
 Data File : PP042706.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jan 2022 16:04
 Operator : AJ\MA
 Sample : N1050-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 VNJ-236

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/10/2022
 Supervised By :mohammad ahmed 01/10/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 01:59:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 05 12:01:35 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.882	4.051	263001	358646	13.575	13.701
2) SA Decachlor...	10.816	9.387	243717	333286	20.774	16.959
Target Compounds						
31) L7 AR-1260-1	7.867	6.911	29876	73335	49.156m	56.361
32) L7 AR-1260-2	8.128	7.108	93692	81330	133.201	53.497m#
33) L7 AR-1260-3	8.497	7.265	18187	60982	32.826m	42.654m#
34) L7 AR-1260-4	8.725	7.751	29408	31055	44.576	28.212 #
35) L7 AR-1260-5	9.043	7.996	58262	91980	48.298	38.107m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010722\
Data File : PP042706.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jan 2022 16:04
Operator : AJ\MA
Sample : N1050-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
VNJ-236


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/10/2022
Supervised By :mohammad ahmed 01/10/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 01:59:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 05 12:01:35 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

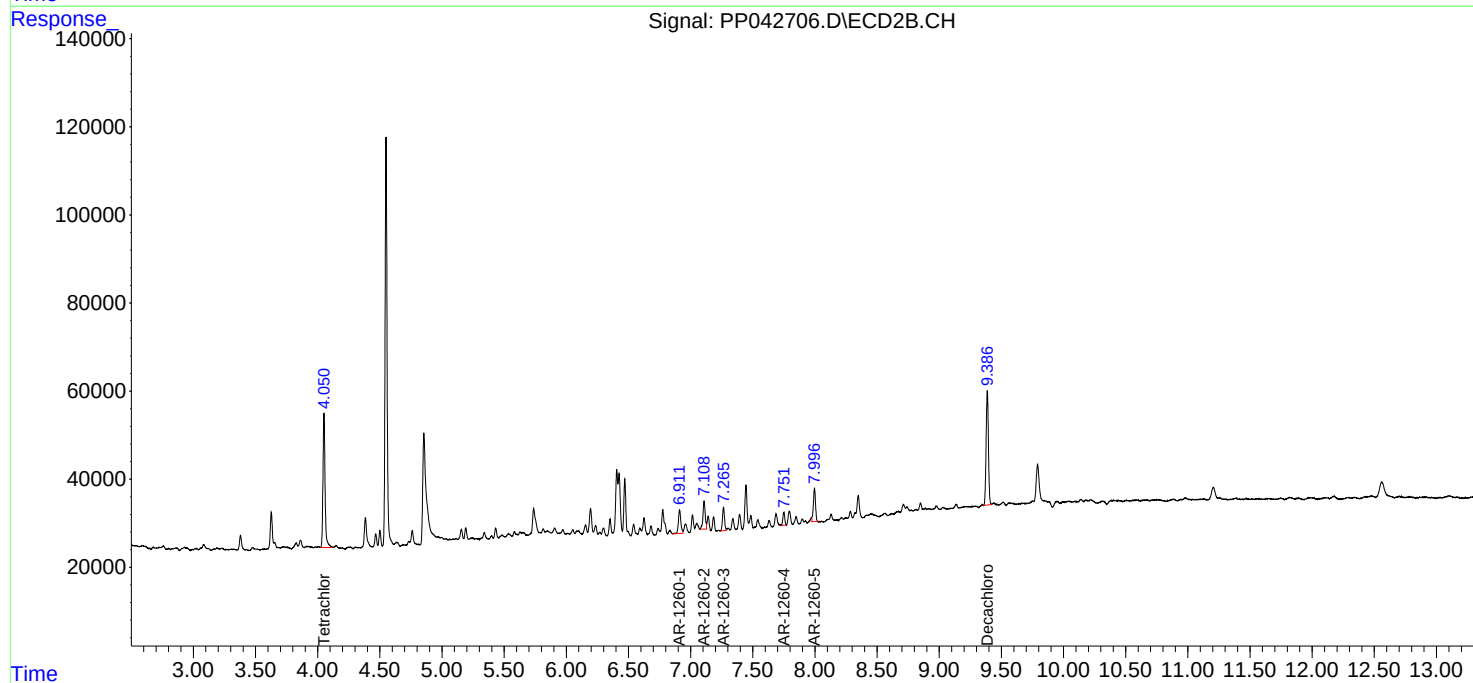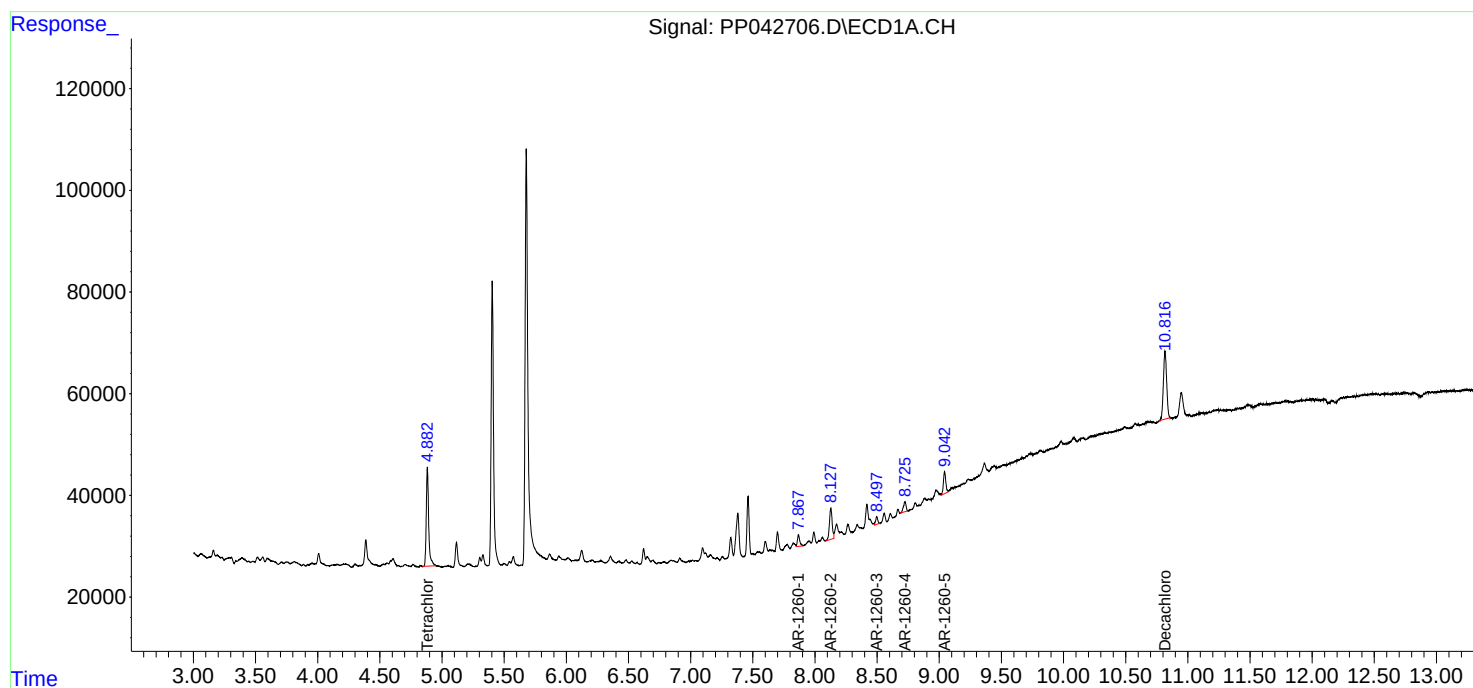

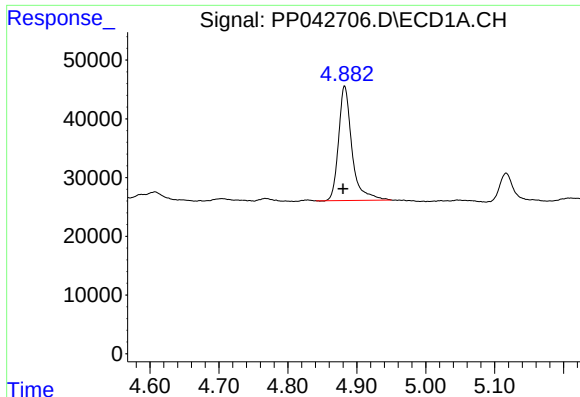


#1 Tetrachloro-m-xylene

R.T.: 4.882 min
Delta R.T.: 0.002 min
Response: 263001
Conc: 13.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
VNJ-236


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/10/2022
Supervised By :mohammad ahmed 01/10/2022

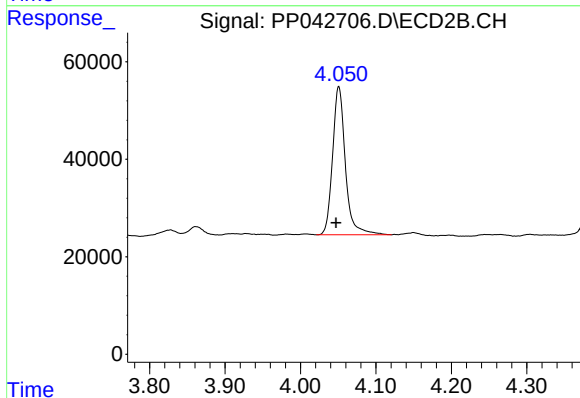


#1 Tetrachloro-m-xylene

R.T.: 4.051 min
Delta R.T.: 0.004 min
Response: 358646
Conc: 13.70 ng/ml

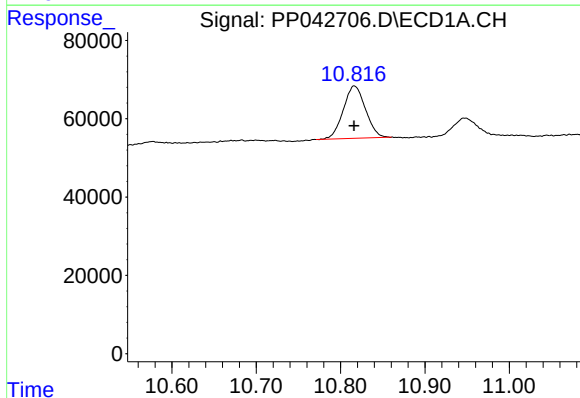


#2 Decachlorobiphenyl

R.T.: 10.816 min
Delta R.T.: 0.000 min
Response: 243717
Conc: 20.77 ng/ml

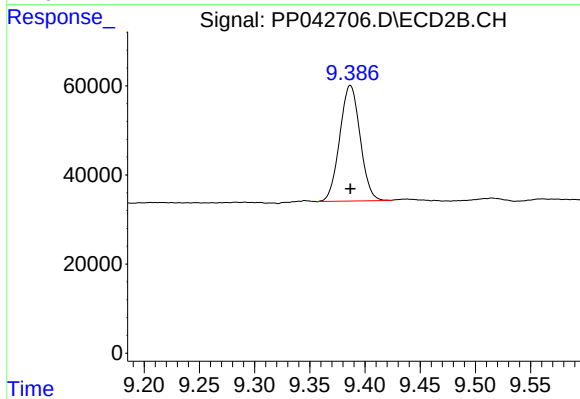

#2 Decachlorobiphenyl

R.T.: 9.387 min
Delta R.T.: 0.000 min
Response: 333286
Conc: 16.96 ng/ml

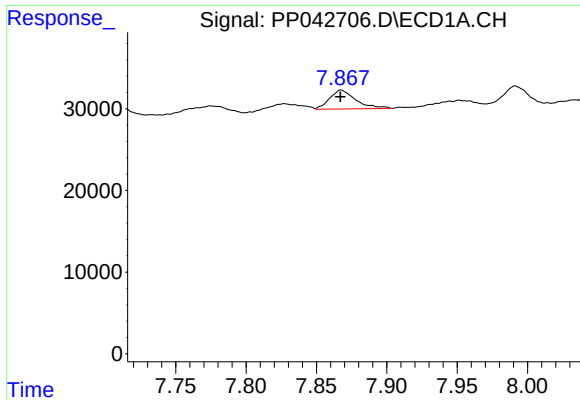


#31 AR-1260-1

R.T.: 7.867 min
Delta R.T.: 0.000 min
Response: 29876
Conc: 49.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
VNJ-236


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/10/2022
Supervised By :mohammad ahmed 01/10/2022

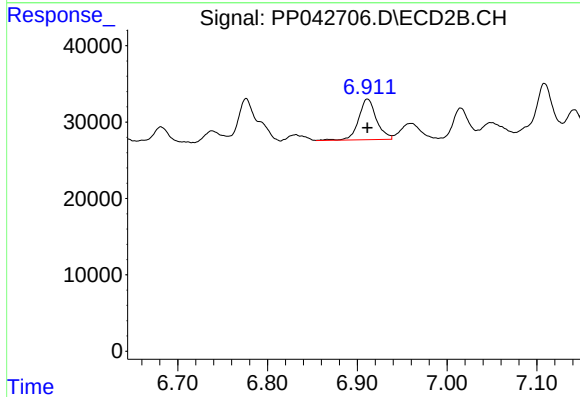


#31 AR-1260-1

R.T.: 6.911 min
Delta R.T.: 0.000 min
Response: 73335
Conc: 56.36 ng/ml

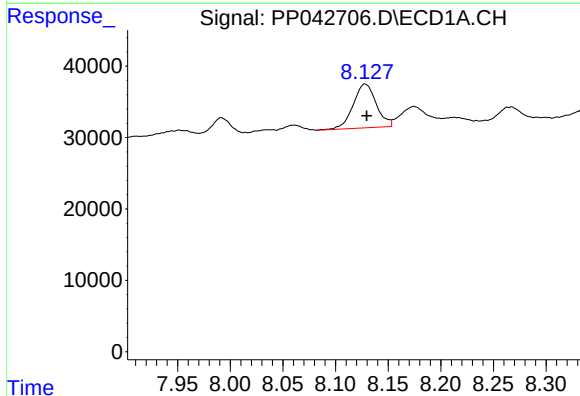


#32 AR-1260-2

R.T.: 8.128 min
Delta R.T.: -0.002 min
Response: 93692
Conc: 133.20 ng/ml

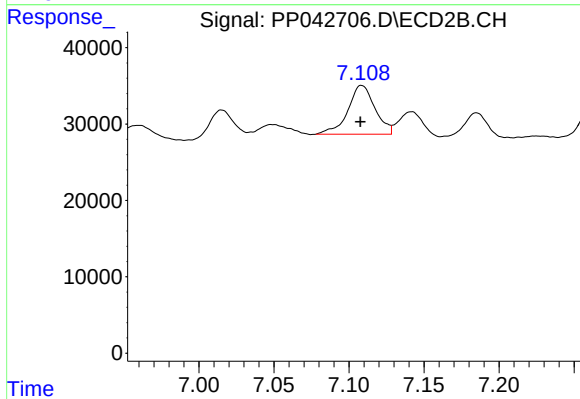

#32 AR-1260-2

R.T.: 7.108 min
Delta R.T.: 0.000 min
Response: 81330
Conc: 53.50 ng/ml m

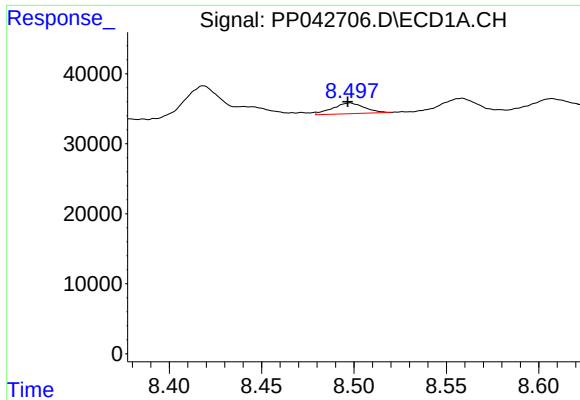


#33 AR-1260-3

R.T.: 8.497 min
Delta R.T.: 0.000 min
Response: 18187
Conc: 32.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
VNJ-236


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/10/2022
Supervised By :mohammad ahmed 01/10/2022

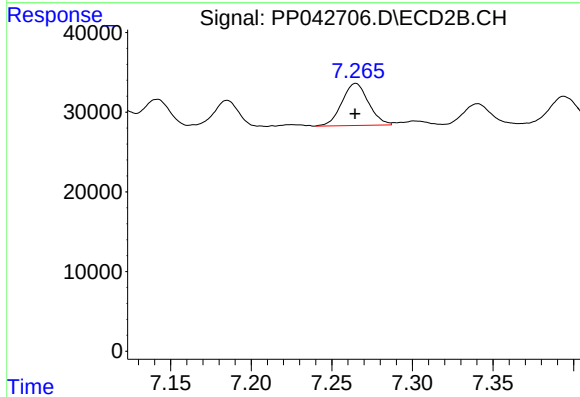


#33 AR-1260-3

R.T.: 7.265 min
Delta R.T.: 0.000 min
Response: 60982
Conc: 42.65 ng/ml m

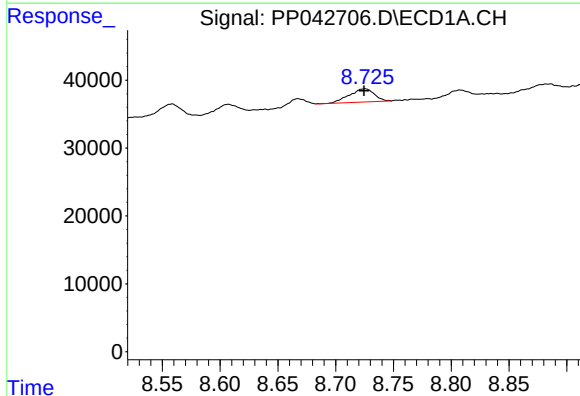


#34 AR-1260-4

R.T.: 8.725 min
Delta R.T.: 0.000 min
Response: 29408
Conc: 44.58 ng/ml

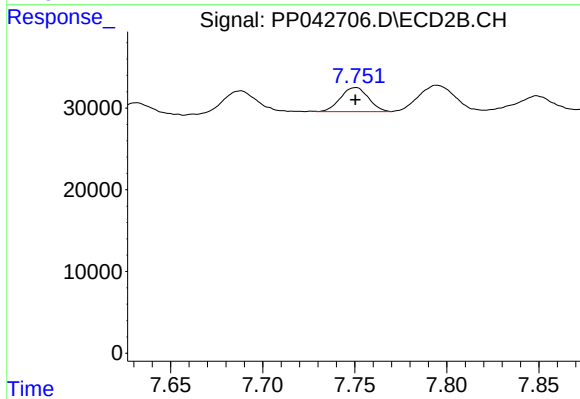

#34 AR-1260-4

R.T.: 7.751 min
Delta R.T.: 0.000 min
Response: 31055
Conc: 28.21 ng/ml

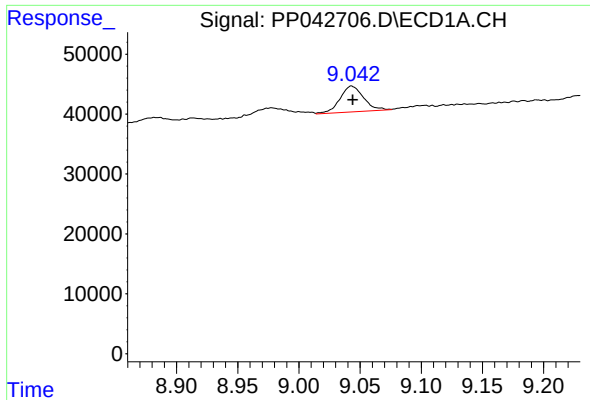


#35 AR-1260-5

R.T.: 9.043 min
Delta R.T.: 0.000 min
Response: 58262
Conc: 48.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
VNJ-236

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/10/2022
Supervised By :mohammad ahmed 01/10/2022

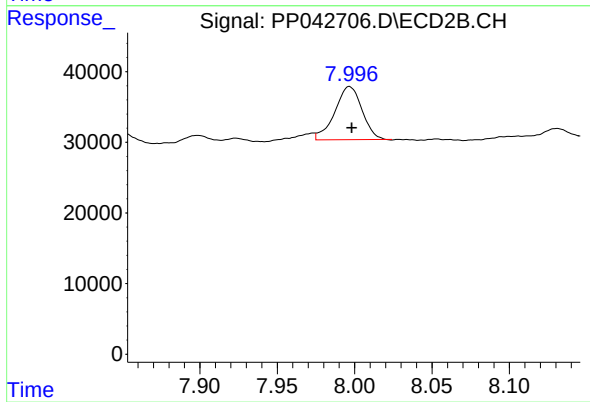

#35 AR-1260-5

R.T.: 7.996 min
Delta R.T.: -0.002 min
Response: 91980
Conc: 38.11 ng/ml m