

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010722\
 Data File : PP042764.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Jan 2022 9:25
 Operator : AJ\MA
 Sample : N1056-07
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMP-3

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/10/2022
 Supervised By :mohammad ahmed 01/10/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 19:39:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 05 12:01:35 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.884	4.052	102598	389223	5.296m	14.869m#
2) SA Decachlor...	10.810	9.383	152049	130666	12.961	6.649 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010722\
Data File : PP042764.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Jan 2022 9:25
Operator : AJ\MA
Sample : N1056-07
Misc :
ALS Vial : 56 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/10/2022
Supervised By :mohammad ahmed 01/10/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 19:39:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010422.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 05 12:01:35 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

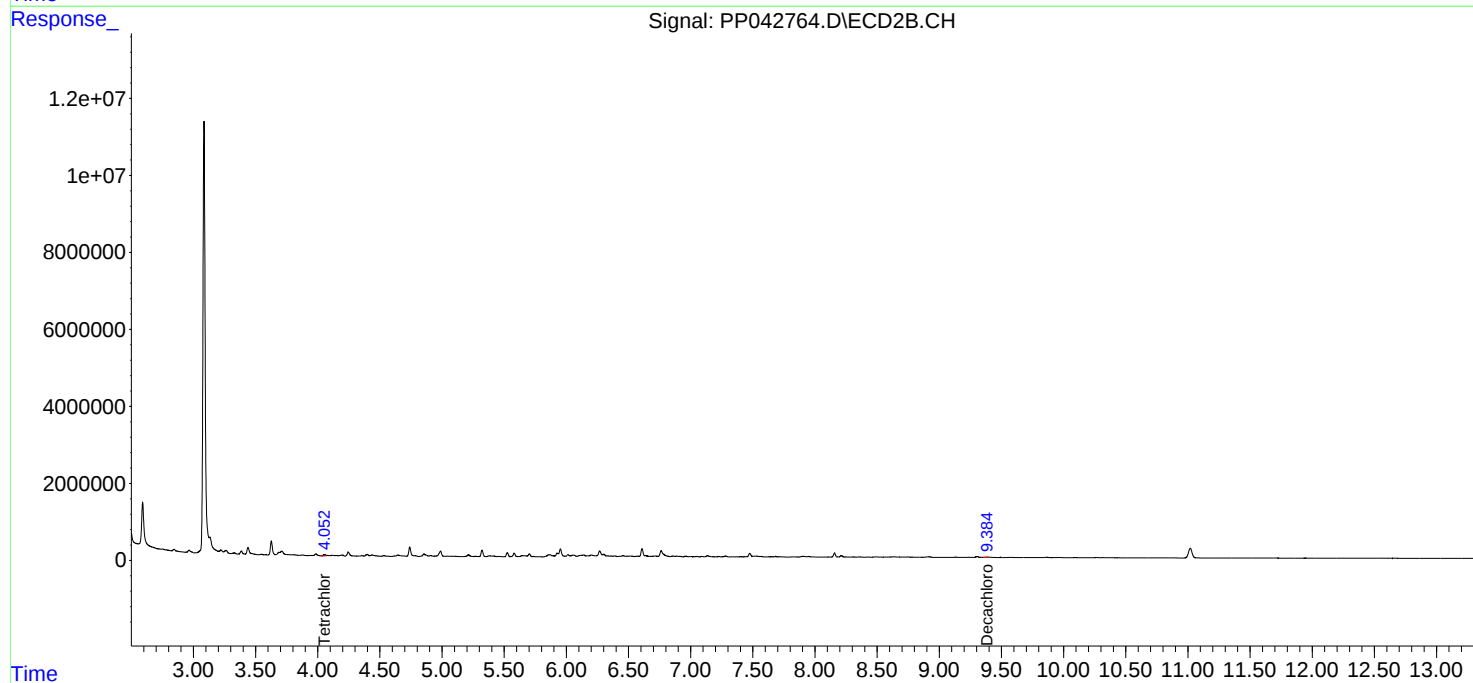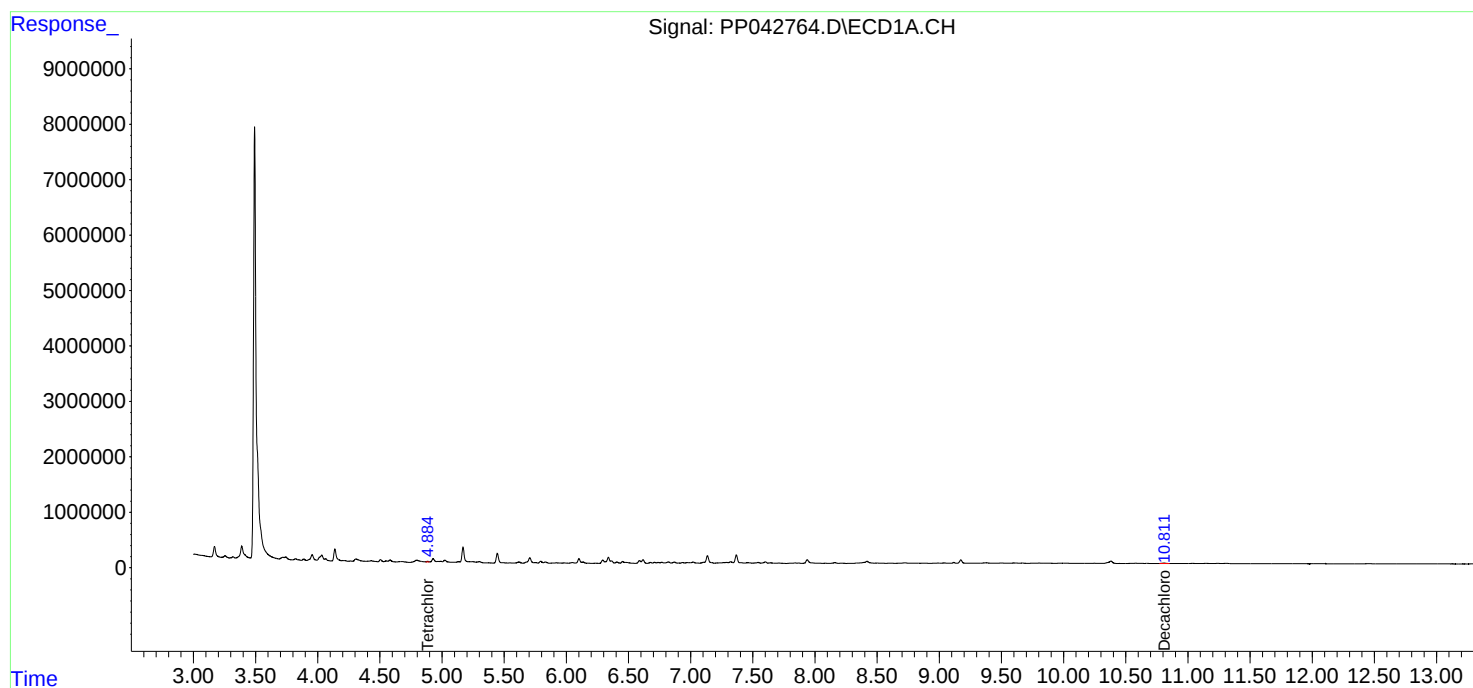

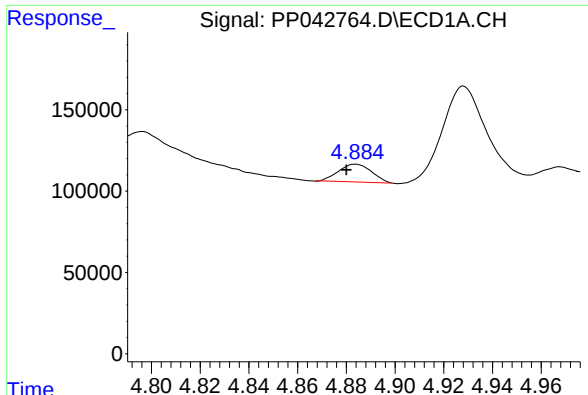


#1 Tetrachloro-m-xylene

R.T.: 4.884 min
 Delta R.T.: 0.004 min
 Response: 102598
 Conc: 5.30 ng/ml

Instrument : ECD_P
 ClientSampleId : COMP-3


Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/10/2022
 Supervised By :mohammad ahmed 01/10/2022

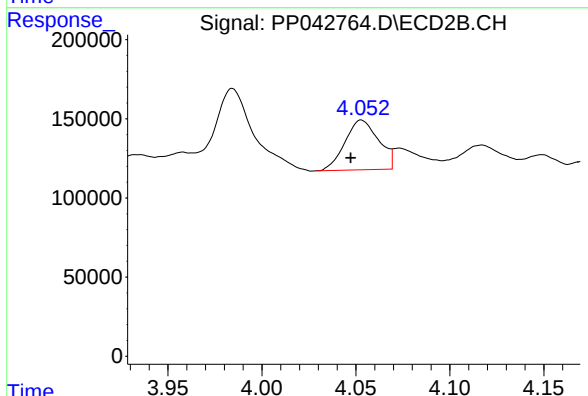


#1 Tetrachloro-m-xylene

R.T.: 4.052 min
 Delta R.T.: 0.005 min
 Response: 389223
 Conc: 14.87 ng/ml m

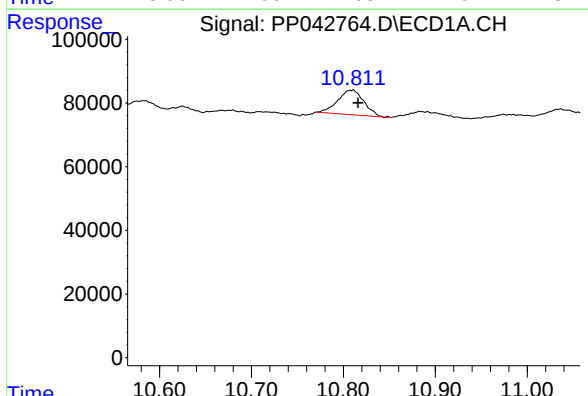

#2 Decachlorobiphenyl

R.T.: 10.810 min
 Delta R.T.: -0.006 min
 Response: 152049
 Conc: 12.96 ng/ml

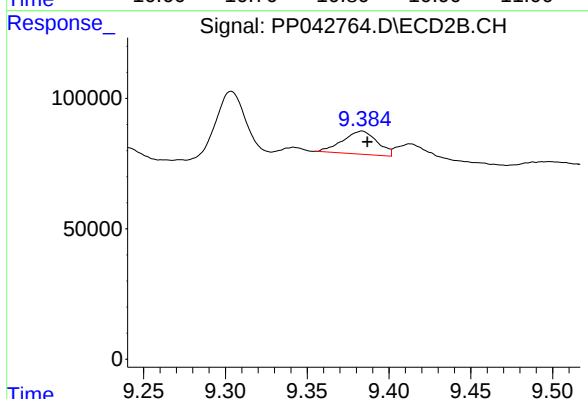

#2 Decachlorobiphenyl

R.T.: 9.383 min
 Delta R.T.: -0.003 min
 Response: 130666
 Conc: 6.65 ng/ml