

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010725\
 Data File : PP068957.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2025 12:21
 Operator : YP\AJ
 Sample : Q1019-02 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 H1H072I-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/08/2025
 Supervised By :Ankita Jodhani 01/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 12:42:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010625.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 07 11:05:55 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.671	3.982	1964308	1557899	1.412	1.596
2) SA Decachlor...	10.521	9.110	2067795	2188930	1.852m	1.822

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010725\
Data File : PP068957.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2025 12:21
Operator : YP\AJ
Sample : Q1019-02 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HH072I-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/08/2025
Supervised By :Ankita Jodhani 01/08/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 12:42:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010625.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 07 11:05:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

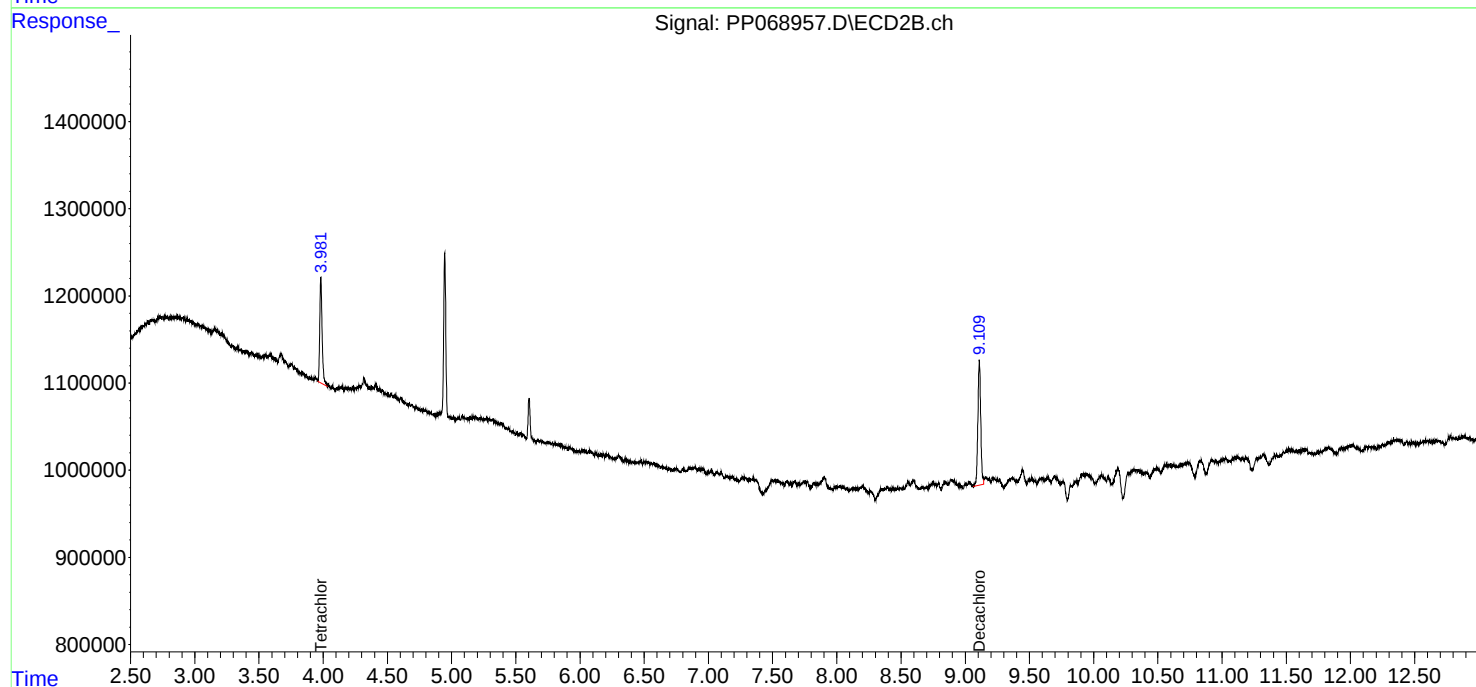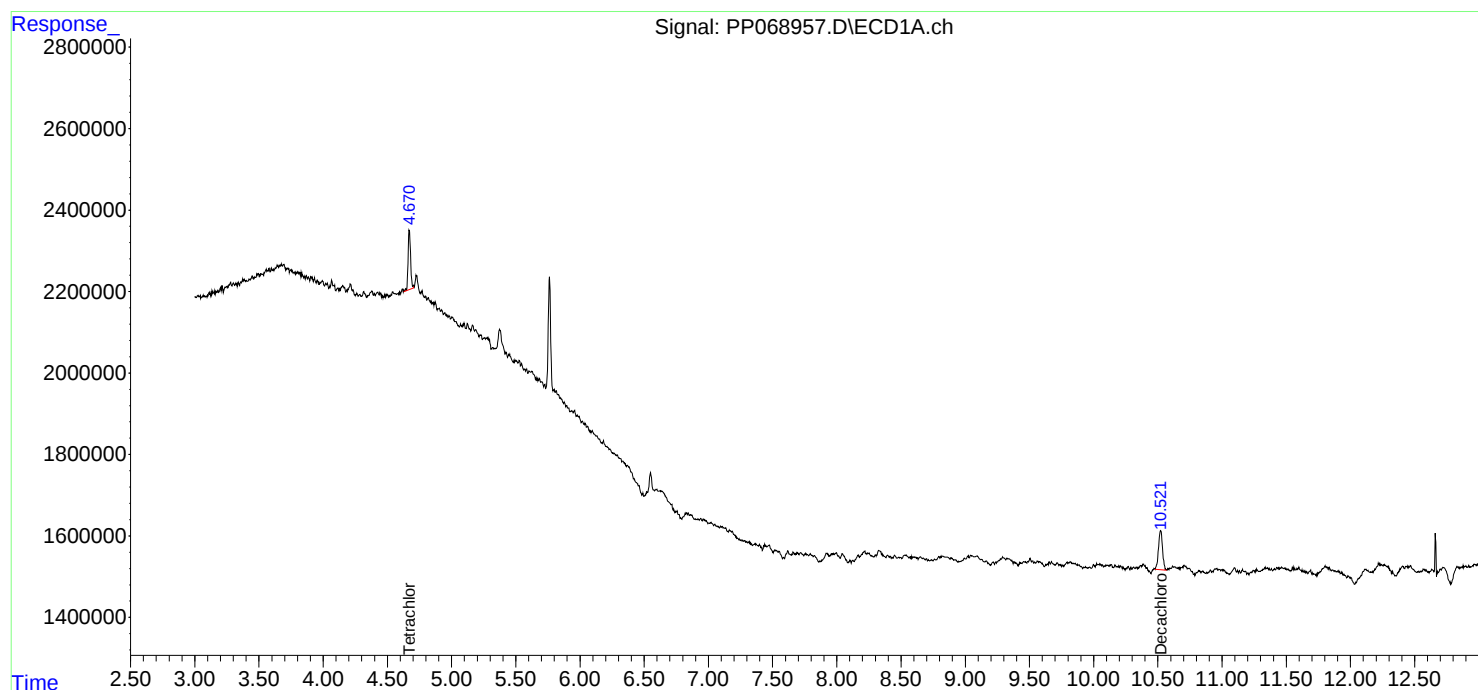

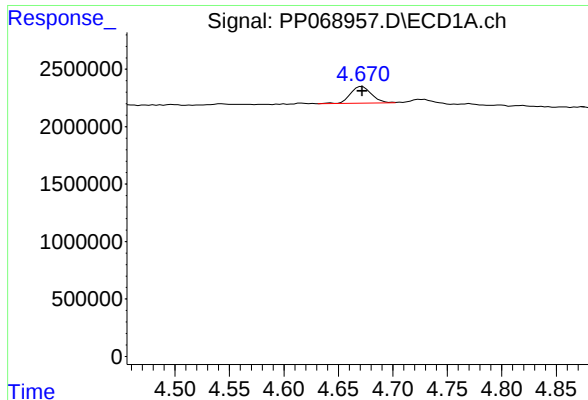


#1 Tetrachloro-m-xylene

R.T.: 4.671 min
Delta R.T.: 0.000 min
Response: 1964308
Conc: 1.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
HH072I-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/08/2025
Supervised By :Ankita Jodhani 01/08/2025

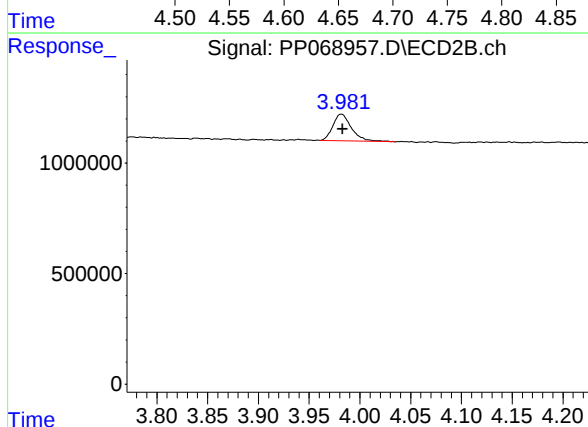


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: -0.001 min
Response: 1557899
Conc: 1.60 ng/ml

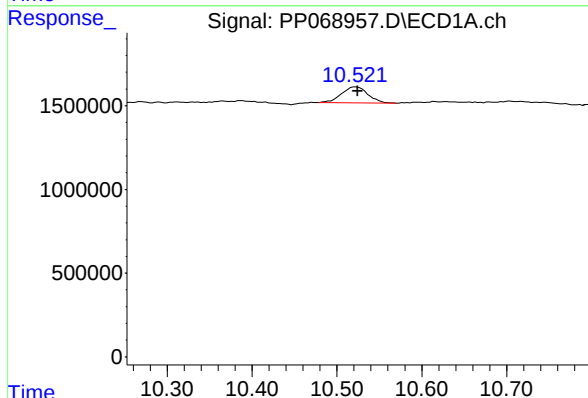

#2 Decachlorobiphenyl

R.T.: 10.521 min
Delta R.T.: -0.003 min
Response: 2067795
Conc: 1.85 ng/ml m

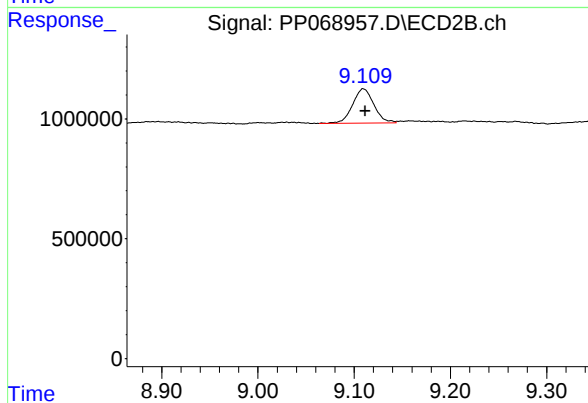

#2 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: -0.002 min
Response: 2188930
Conc: 1.82 ng/ml