

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010725\
 Data File : PP068960.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2025 13:10
 Operator : YP\AJ
 Sample : Q1019-05 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 6-55-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/08/2025
 Supervised By :Ankita Jodhani 01/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 13:42:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010625.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 07 11:05:55 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.670	3.982	2228970	1936326	1.602	1.984
2) SA Decachlor...	10.520	9.109	2074329	2058787	1.858m	1.714

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010725\
Data File : PP068960.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2025 13:10
Operator : YP\AJ
Sample : Q1019-05 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
6-55-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/08/2025
Supervised By :Ankita Jodhani 01/08/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 13:42:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010625.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 07 11:05:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

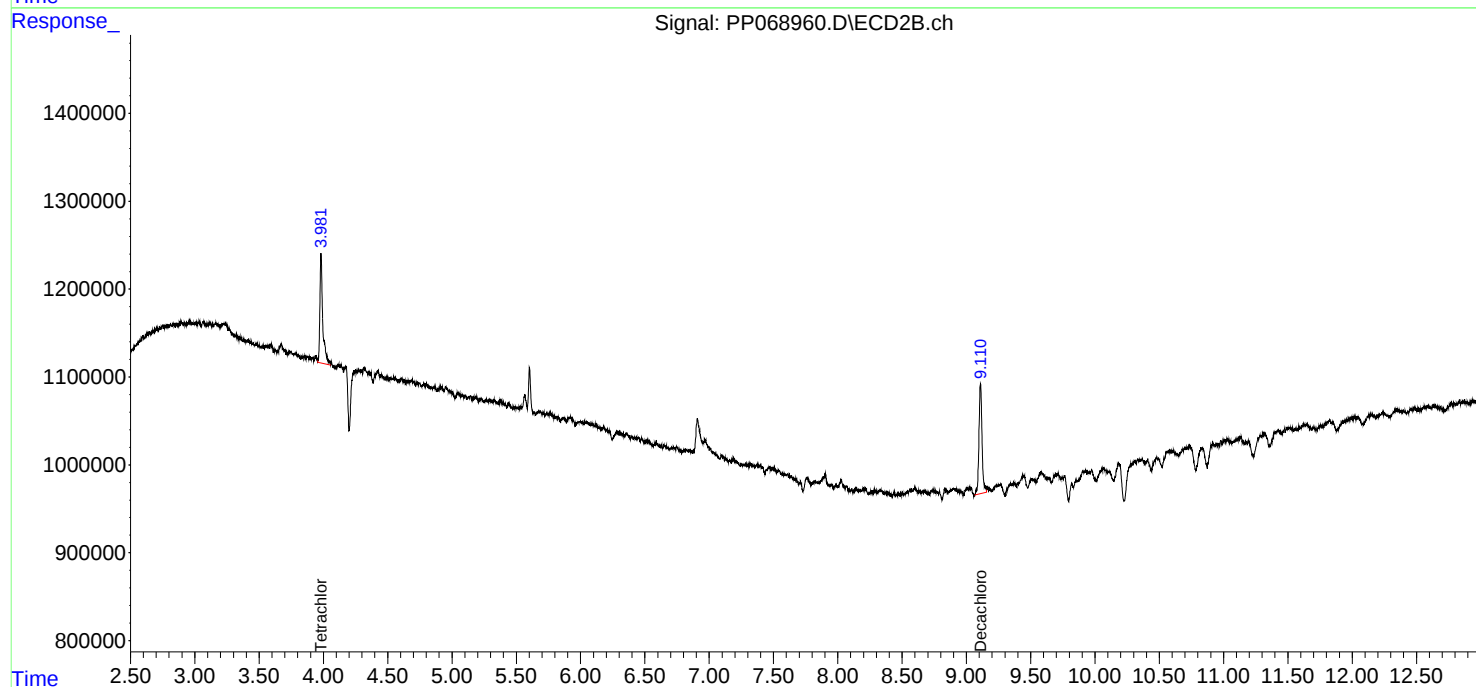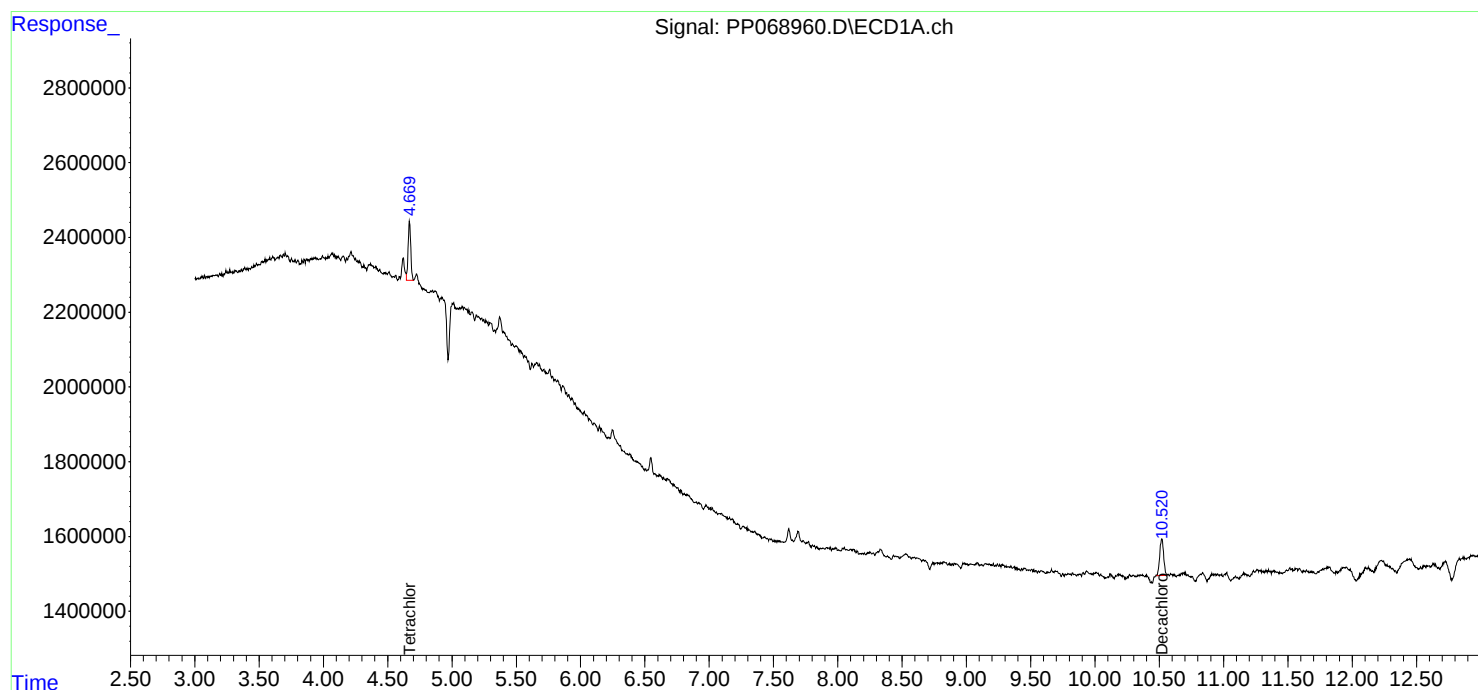

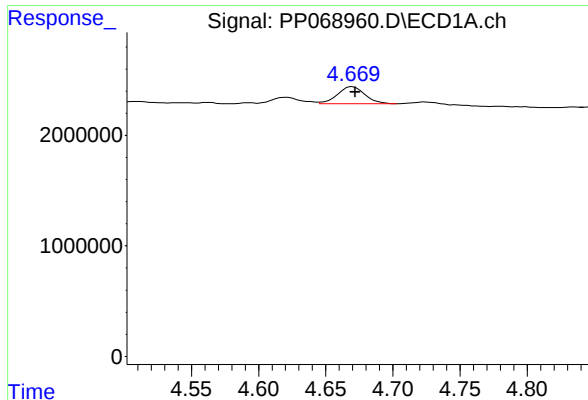


#1 Tetrachloro-m-xylene

R.T.: 4.670 min
Delta R.T.: -0.002 min
Response: 2228970
Conc: 1.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
6-55-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/08/2025
Supervised By :Ankita Jodhani 01/08/2025

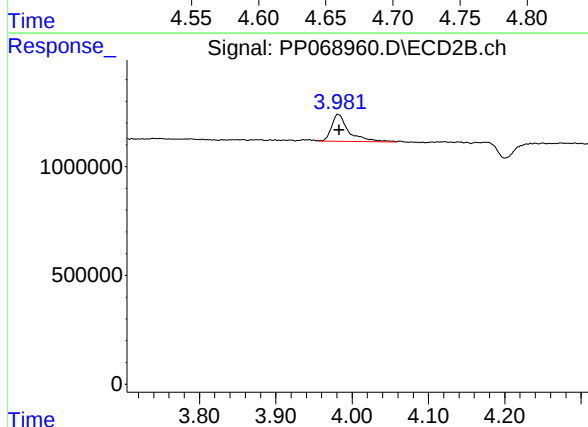


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: -0.001 min
Response: 1936326
Conc: 1.98 ng/ml

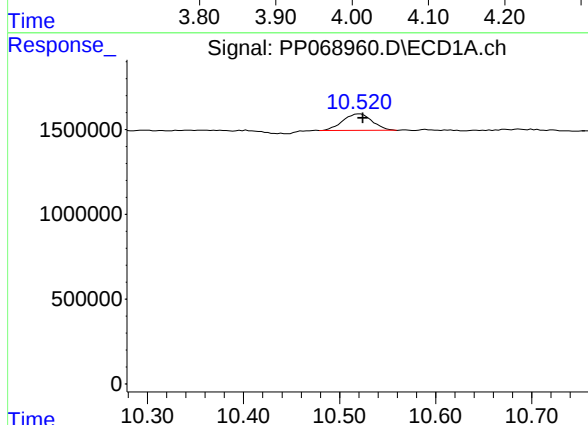

#2 Decachlorobiphenyl

R.T.: 10.520 min
Delta R.T.: -0.004 min
Response: 2074329
Conc: 1.86 ng/ml m

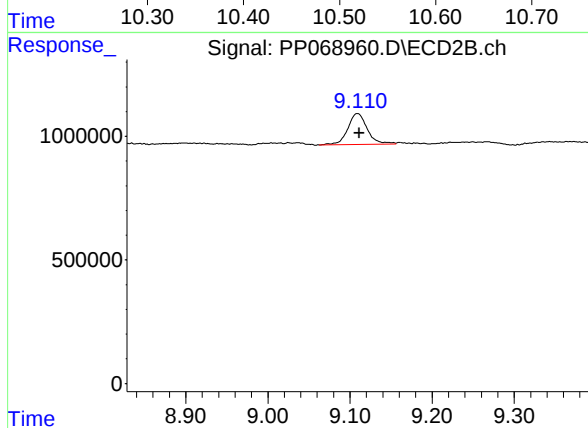

#2 Decachlorobiphenyl

R.T.: 9.109 min
Delta R.T.: -0.002 min
Response: 2058787
Conc: 1.71 ng/ml