

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010725\
 Data File : PP068984.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2025 21:17
 Operator : YP\AJ
 Sample : Q1017-03 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 Y2309-0071-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/08/2025
 Supervised By :Ankita Jodhani 01/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 00:31:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010625.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 07 11:05:55 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.666	3.978	1633926	919852	1.174m	0.942m
2) SA Decachlor...	10.514	9.104	2453550	1810033	2.198	1.507 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010725\
Data File : PP068984.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2025 21:17
Operator : YP\AJ
Sample : Q1017-03 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
Y2309-0071-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/08/2025
Supervised By :Ankita Jodhani 01/08/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 00:31:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010625.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 07 11:05:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

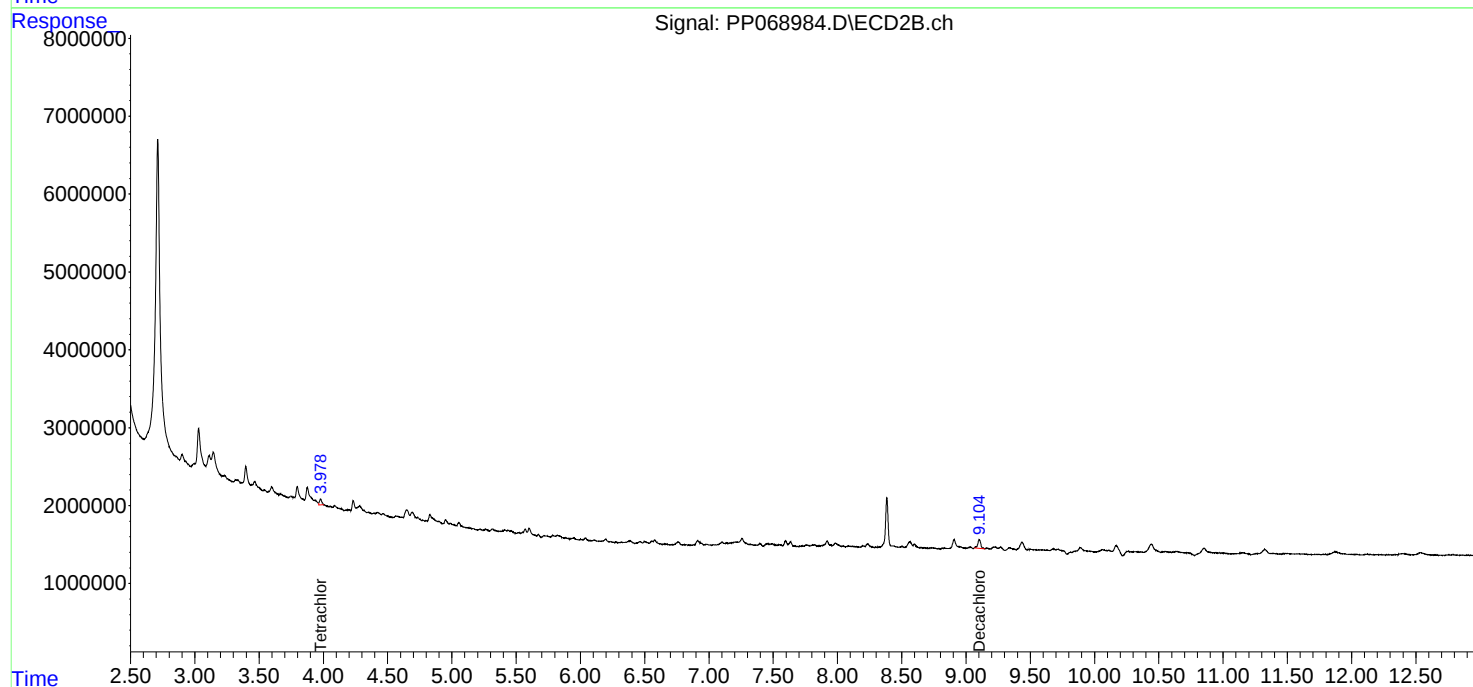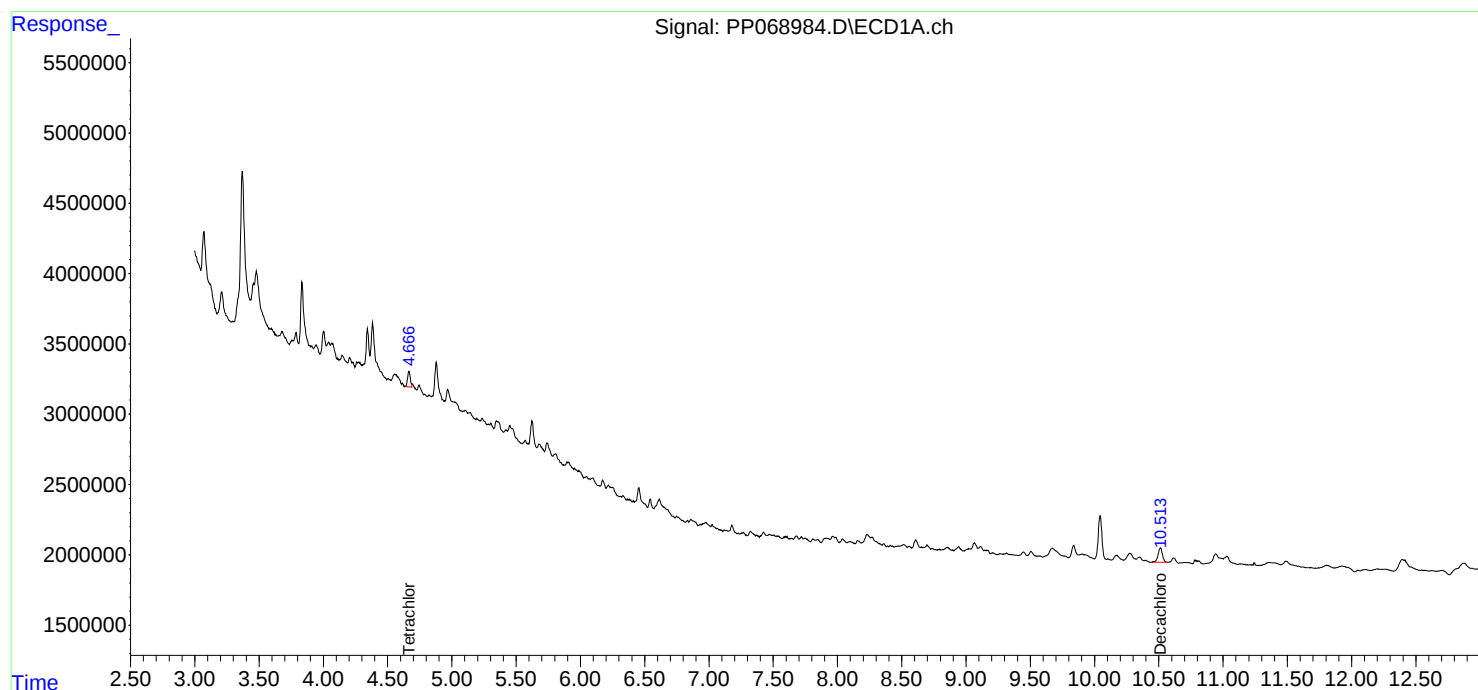

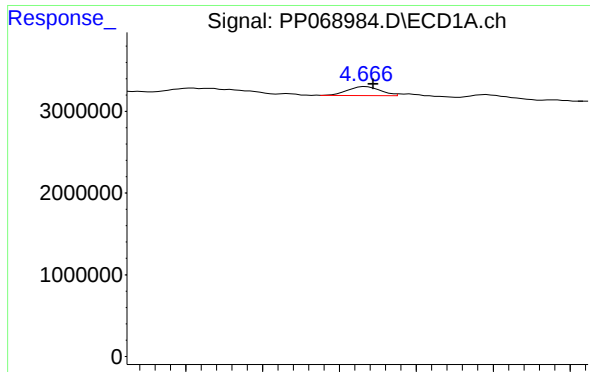


#1 Tetrachloro-m-xylene

R.T.: 4.666 min
Delta R.T.: -0.006 min
Response: 1633926
Conc: 1.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
Y2309-0071-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/08/2025
Supervised By :Ankita Jodhani 01/08/2025

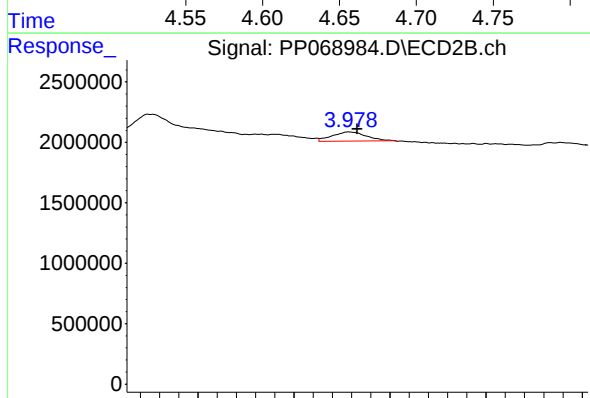


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: -0.005 min
Response: 919852
Conc: 0.94 ng/ml

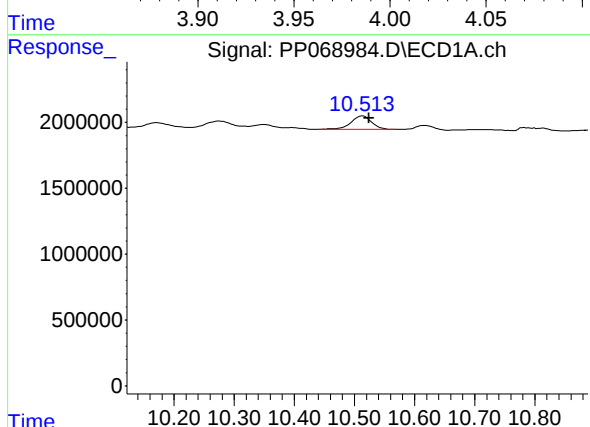

#2 Decachlorobiphenyl

R.T.: 10.514 min
Delta R.T.: -0.010 min
Response: 2453550
Conc: 2.20 ng/ml

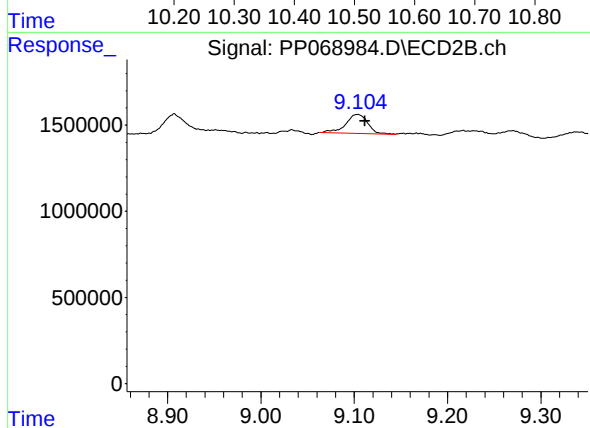

#2 Decachlorobiphenyl

R.T.: 9.104 min
Delta R.T.: -0.008 min
Response: 1810033
Conc: 1.51 ng/ml