

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010819\
 Data File : PP028708.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Jan 2019 21:33
 Operator : EI\MA
 Sample : K1075-13
 Misc : hexane
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 02:51:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010319.M
 Quant Title : 8080.M
 QLast Update : Fri Jan 04 01:40:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	12.135	12.246	46416915	67843352	180.537	155.397
Target Compounds							
1) T	Dalapon	3.322	2.990	82921332	43712083	135.599	74.774 #
6) T	MCP	12.825	12.719	22320360	24101641	45.567	26.058 #
8) T	DICHLORPROP	0.000	13.684	0	16516284	N.D.	38.033 #
12) T	2,4,5-T	0.000	16.010	0	32072598	N.D.	14.785 #
13) T	2,4-DB	16.449	0.000	26498609	0	214.101	N.D. #
14) T	DINOSEB	17.952	17.039	33358379	4882286	15.243	2.782 #
15) T	Picloram	17.805	0.000	1289812	0	16.451	N.D. #
16) T	DCPA	18.269	0.000	45638294	0	11.054	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010819\
Data File : PP028708.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Jan 2019 21:33
Operator : EI\MA
Sample : K1075-13
Misc : hexane
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 02:51:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010319.M
Quant Title : 8080.M
QLast Update : Fri Jan 04 01:40:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

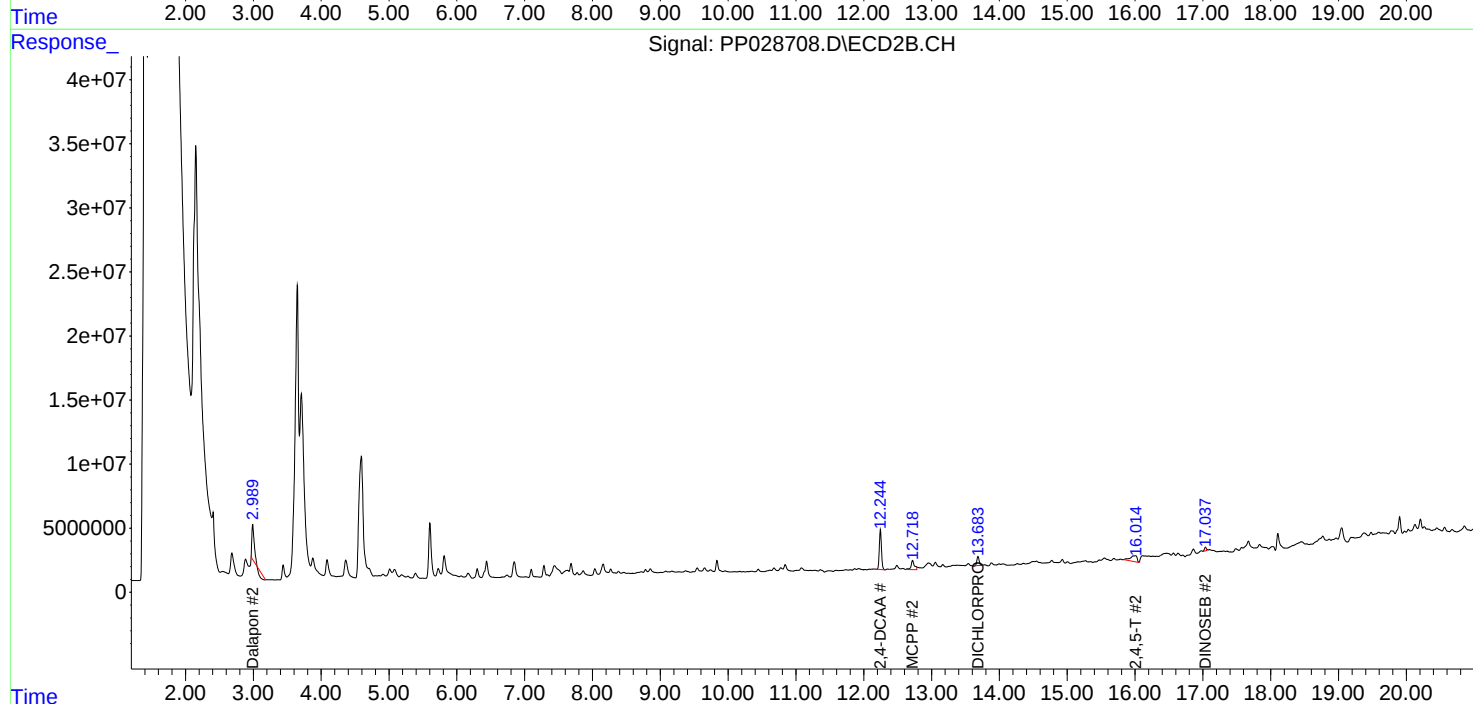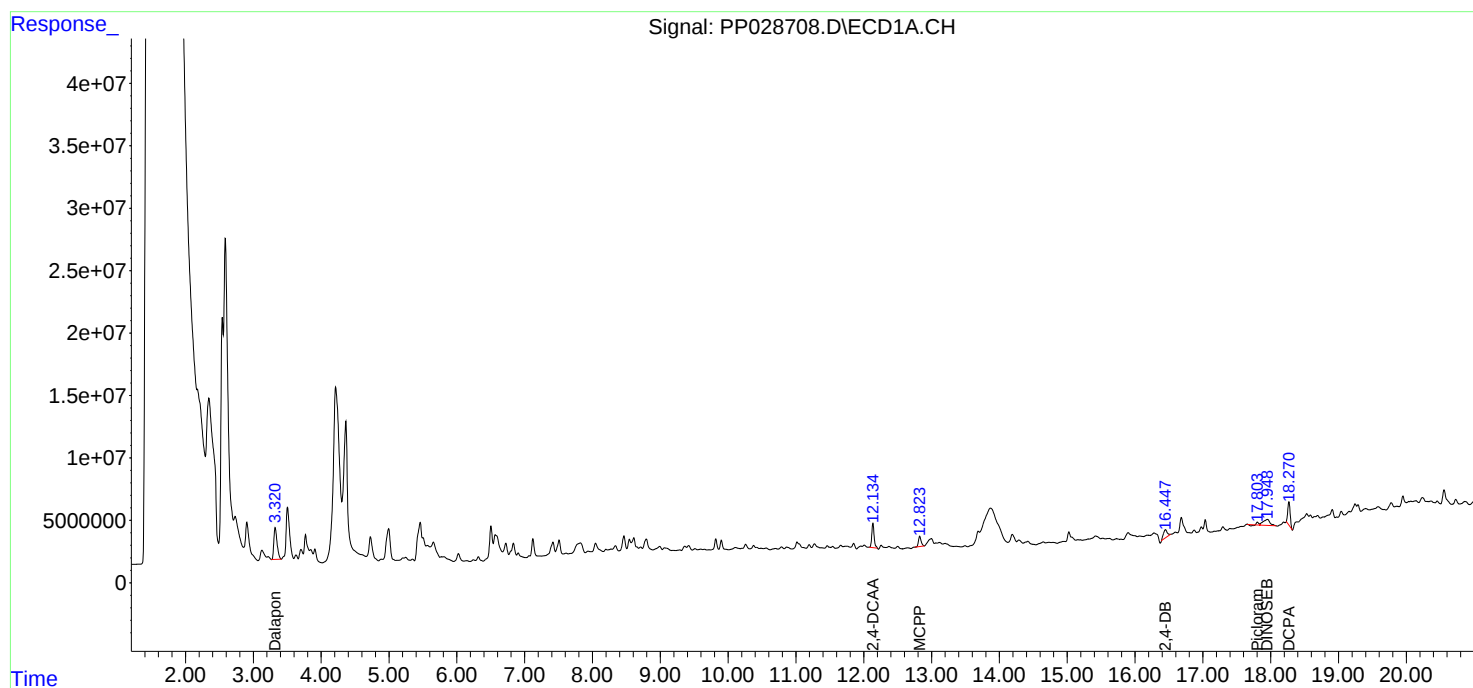


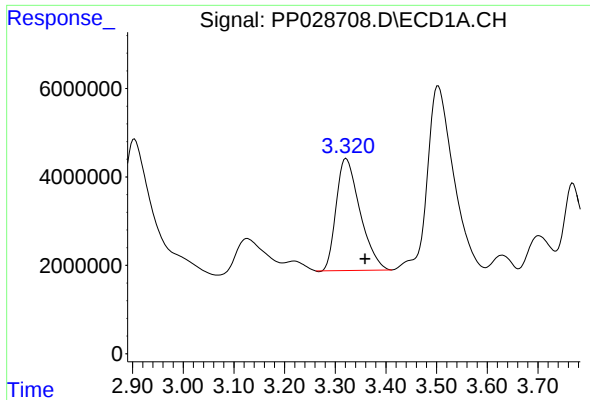

#1 Dalapon


R.T.: 3.322 min
Delta R.T.: -0.037 min
Response: 82921332
Conc: 135.60 ng/ml

Instrument :
ECD_P
ClientSampleId :

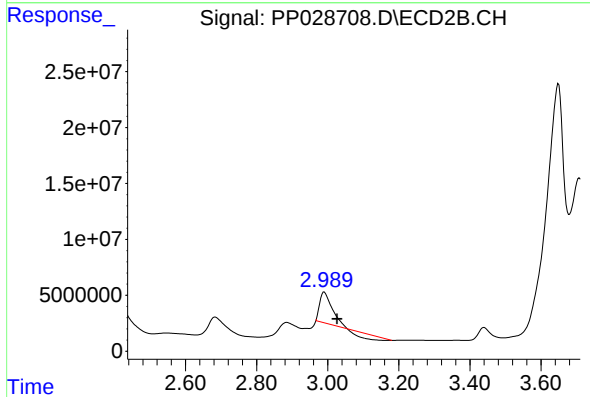


#1 Dalapon

R.T.: 2.990 min
Delta R.T.: -0.036 min
Response: 43712083
Conc: 74.77 ng/ml

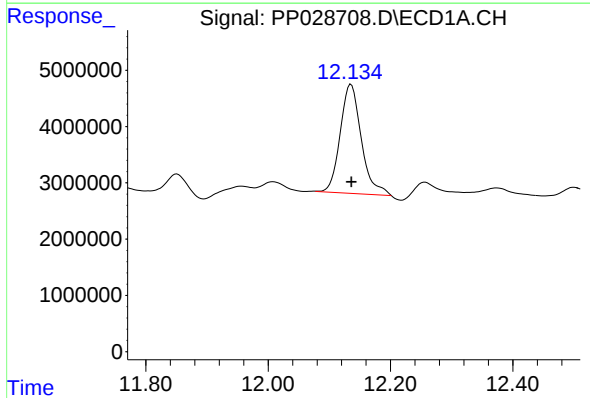


#4 2,4-DCAA

R.T.: 12.135 min
Delta R.T.: 0.000 min
Response: 46416915
Conc: 180.54 ng/ml

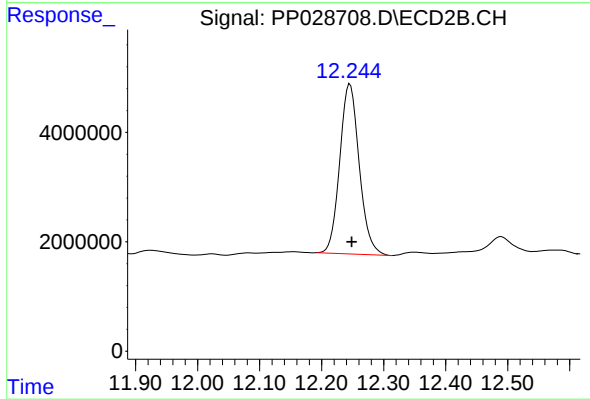

#4 2,4-DCAA


R.T.: 12.246 min
Delta R.T.: -0.003 min
Response: 67843352
Conc: 155.40 ng/ml

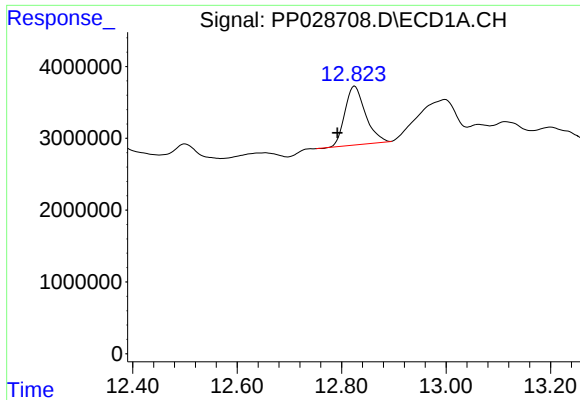

#6 MCP


R.T.: 12.825 min
Delta R.T.: 0.033 min
Response: 22320360
Conc: 45.57 ug/ml

Instrument :
ECD_P
ClientSampleId :

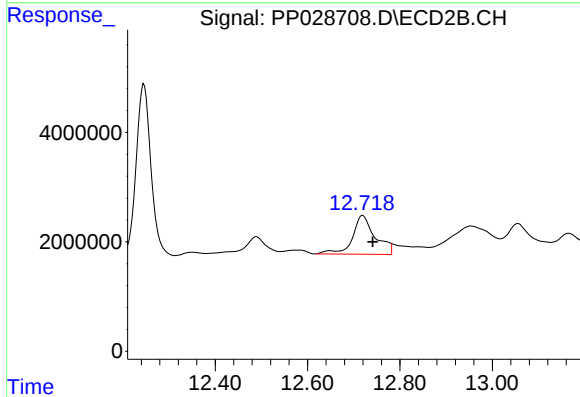


#6 MCP

R.T.: 12.719 min
Delta R.T.: -0.021 min
Response: 24101641
Conc: 26.06 ug/ml

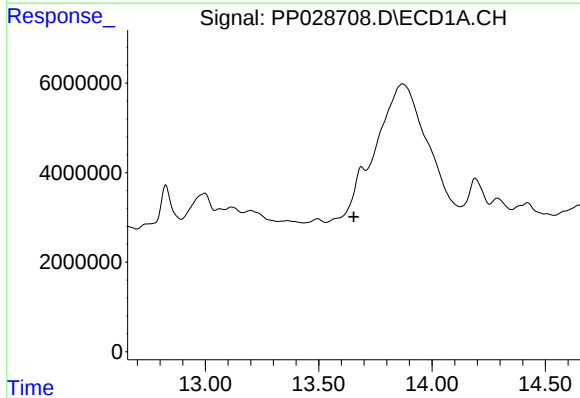


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.655 min
Response: 0
Conc: N.D.

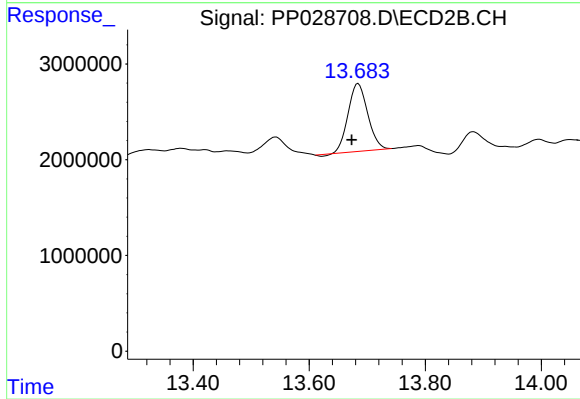

#8 DICHLORPROP


R.T.: 13.684 min
Delta R.T.: 0.011 min
Response: 16516284
Conc: 38.03 ng/ml

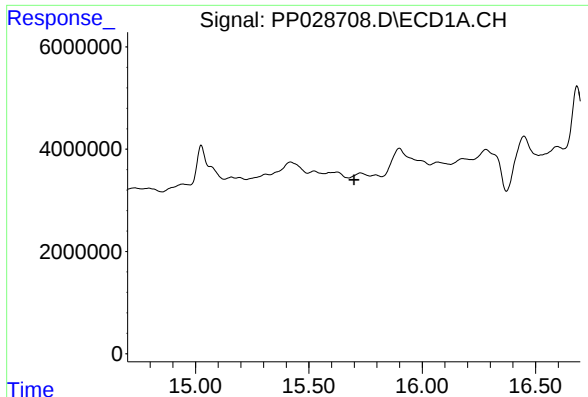

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.699 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

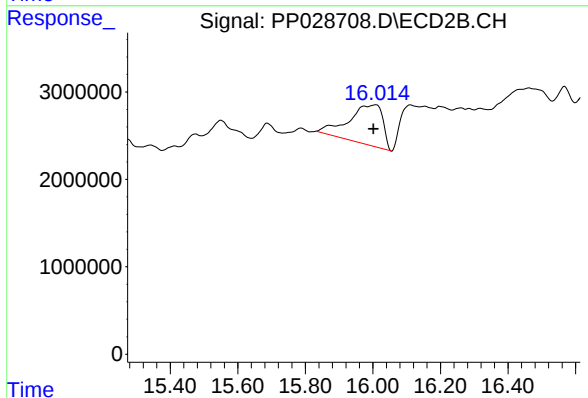


#12 2,4,5-T

R.T.: 16.010 min
Delta R.T.: 0.008 min
Response: 32072598
Conc: 14.79 ng/ml

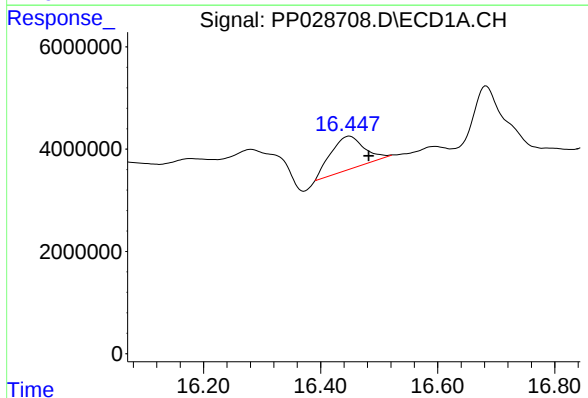


#13 2,4-DB

R.T.: 16.449 min
Delta R.T.: -0.033 min
Response: 26498609
Conc: 214.10 ng/ml

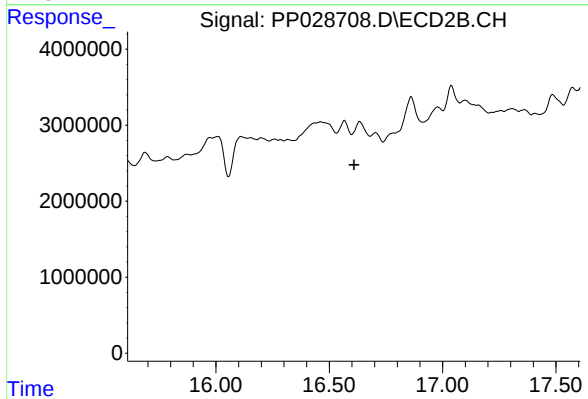

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 16.610 min
Response: 0
Conc: N.D.

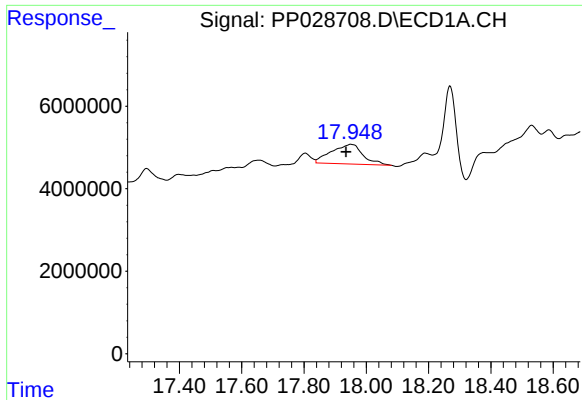

#14 DINOSEB


R.T.: 17.952 min
Delta R.T.: 0.016 min
Response: 33358379
Conc: 15.24 ng/ml

Instrument :
ECD_P
ClientSampleId :

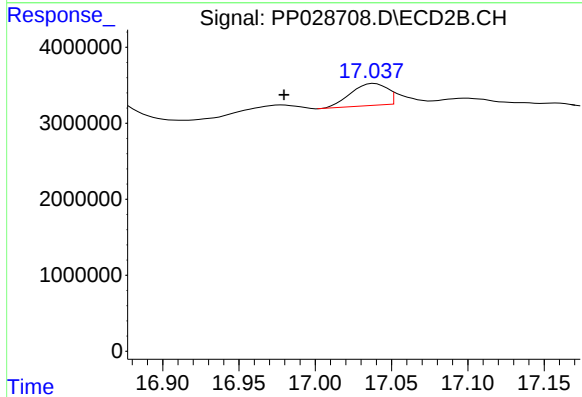


#14 DINOSEB

R.T.: 17.039 min
Delta R.T.: 0.059 min
Response: 4882286
Conc: 2.78 ng/ml

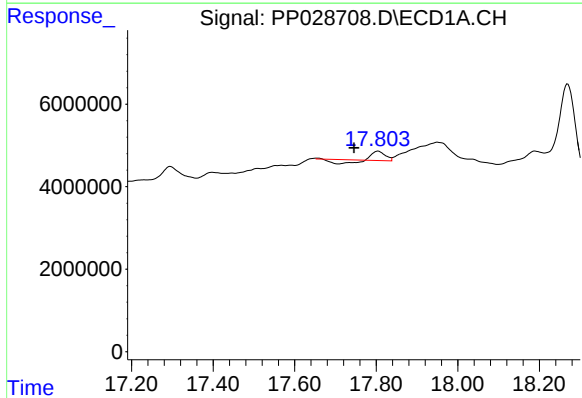


#15 Picloram

R.T.: 17.805 min
Delta R.T.: 0.059 min
Response: 1289812
Conc: 16.45 ng/ml

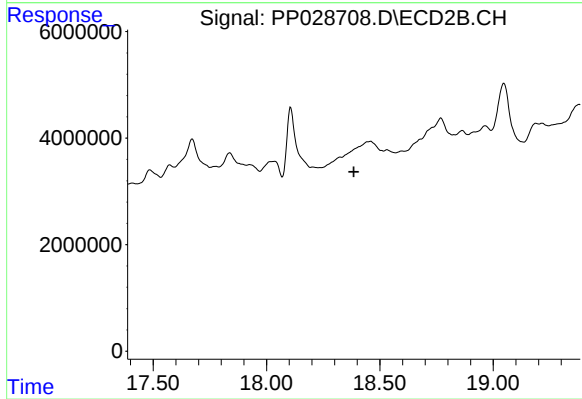

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 18.385 min
Response: 0
Conc: N.D.

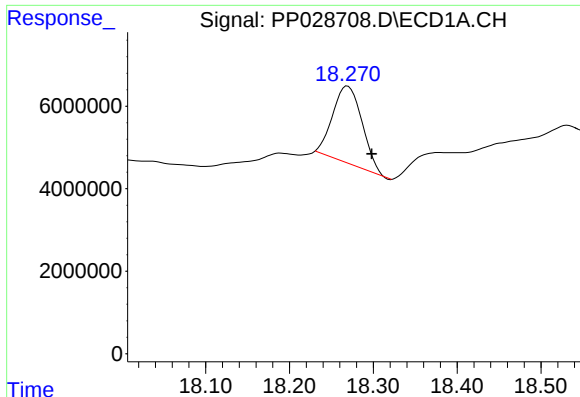

#16 DCPA

R.T.: 18.269 min
Delta R.T.: -0.029 min
Response: 45638294
Conc: 11.05 ng/ml

Instrument :
ECD_P
ClientSampleId :

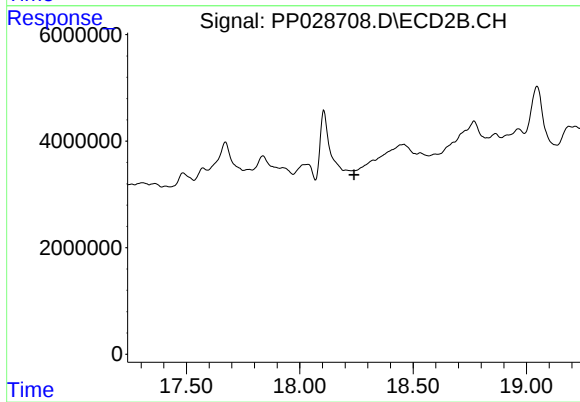

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 18.240 min
Response: 0
Conc: N.D.